

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052419\
 Data File : BF114585.D
 Acq On : 24 May 2019 22:18
 Operator : JU/SJ
 Sample : K3008-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-21

Quant Time: May 25 00:26:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 24 07:23:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	151566	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	573062	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	275529	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	570728	20.00	ng	0.00
76) Chrysene-d12	13.98	240	418432	20.00	ng	0.00
87) Perylene-d12	15.44	264	384678	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	1035205	109.91	ng	0.01
7) Phenol-d6	6.46	99	1229190	110.35	ng	0.00
23) Nitrobenzene-d5	7.37	82	889195	87.08	ng	0.00
42) 2,4,6-Tribromophenol	10.65	330	374106	131.33	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	1546493	84.90	ng	0.00
79) Terphenyl-d14	12.92	244	1784272	87.90	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052419\
Data File : BF114585.D
Acq On : 24 May 2019 22:18
Operator : JU/SJ
Sample : K3008-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-21

Quant Time: May 25 00:26:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 24 07:23:33 2019
Response via : Initial Calibration

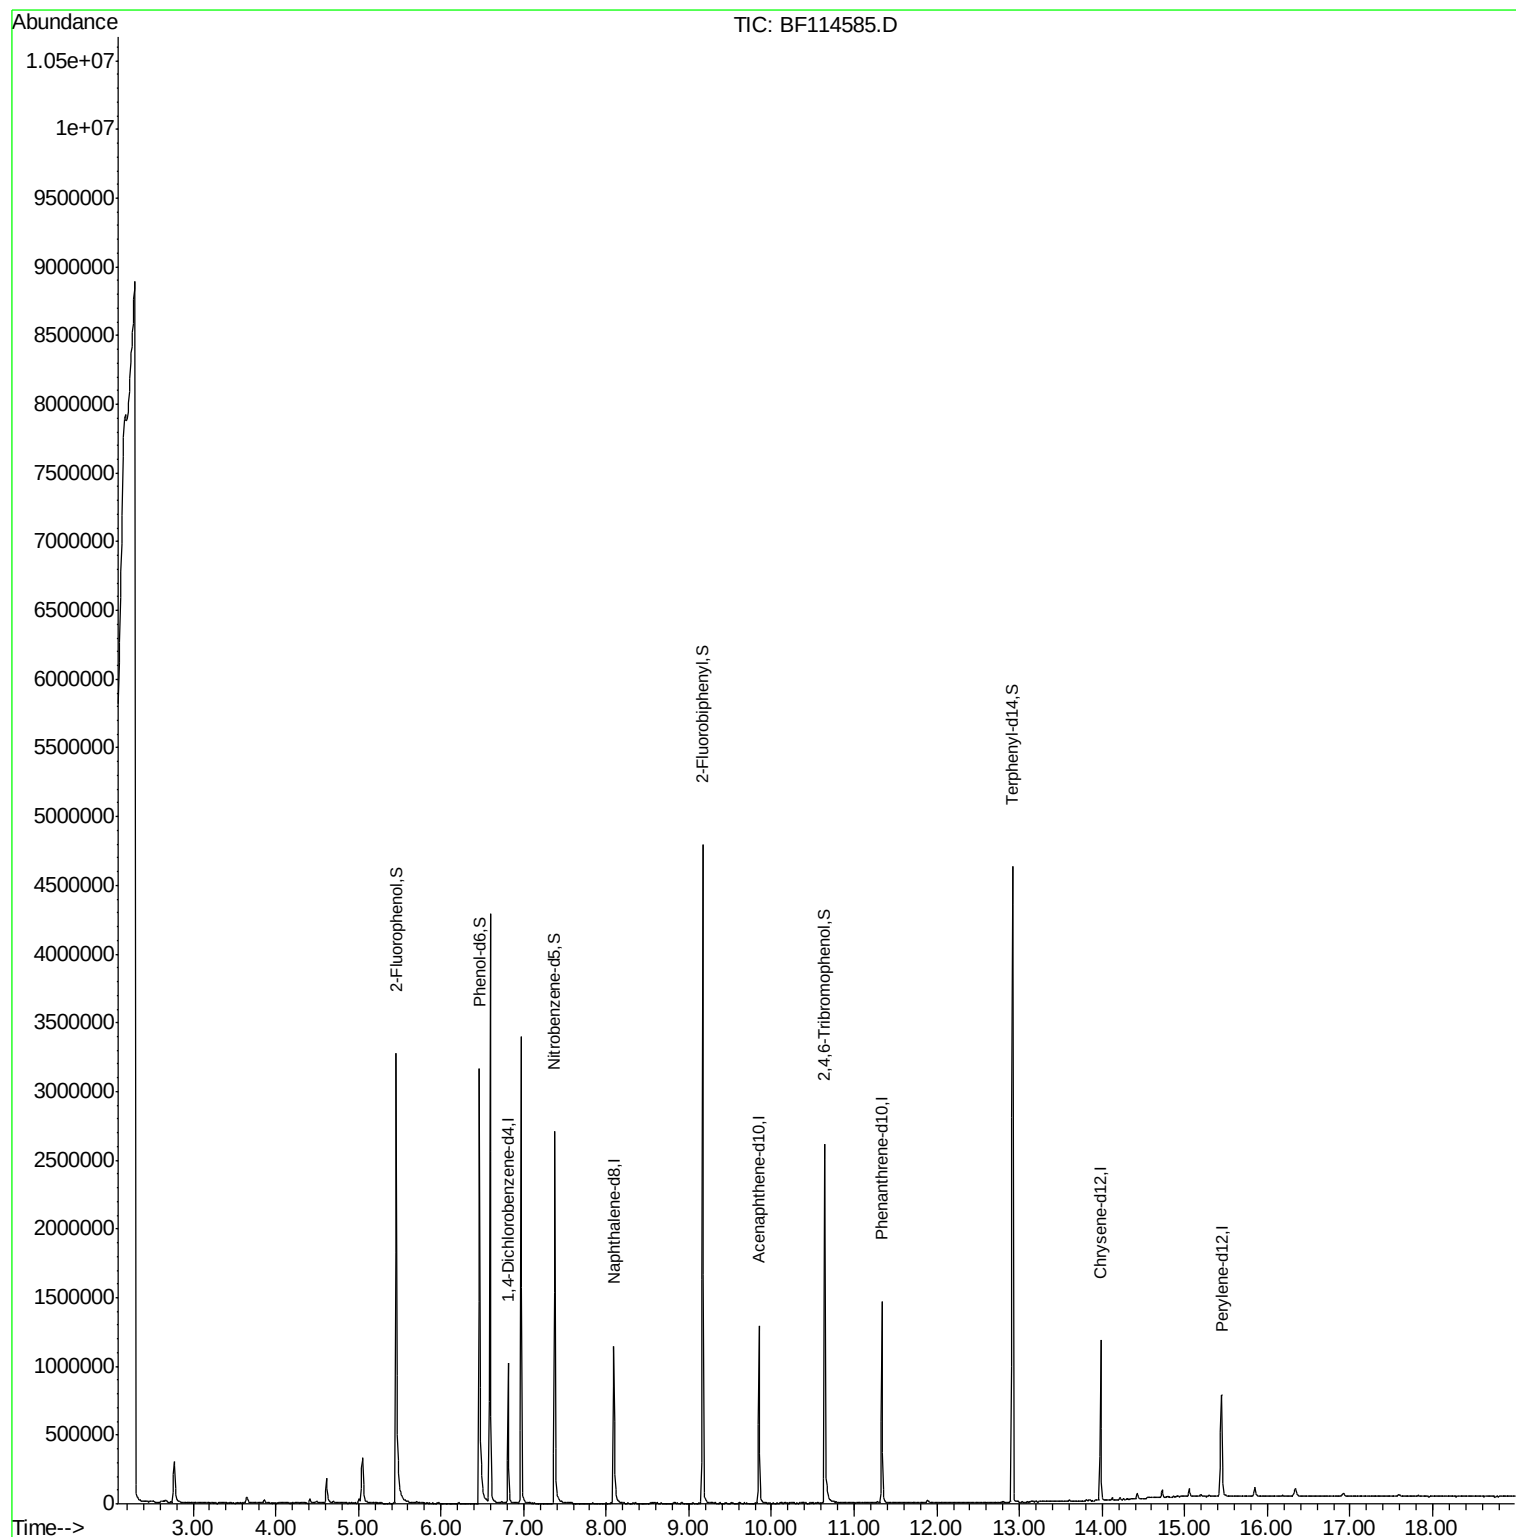

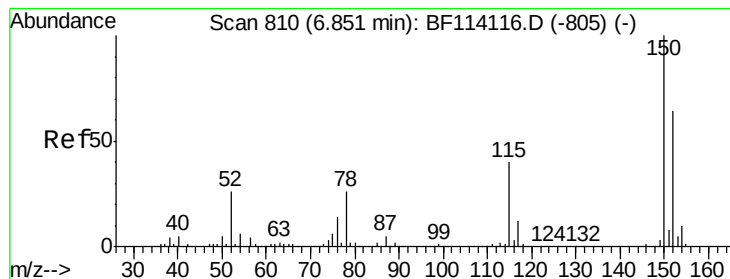


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.81 min Scan# 803
Delta R.T. -0.01 min
Lab File: BF114585.D
Acq: 24 May 2019 22:18

Instrument :
BNA_F
ClientSampleId :
COMP-21

Tot Ion:152 Resp: 151566
Ion Ratio Lower Upper
152 100
150 157.7 124.3 186.5
115 63.4 49.1 73.7

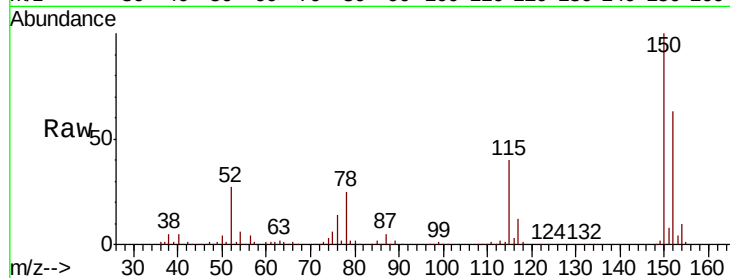


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

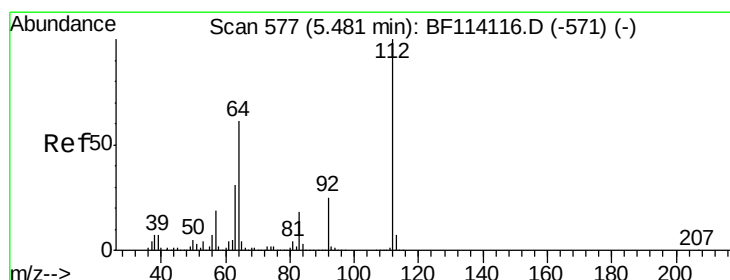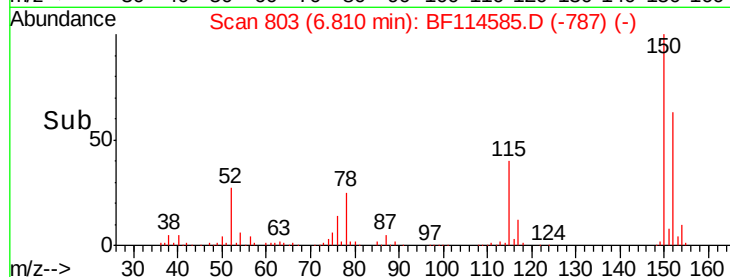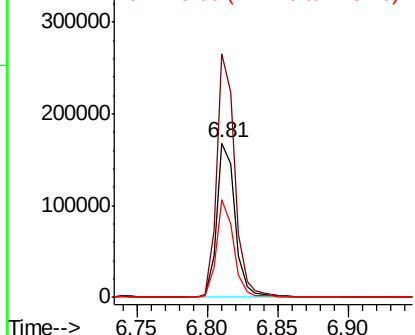



#5


2-Fluorophenol
Concen: 109.914 ng
RT: 5.46 min Scan# 573
Delta R.T. 0.01 min
Lab File: BF114585.D
Acq: 24 May 2019 22:18

Tgt Ion:112 Resp: 1035205
Ion Ratio Lower Upper
112 100
64 65.9 49.0 73.6
63 33.5 24.6 37.0

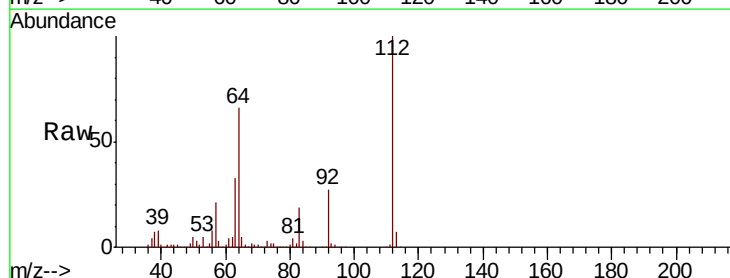

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

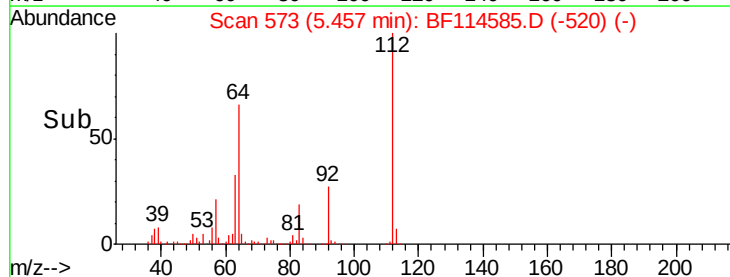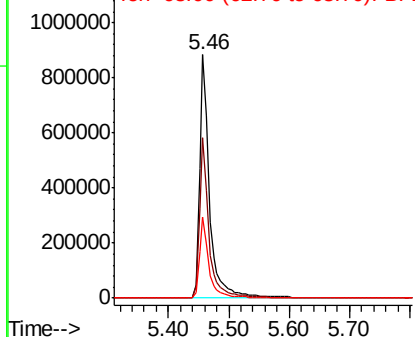

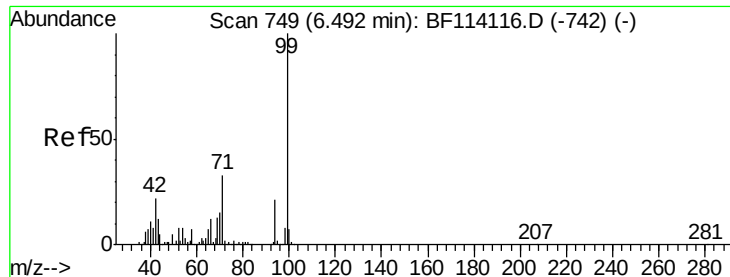

#7

Phenol-d6

Concen: 110.346 ng

RT: 6.46 min Scan# 744

Delta R.T. 0.00 min

Lab File: BF114585.D

Acq: 24 May 2019 22:18

Instrument :

BNA_F

ClientSampled :

COMP-21


Tot Ion: 99 Resp: 1229190

Ion Ratio Lower Upper




99 100

42 23.0 17.9 26.9

71 33.5 26.2 39.2

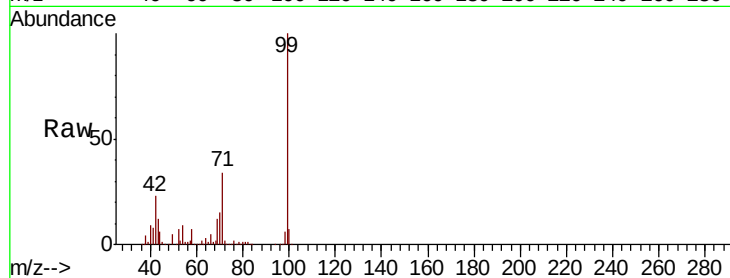

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

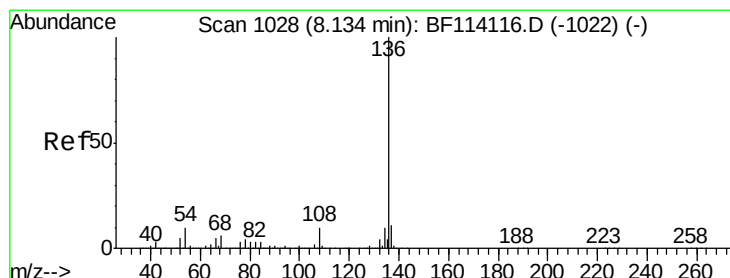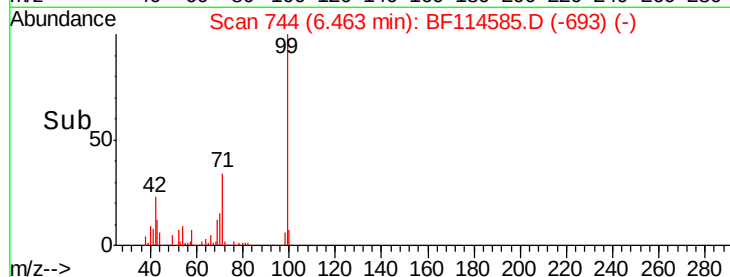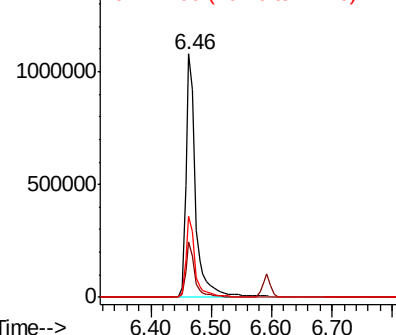

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BF114585.D

Acq: 24 May 2019 22:18

Tgt Ion: 136 Resp: 573062


Ion Ratio Lower Upper

136 100



137 10.6 8.8 13.2


54 9.1 7.8 11.8

68 5.3 5.1 7.7

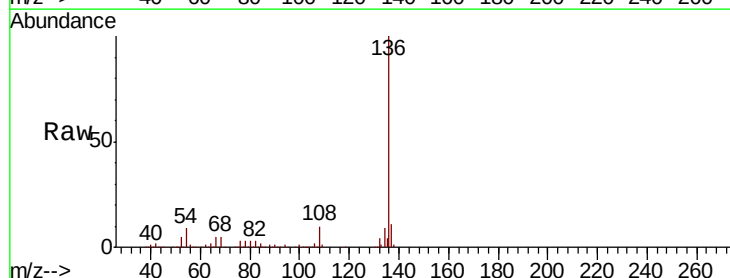

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



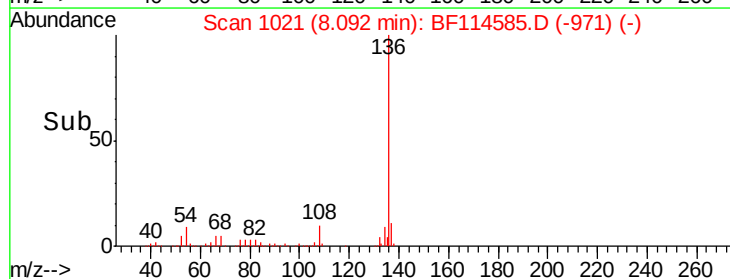
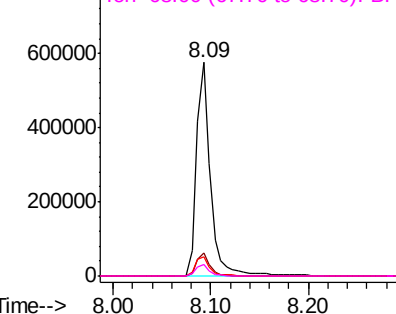


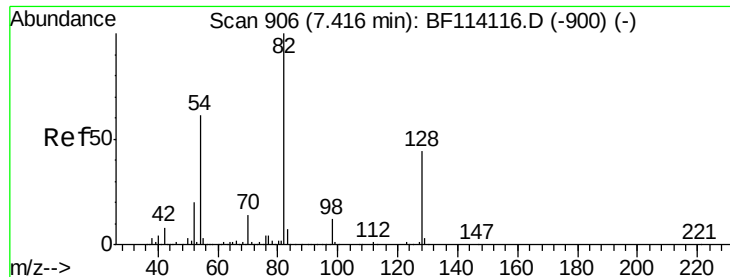

#23
 Nitrobenzene-d5
 Concen: 87.079 ng
 RT: 7.37 min Scan# 899
 Delta R.T. -0.01 min
 Lab File: BF114585.D
 Acq: 24 May 2019 22:18




Instrument :
 BNA_F
 ClientSampleId :
 COMP-21


Tot Ion	82	Resp	889195
Ion Ratio	Lower	Upper	
82	100		
128	43.5	35.5	53.3
54	58.9	48.5	72.7

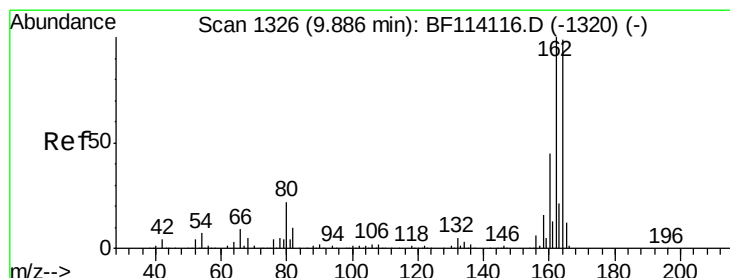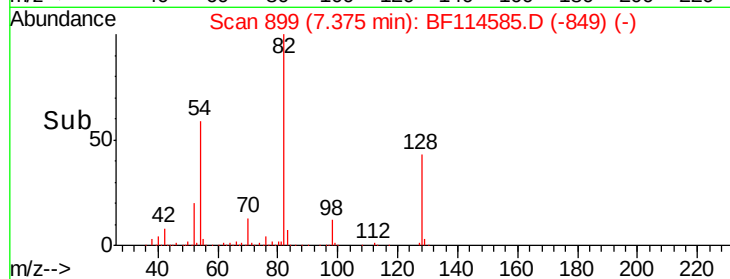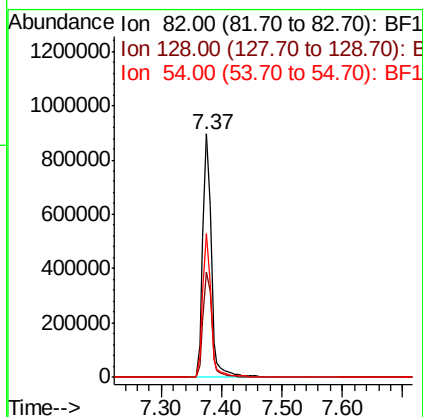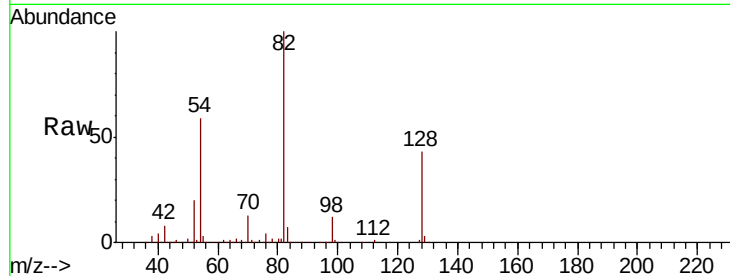

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.85 min Scan# 1319
 Delta R.T. -0.01 min
 Lab File: BF114585.D
 Acq: 24 May 2019 22:18

Tgt Ion	164	Resp	275529
Ion Ratio	Lower	Upper	
164	100		
162	100.3	80.6	120.8
160	45.4	36.5	54.7

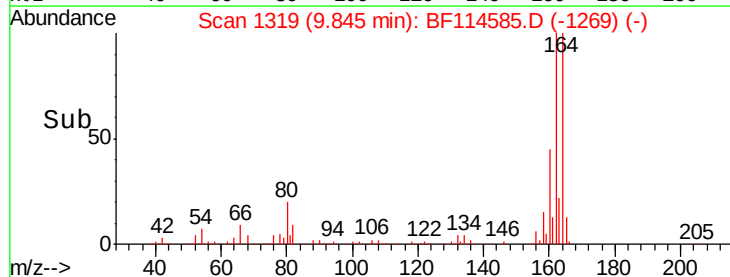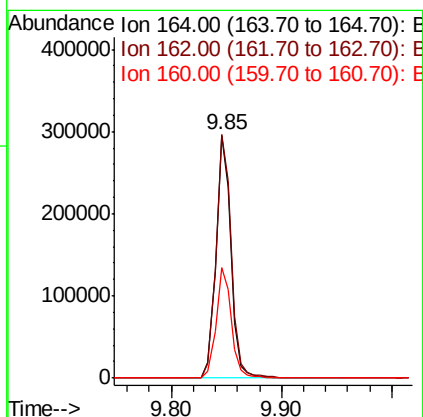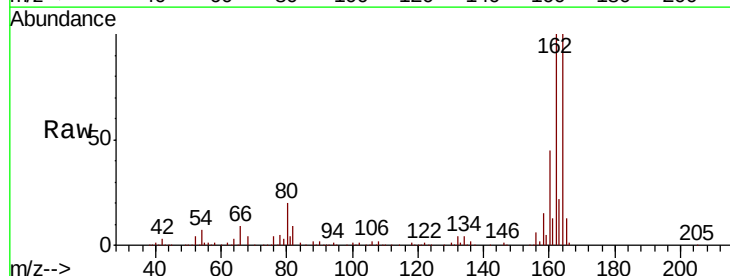

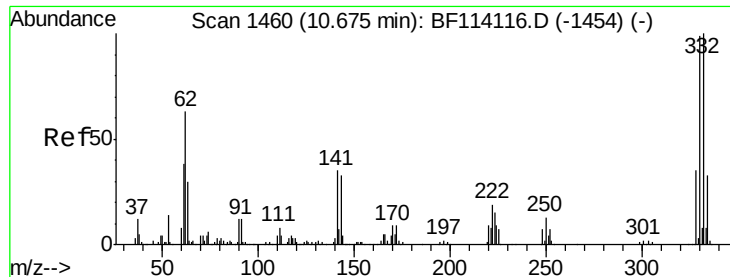

#42

2,4,6-Tribromophenol

Concen: 131.334 ng

RT: 10.65 min Scan# 1455

Delta R.T. 0.00 min

Lab File: BF114585.D

Acq: 24 May 2019 22:18

Instrument :

BNA_F

ClientSampleId :

COMP-21


Tot Ion:330 Resp: 374106

Ion Ratio Lower Upper

330 100

332 102.7 81.4 122.2




141 33.0 26.6 40.0

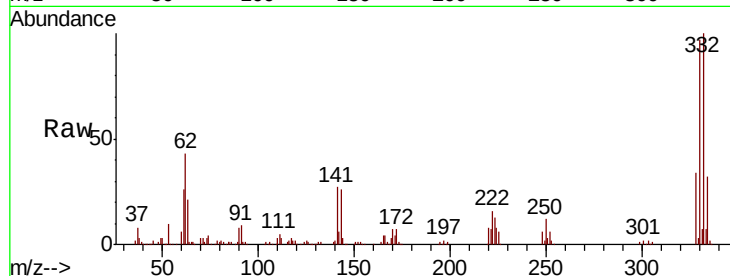

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

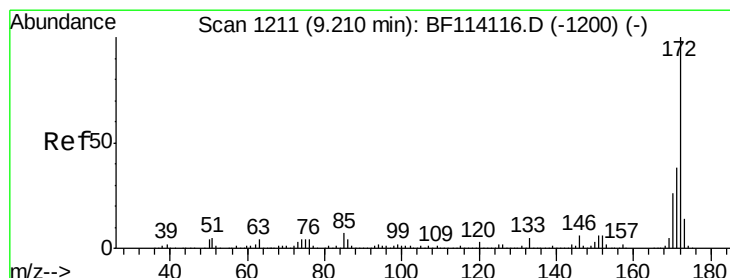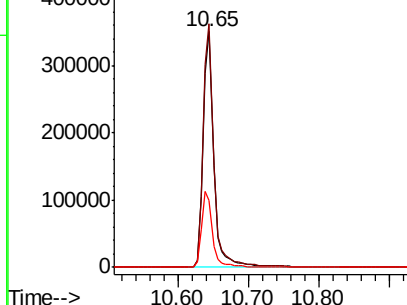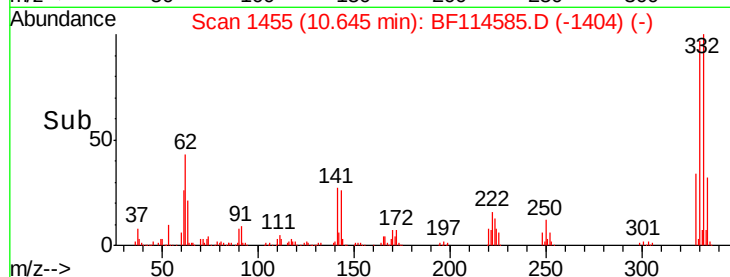

#45

2-Fluorobiphenyl

Concen: 84.903 ng

RT: 9.17 min Scan# 1204

Delta R.T. -0.01 min

Lab File: BF114585.D

Acq: 24 May 2019 22:18


Tgt Ion:172 Resp: 1546493

Ion Ratio Lower Upper

172 100

171 36.7 30.7 46.1



170 24.3 20.5 30.7

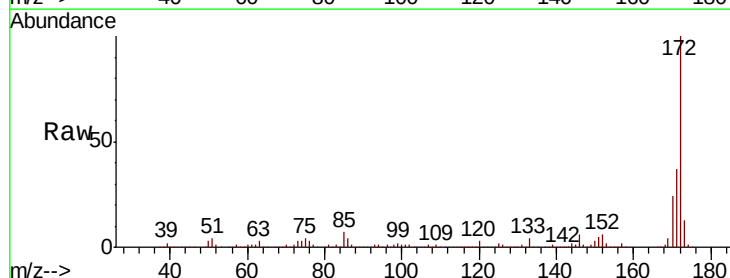


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

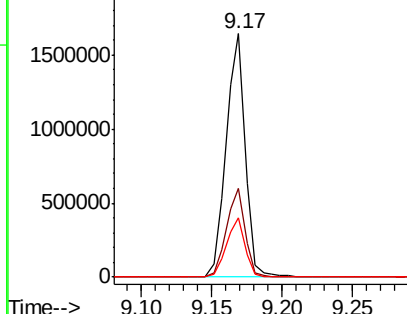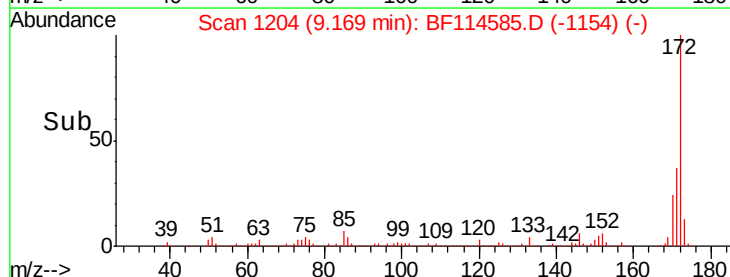

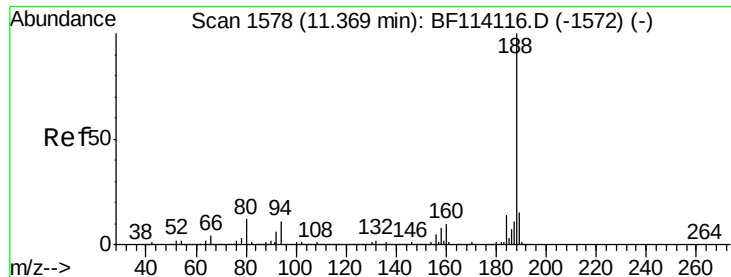

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1572

Delta R.T. -0.01 min

Lab File: BF114585.D

Acq: 24 May 2019 22:18

Instrument :

BNA_F

ClientSampleId :

COMP-21





Tot Ion:188 Resp: 570728

Ion Ratio Lower Upper

188 100

94 10.0 8.4 12.6

80 10.1 9.2 13.8

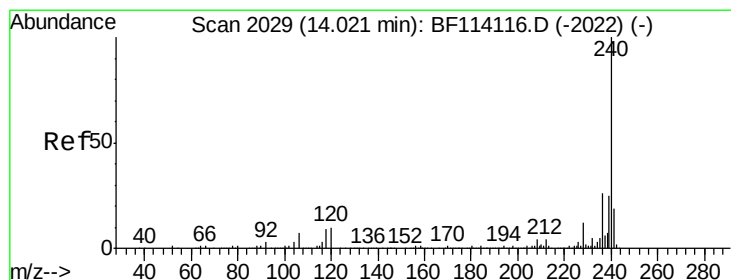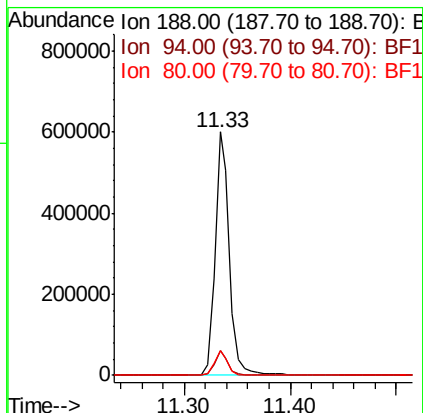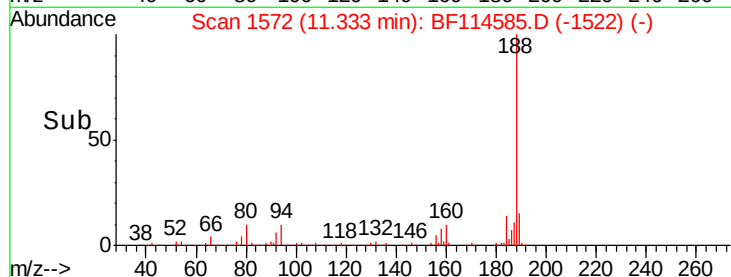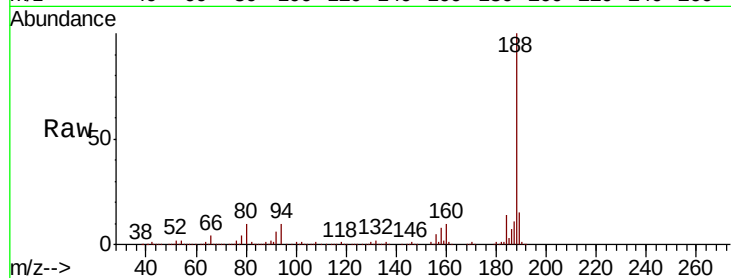

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.98 min Scan# 2022

Delta R.T. -0.01 min

Lab File: BF114585.D

Acq: 24 May 2019 22:18




Tgt Ion:240 Resp: 418432


Ion Ratio Lower Upper

240 100

120 10.4 8.3 12.5

236 26.0 20.8 31.2


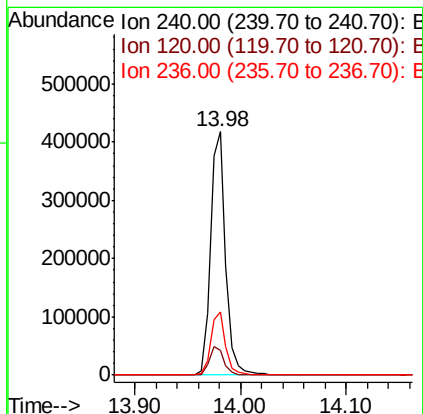
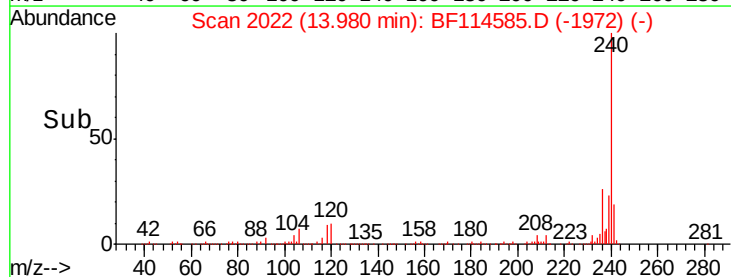
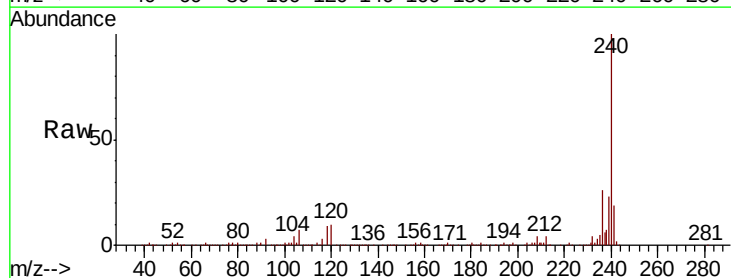


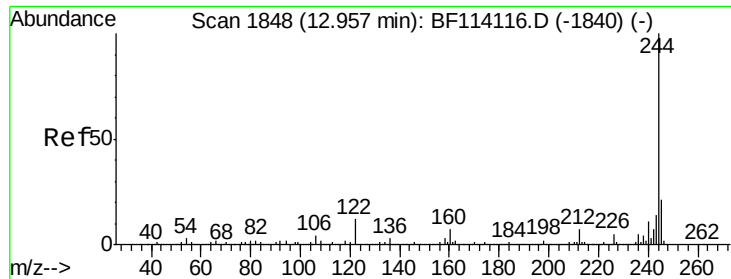

#79
 Terphenyl-d14
 Concen: 87.903 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BF114585.D
 Acq: 24 May 2019 22:18

Instrument :
 BNA_F
 ClientSampleId :
 COMP-21

Tot Ion:244 Resp: 1784272
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 13.1 9.4 14.2

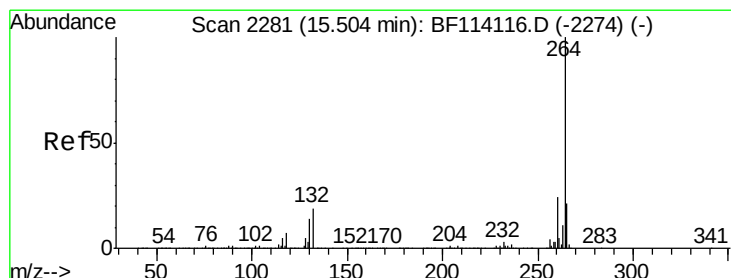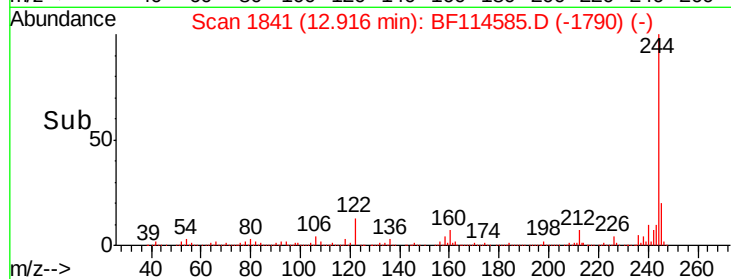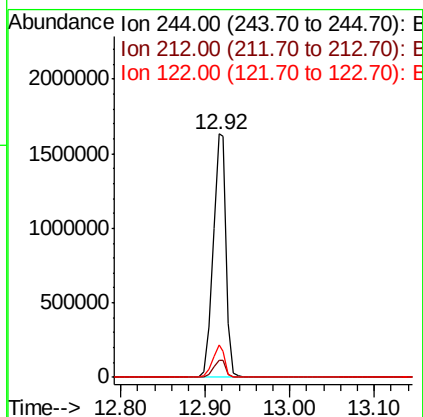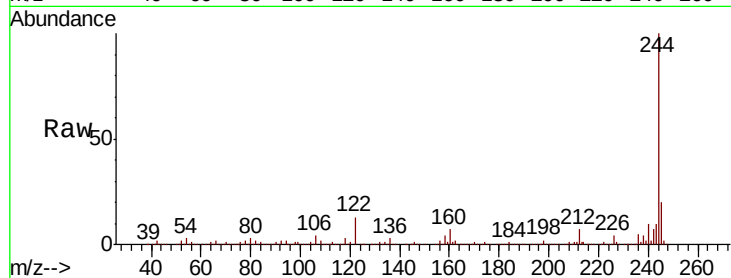

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2271
 Delta R.T. -0.01 min
 Lab File: BF114585.D
 Acq: 24 May 2019 22:18

Tgt Ion:264 Resp: 384678
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.4 29.0
 265 22.3 16.9 25.3

