

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052419\
 Data File : BF114590.D
 Acq On : 25 May 2019 00:29
 Operator : JU/SJ
 Sample : K2954-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20190332A-GLP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	568	571	594	rBV	1890605	2222597	92.94%	10.099%
2	6.457	740	743	762	rBV	1906354	2391542	100.00%	10.867%
3	6.587	762	765	782	rVB	2459641	2323839	97.17%	10.559%
4	6.810	800	803	812	rBV	868582	769849	32.19%	3.498%
5	6.969	826	830	839	rBV	1824283	1633885	68.32%	7.424%
6	7.375	895	899	913	rBV	1444856	1427035	59.67%	6.484%
7	8.092	1018	1021	1043	rVB	1031936	979015	40.94%	4.449%
8	9.163	1200	1203	1216	rBV	2129324	2004022	83.80%	9.106%
9	9.563	1268	1271	1280	rBV	339036	304550	12.73%	1.384%
10	9.845	1316	1319	1332	rBV	1173698	1082112	45.25%	4.917%
11	10.639	1451	1454	1470	rBV	1272394	1308503	54.71%	5.946%
12	11.333	1569	1572	1584	rBV	1214179	1184720	49.54%	5.383%
13	11.863	1659	1662	1669	rBV4	20697	32163	1.34%	0.146%
14	12.910	1837	1840	1844	rBV	1765872	1657742	69.32%	7.533%
15	13.804	1988	1992	2006	rBV	212390	403989	16.89%	1.836%
16	13.980	2018	2022	2029	rBV	985945	965554	40.37%	4.387%
17	14.121	2043	2046	2049	rBV3	20822	24875	1.04%	0.113%
18	14.427	2095	2098	2100	rBV	41990	45415	1.90%	0.206%
19	14.451	2100	2102	2110	rVB6	28568	49499	2.07%	0.225%
20	14.727	2145	2149	2153	rBV	46908	52163	2.18%	0.237%
21	14.798	2158	2161	2165	rVB	43488	43036	1.80%	0.196%
22	15.057	2201	2205	2208	rBV	68489	75870	3.17%	0.345%
23	15.439	2264	2270	2280	rBV	619174	902220	37.73%	4.100%
24	15.845	2336	2339	2345	rVB2	52422	78764	3.29%	0.358%
25	16.339	2419	2423	2428	rBV2	25948	44671	1.87%	0.203%


Sum of corrected areas: 22007630

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052419\
Data File : BF114590.D
Acq On : 25 May 2019 00:29
Operator : JU/SJ
Sample : K2954-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20190332A-GLP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

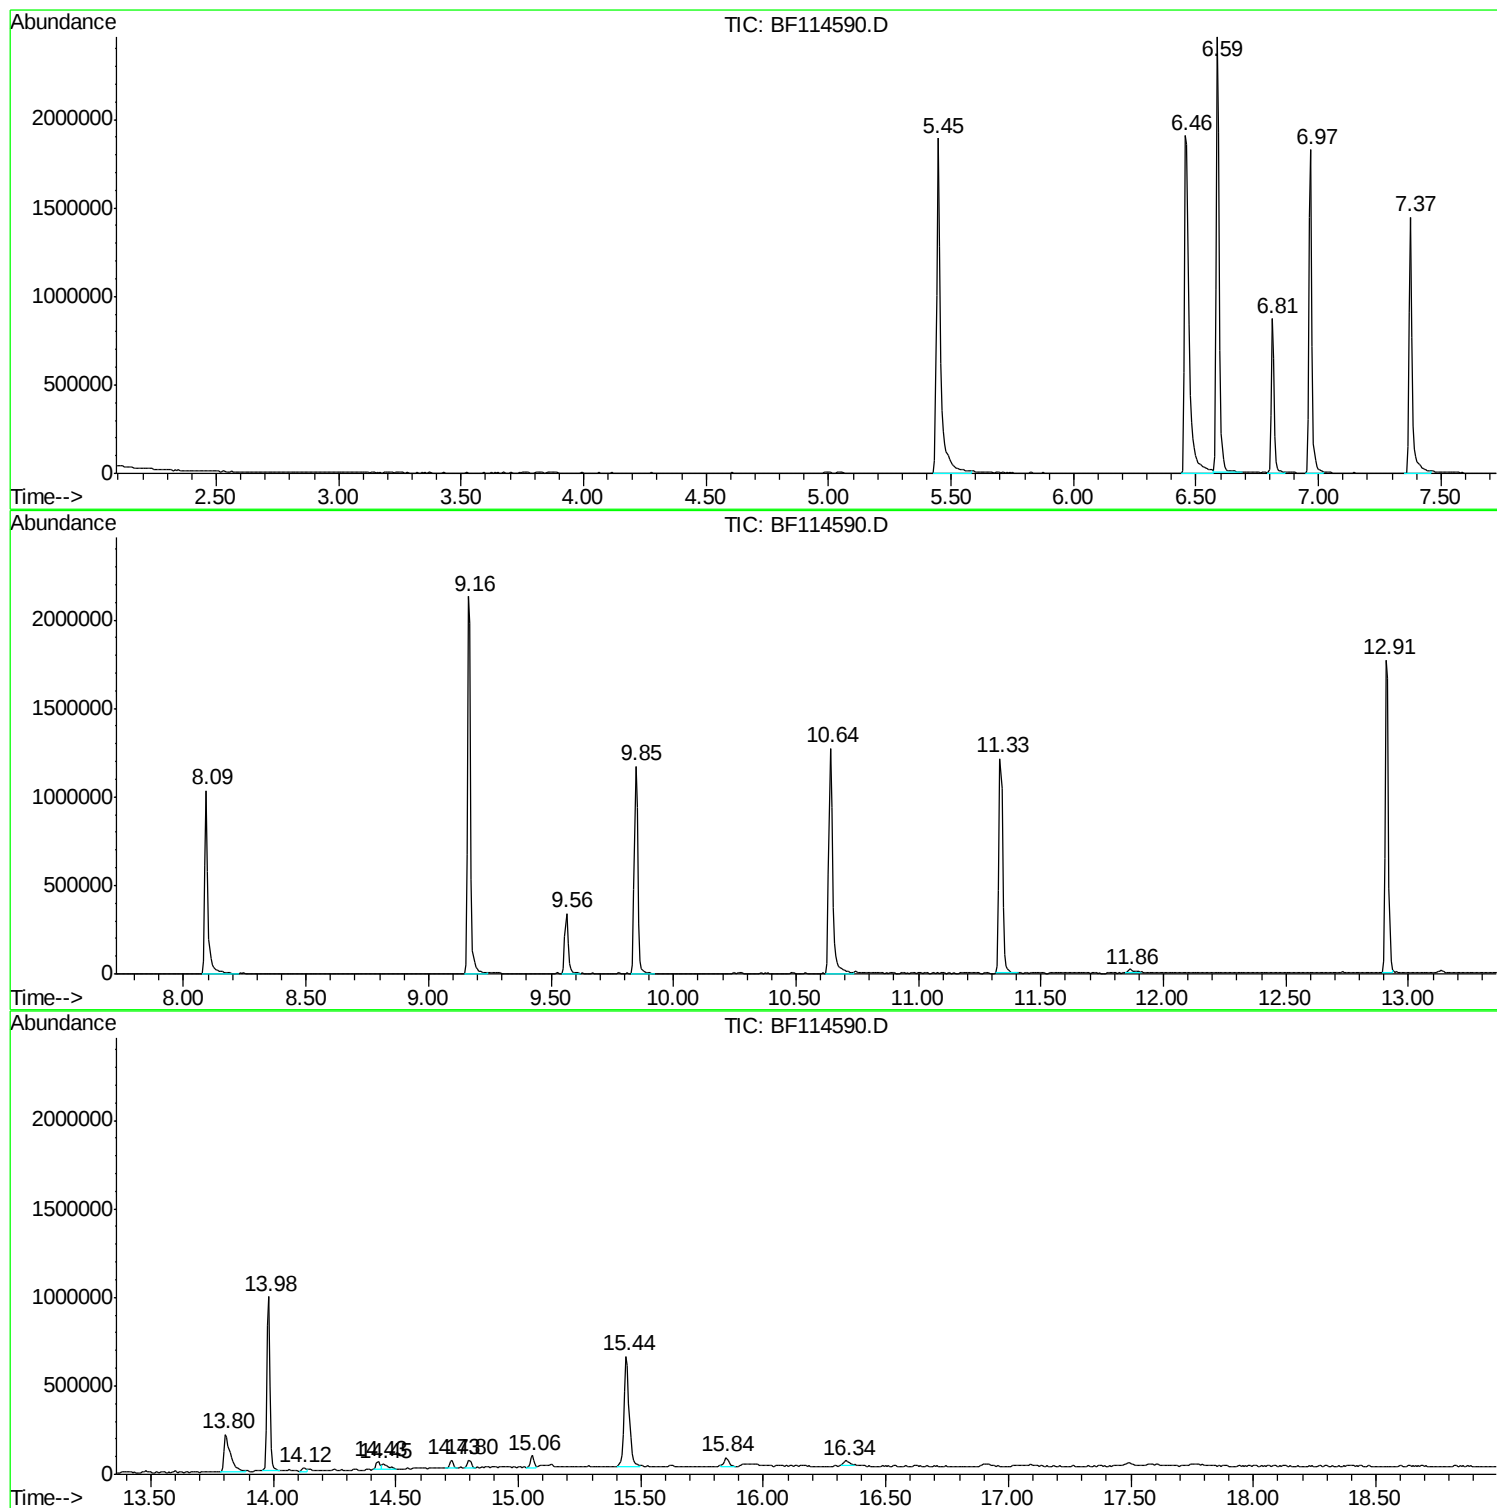

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052419\
Data File : BF114590.D
Acq On : 25 May 2019 00:29
Operator : JU/SJ
Sample : K2954-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20190332A-GLP-1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	60.37 ng	2323840	1,4-Dichlorobenzene-d4	6.81

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27	
2	5-Aminoindole	132	C8H8N2	005192-03-0	12	
3	Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10	
4	1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9	
5	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9	

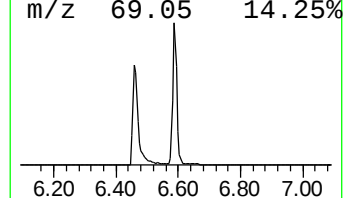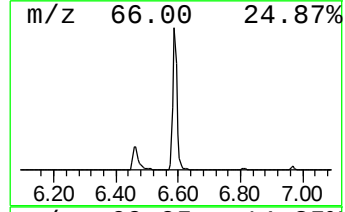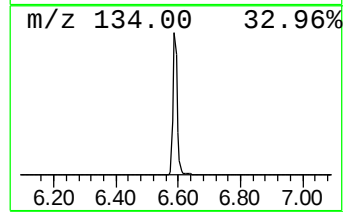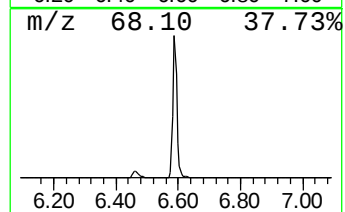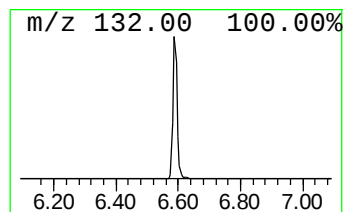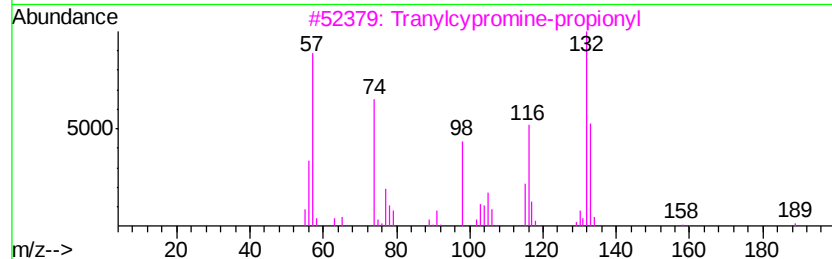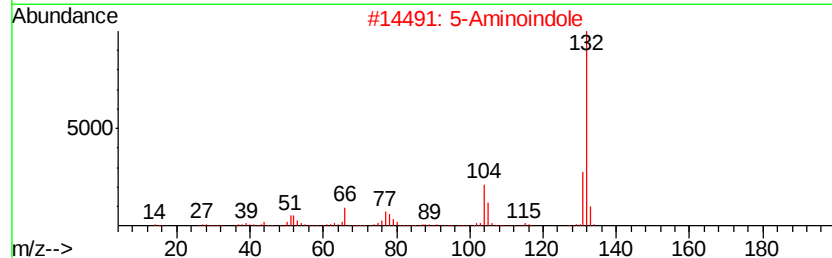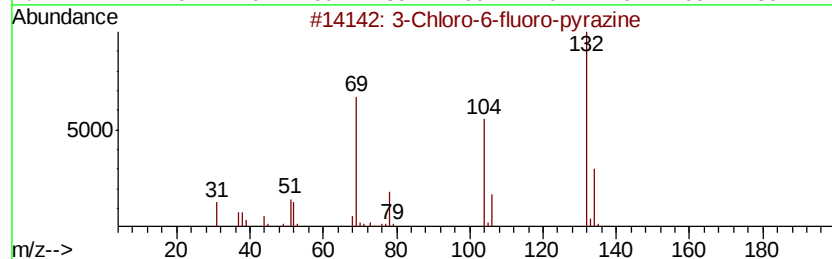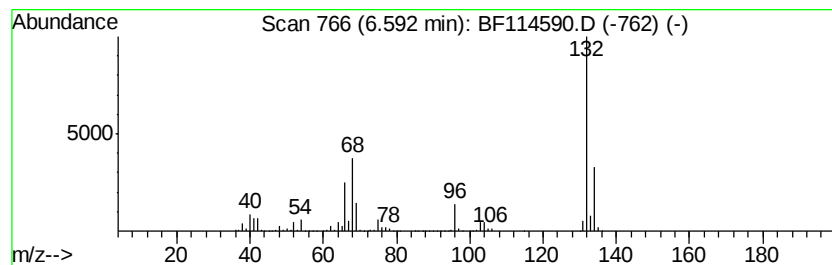

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052419\
Data File : BF114590.D
Acq On : 25 May 2019 00:29
Operator : JU/SJ
Sample : K2954-03
Misc :
ALS Vial : 19 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
20190332A-GLP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Trifluoroacetoxy hexadecane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD		R.T.	
13.80	8.37 ng	403989	Chrysene-d12		13.98	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Trifluoroacetoxv hexadecane	338	C18H33F3O2	006222-03-3	91
2		Heptadecyl trifluoroacetate	352	C19H35F3O2	1000351-87-0	91
3		3-Chloropropionic acid, heptadec...	346	C20H39ClO2	1000283-05-1	91
4		Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	87
5		1-Heneicosanol	312	C21H44O	015594-90-8	87

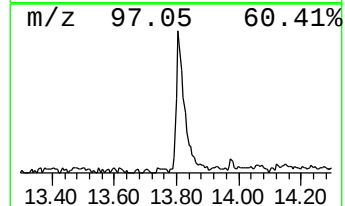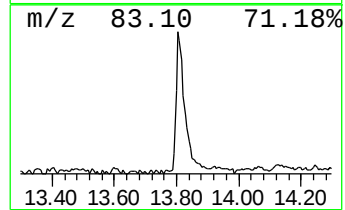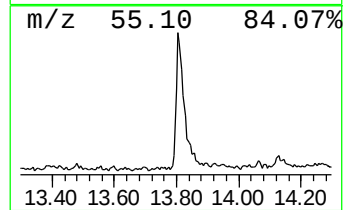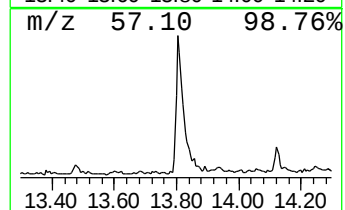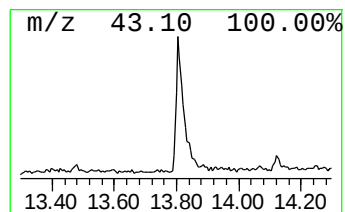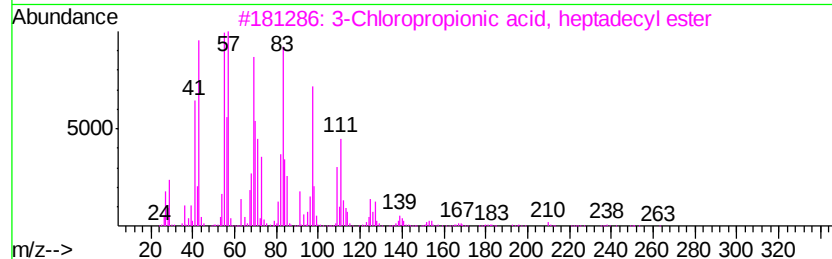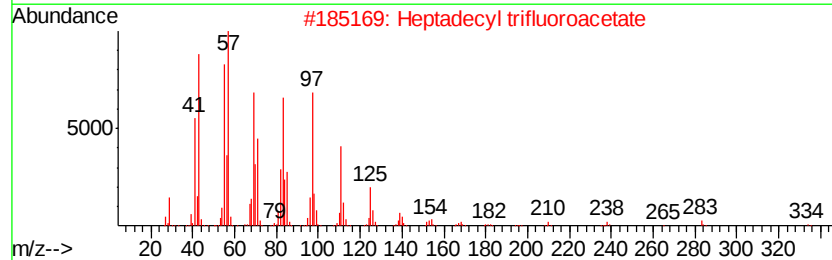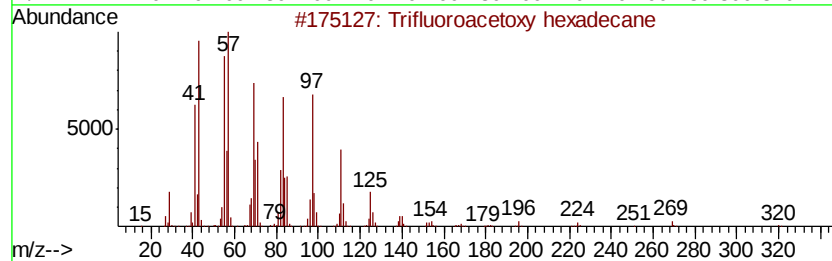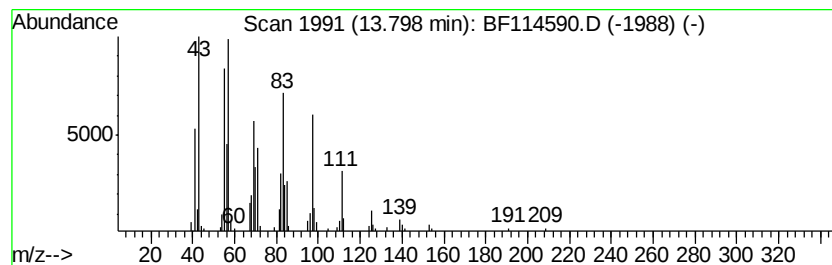

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052419\
Data File : BF114590.D
Acq On : 25 May 2019 00:29
Operator : JU/SJ
Sample : K2954-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20190332A-GLP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.59	6.59	60.4	ng	2323840	1	6.81	769849	20.0
Trifluoroacetoxy ...	13.80	8.4	ng	403989	5	13.98	965554	20.0