


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052419\
 Data File : BF114572.D
 Acq On : 24 May 2019 16:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 07:23:33 2019

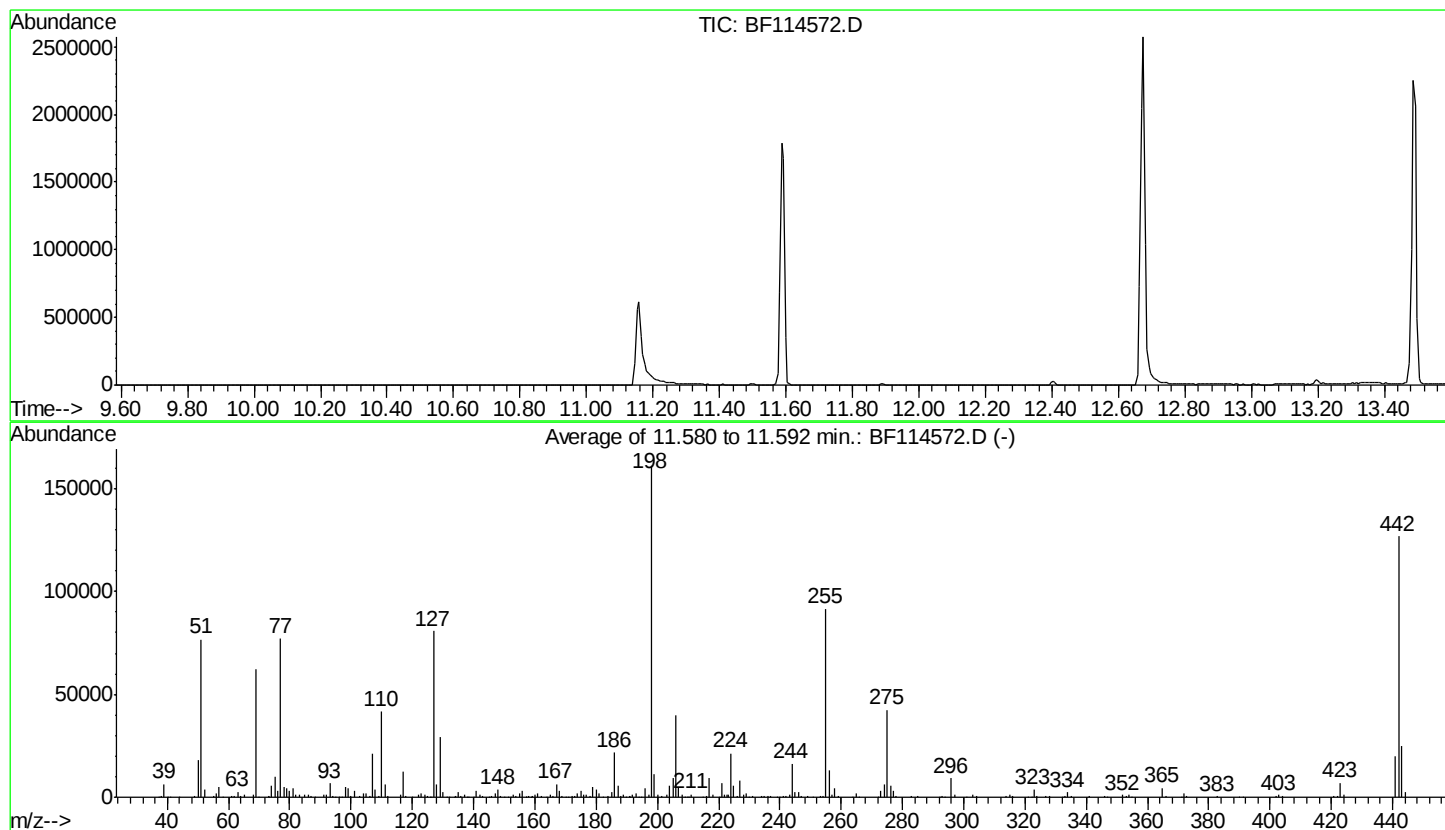

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	76813	PASS
68	69	0.00	2	1.6	975	PASS
69	198	0.00	100	38.7	62416	PASS
70	69	0.00	2	0.4	256	PASS
127	198	10	80	50.1	80818	PASS
197	198	0.00	2	0.7	1182	PASS
198	198	100	100	100.0	161176	PASS
199	198	5	9	6.8	11026	PASS
275	198	10	60	26.3	42432	PASS
365	198	1	100	2.7	4387	PASS
441	198	0.01	100	12.5	20160	PASS
442	198	50	100	78.7	126770	PASS
443	442	15	24	19.4	24649	PASS