


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052419\
Data File : BF114596.D
Acq On : 25 May 2019 3:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 24 07:23:33 2019

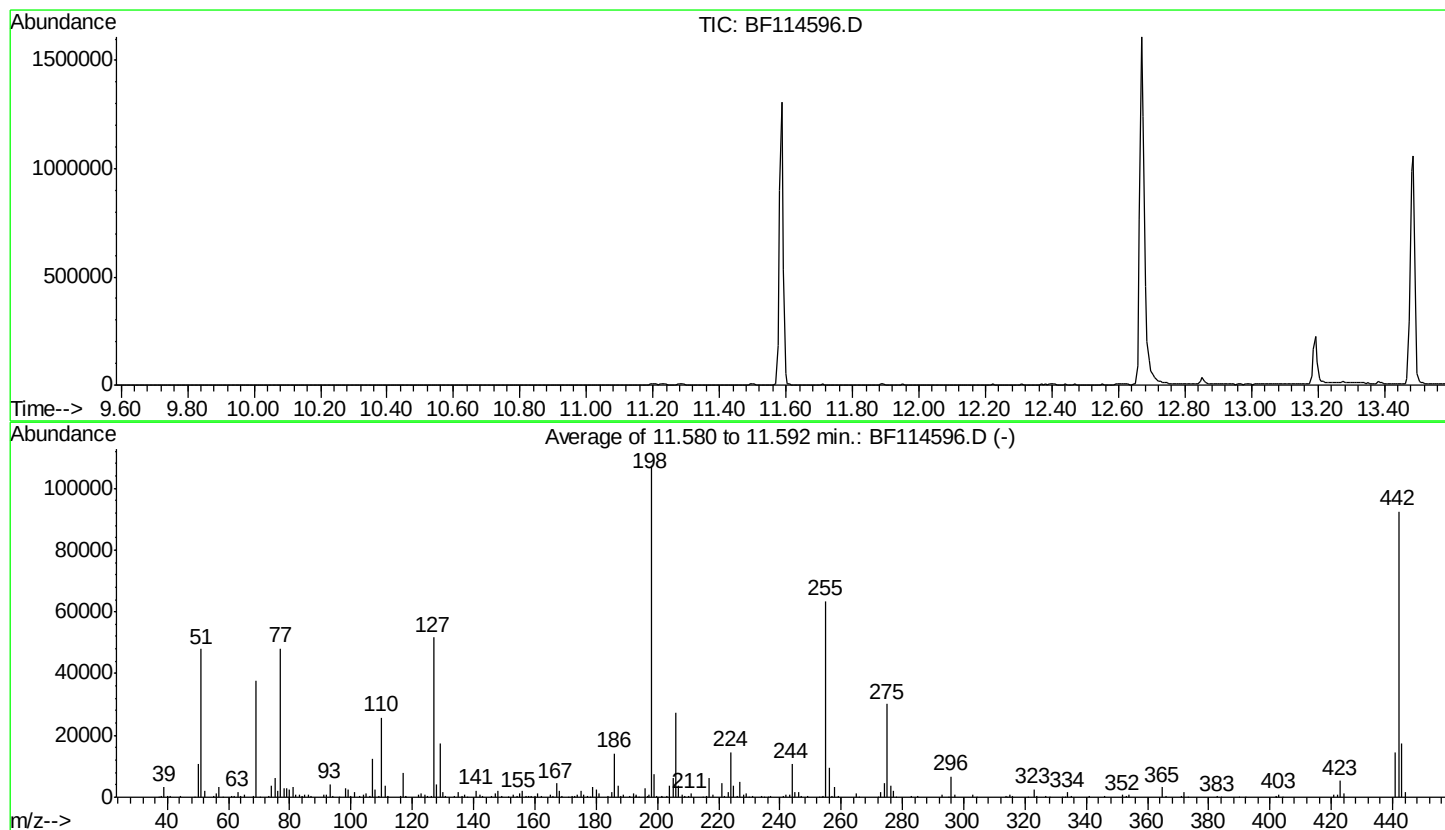

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	47896	PASS
68	69	0.00	2	1.6	609	PASS
69	198	0.00	100	35.3	37864	PASS
70	69	0.00	2	0.4	161	PASS
127	198	10	80	48.2	51661	PASS
197	198	0.00	2	0.7	716	PASS
198	198	100	100	100.0	107288	PASS
199	198	5	9	6.8	7281	PASS
275	198	10	60	28.0	30088	PASS
365	198	1	100	3.1	3306	PASS
441	198	0.01	100	13.4	14372	PASS
442	198	50	100	86.3	92538	PASS
443	442	15	24	18.7	17286	PASS