

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052519\
 Data File : BF114607.D
 Acq On : 25 May 2019 16:46
 Operator : JU/SJ
 Sample : PB119807BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB119807BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	5	23	rVB	73396	127458	2.40%	0.291%
2	5.439	566	570	604	rBV	4274003	4542729	85.36%	10.359%
3	6.451	737	742	759	rBV	4280991	4761922	89.48%	10.859%
4	6.575	759	763	781	rVB	4724618	4590517	86.26%	10.468%
5	6.798	798	801	812	rBV	1266090	1125675	21.15%	2.567%
6	6.957	824	828	846	rBV	3773888	3653765	68.66%	8.332%
7	7.363	893	897	916	rBV	2767769	3038659	57.10%	6.929%
8	8.080	1015	1019	1039	rBV	1462497	1453291	27.31%	3.314%
9	9.157	1197	1202	1205	rBV	5474633	5321600	100.00%	12.136%
10	9.833	1313	1317	1332	rBV	1660074	1652923	31.06%	3.769%
11	10.627	1448	1452	1478	rBV	3120592	3288763	61.80%	7.500%
12	11.321	1567	1570	1581	rBV	1936440	1788314	33.60%	4.078%
13	12.910	1835	1840	1843	rBV	5006814	5203722	97.78%	11.867%
14	13.968	2016	2020	2031	rBV	1543395	1540520	28.95%	3.513%
15	15.039	2198	2202	2207	rBV	58709	71845	1.35%	0.164%
16	15.421	2260	2267	2278	rVB	1088598	1502664	28.24%	3.427%
17	15.827	2331	2336	2341	rVB	71214	104115	1.96%	0.237%
18	16.309	2414	2418	2423	rBV2	50080	82774	1.56%	0.189%


Sum of corrected areas: 43851256

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052519\
Data File : BF114607.D
Acq On : 25 May 2019 16:46
Operator : JU/SJ
Sample : PB119807BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119807BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

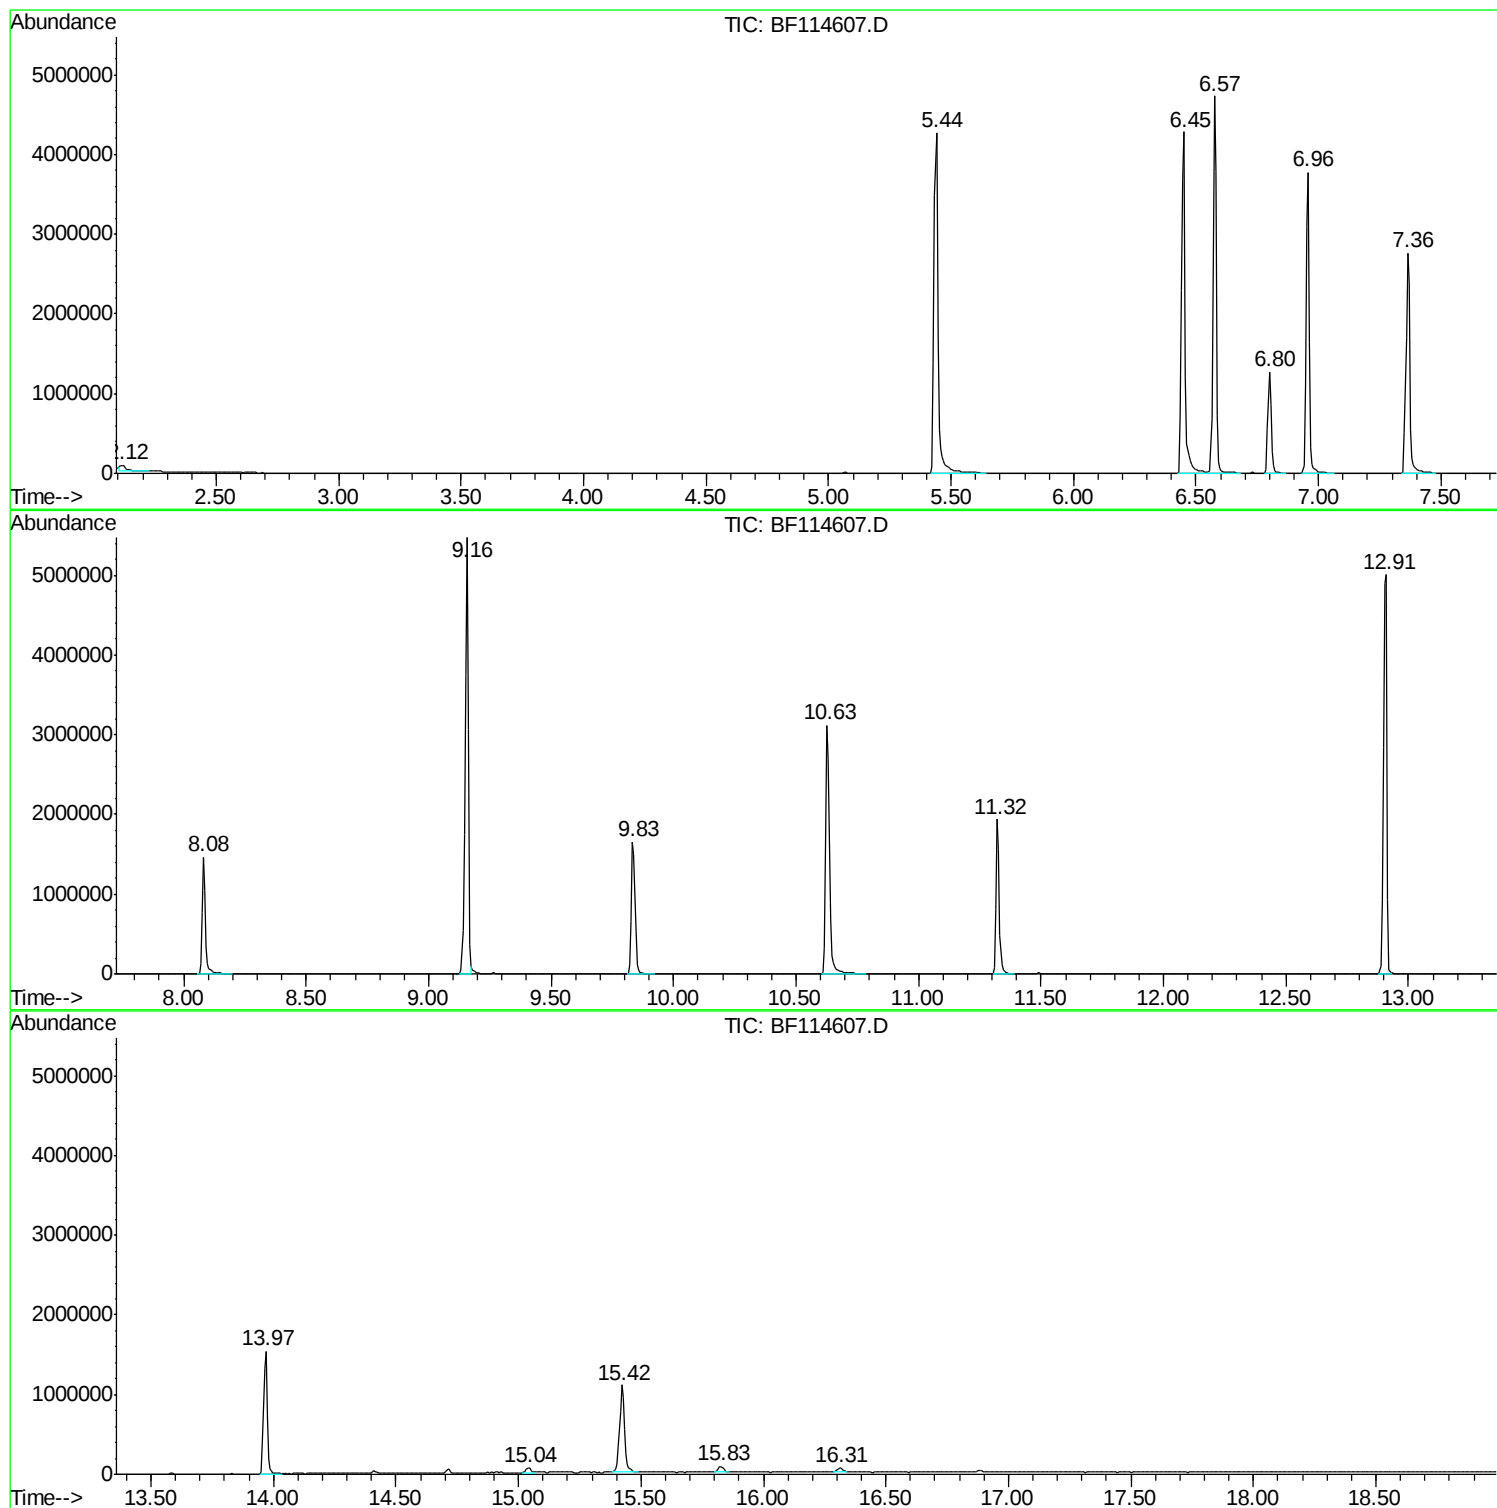

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052519\
Data File : BF114607.D
Acq On : 25 May 2019 16:46
Operator : JU/SJ
Sample : PB119807BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119807BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052519\
Data File : BF114607.D
Acq On : 25 May 2019 16:46
Operator : JU/SJ
Sample : PB119807BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119807BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc