


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052519\
 Data File : BF114601.D
 Acq On : 25 May 2019 13:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 07:23:33 2019

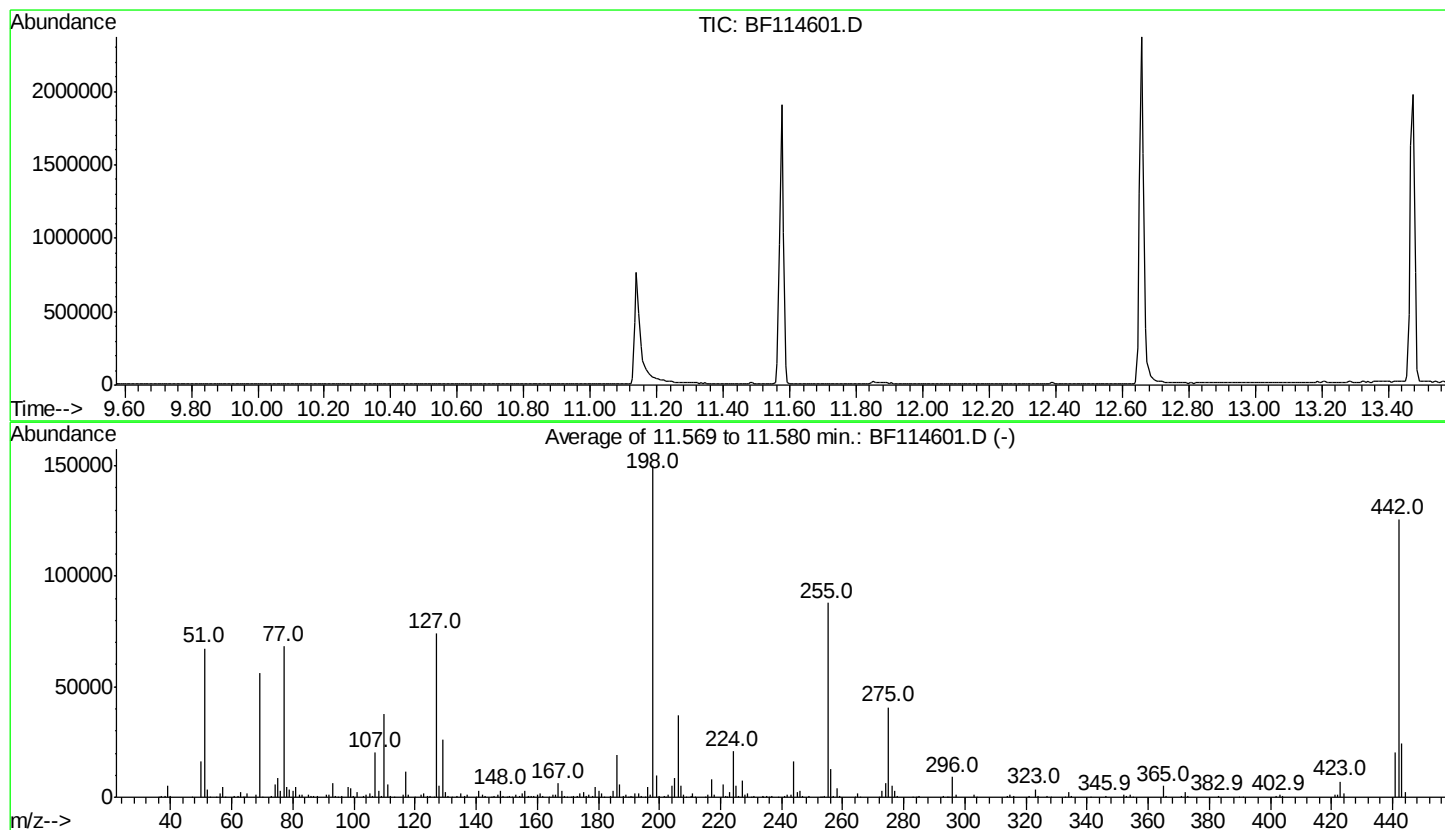

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	67381	PASS
68	69	0.00	2	1.7	959	PASS
69	198	0.00	100	37.4	56189	PASS
70	69	0.00	2	0.3	175	PASS
127	198	10	80	49.3	74010	PASS
197	198	0.00	2	0.7	1012	PASS
198	198	100	100	100.0	150082	PASS
199	198	5	9	6.6	9972	PASS
275	198	10	60	27.2	40858	PASS
365	198	1	100	3.3	4984	PASS
441	198	0.01	100	13.5	20197	PASS
442	198	50	100	83.7	125640	PASS
443	442	15	24	19.5	24454	PASS