
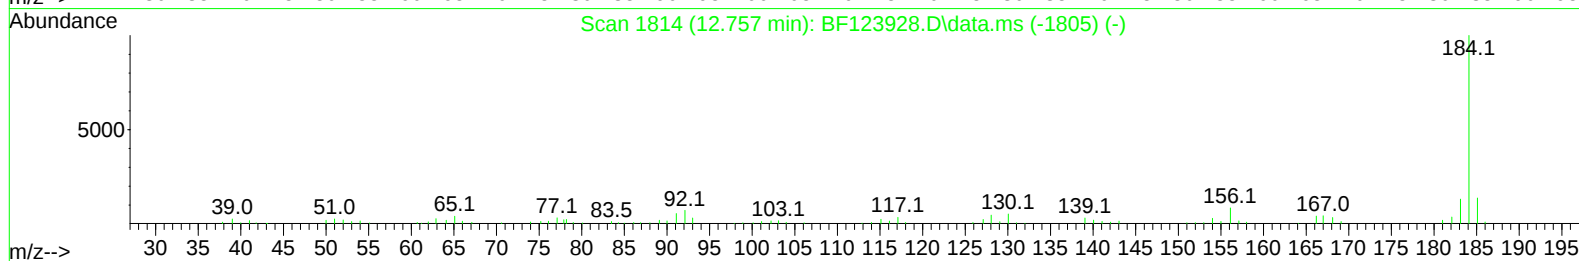
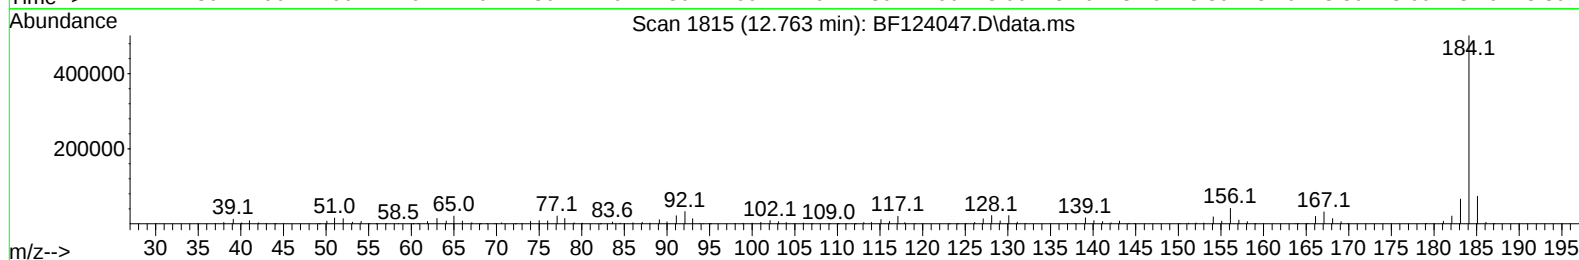


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052521\  
 Data File : BF124047.D  
 Acq On : 25 May 2021 15:47  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 16:22:27 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051421.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri May 14 19:05:57 2021  
 Response via : Initial Calibration

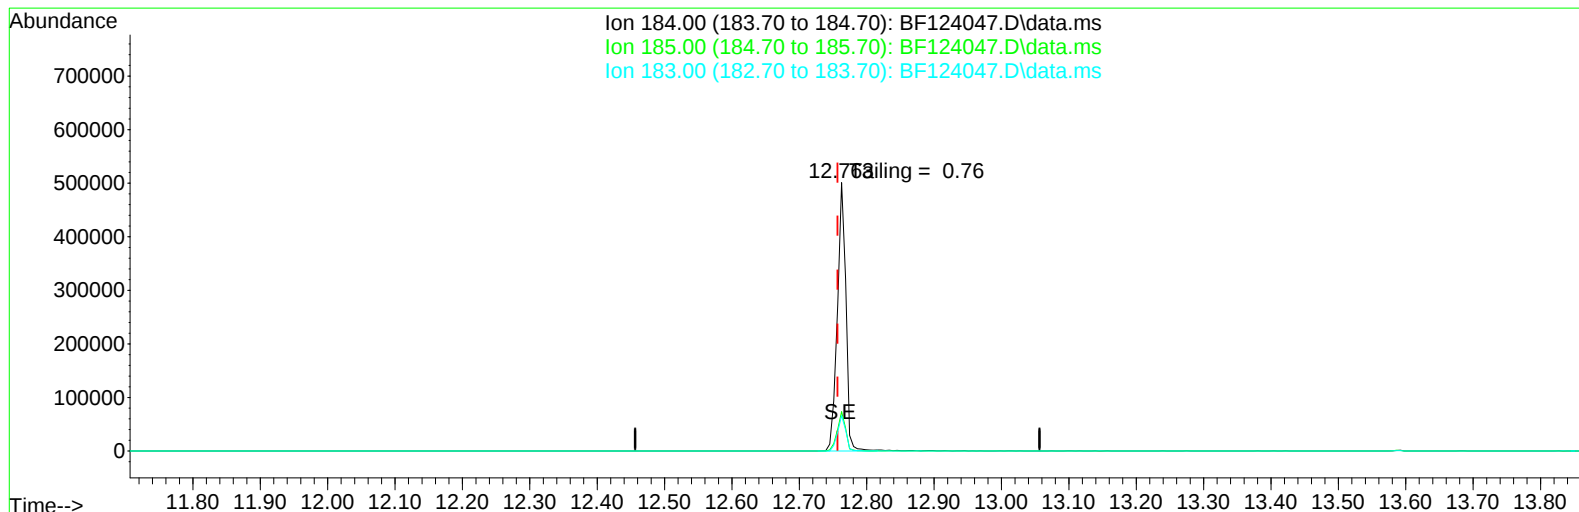

TIC: BF124047.D\data.ms

**(77) Benzidine**




12.763min (+ 0.006) 0.00 ng

response 446727

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 14.66  |
| 183.00 | 9.80   | 13.18# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052521\  
Data File : BF124047.D  
Acq On : 25 May 2021 15:47  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 16:22:27 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 14 19:05:57 2021  
Response via : Initial Calibration

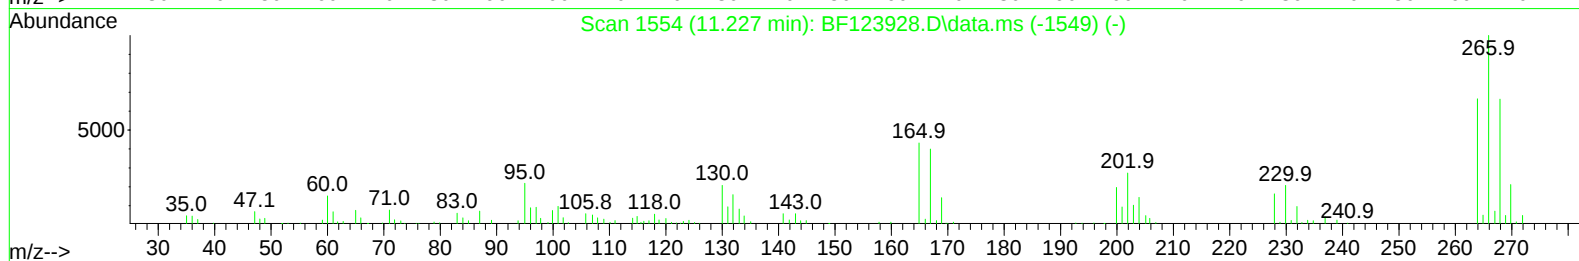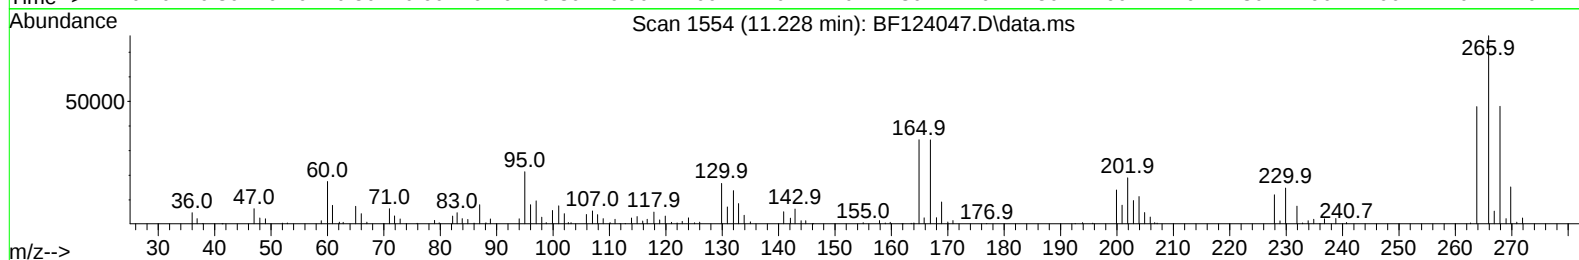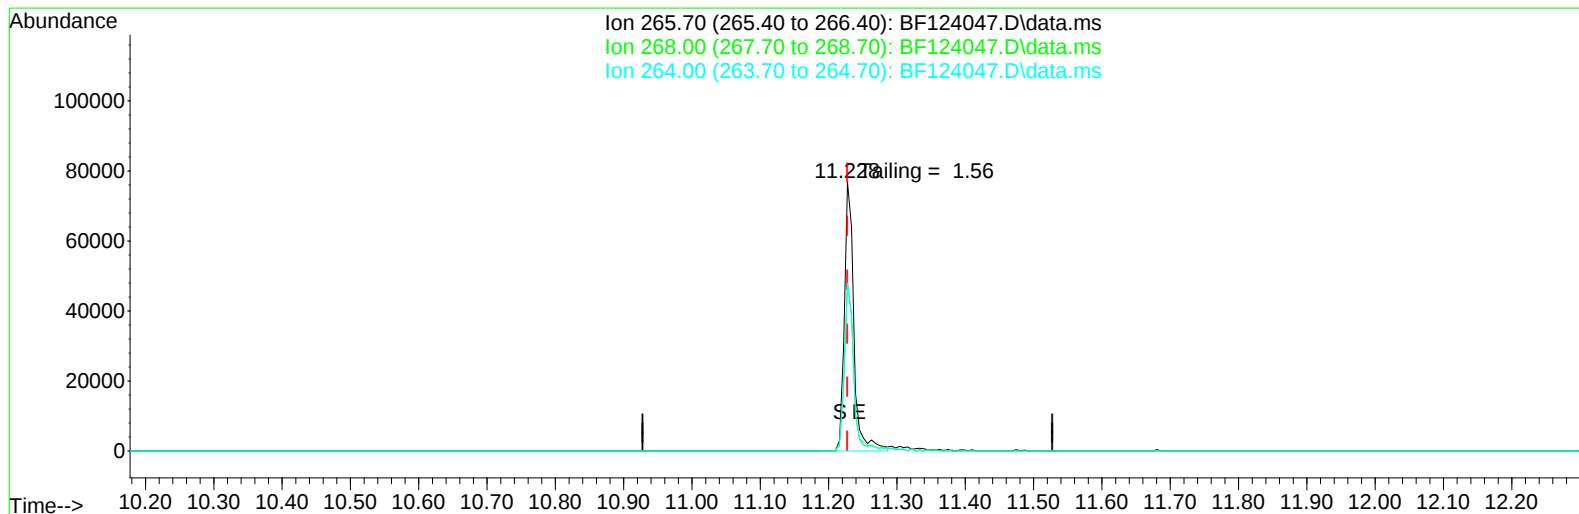

TIC: BF124047.D\data.ms

**(70) Pentachlorophenol (C)**

11.228min (+ 0.000) 16563.56 ng

response 75060

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 62.60  |
| 264.00 | 65.70  | 62.49  |
| 0.00   | 0.00   | 0.00   |