
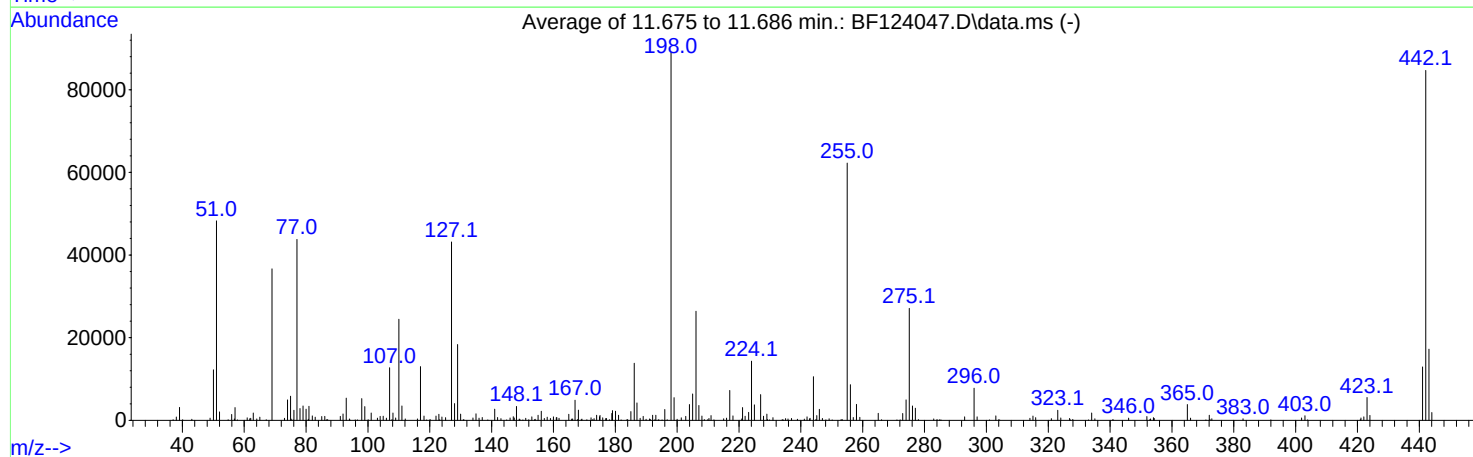


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052521\
 Data File : BF124047.D
 Acq On : 25 May 2021 15:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

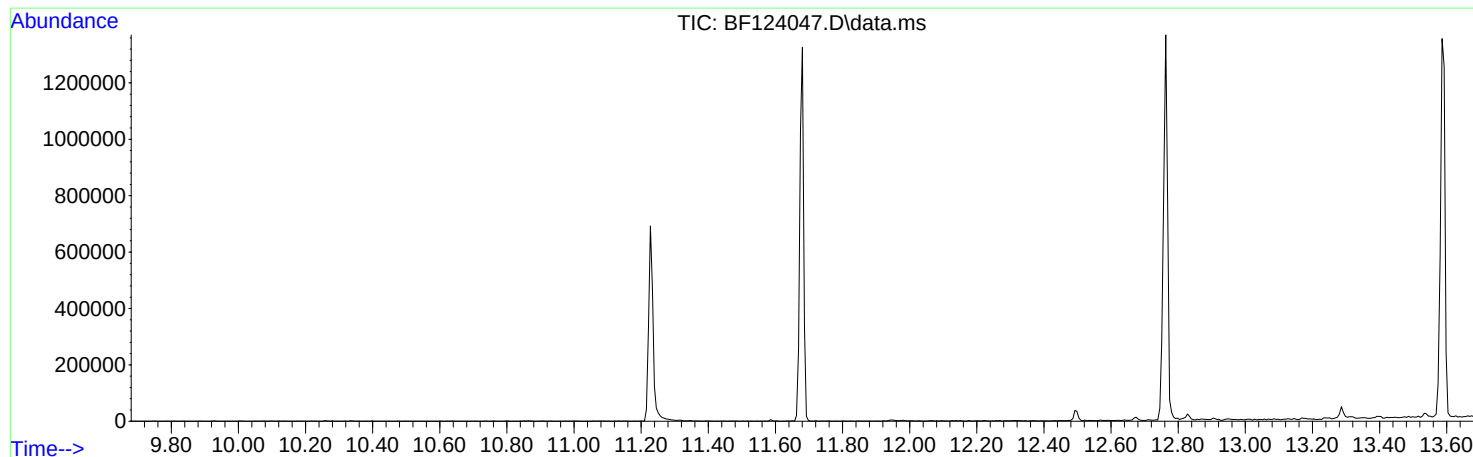




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	48275	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.2	36673	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	43162	PASS
197	198	0.00	2	0.2	154	PASS
198	198	100	100	100.0	89003	PASS
199	198	5	9	6.2	5516	PASS
275	198	10	60	30.5	27114	PASS
365	198	1	100	4.3	3824	PASS
441	198	0.01	100	14.5	12930	PASS
442	442	50	100	100.0	84669	PASS
443	442	15	24	20.3	17230	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052521\  
Data File : BF124047.D  
Acq On    : 25 May 2021  15:47  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 25 16:22:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

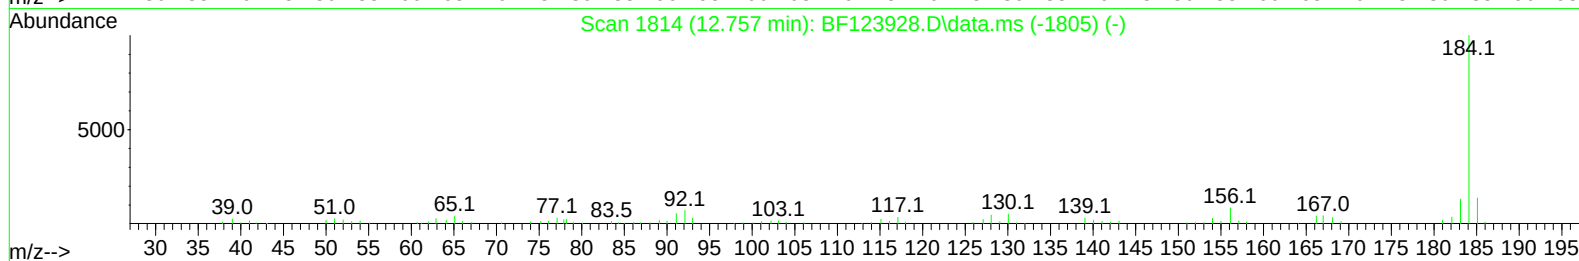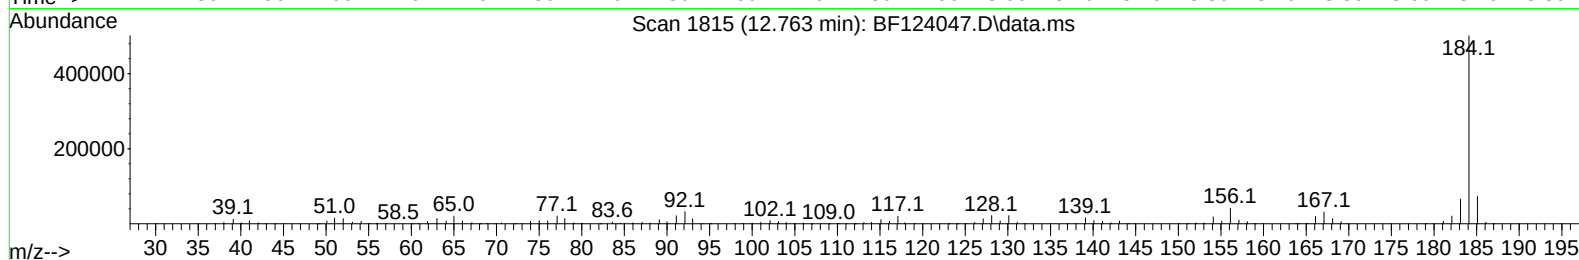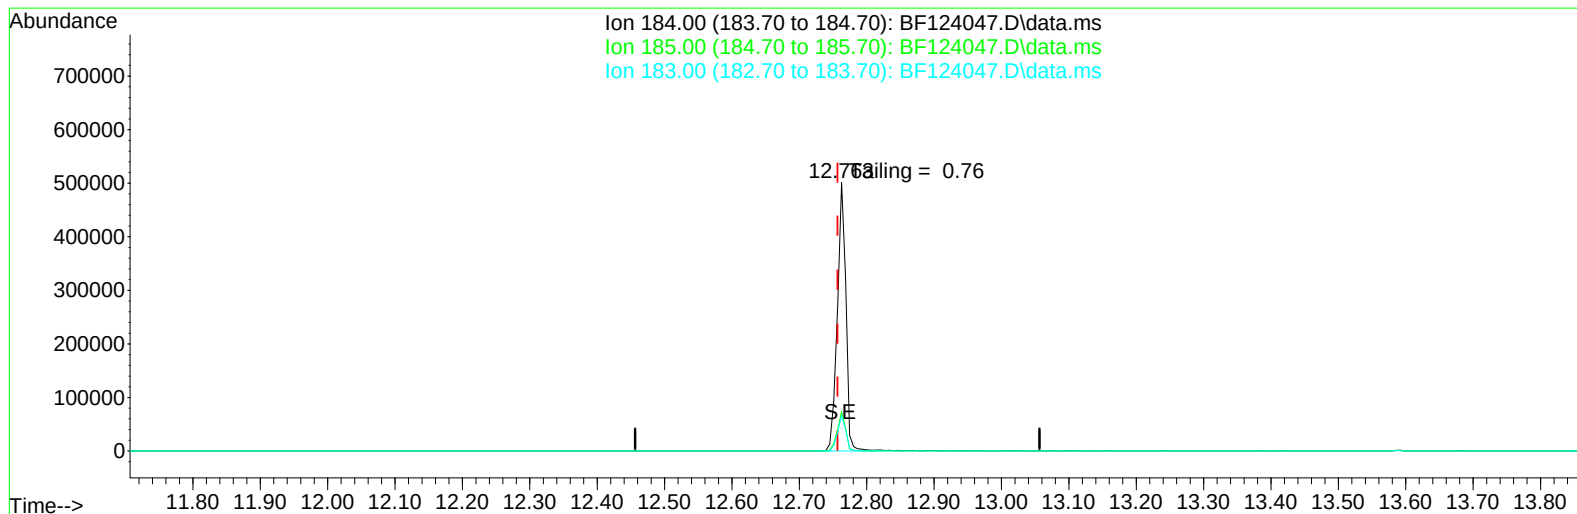

TIC: BF124047.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng




response 446727

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.66
183.00	9.80	13.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052521\
Data File : BF124047.D
Acq On : 25 May 2021 15:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 25 16:22:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

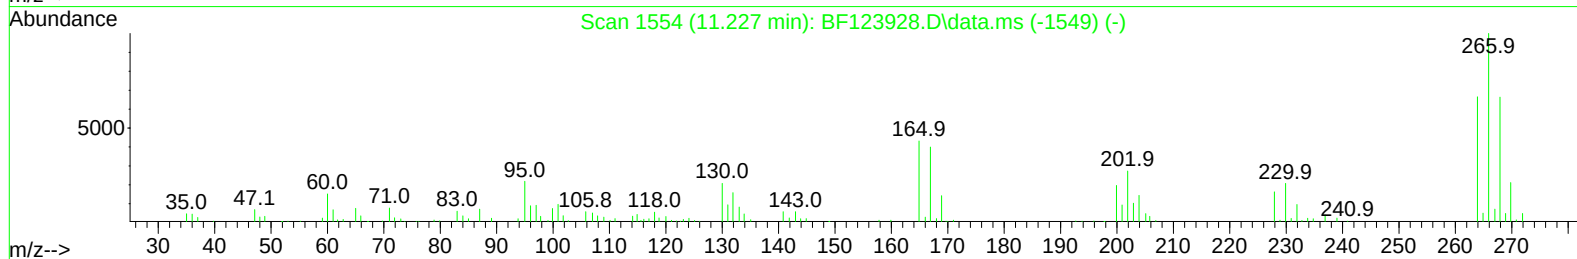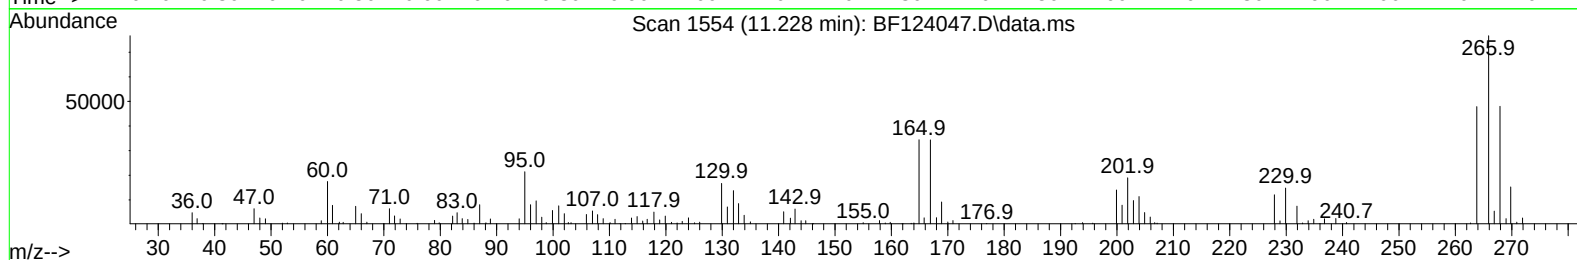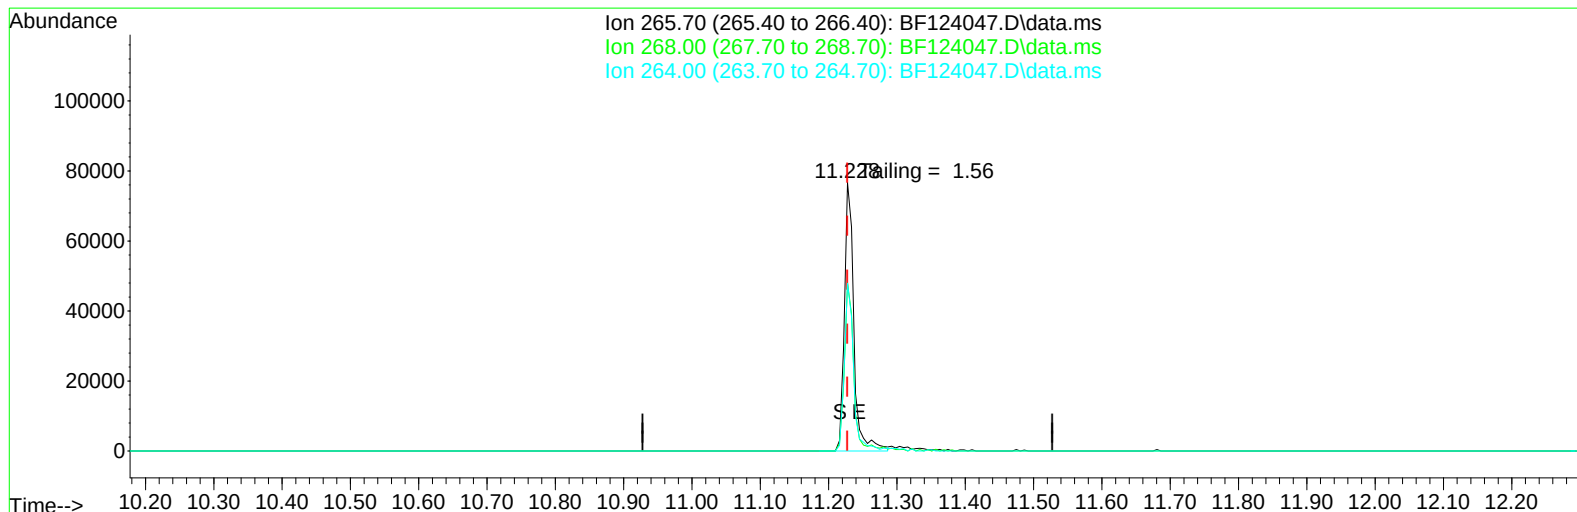

TIC: BF124047.D\data.ms

(70) Pentachlorophenol (C)

11.228min (+ 0.000) 16563.56 ng

response 75060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.60
264.00	65.70	62.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/25/2021	BNA_F	<u>BF124047.D</u>
Compound Name	Response	Retention Time
DDT	223902	13.59
DDD	6014	13.28
DDE	554	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6568	230470	2.85