
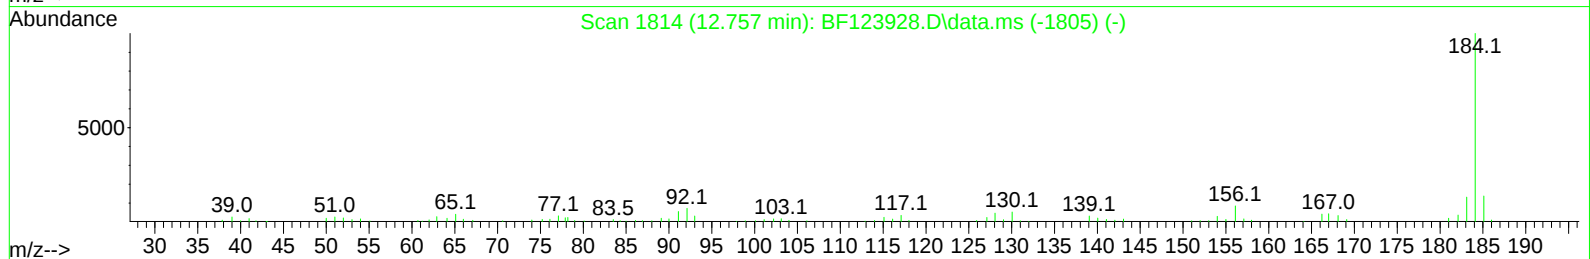
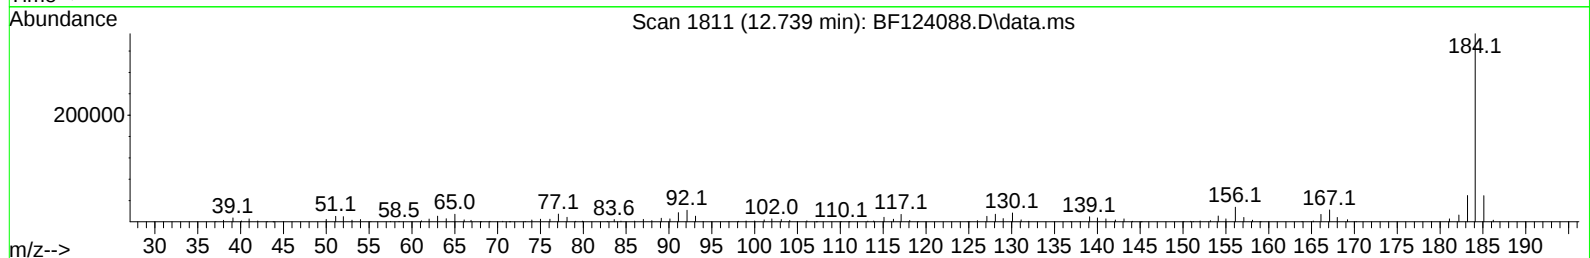


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052721\
Data File : BF124088.D
Acq On : 27 May 2021 10:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 12:52:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

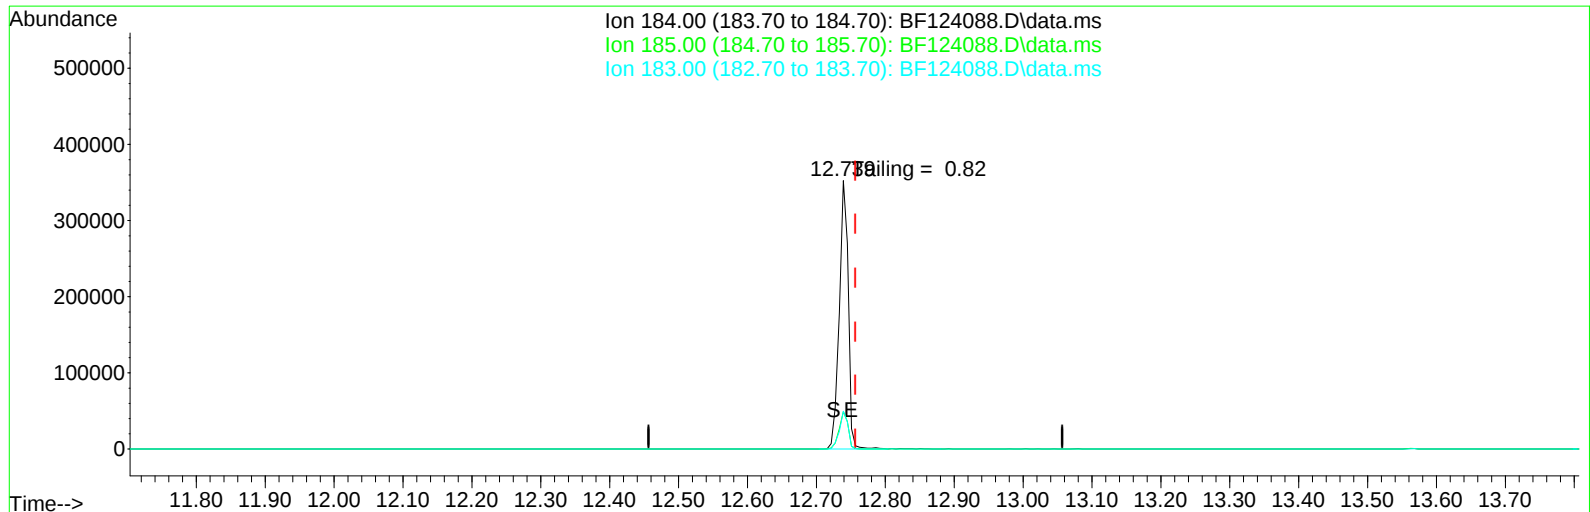

TIC: BF124088.D\data.ms

(77) Benzidine




12.739min (-0.018) 0.00 ng

response 317897

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.97
183.00	9.80	14.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052721\
Data File : BF124088.D
Acq On : 27 May 2021 10:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 12:52:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

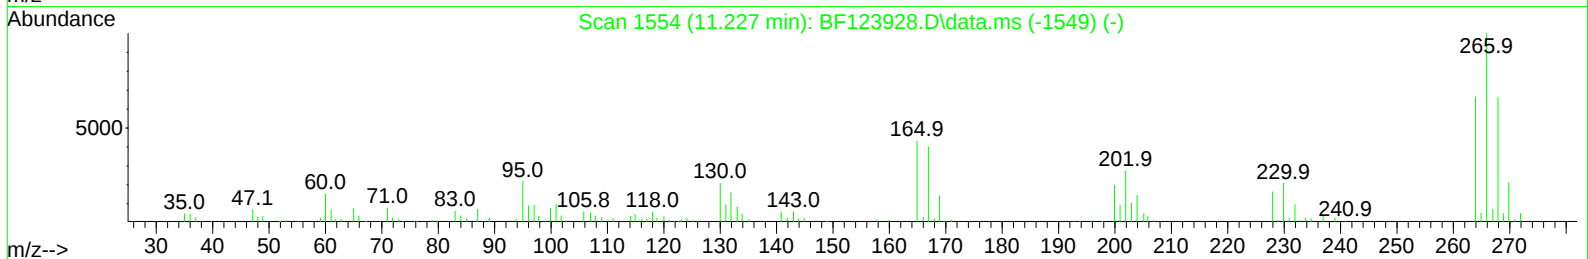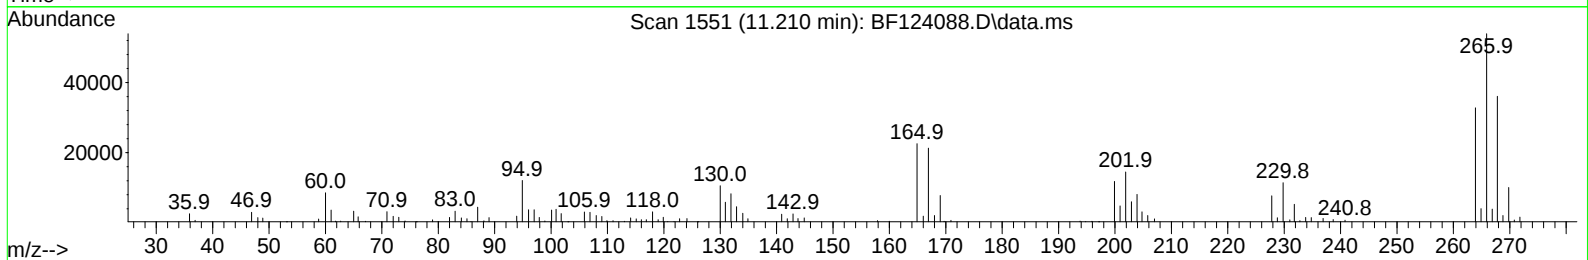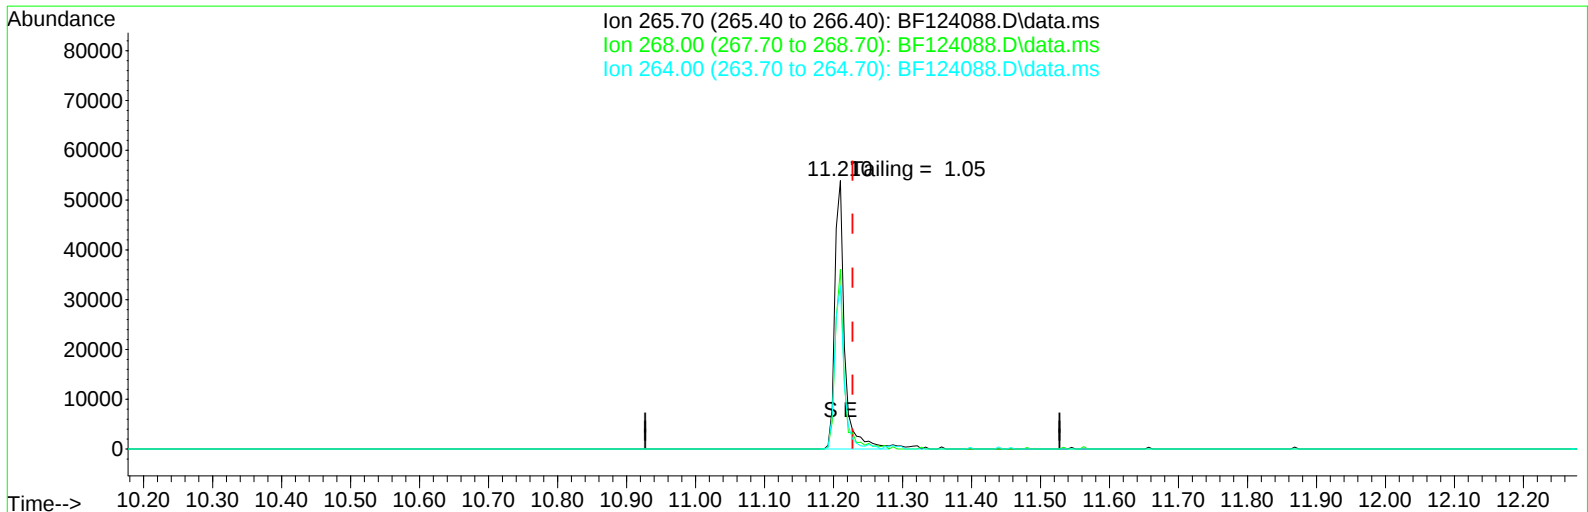

TIC: BF124088.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.018) 16616.56 ng

response 52898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	66.88
264.00	65.70	60.81
0.00	0.00	0.00