
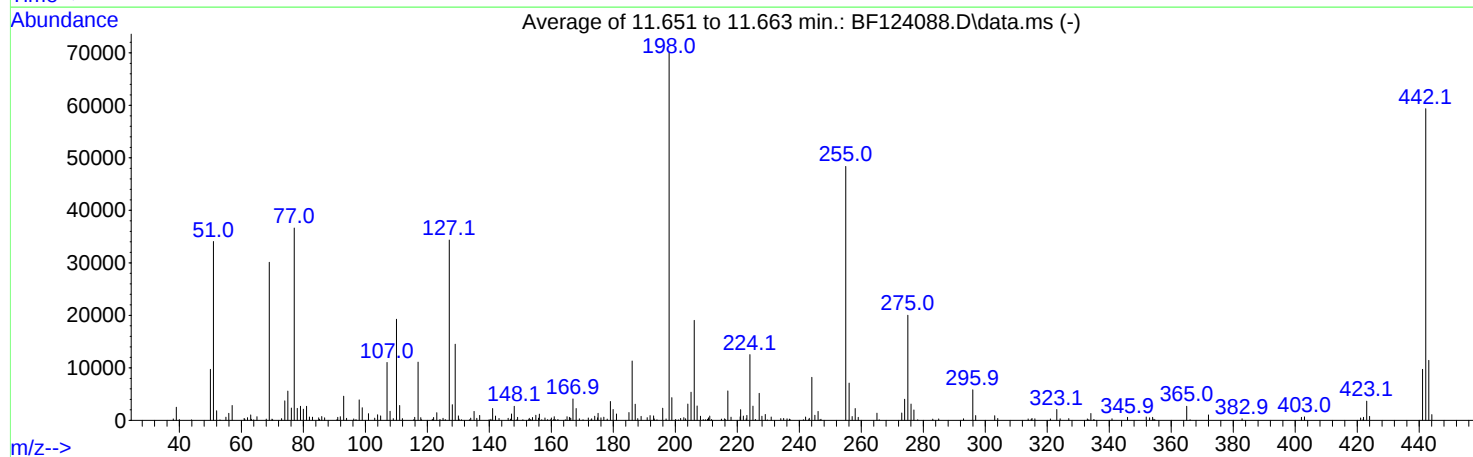


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052721\
 Data File : BF124088.D
 Acq On : 27 May 2021 10:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 13:12:25 2021

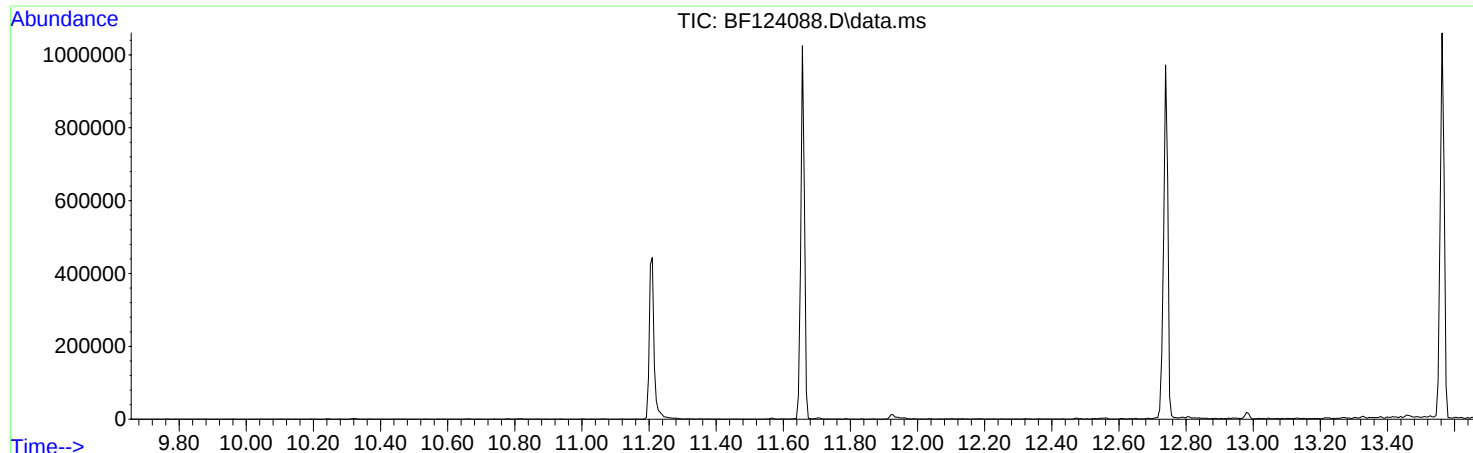




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	34061	PASS
68	69	0.00	2	0.8	242	PASS
69	198	0.00	100	43.0	30117	PASS
70	69	0.00	2	0.9	259	PASS
127	198	10	80	49.0	34352	PASS
197	198	0.00	2	0.4	274	PASS
198	198	100	100	100.0	70061	PASS
199	198	5	9	6.2	4329	PASS
275	198	10	60	28.6	20020	PASS
365	198	1	100	3.8	2689	PASS
441	198	0.01	100	13.9	9709	PASS
442	442	50	100	100.0	59379	PASS
443	442	15	24	19.3	11441	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052721\
 Data File : BF124088.D
 Acq On : 27 May 2021 10:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 27 12:52:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

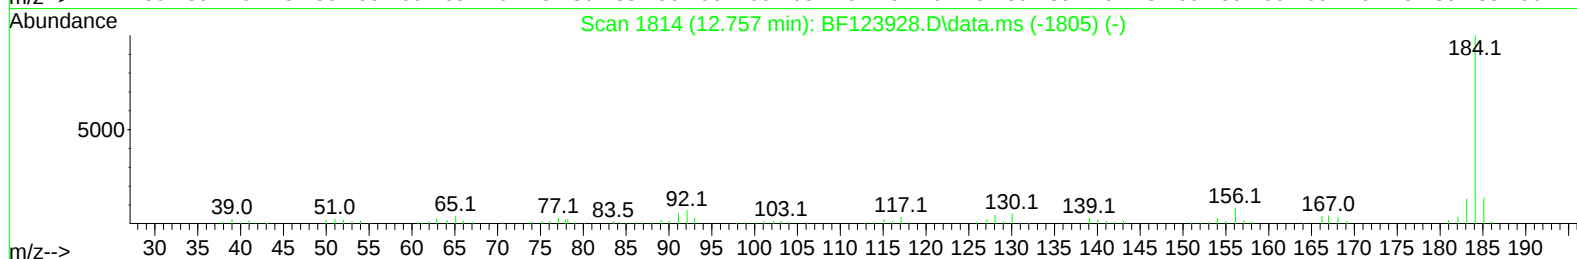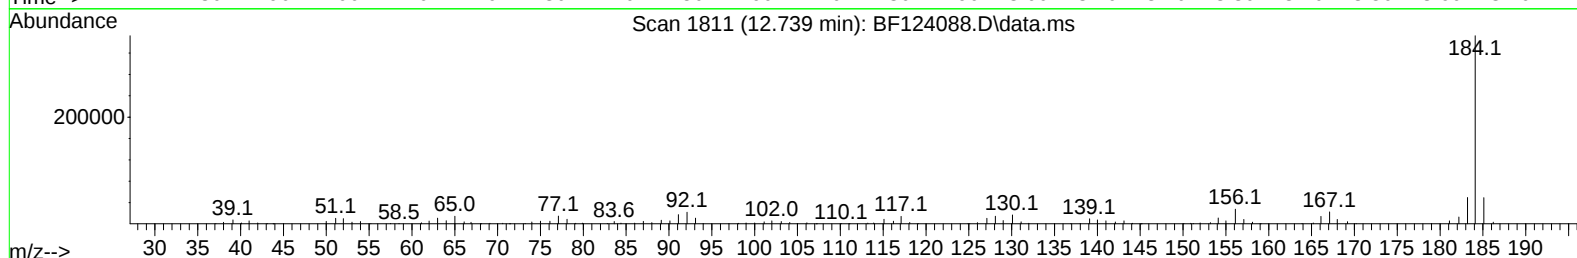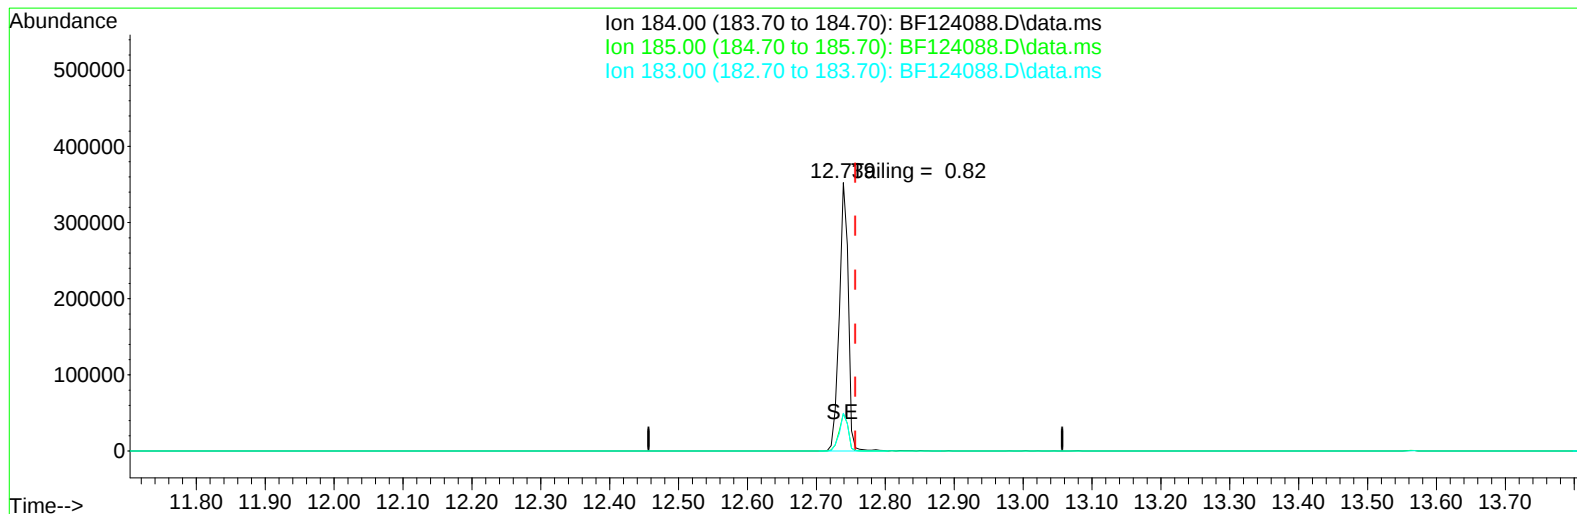

TIC: BF124088.D\data.ms

(77) Benzidine

12.739min (-0.018) 0.00 ng




response 317897

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.97
183.00	9.80	14.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052721\
Data File : BF124088.D
Acq On : 27 May 2021 10:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 27 12:52:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

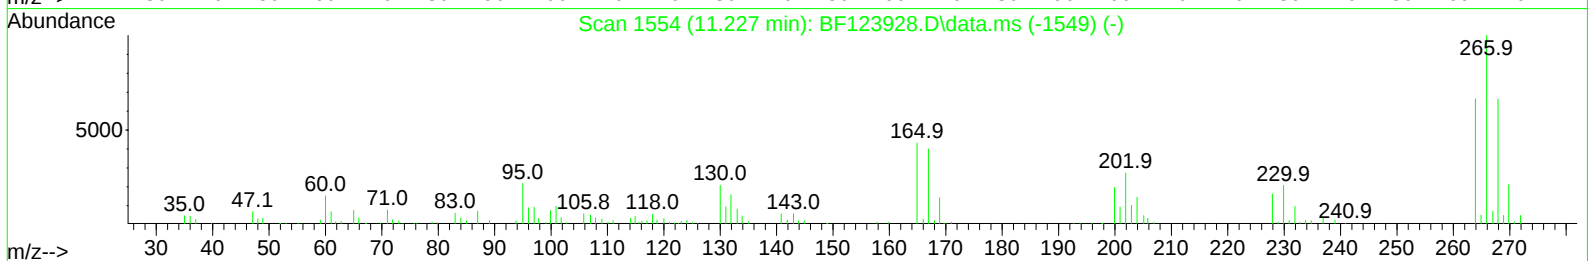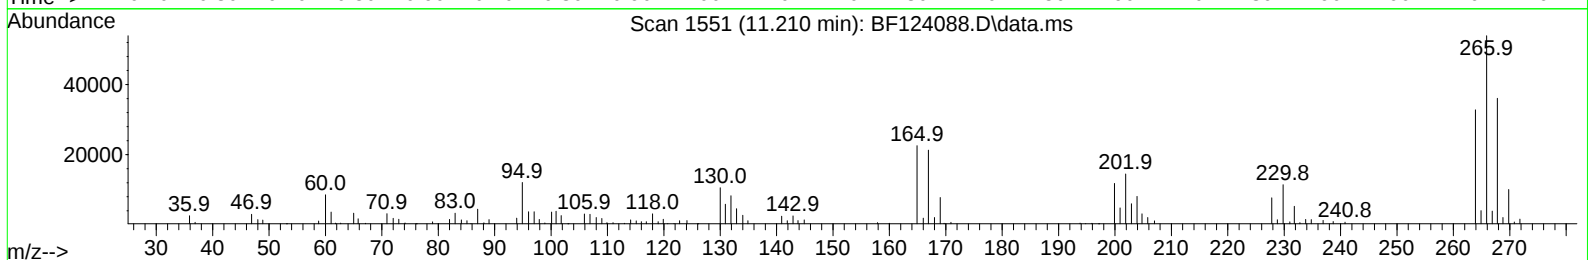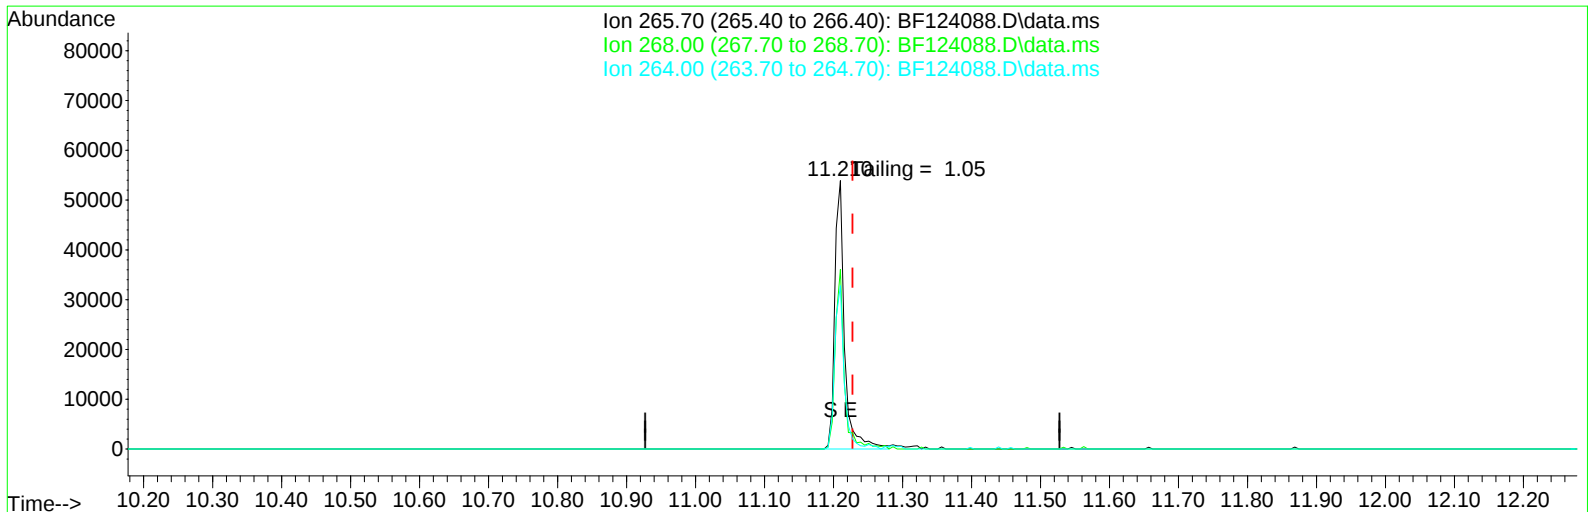

TIC: BF124088.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.018) 16616.56 ng

response 52898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	66.88
264.00	65.70	60.81
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
5/27/2021	BNA_F	<u>BF124088.D</u>
Compound Name	Response	Retention Time
DDT	157202	13.56
DDD	1368	13.28
DDE	243	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1611	158813	1.01