
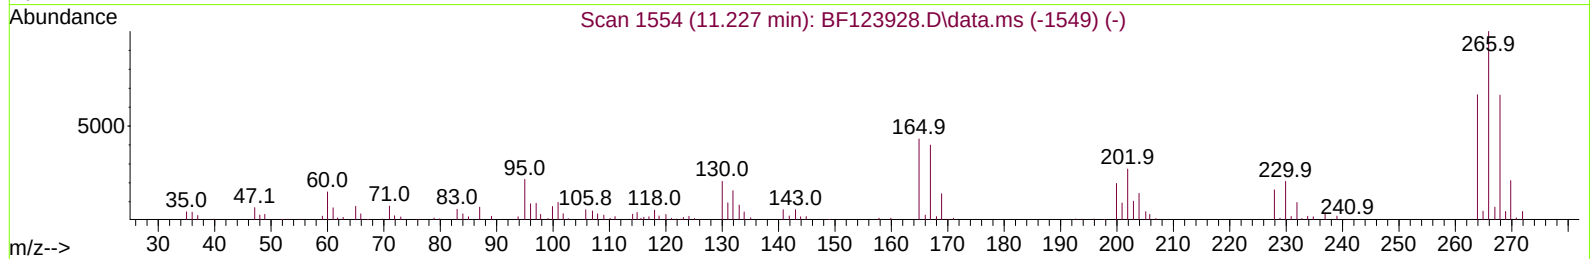
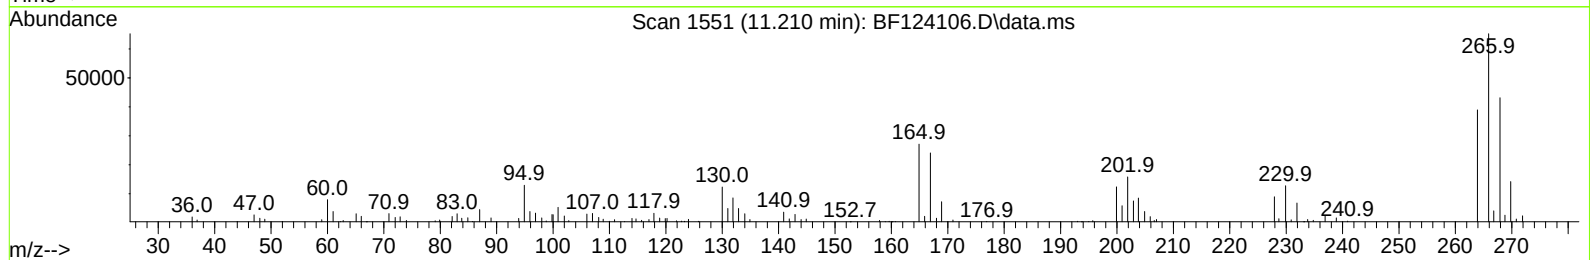


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052821\
Data File : BF124106.D
Acq On : 28 May 2021 13:03
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 15:00:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 13:12:25 2021
Response via : Initial Calibration

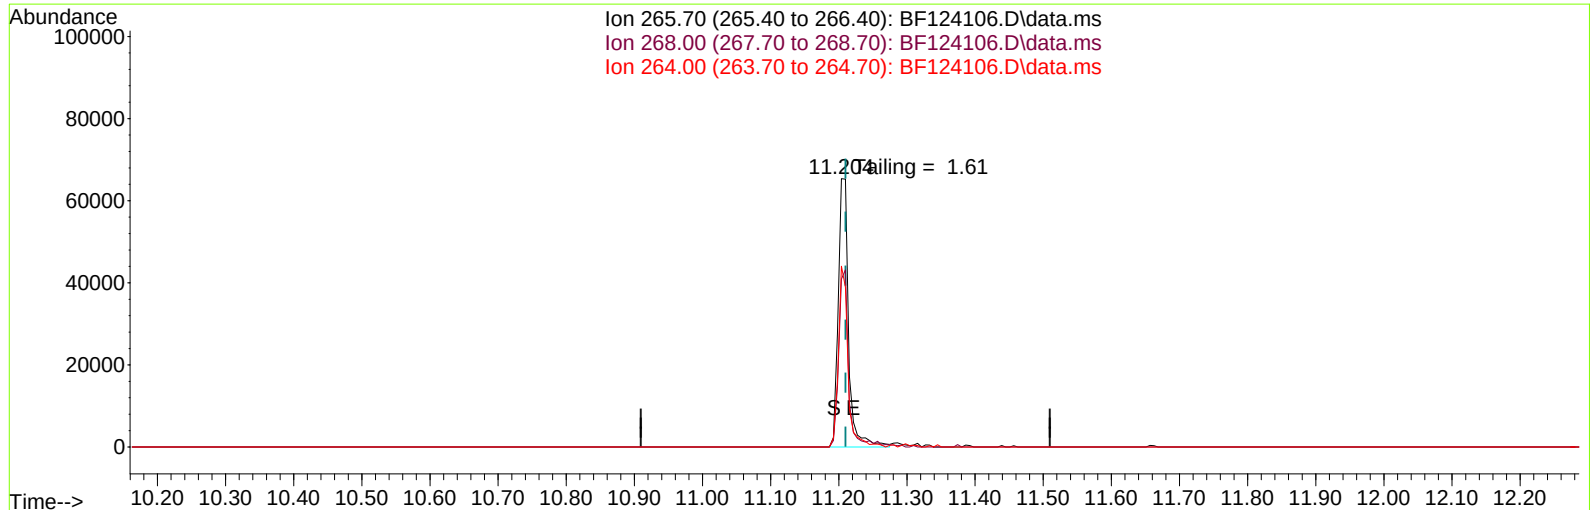

TIC: BF124106.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 14145.66 ng

response 61027

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.39
264.00	65.70	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052821\
Data File : BF124106.D
Acq On : 28 May 2021 13:03
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 15:00:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 13:12:25 2021
Response via : Initial Calibration

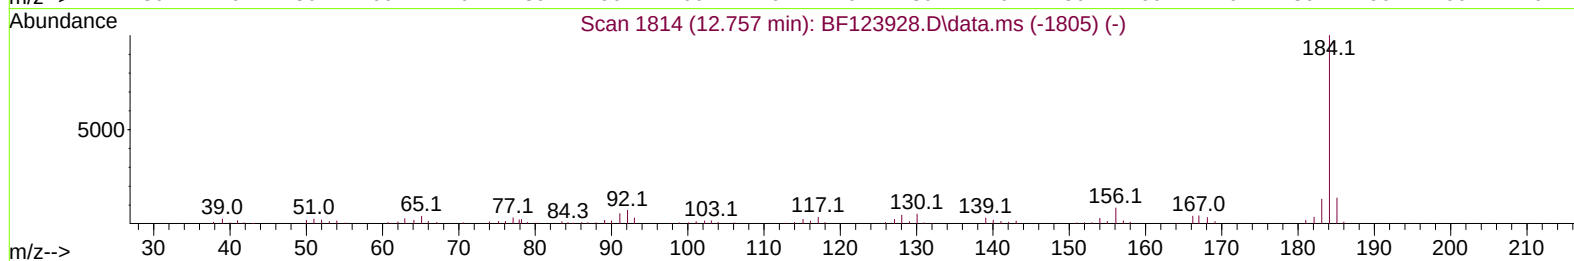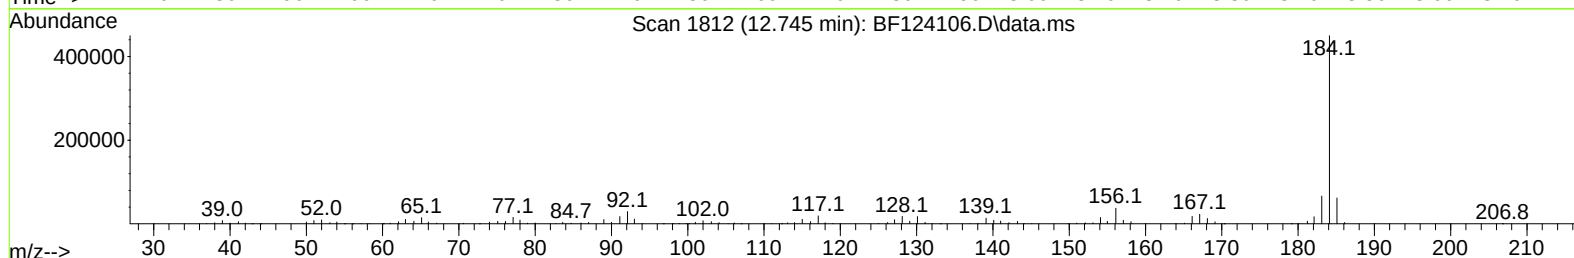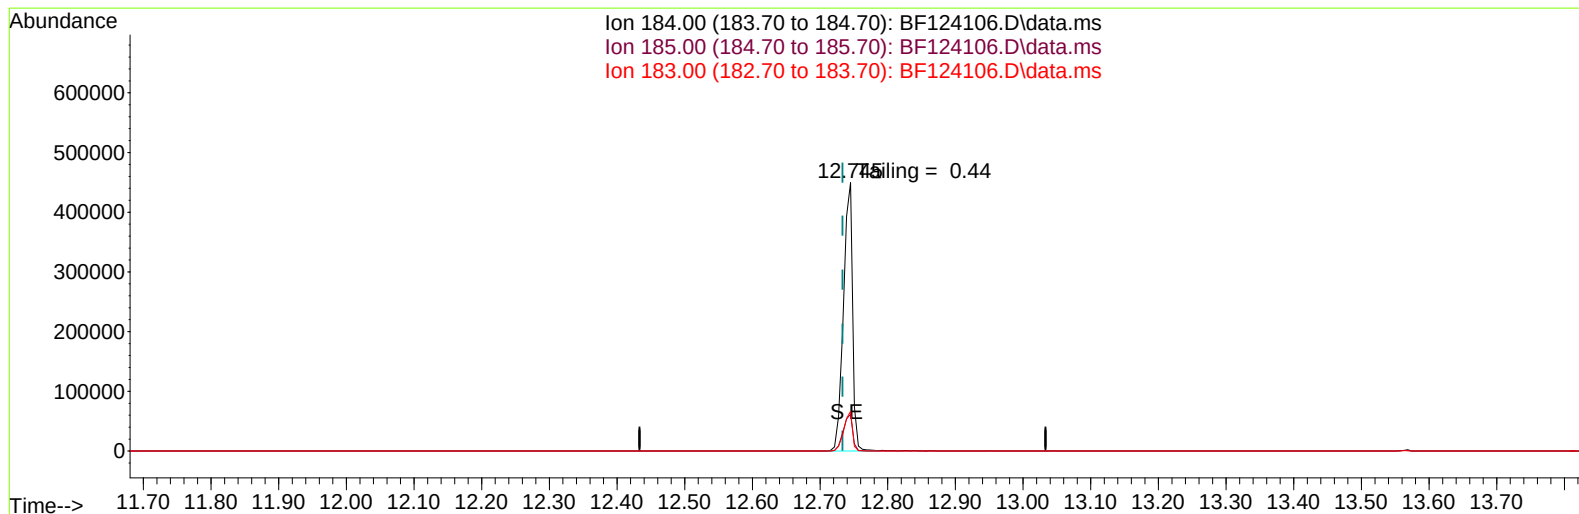

TIC: BF124106.D\data.ms

(77) Benzidine

12.745min (+ 0.012) 0.00 ng

response 387469

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.29
183.00	9.80	13.54#
0.00	0.00	0.00