


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052821\
 Data File : BF124106.D
 Acq On : 28 May 2021 13:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 13:12:25 2021

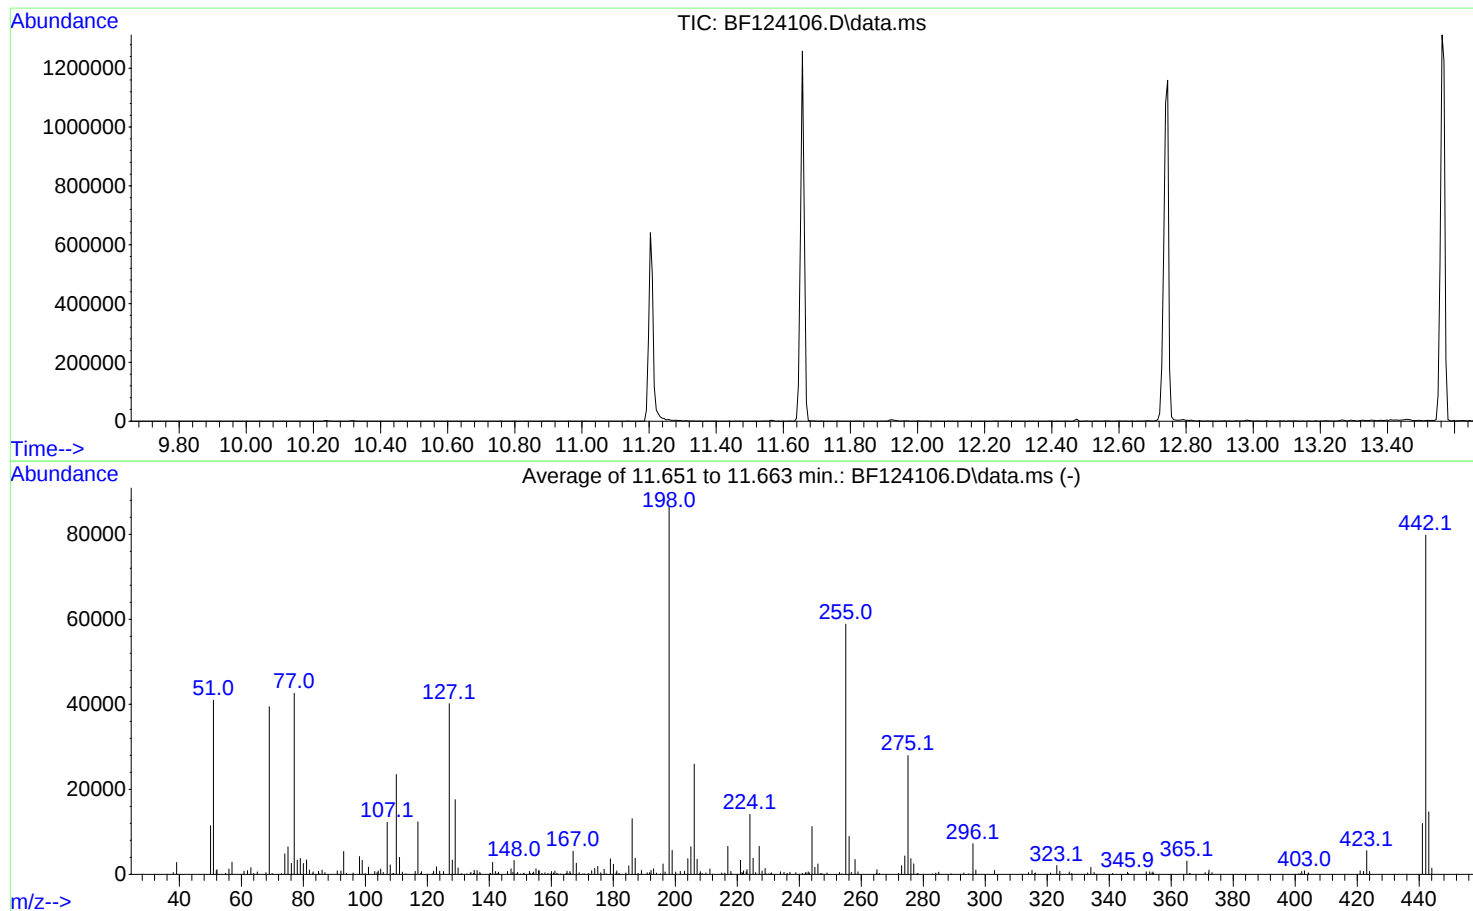

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	40979	PASS
68	69	0.00	2	1.1	422	PASS
69	198	0.00	100	45.6	39435	PASS
70	69	0.00	2	0.3	136	PASS
127	198	10	80	46.4	40160	PASS
197	198	0.00	2	0.6	550	PASS
198	198	100	100	100.0	86536	PASS
199	198	5	9	6.5	5639	PASS
275	198	10	60	32.3	27968	PASS
365	198	1	100	3.6	3138	PASS
441	198	0.01	100	13.8	11968	PASS
442	442	50	100	100.0	79792	PASS
443	442	15	24	18.4	14705	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2021	BNA_F	<u>BF124106.D</u>
Compound Name	Response	Retention Time
DDT	214024	13.568
DDD	1906	13.292
DDE	215	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2121	216145	0.98

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052821\
 Data File : BF124106.D
 Acq On : 28 May 2021 13:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 28 15:00:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 13:12:25 2021
 Response via : Initial Calibration

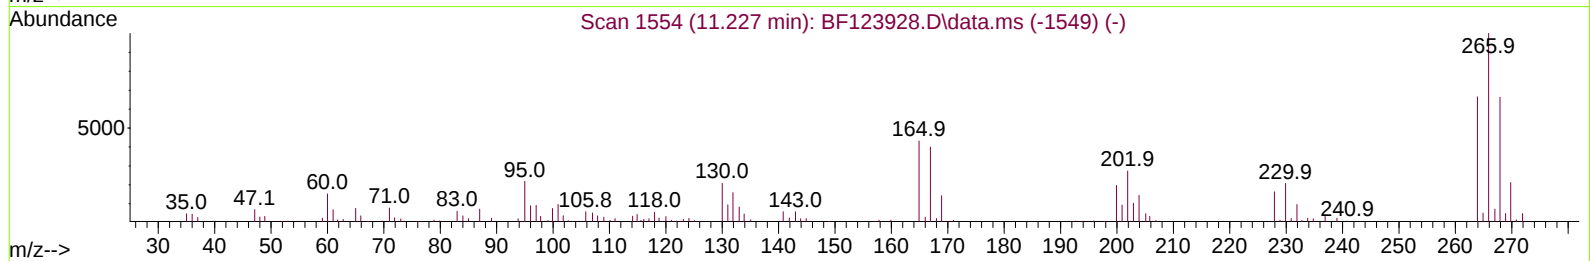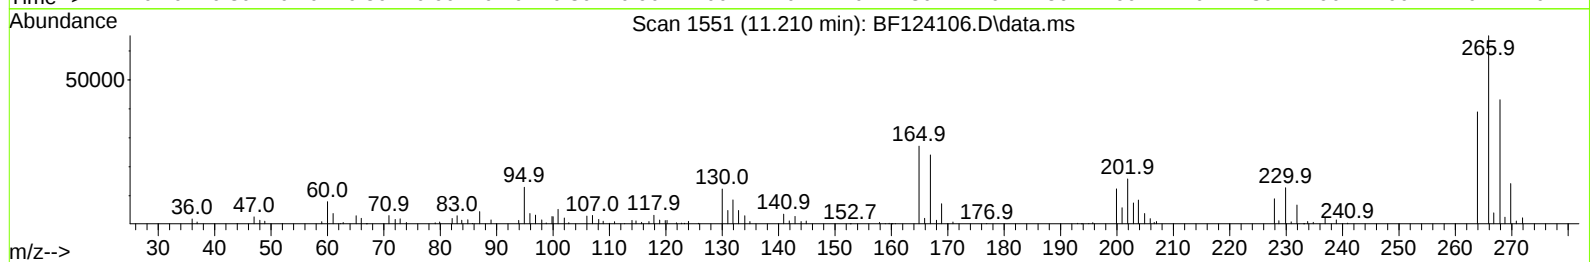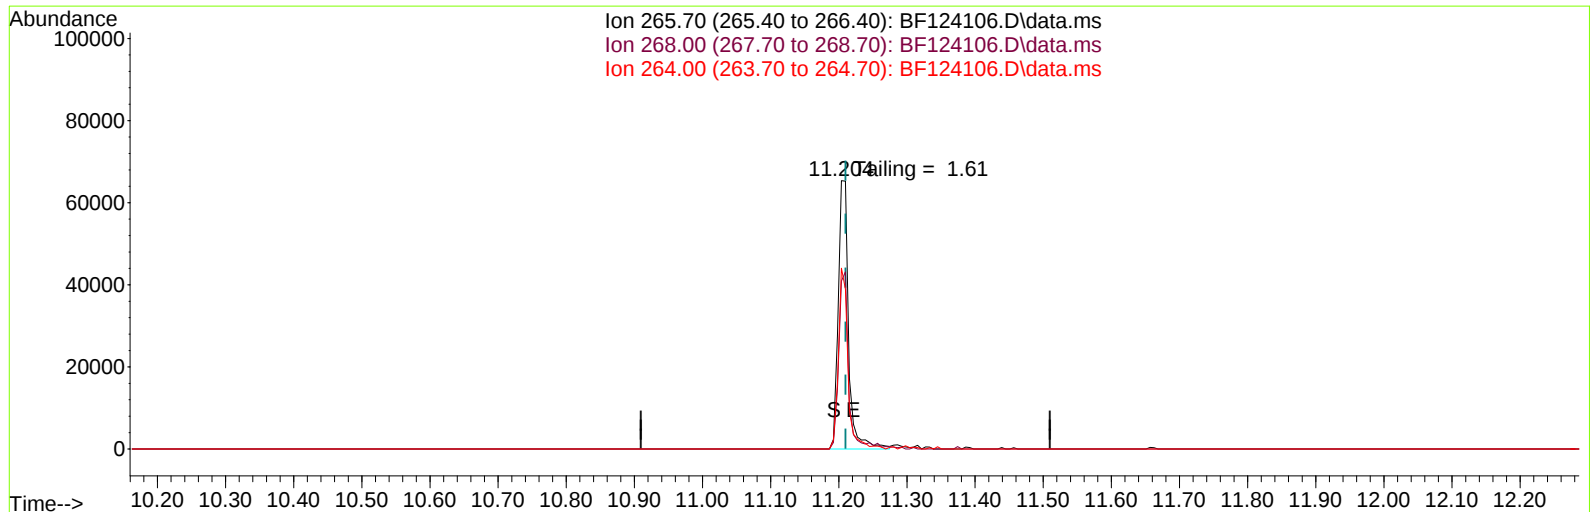

TIC: BF124106.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 14145.66 ng




response 61027

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.39
264.00	65.70	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052821\
Data File : BF124106.D
Acq On : 28 May 2021 13:03
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 28 15:00:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 13:12:25 2021
Response via : Initial Calibration

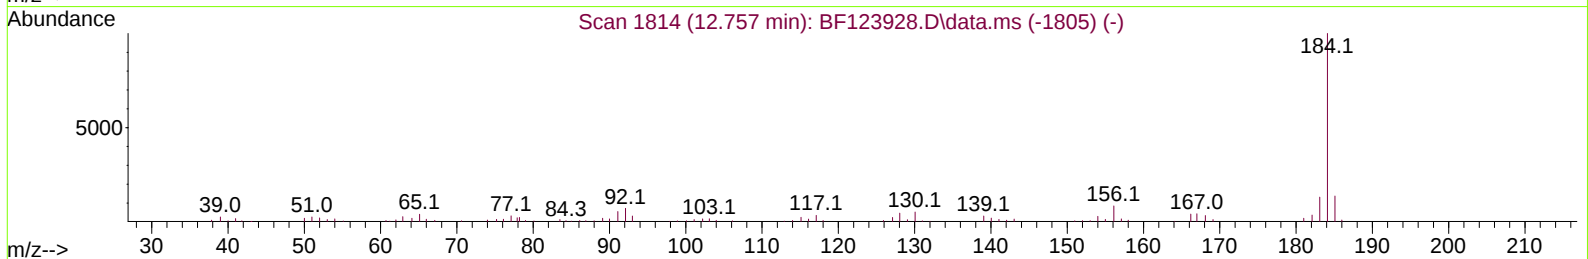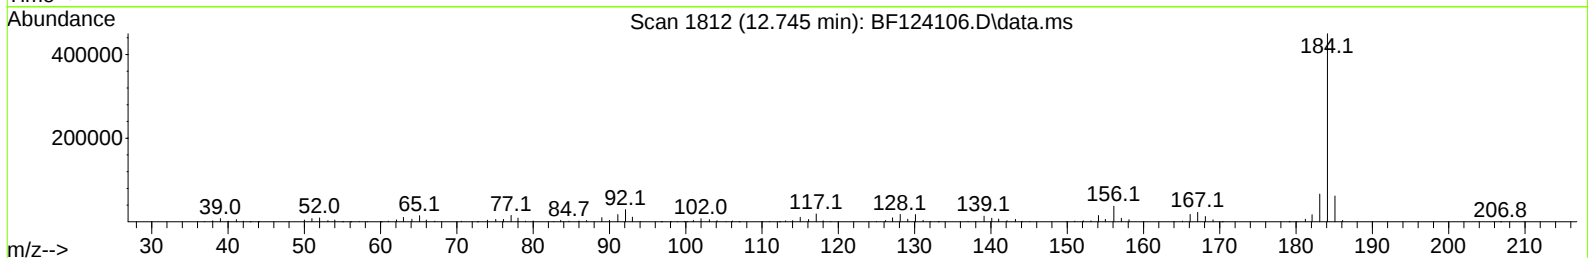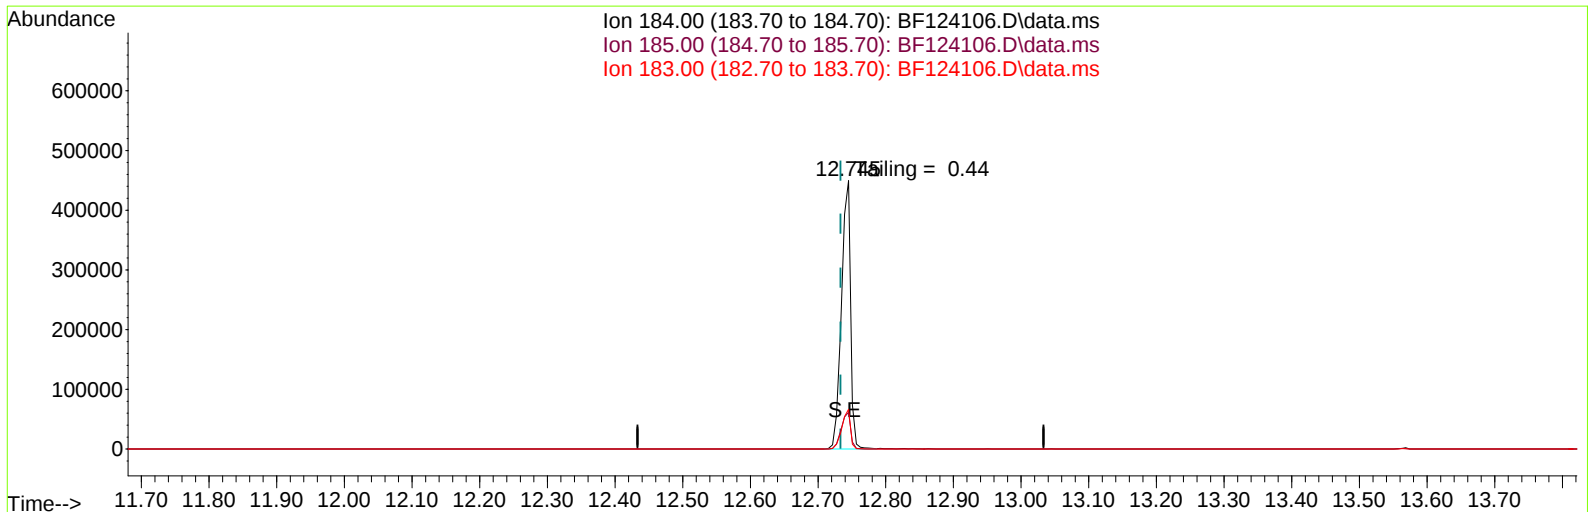

TIC: BF124106.D\data.ms

(77) Benzidine

12.745min (+ 0.012) 0.00 ng

response 387469

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.29
183.00	9.80	13.54#
0.00	0.00	0.00