

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052919\
 Data File : BF114648.D
 Acq On : 30 May 2019 1:50
 Operator : HP/JU
 Sample : K3065-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-14-11-12.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.716	258	277	280	rBV	11855120	39511497	100.00%	7.585%
2	5.187	518	527	530	rVV2	12605018	34360117	86.96%	6.596%
3	5.310	539	548	551	rVV3	13317850	38067106	96.34%	7.308%
4	5.381	555	560	566	rVB2	740440	840554	2.13%	0.161%
5	5.481	570	577	581	rVB2	379425	413491	1.05%	0.079%
6	5.569	581	592	595	rBV2	13087114	27421765	69.40%	5.264%
7	5.869	639	643	647	rBV	5739469	5586551	14.14%	1.073%
8	6.087	676	680	684	rVB	3454095	3108760	7.87%	0.597%
9	6.163	684	693	700	rBV	3032395	3190787	8.08%	0.613%
10	6.251	700	708	709	rBV	12814812	23781500	60.19%	4.566%
11	6.275	709	712	715	rVV	12174853	13162625	33.31%	2.527%
12	6.316	715	719	721	rVV	11511520	13822506	34.98%	2.654%
13	6.340	721	723	728	rVB2	6130918	5704616	14.44%	1.095%
14	6.392	728	732	734	rBV	5305341	4649307	11.77%	0.893%
15	6.416	734	736	740	rVV2	2909042	3038412	7.69%	0.583%
16	6.469	740	745	748	rVV	7350563	9675927	24.49%	1.858%
17	6.492	748	749	750	rVV	1908606	993910	2.52%	0.191%
18	6.557	750	760	762	rVV2	13465480	29226800	73.97%	5.611%
19	6.581	762	764	767	rVB	3050459	2152560	5.45%	0.413%
20	6.657	773	777	781	rBV4	480785	758717	1.92%	0.146%
21	6.698	781	784	788	rVB	2396691	2175379	5.51%	0.418%
22	6.769	788	796	799	rBV2	8382678	12355650	31.27%	2.372%
23	6.816	799	804	808	rVV2	5466179	10229710	25.89%	1.964%
24	6.898	808	818	820	rVV2	12410714	31242716	79.07%	5.998%
25	6.945	823	826	827	rBV2	1747188	1753503	4.44%	0.337%
26	6.981	827	832	835	rVB	12053105	20979819	53.10%	4.028%
27	7.028	837	840	843	rBV	5913311	4770519	12.07%	0.916%
28	7.098	849	852	855	rBV2	1922666	1779332	4.50%	0.342%
29	7.169	860	864	866	rVV2	1430656	1554991	3.94%	0.299%
30	7.192	866	868	870	rVV	1216128	1248267	3.16%	0.240%
31	7.210	870	871	873	rVV2	973645	879600	2.23%	0.169%
32	7.245	873	877	878	rVV	5673748	6546424	16.57%	1.257%
33	7.281	881	883	886	rVV2	964139	1007195	2.55%	0.193%
34	7.316	886	889	892	rVV	3225541	3461979	8.76%	0.665%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052919\
 Data File : BF114648.D
 Acq On : 30 May 2019 1:50
 Operator : HP/JU
 Sample : K3065-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-14-11-12.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	7.345	892	894	895	rVV2	906509	800255	2.03%	0.154%
36	7.363	895	897	899	rVV	834820	660872	1.67%	0.127%
37	7.404	899	904	906	rVV3	1072388	1455713	3.68%	0.279%
38	7.475	913	916	918	rVV	2109816	1815770	4.60%	0.349%
39	7.498	918	920	924	rVV	3610408	3084941	7.81%	0.592%
40	7.534	924	926	929	rVV2	707914	728199	1.84%	0.140%
41	7.569	929	932	934	rVV	1258915	1147076	2.90%	0.220%
42	7.657	938	947	950	rVV	3417919	4035694	10.21%	0.775%
43	7.734	954	960	963	rBV3	7954887	11862019	30.02%	2.277%
44	7.769	963	966	972	rVB	7323825	10440323	26.42%	2.004%
45	7.851	977	980	982	rVB2	1331770	1135142	2.87%	0.218%
46	8.010	997	1007	1010	rBV3	11890378	32169585	81.42%	6.176%
47	8.057	1012	1015	1017	rVV	2689452	1939495	4.91%	0.372%
48	8.416	1071	1076	1078	rBV	493471	655417	1.66%	0.126%
49	8.439	1078	1080	1082	rVV2	423578	471842	1.19%	0.091%
50	8.557	1097	1100	1102	rVV	589071	543315	1.38%	0.104%
51	8.686	1117	1122	1126	rVB	8497719	9355410	23.68%	1.796%
52	8.786	1133	1139	1142	rBV	6322225	6040864	15.29%	1.160%
53	9.051	1179	1184	1187	rVB	8362866	8128766	20.57%	1.561%
54	9.145	1195	1200	1203	rBV	946898	804035	2.03%	0.154%
55	9.216	1208	1212	1220	rVB2	5251670	6568844	16.63%	1.261%
56	9.304	1221	1227	1231	rVB2	1173416	1789303	4.53%	0.344%
57	9.351	1231	1235	1237	rBV	1428784	1293938	3.27%	0.248%
58	9.381	1237	1240	1242	rVV	1652621	1409785	3.57%	0.271%
59	9.404	1242	1244	1247	rVB	1060173	898793	2.27%	0.173%
60	9.439	1247	1250	1256	rVB4	1165556	1437533	3.64%	0.276%
61	9.498	1256	1260	1262	rBV	766588	760149	1.92%	0.146%
62	9.575	1269	1273	1276	rBV	1662100	1466538	3.71%	0.282%
63	9.692	1291	1293	1295	rVV	1474010	1364160	3.45%	0.262%
64	9.716	1295	1297	1299	rVV	3399218	3306265	8.37%	0.635%
65	9.739	1299	1301	1305	rVV2	2614789	2969377	7.52%	0.570%
66	9.775	1305	1307	1309	rVV2	623650	497505	1.26%	0.096%
67	9.904	1324	1329	1331	rBV2	761212	990131	2.51%	0.190%
68	10.169	1371	1374	1376	rVV2	442599	399338	1.01%	0.077%
69	10.263	1387	1390	1393	rBV2	972317	931993	2.36%	0.179%
70	10.498	1423	1430	1434	rBV2	5536435	6439486	16.30%	1.236%
71	11.192	1544	1548	1550	rBV	3921597	3550461	8.99%	0.682%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052919\
 Data File : BF114648.D
 Acq On : 30 May 2019 1:50
 Operator : HP/JU
 Sample : K3065-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-14-11-12.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.216	1550	1552	1555	rVB	2795912	2028413	5.13%	0.389%
73	11.263	1557	1560	1563	rVB	679038	530612	1.34%	0.102%
74	11.692	1630	1633	1635	rBV	513883	481578	1.22%	0.092%
75	11.716	1635	1637	1639	rVV2	801521	676030	1.71%	0.130%
76	11.739	1639	1641	1643	rVV	811559	625467	1.58%	0.120%
77	11.798	1648	1651	1654	rBV	755995	770009	1.95%	0.148%
78	12.392	1749	1752	1758	rBV	1042405	916205	2.32%	0.176%
79	12.516	1771	1773	1781	rBV4	385116	566633	1.43%	0.109%
80	12.616	1786	1790	1793	rVV	1194917	1190773	3.01%	0.229%
81	12.780	1813	1818	1821	rBV	7986448	8738118	22.12%	1.678%
82	13.027	1856	1860	1862	rVB2	378890	480947	1.22%	0.092%
83	13.680	1968	1971	1979	rBV	1899951	2279779	5.77%	0.438%
84	13.810	1988	1993	1996	rBV	3135990	3350631	8.48%	0.643%
85	14.316	2076	2079	2087	rBV3	707403	954379	2.42%	0.183%
86	14.610	2126	2129	2134	rVB	389493	395339	1.00%	0.076%
87	14.915	2178	2181	2191	rVB4	319947	496604	1.26%	0.095%
88	15.198	2224	2229	2233	rVV	2305053	2671702	6.76%	0.513%
89	15.262	2237	2240	2250	rVB	261988	415895	1.05%	0.080%
90	15.698	2311	2314	2324	rVB2	329880	514128	1.30%	0.099%


Sum of corrected areas: 520884166

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052919\
Data File : BF114648.D
Acq On : 30 May 2019 1:50
Operator : HP/JU
Sample : K3065-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-14-11-12.0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

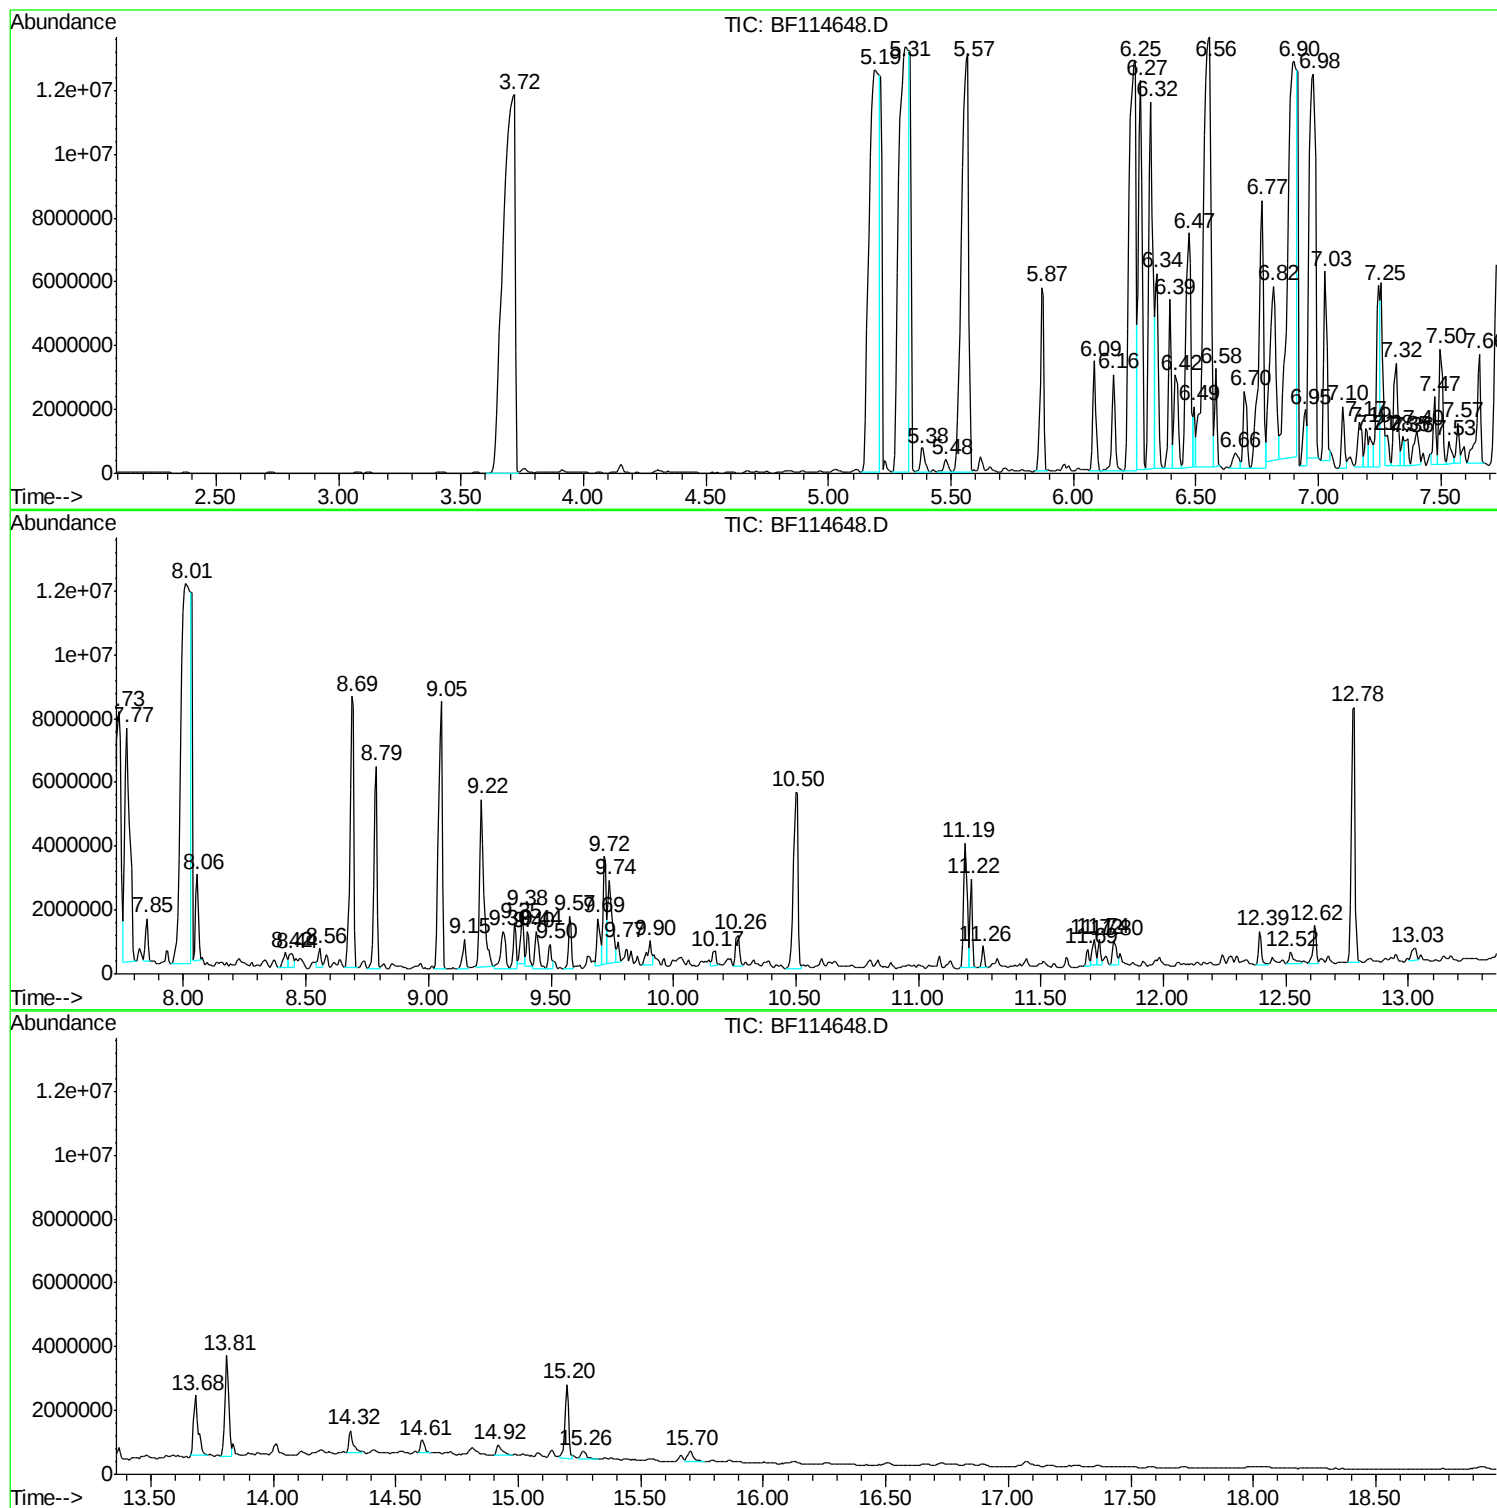

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052919\
Data_File : BF114648.D
Acq_On : 30 May, 2019 1:500
Operator : HP/JUU
Sample : K3065-088
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
B-14-11-12.0

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
