


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052919\
 Data File : BF114631.D
 Acq On : 29 May 2019 13:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 19:08:51 2019

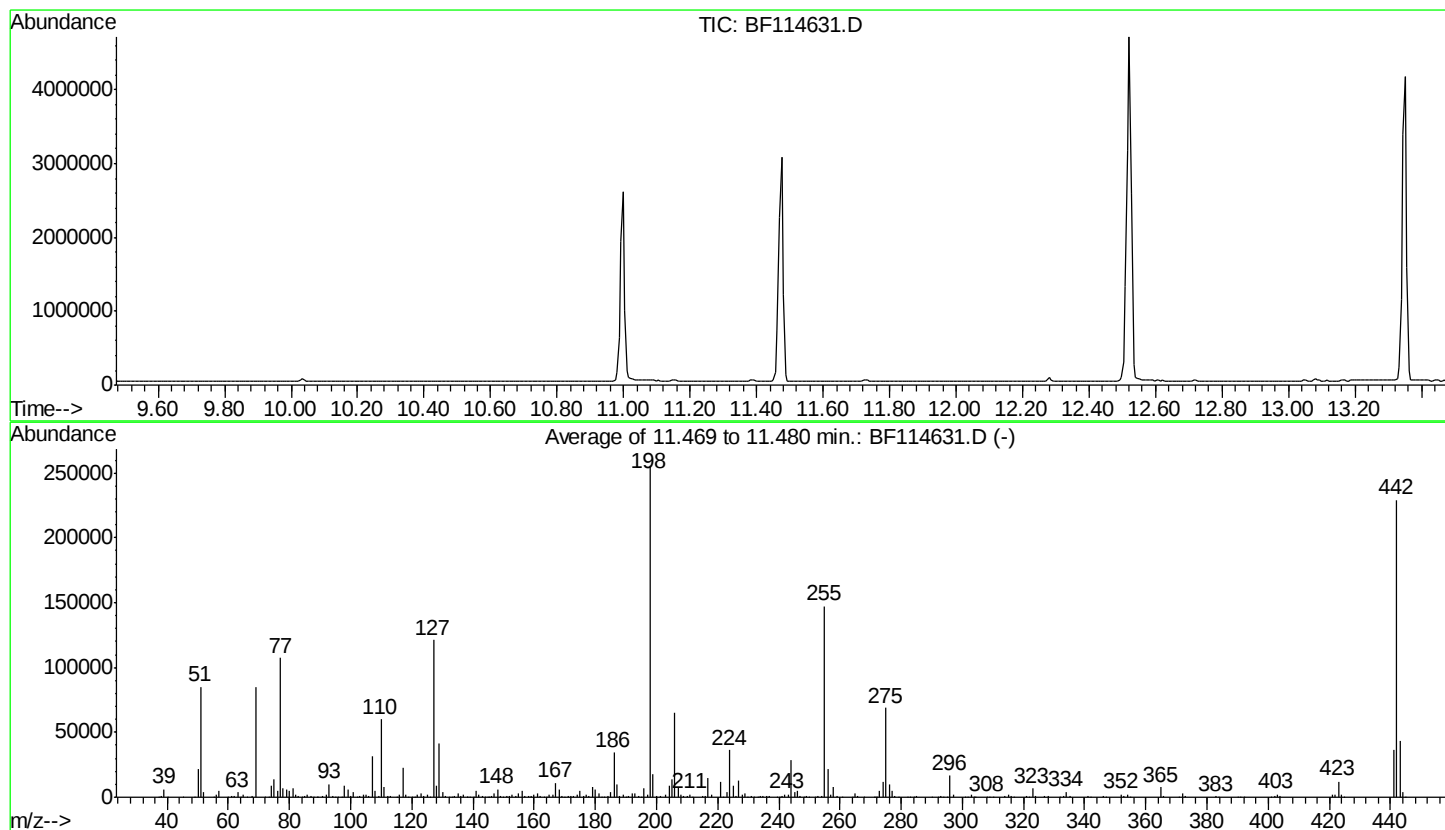

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	85189	PASS
68	69	0.00	2	1.6	1366	PASS
69	198	0.00	100	33.1	84664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	121240	PASS
197	198	0.00	2	0.6	1597	PASS
198	198	100	100	100.0	255592	PASS
199	198	5	9	6.8	17392	PASS
275	198	10	60	26.9	68749	PASS
365	198	1	100	3.0	7683	PASS
441	198	0.01	100	14.2	36232	PASS
442	198	50	100	89.7	229226	PASS
443	442	15	24	19.1	43789	PASS