

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053019\
 Data File : BF114659.D
 Acq On : 30 May 2019 14:26
 Operator : HP/JU
 Sample : PB118819BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118819BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.316	542	549	552	rBV	7980082	9551002	78.74%	9.856%
2	6.334	714	722	724	rBV	7885825	9648792	79.54%	9.957%
3	6.463	738	744	747	rBV	8568778	10174417	83.88%	10.499%
4	6.692	779	783	786	rBV	3161771	2579429	21.26%	2.662%
5	6.851	805	810	813	rBV	8274546	8169337	67.35%	8.430%
6	7.251	872	878	881	rBV	5493704	6735180	55.52%	6.950%
7	7.969	995	1000	1004	rBV	3255240	3372242	27.80%	3.480%
8	9.051	1177	1184	1187	rBV	10257493	12130222	100.00%	12.517%
9	9.716	1291	1297	1301	rBV	4008433	3953788	32.59%	4.080%
10	10.504	1423	1431	1434	rBV	6604251	7563494	62.35%	7.805%
11	11.192	1541	1548	1551	rBV	4758857	4173476	34.41%	4.307%
12	12.780	1810	1818	1821	rBV	10315467	11892993	98.04%	12.273%
13	13.810	1989	1993	1997	rBV	3996097	3626151	29.89%	3.742%
14	15.198	2223	2229	2236	rBV	2797049	3336346	27.50%	3.443%


Sum of corrected areas: 96906869

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF053019\
Data File : BF114659.D
Acq On : 30 May 2019 14:26
Operator : HP/JU
Sample : PB118819BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118819BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

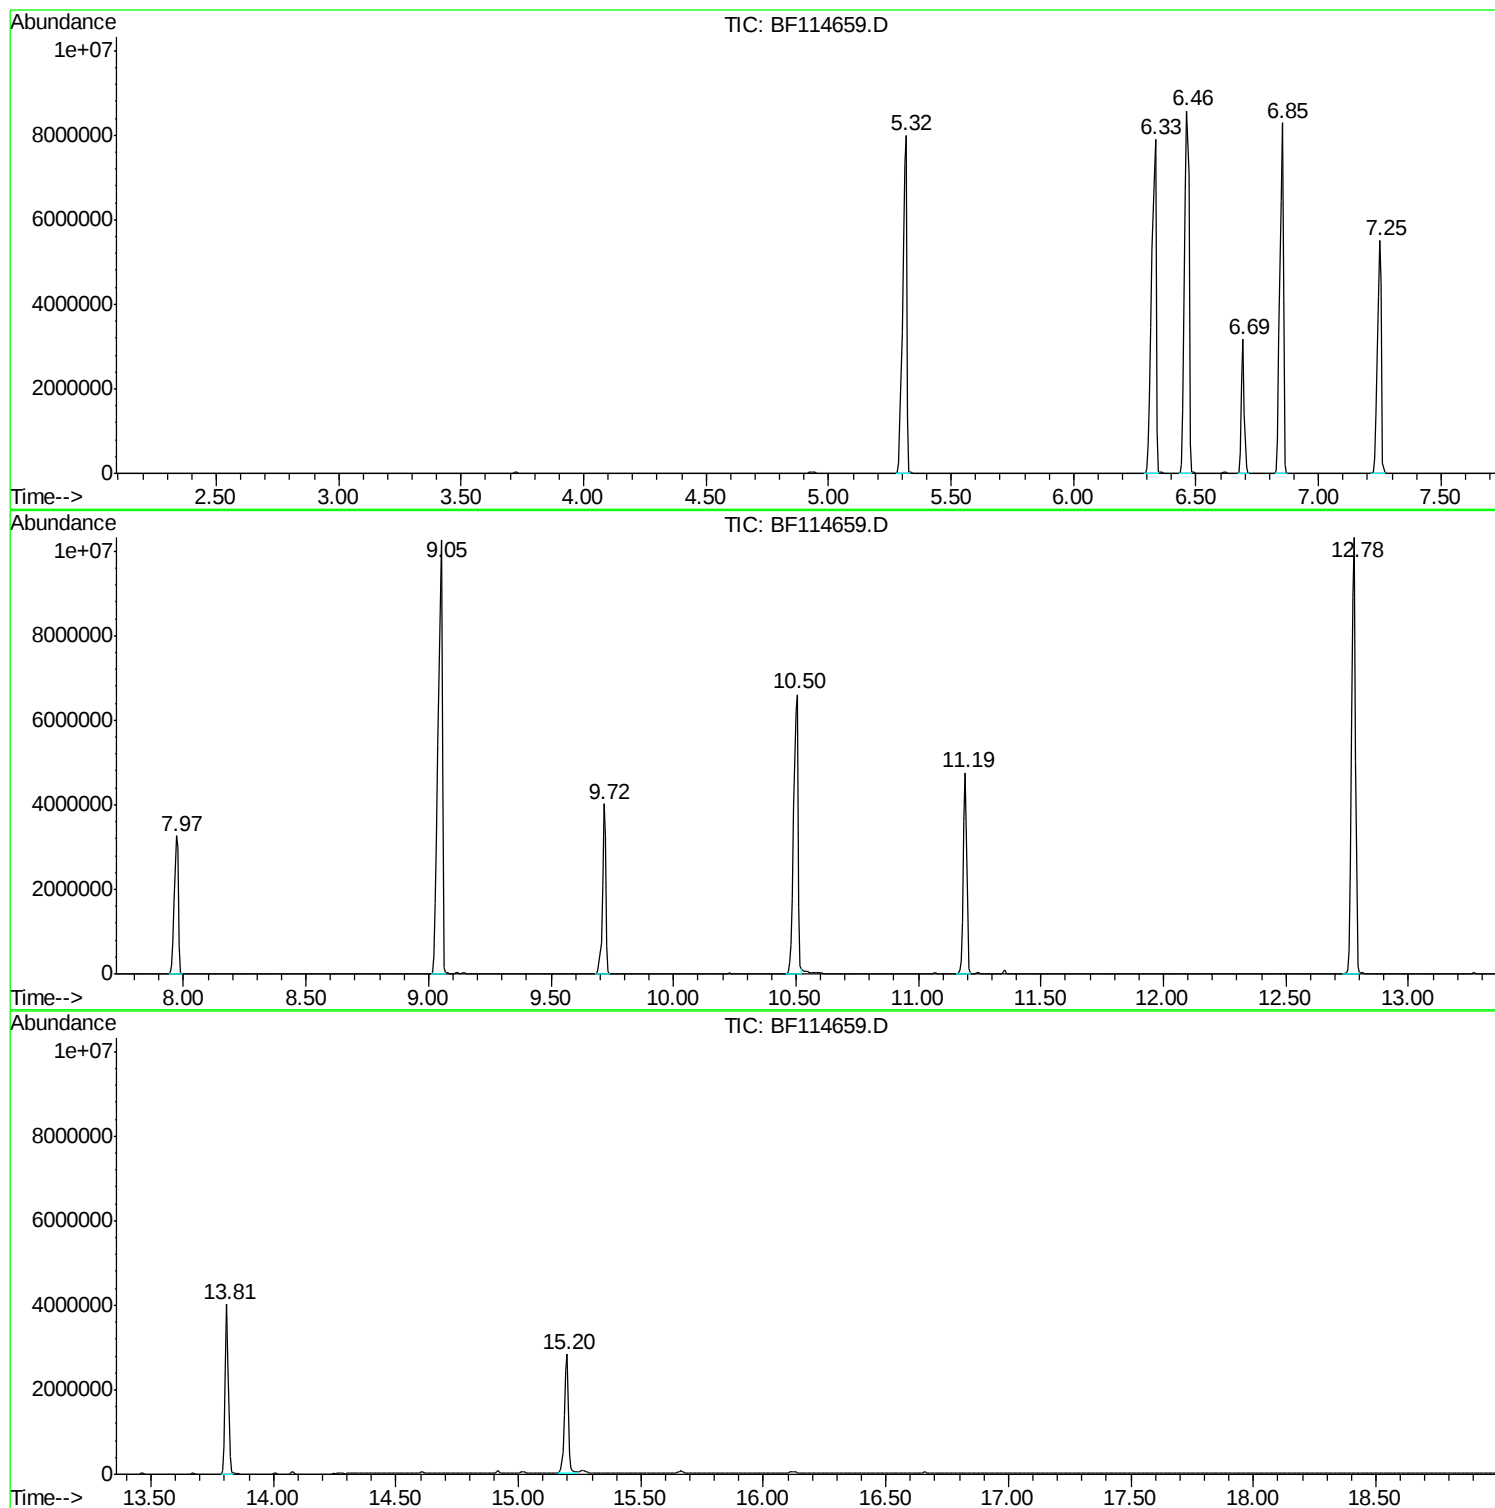

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF053019\
Data File : BF114659.D
Acq On : 30 May 2019 14:26
Operator : HP/JU
Sample : PB118819BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118819BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	78.89 ng	10174400	1,4-Dichlorobenzene-d4	6.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	30
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

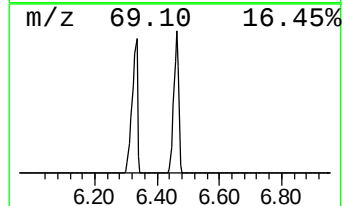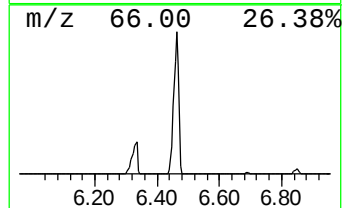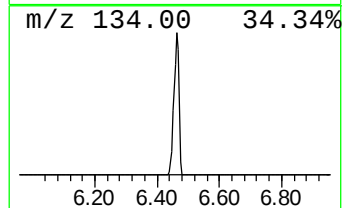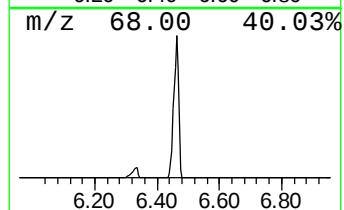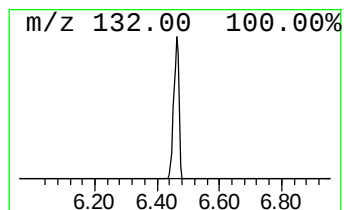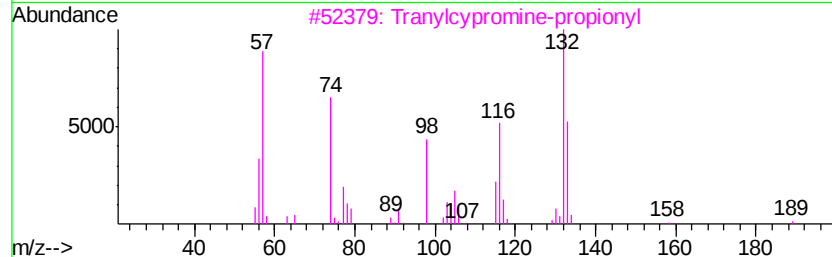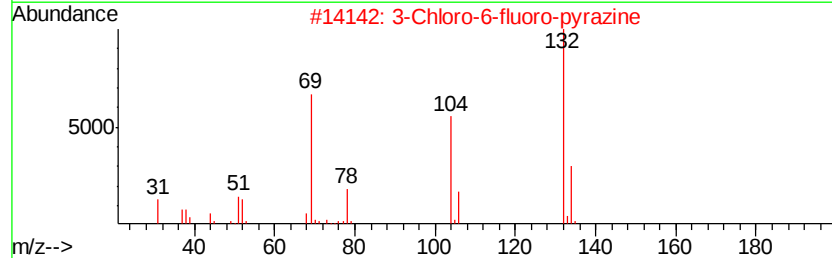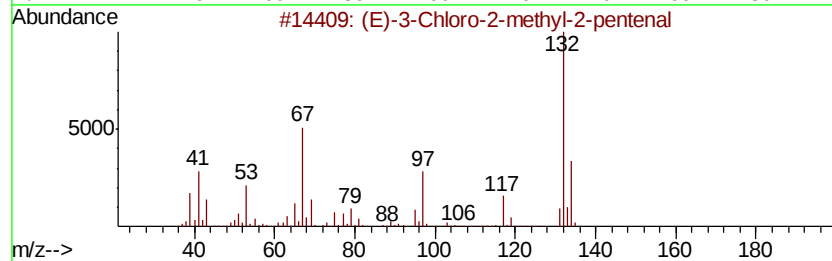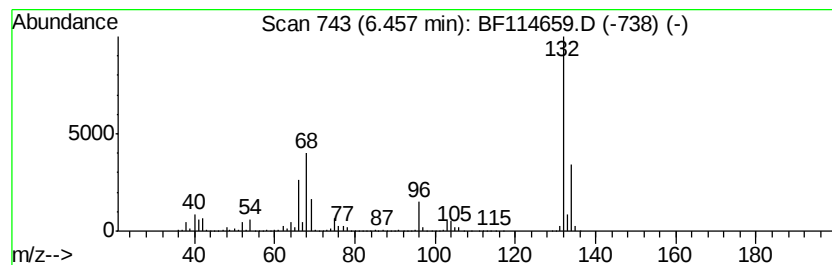

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053019\
Data File : BF114659.D
Acq On : 30 May 2019 14:26
Operator : HP/JU
Sample : PB118819BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118819BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.46	6.46	78.9	ng	10174400	1	6.69	2579430	20.0