


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053019\
Data File : BF114649.D
Acq On : 30 May 2019 8:26
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 31 12:07:00 2019

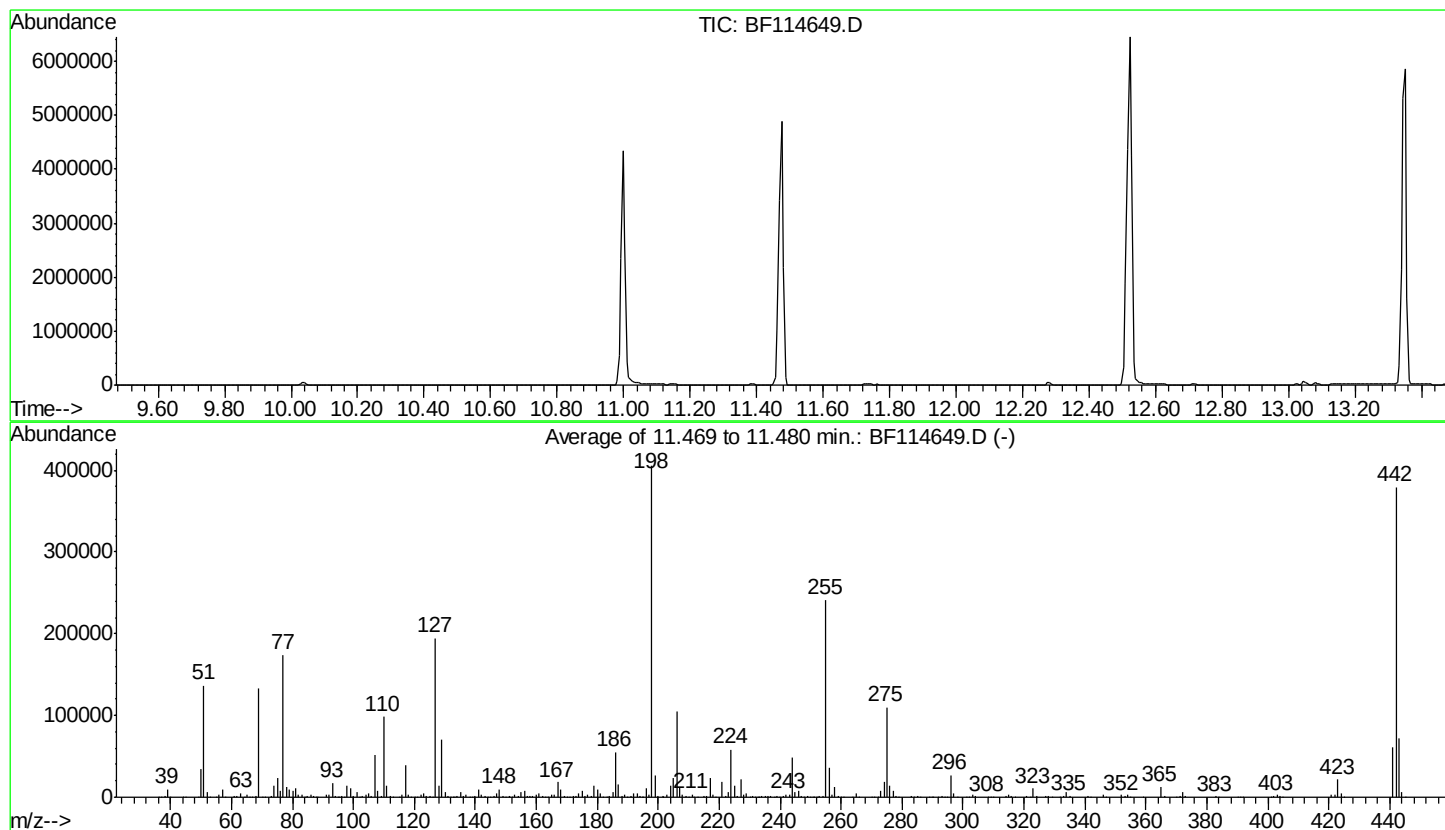

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	136306	PASS
68	69	0.00	2	1.8	2337	PASS
69	198	0.00	100	32.9	133416	PASS
70	69	0.00	2	0.6	783	PASS
127	198	10	80	47.9	194368	PASS
197	198	0.00	2	0.6	2622	PASS
198	198	100	100	100.0	405610	PASS
199	198	5	9	6.7	27190	PASS
275	198	10	60	27.1	110098	PASS
365	198	1	100	3.2	12797	PASS
441	198	0.01	100	15.0	60714	PASS
442	198	50	100	93.5	379114	PASS
443	442	15	24	19.2	72640	PASS