


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053019\
 Data File : BF114668.D
 Acq On : 30 May 2019 18:57
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 31 12:07:00 2019

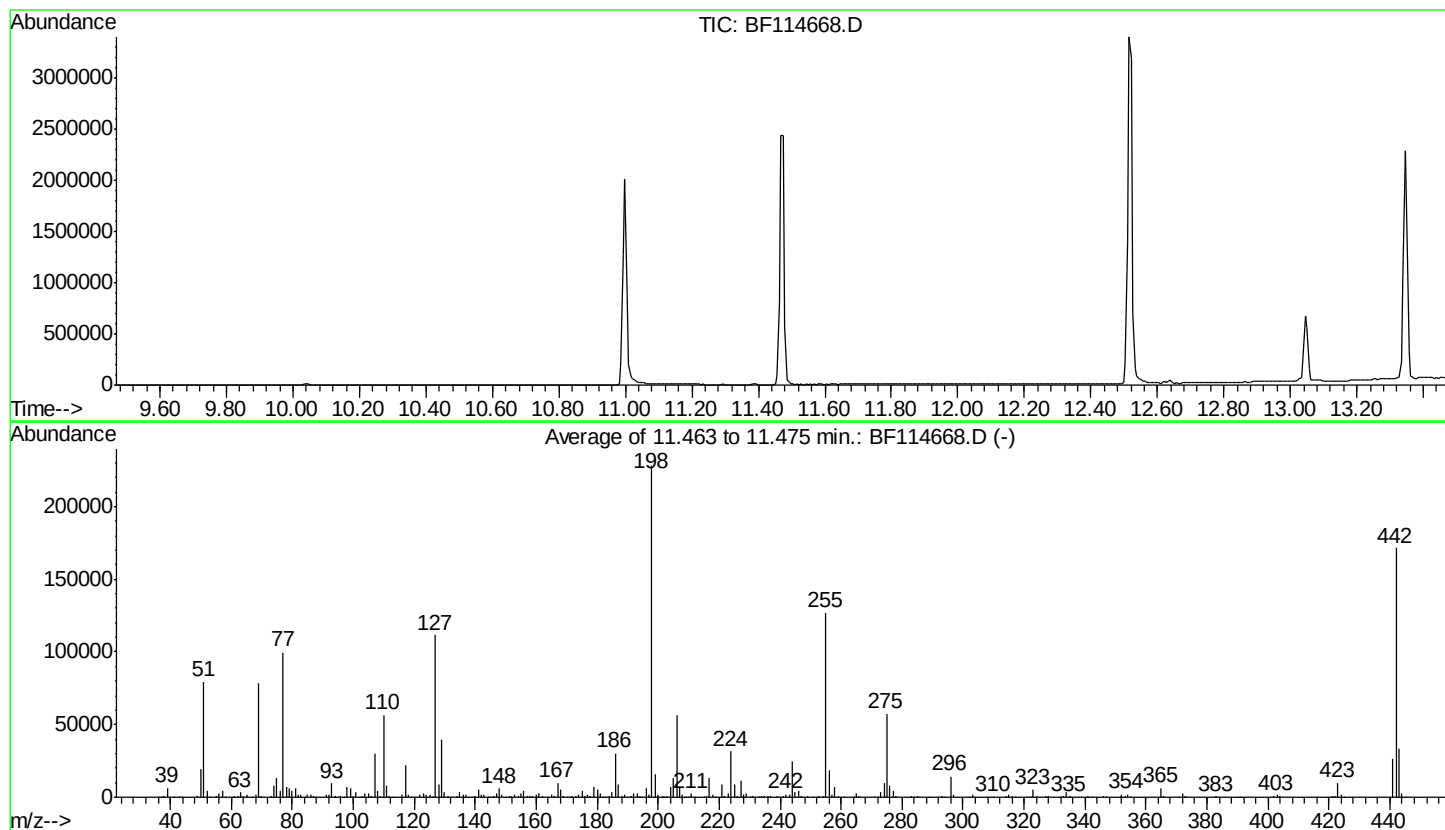

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	79408	PASS
68	69	0.00	2	1.8	1442	PASS
69	198	0.00	100	34.5	78773	PASS
70	69	0.00	2	0.9	680	PASS
127	198	10	80	48.9	111480	PASS
197	198	0.00	2	0.6	1358	PASS
198	198	100	100	100.0	228154	PASS
199	198	5	9	6.8	15468	PASS
275	198	10	60	25.1	57301	PASS
365	198	1	100	2.8	6286	PASS
441	198	0.01	100	11.6	26471	PASS
442	198	50	100	75.2	171461	PASS
443	442	15	24	19.6	33625	PASS