

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053024\
 Data File : BF138075.D
 Acq On : 30 May 2024 14:57
 Operator : CG\JU
 Sample : P2612-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11933

Quant Time: May 30 15:37:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 15 04:12:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.034	152	90486	20.000	ng	-0.01
21) Naphthalene-d8	8.316	136	347277	20.000	ng	-0.01
39) Acenaphthene-d10	10.080	164	209300	20.000	ng	0.00
64) Phenanthrene-d10	11.574	188	339330	20.000	ng	0.00
76) Chrysene-d12	14.233	240	133816	20.000	ng	0.00
86) Perylene-d12	15.815	264	66378m	20.000	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.681	112	652592	122.508	ng	0.02
7) Phenol-d6	6.663	99	703827	107.259	ng	0.00
23) Nitrobenzene-d5	7.598	82	533716	90.445	ng	-0.01
42) 2,4,6-Tribromophenol	10.880	330	312873	148.255	ng	0.00
45) 2-Fluorobiphenyl	9.398	172	1228982	90.450	ng	0.00
79) Terphenyl-d14	13.168	244	1126724	124.093	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053024\
Data File : BF138075.D
Acq On : 30 May 2024 14:57
Operator : CG\JU
Sample : P2612-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11933

Quant Time: May 30 15:37:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration




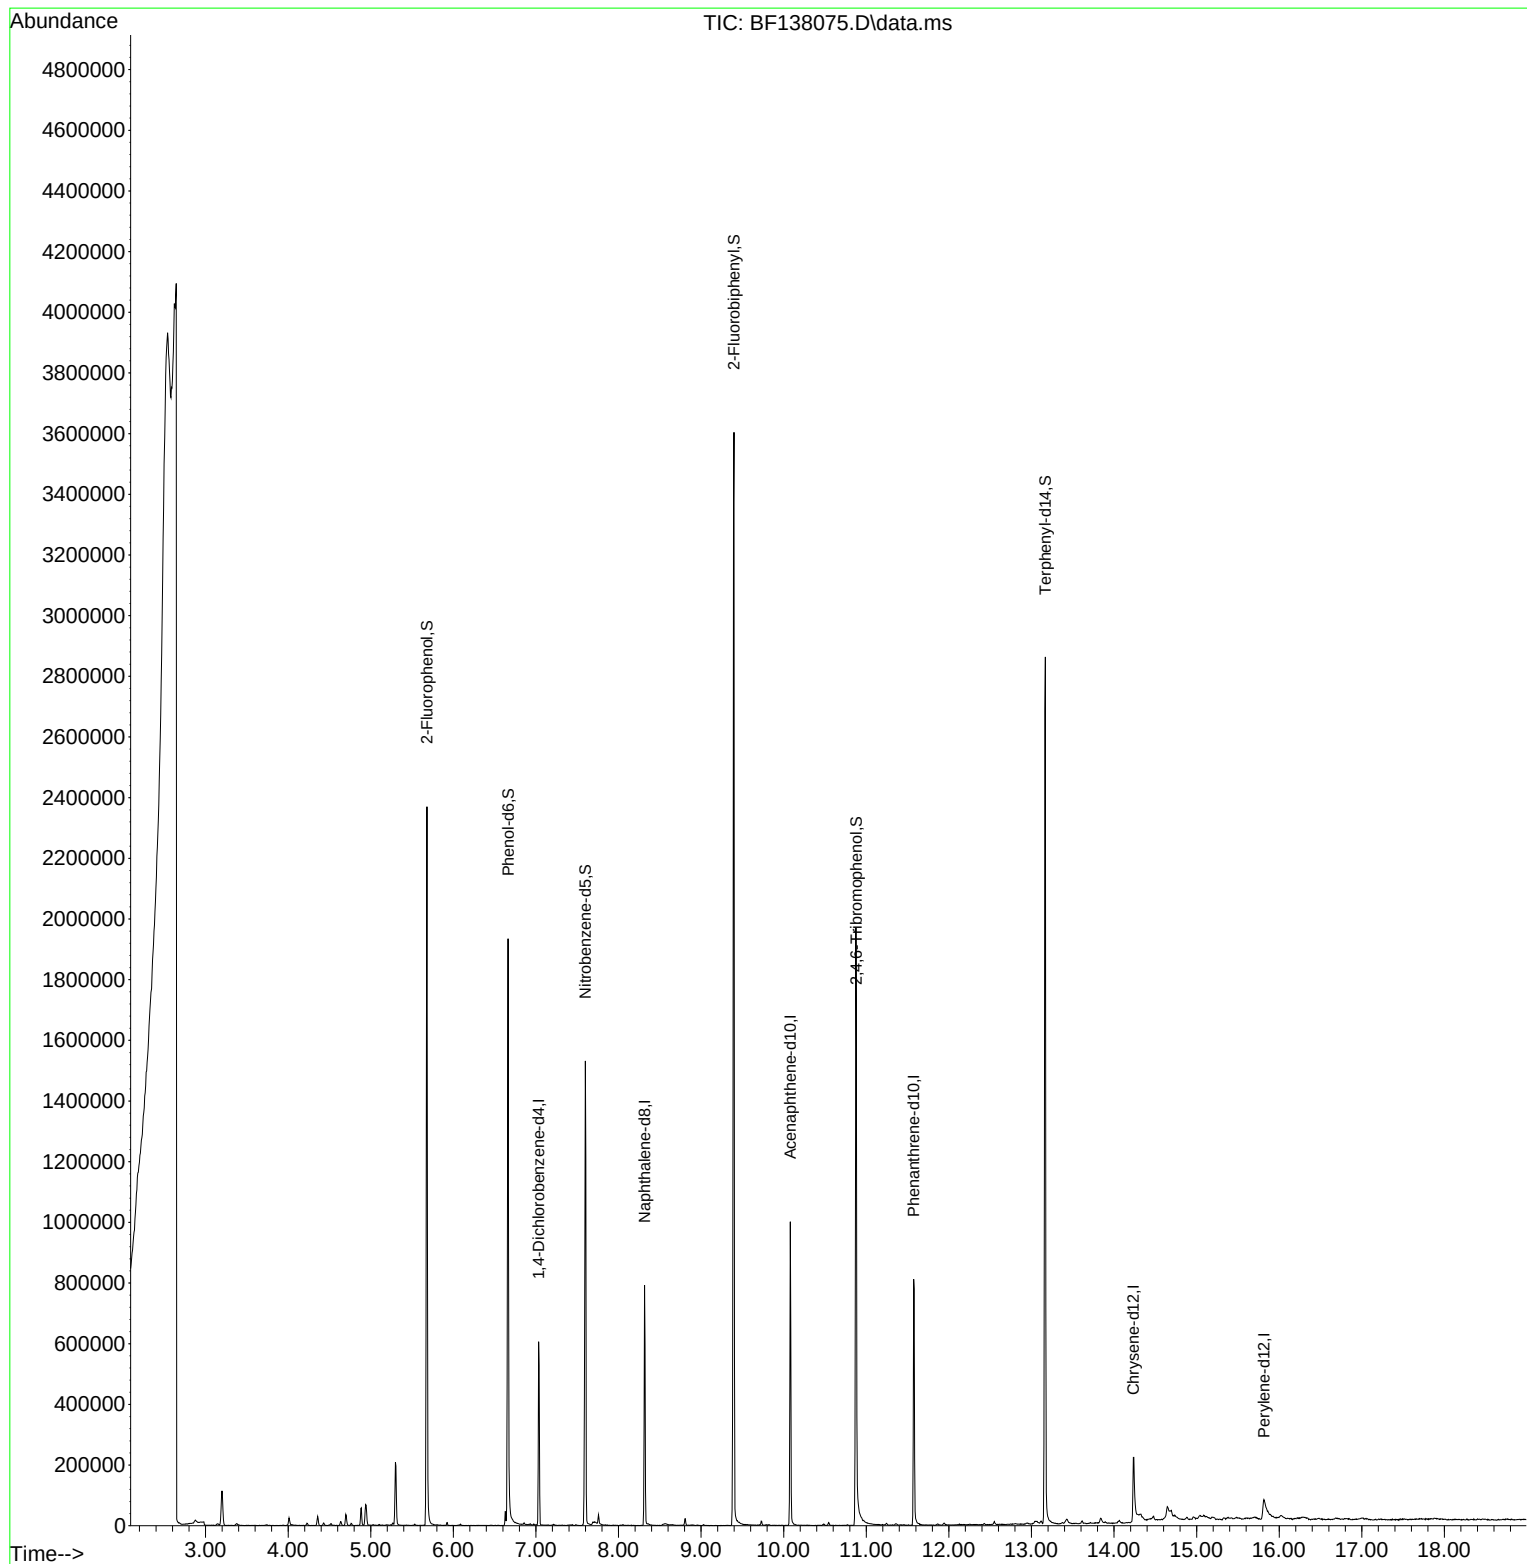


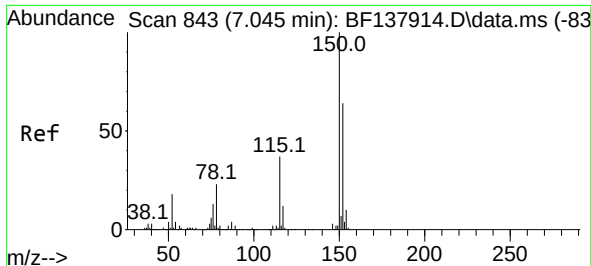

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.034 min Scan# 84
Delta R.T. -0.011 min
Lab File: BF138075.D
Acq: 30 May 2024 14:57




Instrument :
BNA_F
ClientSampleId :
72-11933


Tgt Ion:152 Resp: 90486
Ion Ratio Lower Upper
152 100
150 160.9 125.7 188.5
115 64.4 47.0 70.6

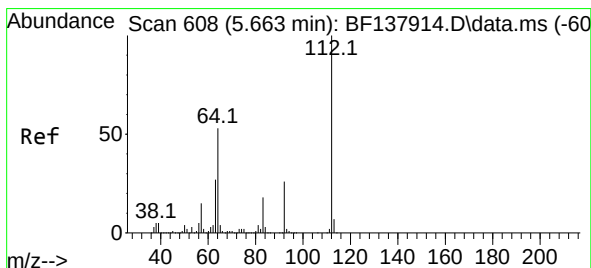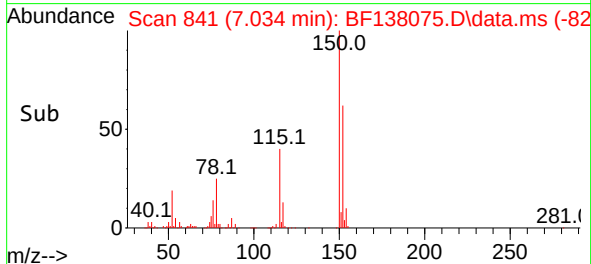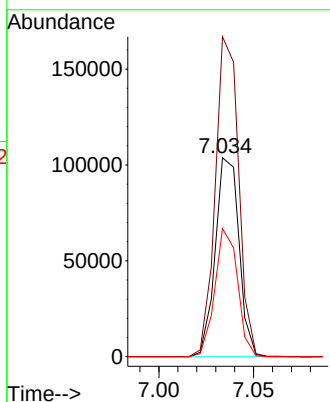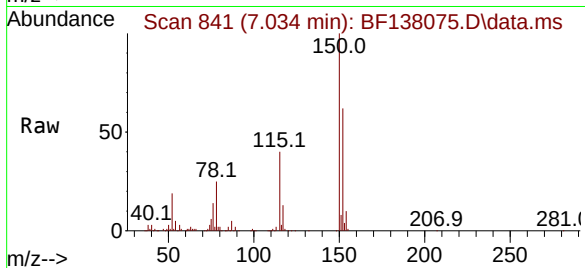

#5
2-Fluorophenol
Concen: 122.508 ng
RT: 5.681 min Scan# 611
Delta R.T. 0.018 min
Lab File: BF138075.D
Acq: 30 May 2024 14:57

Tgt Ion:112 Resp: 652592
Ion Ratio Lower Upper
112 100
64 53.3 42.4 63.6
63 28.0 21.4 32.2


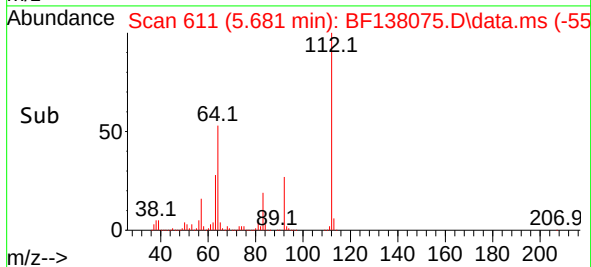
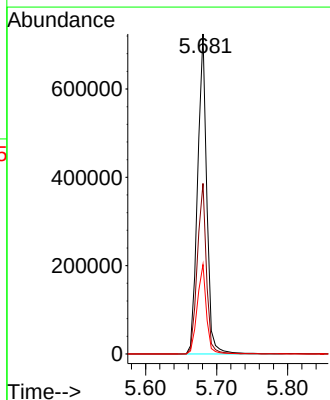
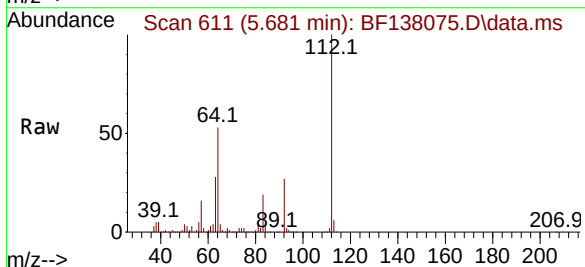


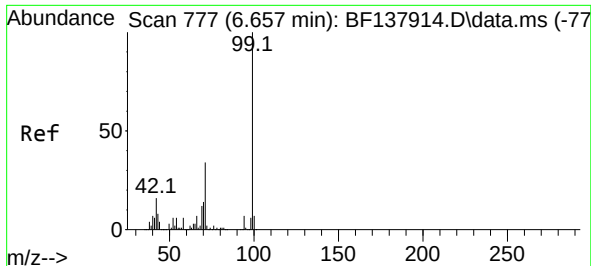

#7
Phenol-d6
Concen: 107.259 ng
RT: 6.663 min Scan# 71
Delta R.T. 0.006 min
Lab File: BF138075.D
Acq: 30 May 2024 14:57




Instrument :
BNA_F
ClientSampleId :
72-11933


Tgt Ion: 99 Resp: 703827
Ion Ratio Lower Upper
99 100
42 15.3 12.6 18.8
71 35.2 27.1 40.7

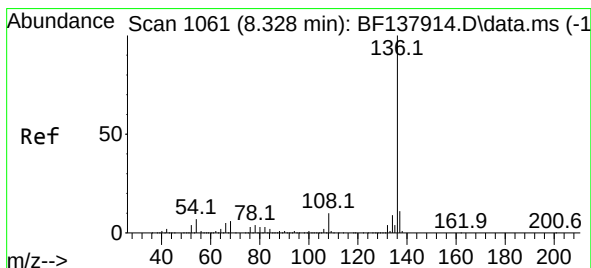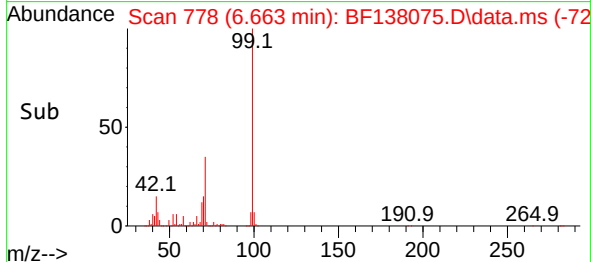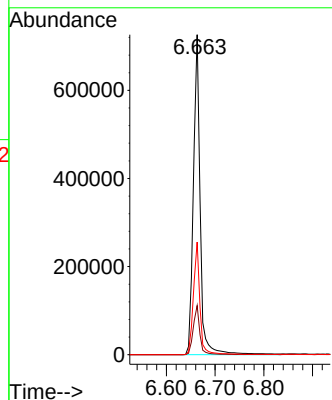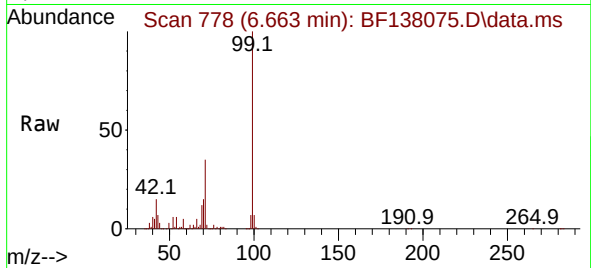

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.316 min Scan# 1059
Delta R.T. -0.012 min
Lab File: BF138075.D
Acq: 30 May 2024 14:57

Tgt Ion: 136 Resp: 347277
Ion Ratio Lower Upper
136 100
137 11.1 8.7 13.1
54 6.4 5.4 8.2
68 5.5 4.6 7.0

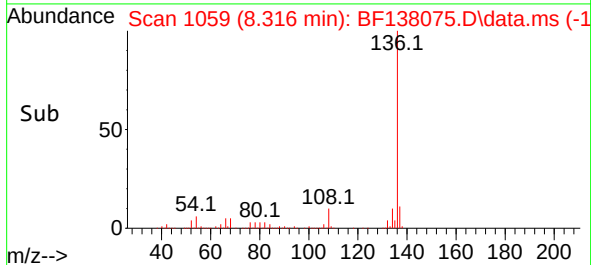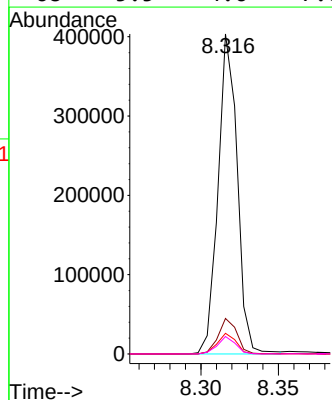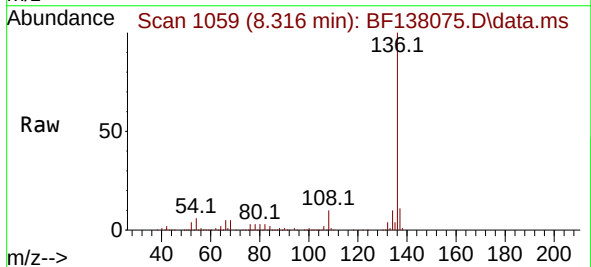

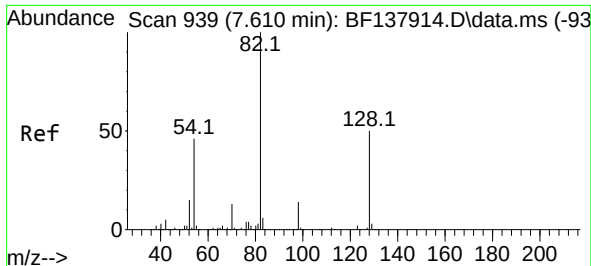

#23

Nitrobenzene-d5

Concen: 90.445 ng

RT: 7.598 min Scan# 91

Delta R.T. -0.012 min

Lab File: BF138075.D

Acq: 30 May 2024 14:57

Instrument :

BNA_F

ClientSampleId :

72-11933





Tgt Ion: 82 Resp: 533716

Ion Ratio Lower Upper

82 100

128 49.3 40.3 60.5

54 46.5 36.8 55.2

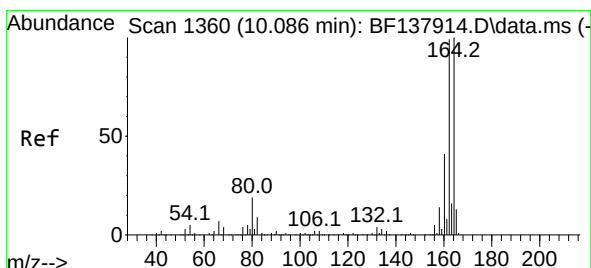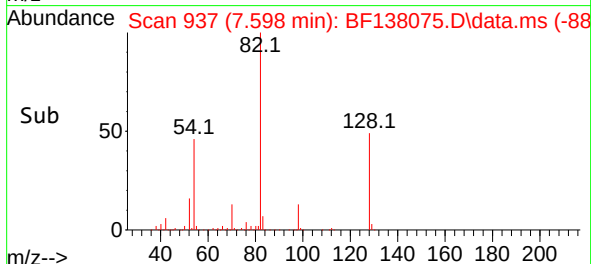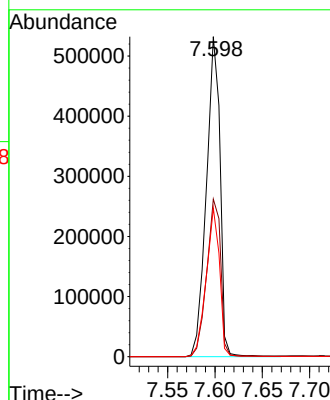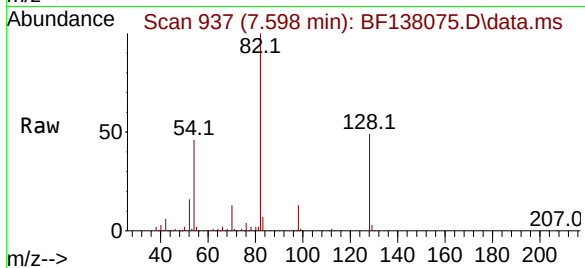

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.080 min Scan# 1359

Delta R.T. -0.006 min

Lab File: BF138075.D

Acq: 30 May 2024 14:57




Tgt Ion:164 Resp: 209300


Ion Ratio Lower Upper

164 100

162 99.9 79.4 119.2

160 43.0 33.1 49.7


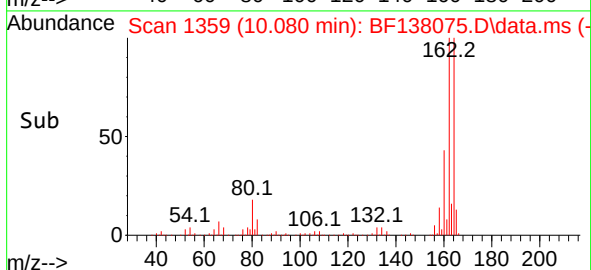
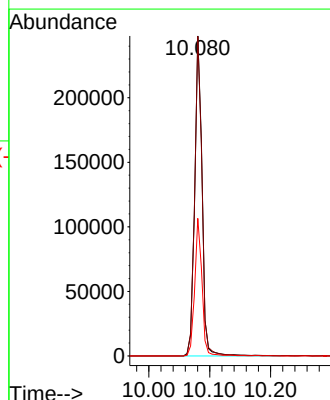
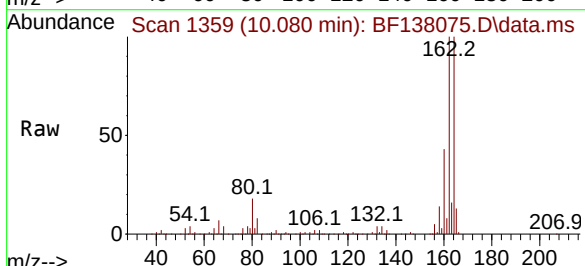


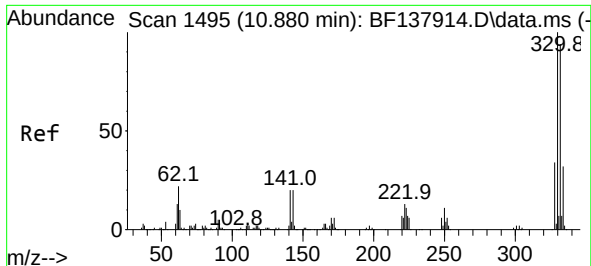

#42
2,4,6-Tribromophenol
Concen: 148.255 ng
RT: 10.880 min Scan# 1495
Delta R.T. 0.000 min
Lab File: BF138075.D
Acq: 30 May 2024 14:57




Instrument :
BNA_F
ClientSampleId :
72-11933


Tgt Ion: 330 Resp: 312873
Ion Ratio Lower Upper
330 100
332 95.8 75.8 113.8
141 27.0 23.8 35.6

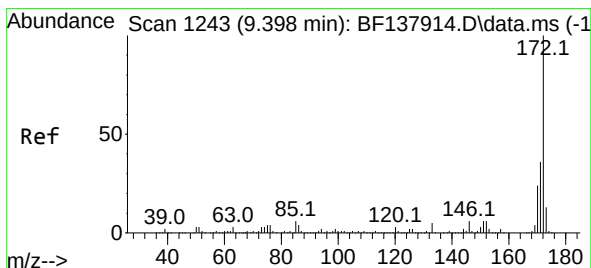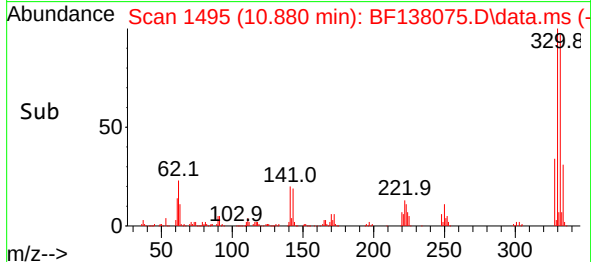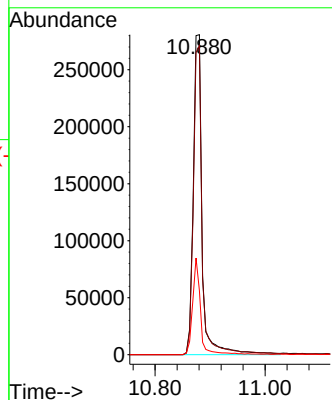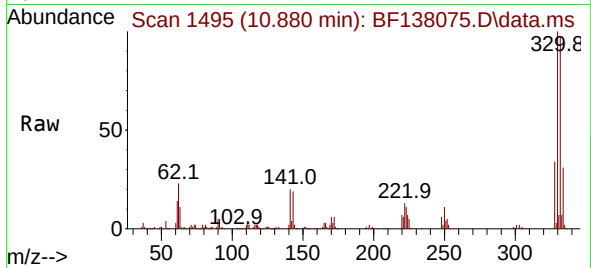

#45
2-Fluorobiphenyl
Concen: 90.450 ng
RT: 9.398 min Scan# 1243
Delta R.T. 0.000 min
Lab File: BF138075.D
Acq: 30 May 2024 14:57

Tgt Ion: 172 Resp: 1228982
Ion Ratio Lower Upper
172 100
171 36.4 28.9 43.3
170 22.9 18.9 28.3

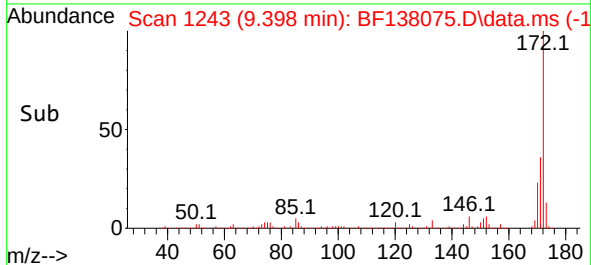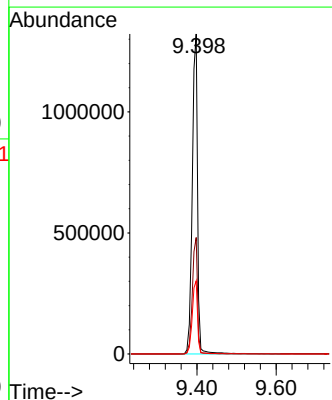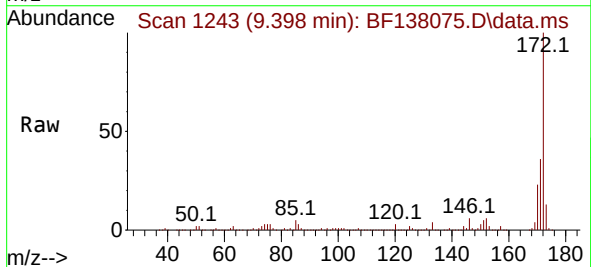

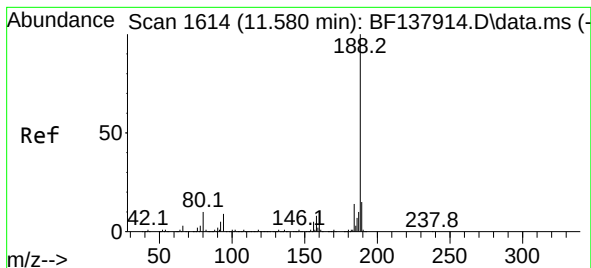

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.574 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF138075.D

Acq: 30 May 2024 14:57

Instrument :

BNA_F

ClientSampleId :

72-11933





Tgt Ion:188 Resp: 339330

Ion Ratio Lower Upper

188 100

94 9.1 7.0 10.4

80 10.2 7.7 11.5

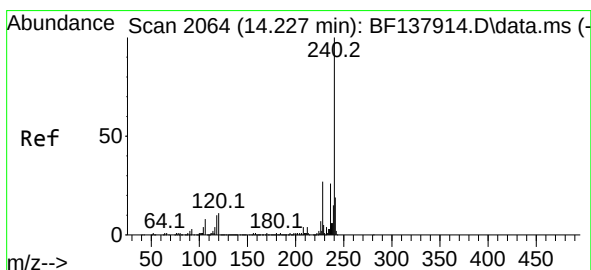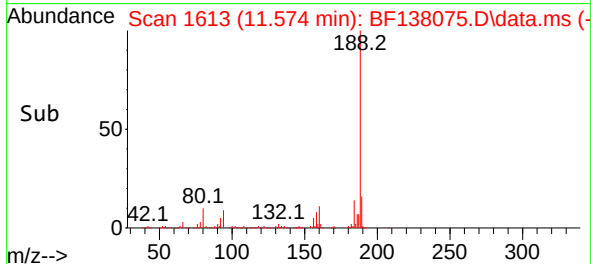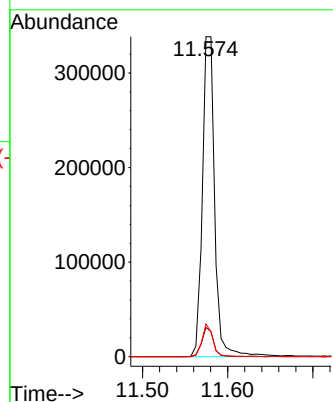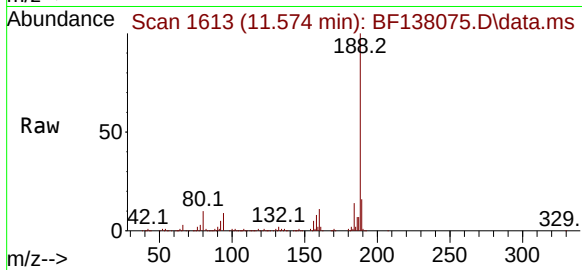

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.233 min Scan# 2065

Delta R.T. 0.006 min

Lab File: BF138075.D

Acq: 30 May 2024 14:57




Tgt Ion:240 Resp: 133816


Ion Ratio Lower Upper

240 100

120 11.4 8.9 13.3

236 24.9 21.0 31.4


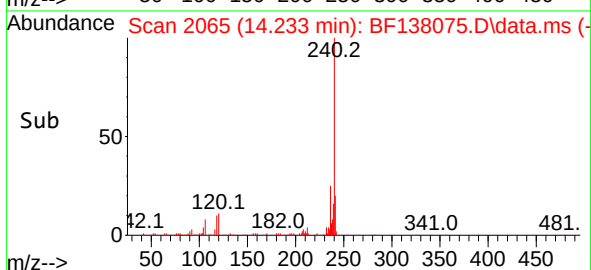
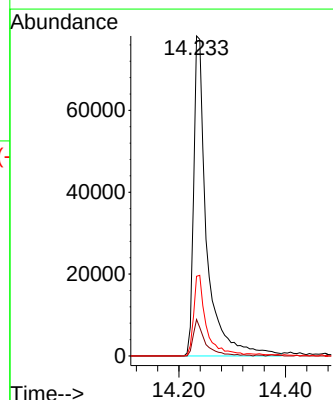
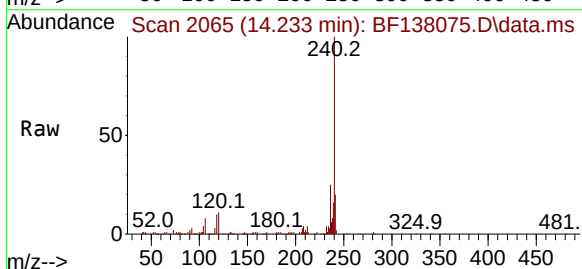


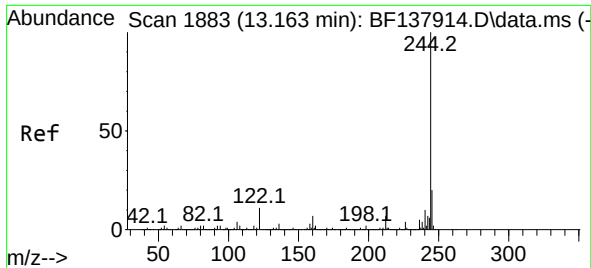

#79
 Terphenyl-d14
 Concen: 124.093 ng
 RT: 13.168 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BF138075.D
 Acq: 30 May 2024 14:57

Instrument :
 BNA_F
 ClientSampleId :
 72-11933

Tgt Ion:244 Resp: 1126724
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.6 8.4
 122 8.7 8.8 13.2#

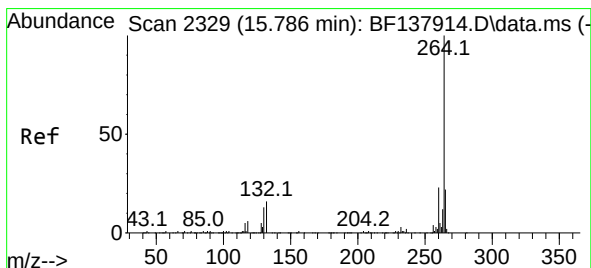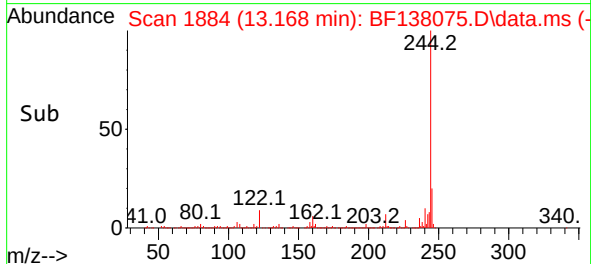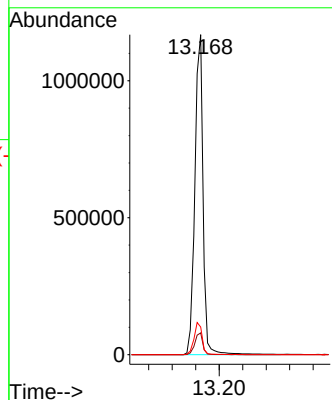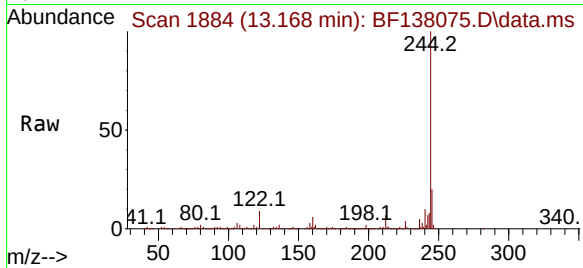

#86
 Perylene-d12
 Concen: 20.000 ng m
 RT: 15.815 min Scan# 2334
 Delta R.T. 0.029 min
 Lab File: BF138075.D
 Acq: 30 May 2024 14:57

Tgt Ion:264 Resp: 66378
 Ion Ratio Lower Upper
 264 100
 260 26.8 18.3 27.5
 265 22.3 17.6 26.4

