


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053024\
Data File : BF138065.D
Acq On : 30 May 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

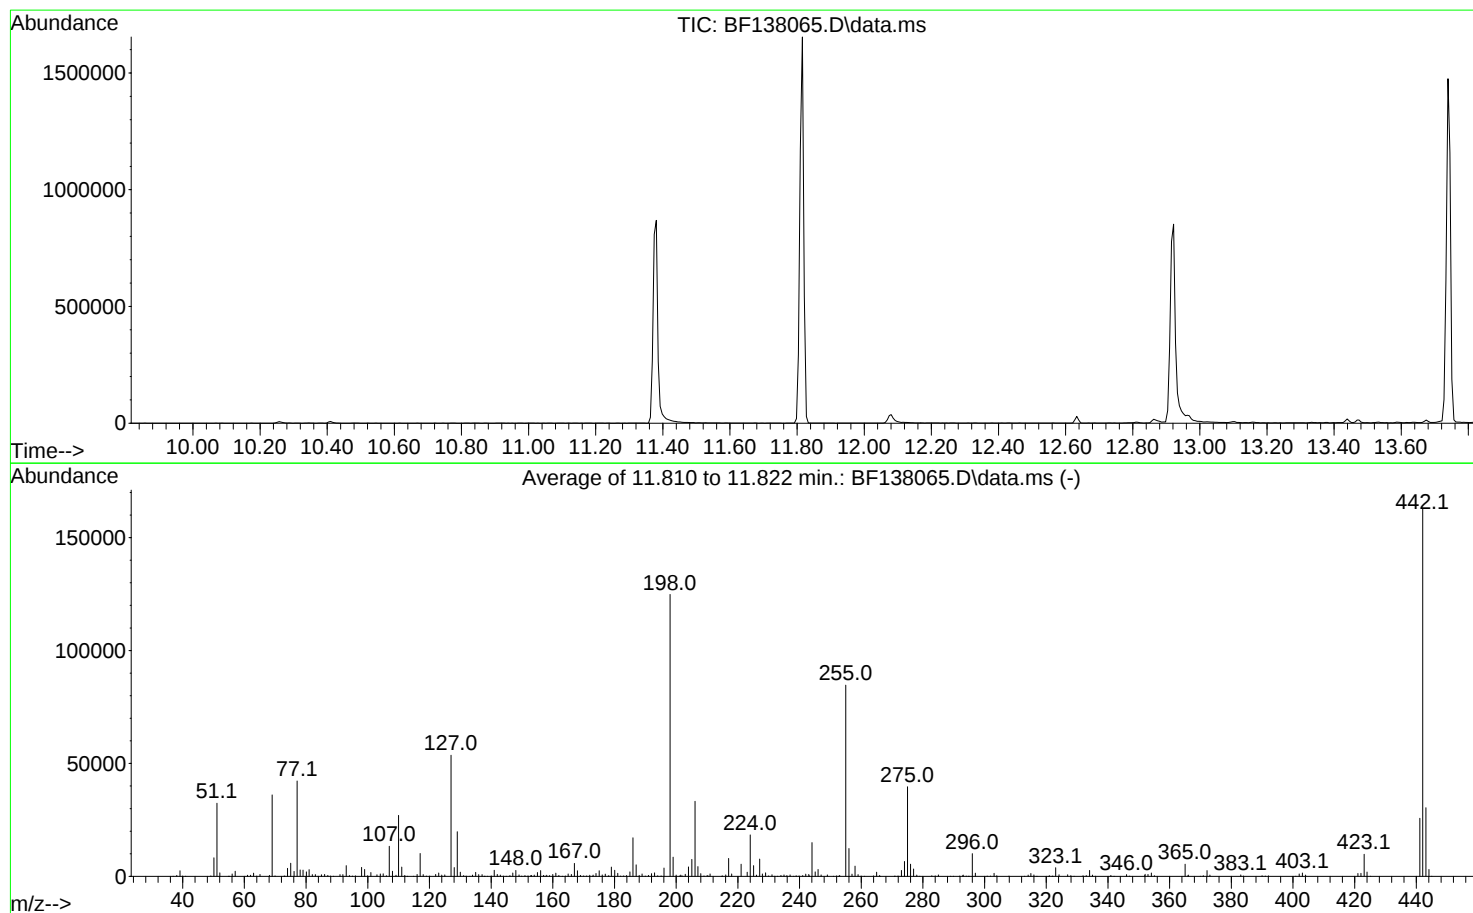

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	32411	PASS
68	69	0.00	2	1.2	428	PASS
69	198	0.00	100	28.9	36045	PASS
70	69	0.00	2	0.6	217	PASS
127	198	10	80	43.0	53648	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124840	PASS
199	198	5	9	6.8	8509	PASS
275	198	10	60	31.8	39672	PASS
365	198	1	100	4.3	5355	PASS
441	198	0.01	100	20.6	25759	PASS
442	442	50	100	100.0	162899	PASS
443	442	15	24	18.7	30408	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/30/2024	BNA_F	<u>BF138065.D</u>
Compound Name	Response	Retention Time
DDT	264346	13.739
DDD	6540	13.439
DDE	1013	13.104
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7553	271899	2.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053024\
Data File : BF138065.D
Acq On : 30 May 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 12:00:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

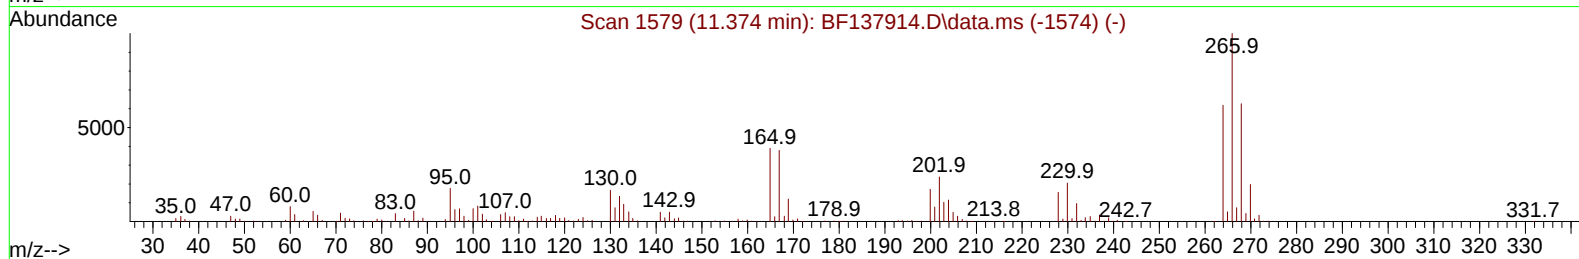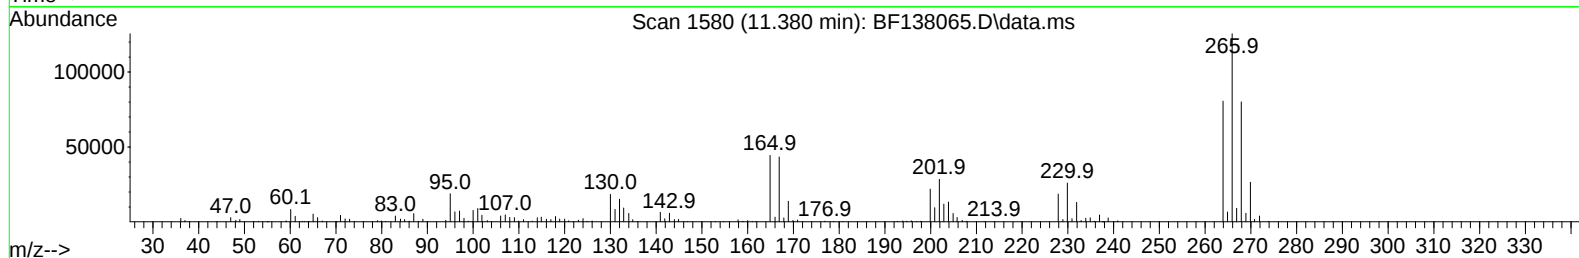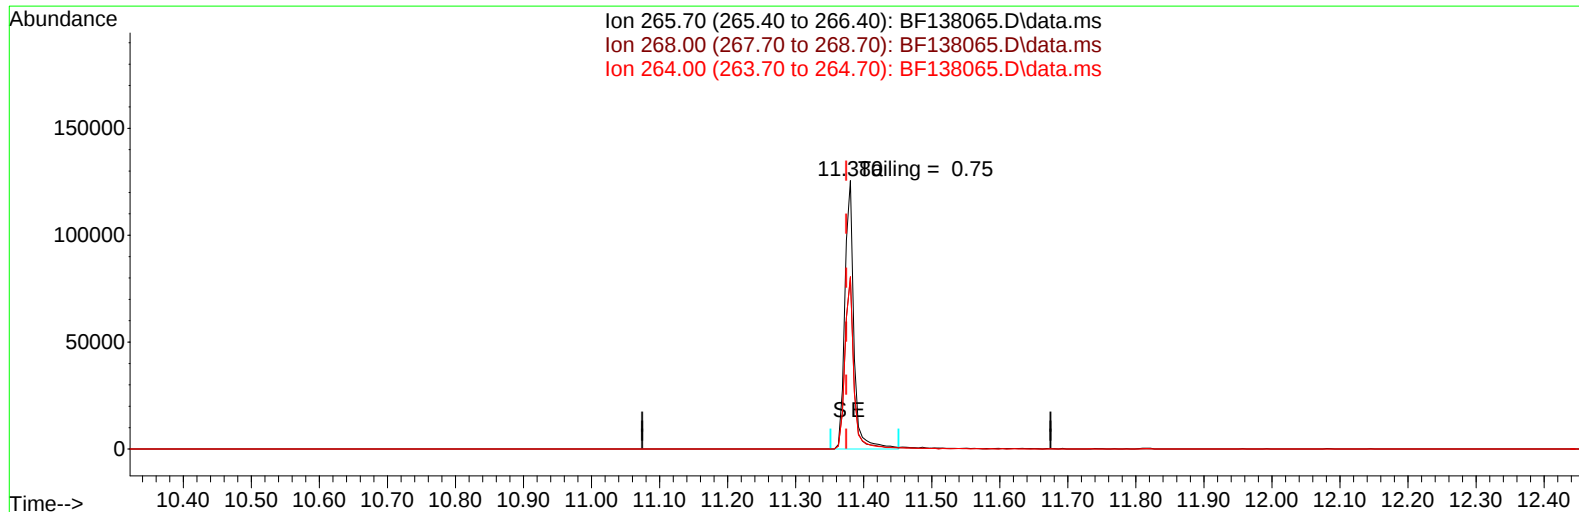

TIC: BF138065.D\data.ms

(70) Pentachlorophenol (C)

11.380min (+ 0.006) 32424.48 ng




response 116002

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.76
264.00	61.80	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053024\
Data File : BF138065.D
Acq On : 30 May 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 12:00:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

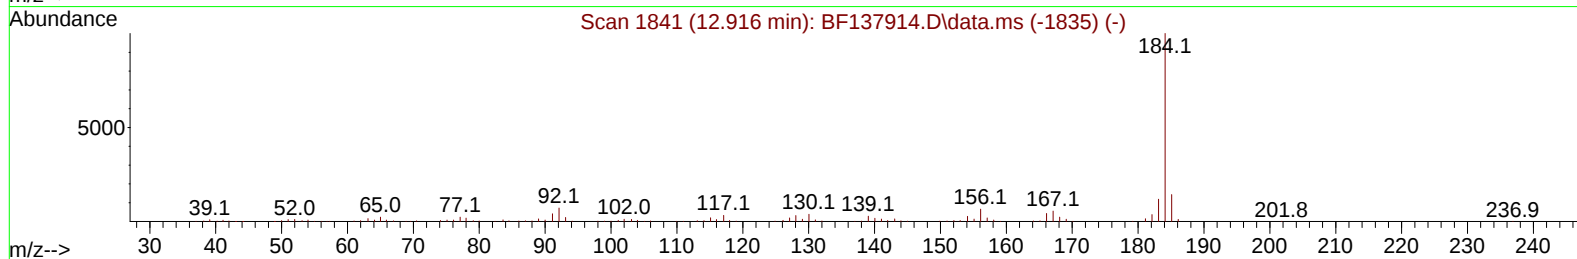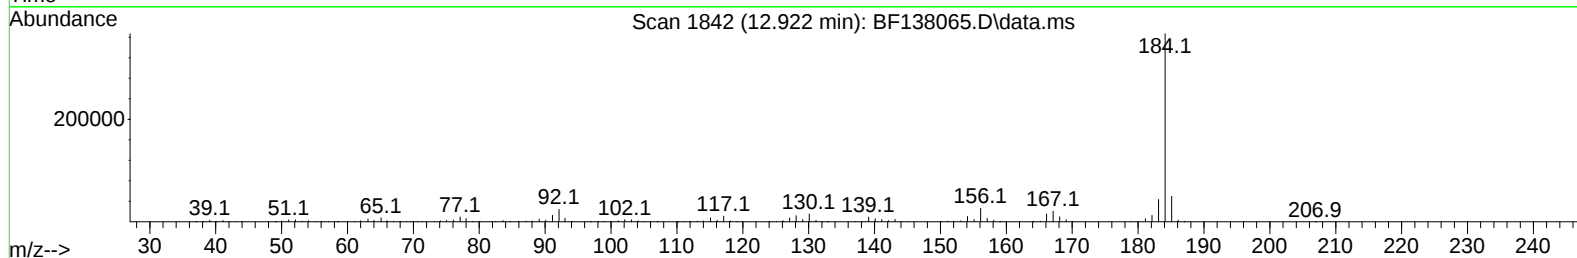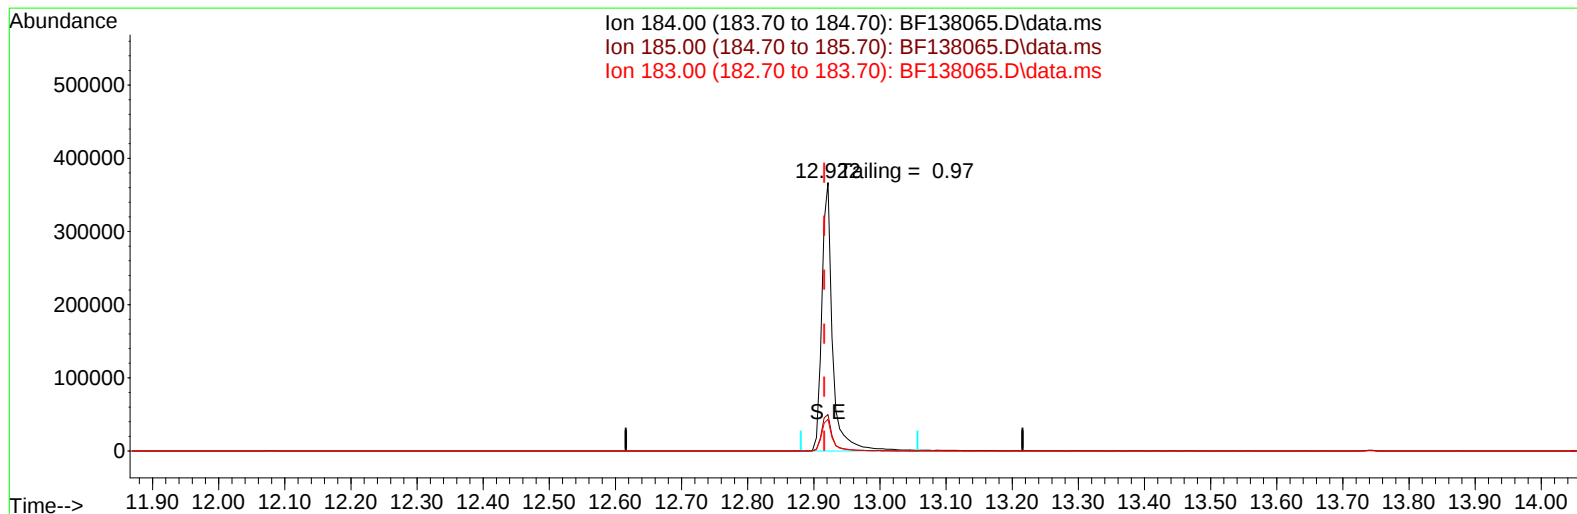

TIC: BF138065.D\data.ms

(77) Benzidine

12.922min (+ 0.006) 0.00 ng

response 414443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.59
183.00	11.90	11.83
0.00	0.00	0.00