

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053119\
 Data File : BF114706.D
 Acq On : 31 May 2019 14:18
 Operator : HP/JU
 Sample : K2986-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FESB-21(4.5-5)

Quant Time: Jun 01 00:22:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 29 19:08:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	271862	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	973087	20.00	ng	0.00
39) Acenaphthene-d10	9.72	164	486582	20.00	ng	0.00
64) Phenanthrene-d10	11.19	188	978123	20.00	ng	0.00
76) Chrysene-d12	13.82	240	796568	20.00	ng	0.00
87) Perylene-d12	15.21	264	725693	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.30	112	2179779	140.77	ng	0.01
7) Phenol-d6	6.33	99	2650438	142.04	ng	0.00
23) Nitrobenzene-d5	7.26	82	1656821	106.23	ng	0.00
42) 2,4,6-Tribromophenol	10.50	330	743419	160.35	ng	0.00
45) 2-Fluorobiphenyl	9.05	172	3005927	123.25	ng	0.00
79) Terphenyl-d14	12.78	244	3460354	81.68	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.33	77	4607	Below Cal	#	1
10) Phenol	6.34	94	46218	2.050	ng	72
19) n-Nitroso-di-n-propylamine	7.26	70	226155	17.559	ng	75
25) Isophorone	7.26	82	1616251	51.635	ng	63
50) Dimethylphthalate	9.44	163	498534	14.704	ng	98
57) 2,4-Dinitrotoluene	9.72	165	63306	6.261	ng	23
58) Fluorene	10.50	166	33339	Below Cal	#	93
67) 4-Bromophenyl-phenylether	10.50	248	48297	4.605	ng	1
74) Di-n-butylphthalate	11.77	149	8844	Below Cal	#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053119\
Data File : BF114706.D
Acq On : 31 May 2019 14:18
Operator : HP/JU
Sample : K2986-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FESB-21(4.5-5)

Quant Time: Jun 01 00:22:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 19:08:51 2019
Response via : Initial Calibration

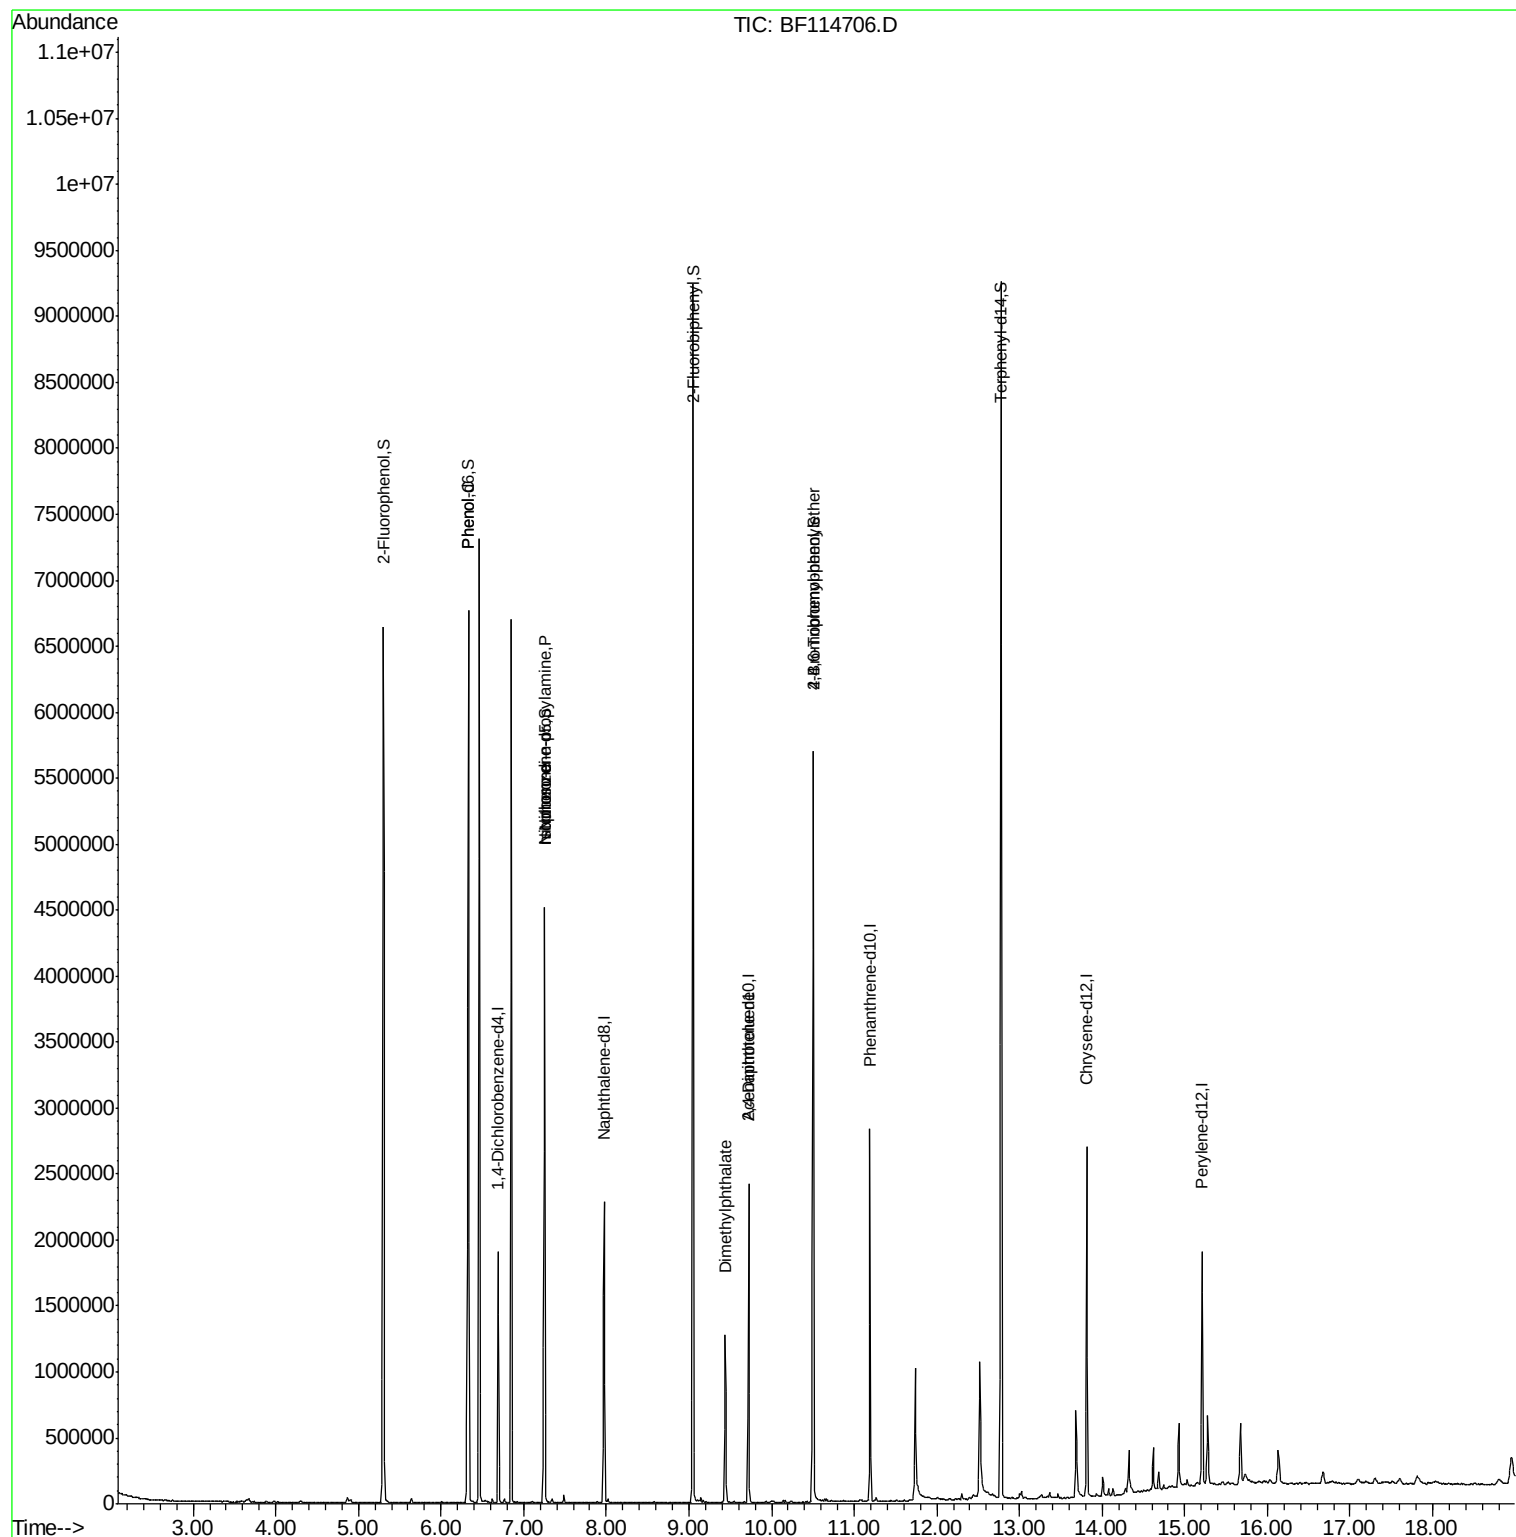

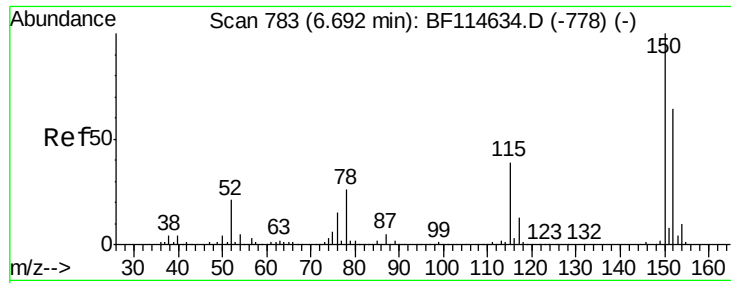


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.69 min Scan# 783
 Delta R.T. -0.00 min
 Lab File: BF114706.D
 Acq: 31 May 2019 14:18

Instrument :
 BNA_F
 ClientSampleId :
 FESB-21(4.5-5)

Tgt Ion:152 Resp: 271862
 Ion Ratio Lower Upper
 152 100
 150 161.0 124.4 186.6
 115 60.2 48.7 73.1




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

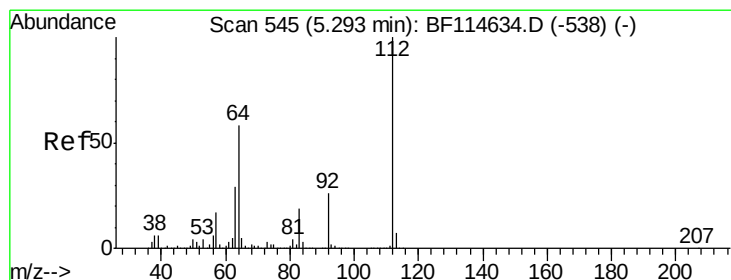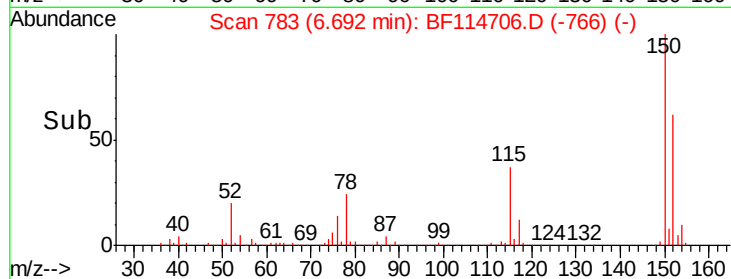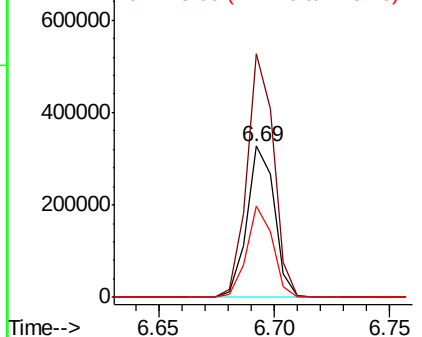



#5




2-Fluorophenol
 Concen: 140.772 ng
 RT: 5.30 min Scan# 547
 Delta R.T. 0.01 min
 Lab File: BF114706.D
 Acq: 31 May 2019 14:18

Tgt Ion:112 Resp: 2179779
 Ion Ratio Lower Upper
 112 100
 64 55.6 46.1 69.1
 63 29.0 23.4 35.2

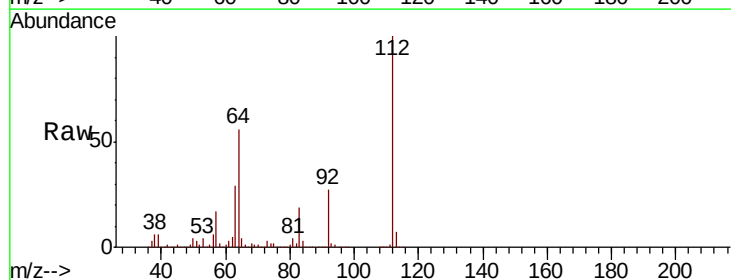

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

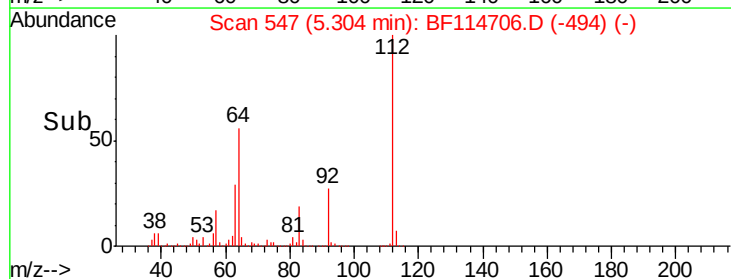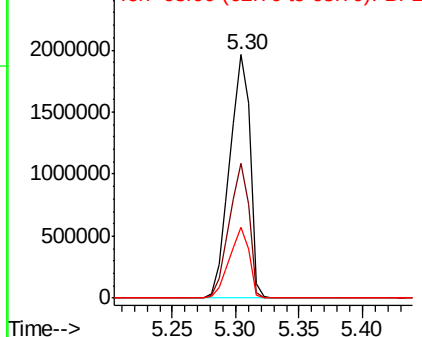

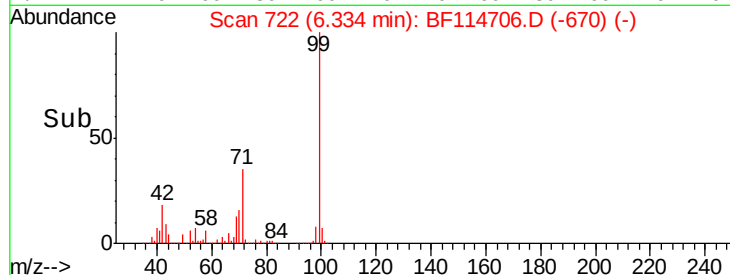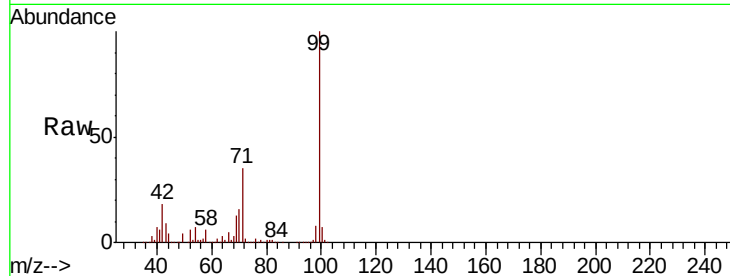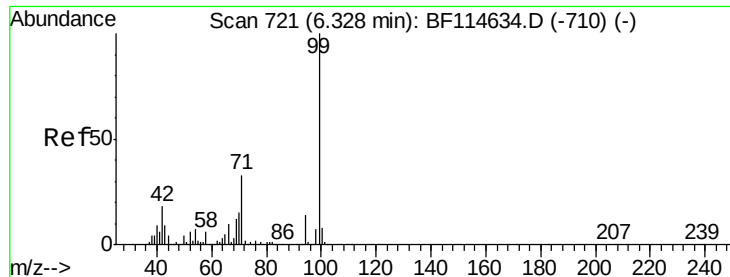

#7

Phenol-d6

Concen: 142.044 ng

RT: 6.33 min Scan# 722

Delta R.T. 0.01 min

Lab File: BF114706.D

Acq: 31 May 2019 14:18

Instrument :

BNA_F

ClientSampleId :

FESB-21(4.5-5)





Tgt Ion: 99 Resp: 2650438

Ion Ratio Lower Upper

99 100

42 17.7 14.7 22.1

71 34.9 26.6 40.0

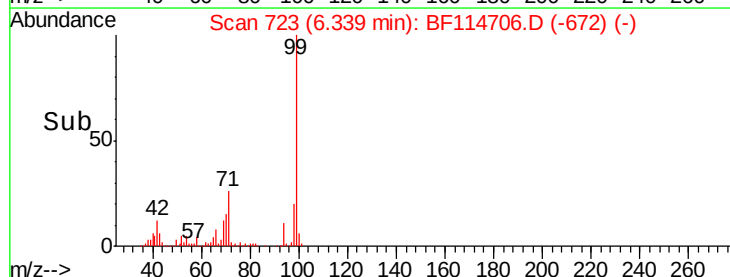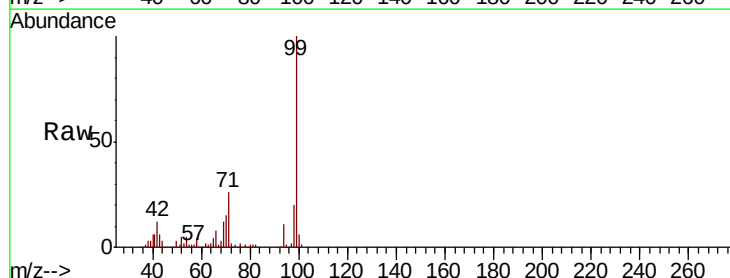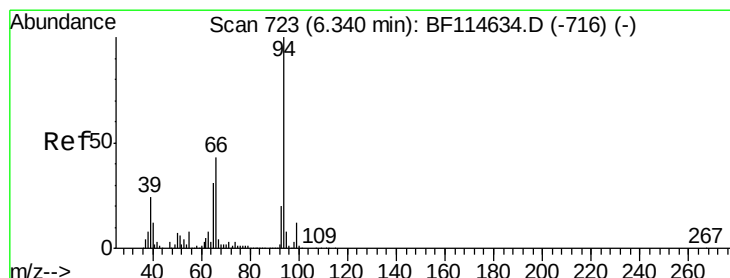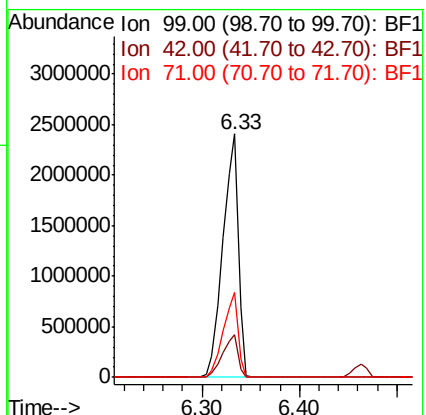

#10

Phenol

Concen: 2.050 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.00 min

Lab File: BF114706.D

Acq: 31 May 2019 14:18


Tgt Ion: 94 Resp: 46218


Ion Ratio Lower Upper

94 100

65 34.0 11.0 51.0

66 70.8 23.0 63.0#




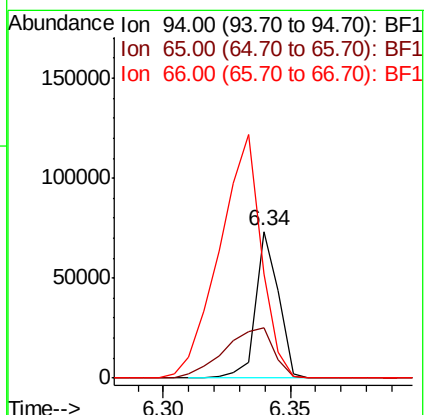




#19
n-Nitroso-di-n-propylamine
Concen: 17.559 ng
RT: 7.26 min Scan# 879
Delta R.T. 0.14 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18




Instrument :
BNA_F
ClientSampleId :
FESB-21(4.5-5)


Tgt Ion:	70	Resp:	226155
Ion	Ratio	Lower	Upper
70	100		
42	44.1	44.4	66.6#
101	0.0	8.2	12.4#
130	2.5	19.4	29.0#

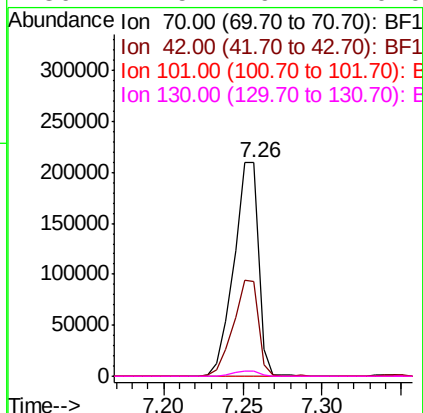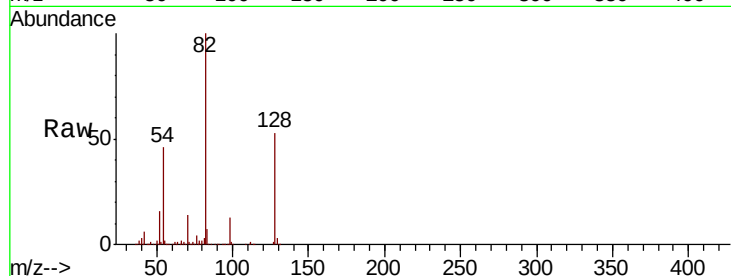

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.97 min Scan# 1001
Delta R.T. -0.00 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Tgt Ion:	136	Resp:	973087
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.3	13.9
54	6.6	6.3	9.5
68	5.8	5.4	8.0

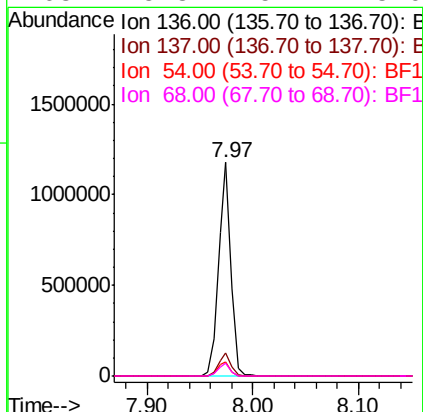


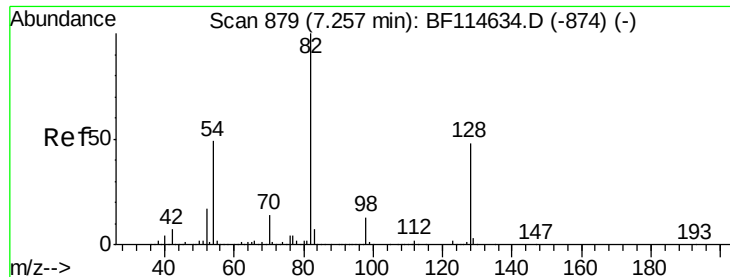




#23
Nitrobenzene-d5
Concen: 106.226 ng
RT: 7.26 min Scan# 879
Delta R.T. -0.00 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Instrument :
BNA_F
ClientSampleId :
FESB-21(4.5-5)

Tgt Ion: 82 Resp: 1656821
Ion Ratio Lower Upper
82 100
128 53.4 38.5 57.7
54 46.4 39.1 58.7

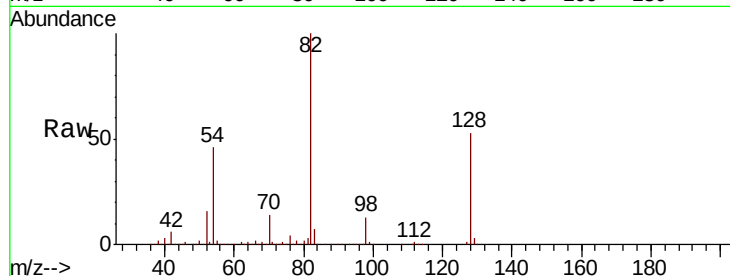


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

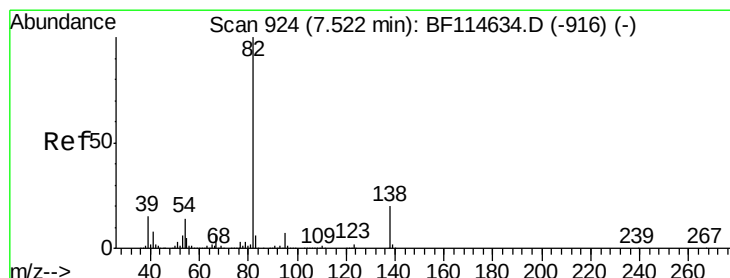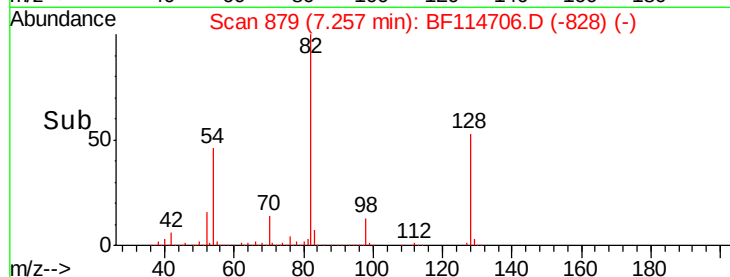
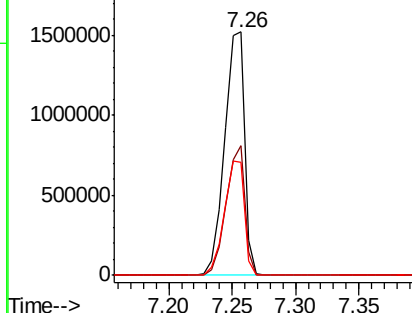



#25
Isophorone
Concen: 51.635 ng
RT: 7.26 min Scan# 879
Delta R.T. -0.26 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Tgt Ion: 82 Resp: 1616251
Ion Ratio Lower Upper
82 100
95 0.0 5.6 8.4#
138 0.0 15.9 23.9#

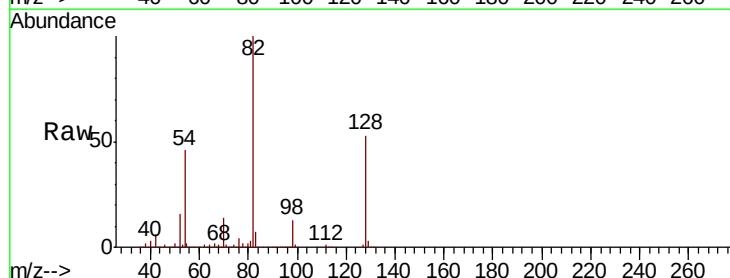

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

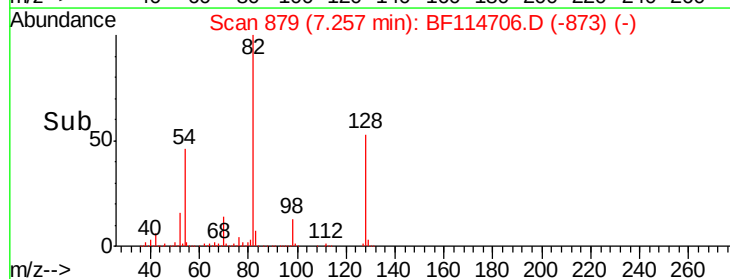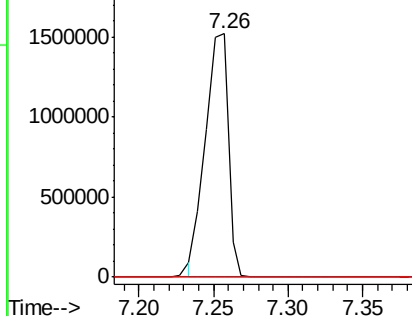







#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.72 min Scan# 1298
Delta R.T. -0.00 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Instrument :
BNA_F
ClientSampleId :
FESB-21(4.5-5)

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.9	81.4	122.2
160	46.6	36.6	54.8




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

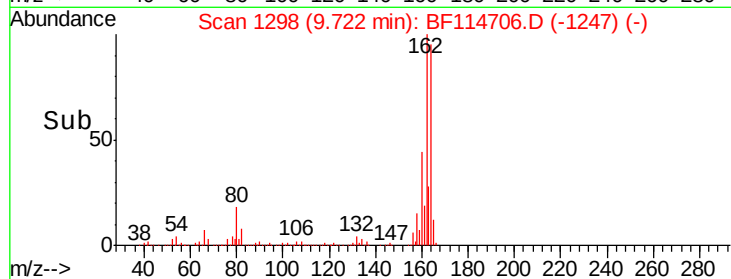
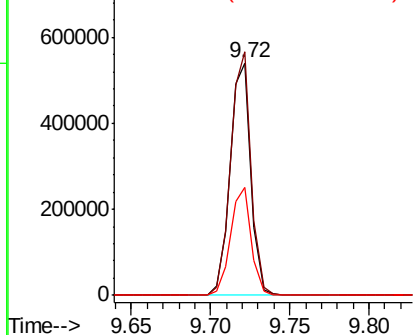



#42
2,4,6-Tribromophenol
Concen: 160.345 ng
RT: 10.50 min Scan# 1431
Delta R.T. -0.00 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.2	75.8	113.8
141	32.2	27.8	41.8



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

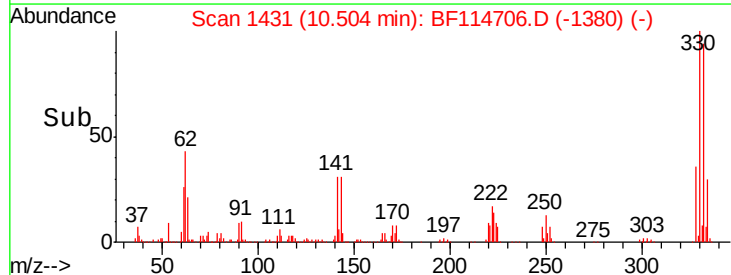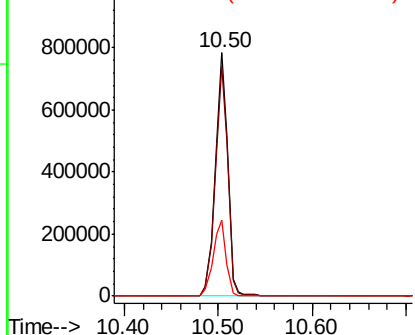







#45
 2-Fluorobiphenyl
 Concen: 123.246 ng
 RT: 9.05 min Scan# 1184
 Delta R.T. 0.00 min
 Lab File: BF114706.D
 Acq: 31 May 2019 14:18

Instrument :
 BNA_F
 ClientSampleId :
 FESB-21(4.5-5)

Tgt Ion:172 Resp: 3005927
 Ion Ratio Lower Upper
 172 100
 171 38.4 30.6 45.8
 170 26.7 20.7 31.1




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


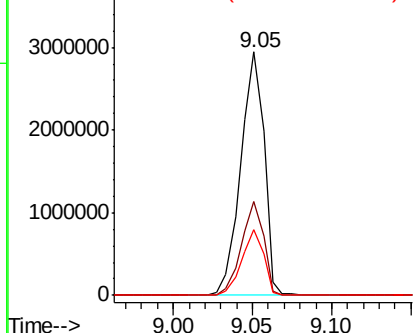



#50
 Dimethylphthalate
 Concen: 14.704 ng
 RT: 9.44 min Scan# 1250
 Delta R.T. -0.02 min
 Lab File: BF114706.D
 Acq: 31 May 2019 14:18

Tgt Ion:163 Resp: 498534
 Ion Ratio Lower Upper
 163 100
 194 3.8 3.4 5.0
 164 10.0 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E




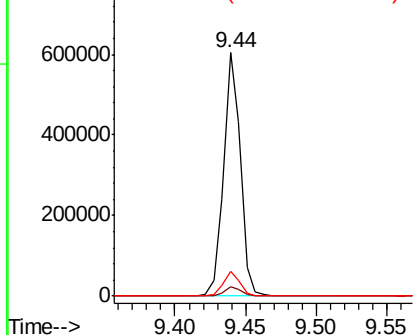




#57
2,4-Dinitrotoluene
Concen: 6.261 ng
RT: 9.72 min Scan# 1298
Delta R.T. -0.18 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18




Instrument :
BNA_F
ClientSampleId :
FESB-21(4.5-5)


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.1	34.8	52.2#
89	1.3	58.5	87.7#
182	0.0	2.2	3.2#

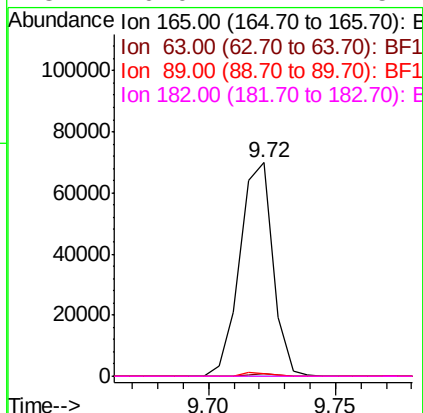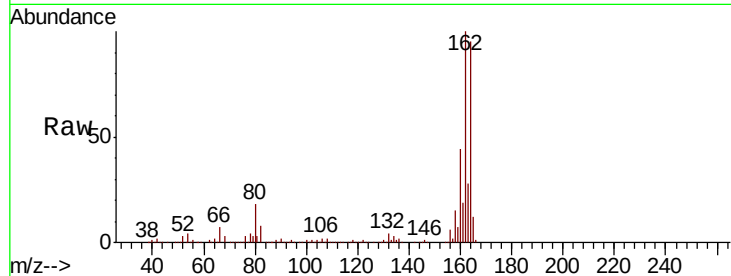

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1548
Delta R.T. -0.00 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.0	8.6	13.0
80	10.2	9.0	13.6

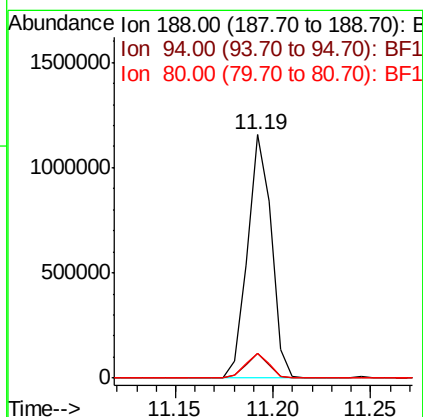


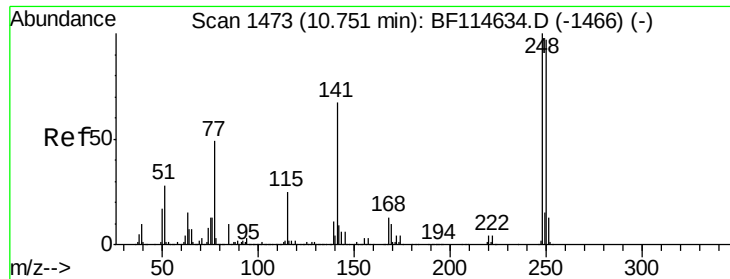




#67
4-Bromophenyl-phenylether
Concen: 4.605 ng
RT: 10.50 min Scan# 1431
Delta R.T. -0.25 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Instrument :
BNA_F
ClientSampleId :
FESB-21(4.5-5)

Tgt Ion:248 Resp: 48297
Ion Ratio Lower Upper
248 100
250 186.7 78.0 117.0#
141 449.0 53.8 80.8#

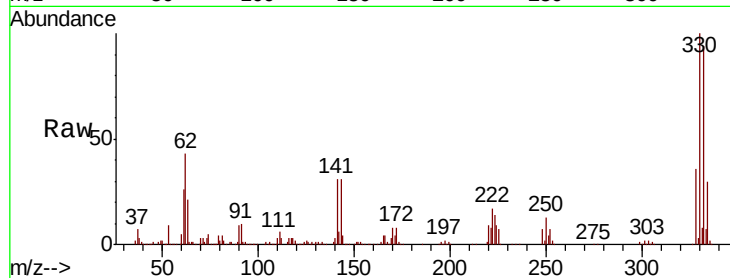


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

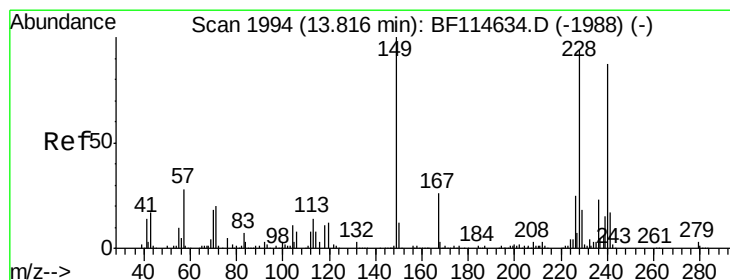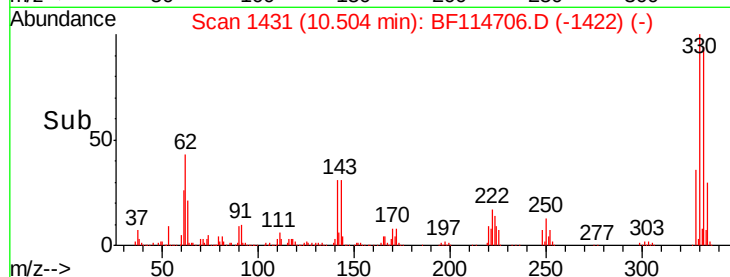
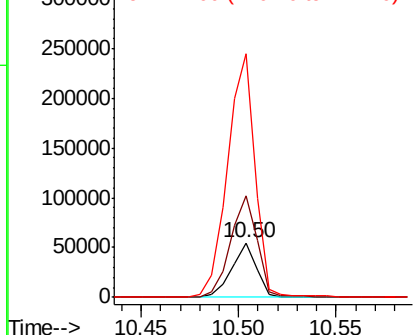



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.82 min Scan# 1994
Delta R.T. -0.00 min
Lab File: BF114706.D
Acq: 31 May 2019 14:18

Tgt Ion:240 Resp: 796568
Ion Ratio Lower Upper
240 100
120 11.3 11.2 16.8
236 27.2 21.2 31.8

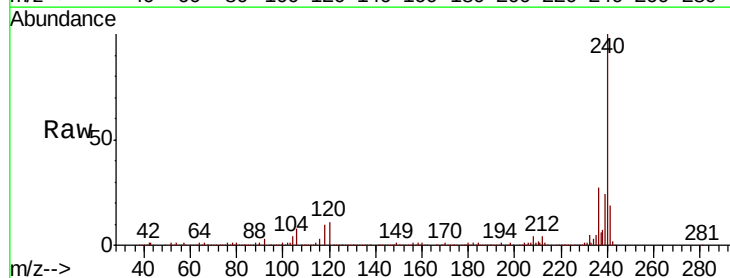

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

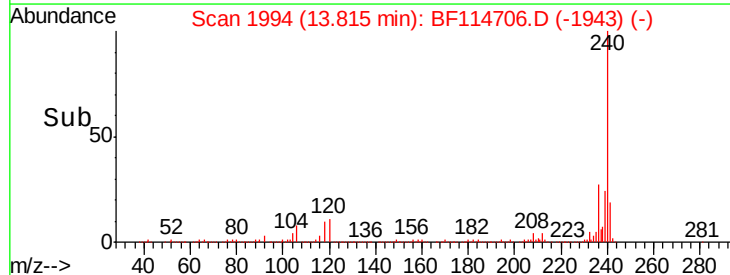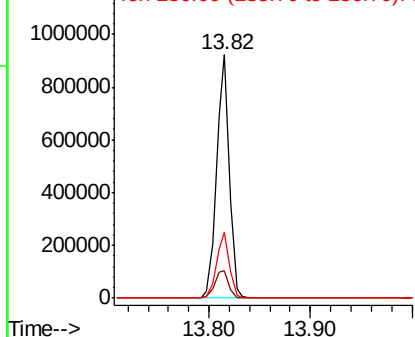



#79

Terphenyl-d14

Concen: 81.675 ng

RT: 12.78 min Scan# 1818

Delta R.T. -0.00 min

Lab File: BF114706.D

Acq: 31 May 2019 14:18

Instrument :

BNA_F

ClientSampleId :

FESB-21(4.5-5)


Tgt Ion:244 Resp: 3460354

Ion Ratio Lower Upper

244 100

212 7.8 6.1 9.1




122 13.0 9.8 14.8

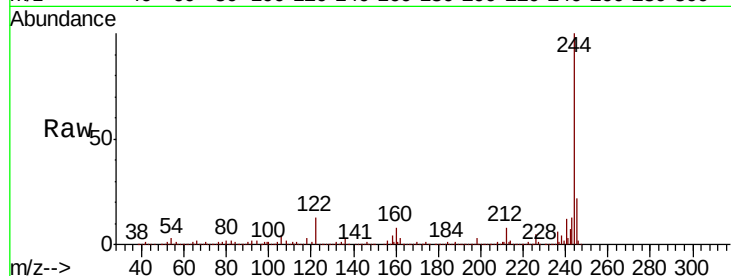

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

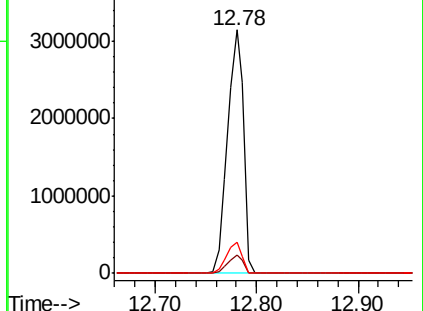

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.21 min Scan# 2231

Delta R.T. -0.00 min

Lab File: BF114706.D

Acq: 31 May 2019 14:18


Tgt Ion:264 Resp: 725693

Ion Ratio Lower Upper

264 100

260 24.4 19.7 29.5

265 21.9 18.1 27.1



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

