

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF053119\
 Data File : BF114736.D
 Acq On : 1 Jun 2019 4:33
 Operator : HP/JU
 Sample : K3090-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-4-D

Quant Time: Jun 01 06:55:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 29 19:08:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	481093	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	1780240	20.00	ng	0.00
39) Acenaphthene-d10	9.72	164	810846	20.00	ng	0.00
64) Phenanthrene-d10	11.19	188	1319986	20.00	ng	0.00
76) Chrysene-d12	13.81	240	879377	20.00	ng	0.00
87) Perylene-d12	15.20	264	805865	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	2775394	101.29	ng	0.04
7) Phenol-d6	6.34	99	2997767	90.79	ng	0.01
23) Nitrobenzene-d5	7.26	82	2353931	82.49	ng	0.00
42) 2,4,6-Tribromophenol	10.50	330	885234	114.58	ng	0.00
45) 2-Fluorobiphenyl	9.05	172	3959158	93.28	ng	0.00
79) Terphenyl-d14	12.78	244	3318210	70.94	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF053119\
Data File : BF114736.D
Acq On : 1 Jun 2019 4:33
Operator : HP/JU
Sample : K3090-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-D

Quant Time: Jun 01 06:55:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 19:08:51 2019
Response via : Initial Calibration

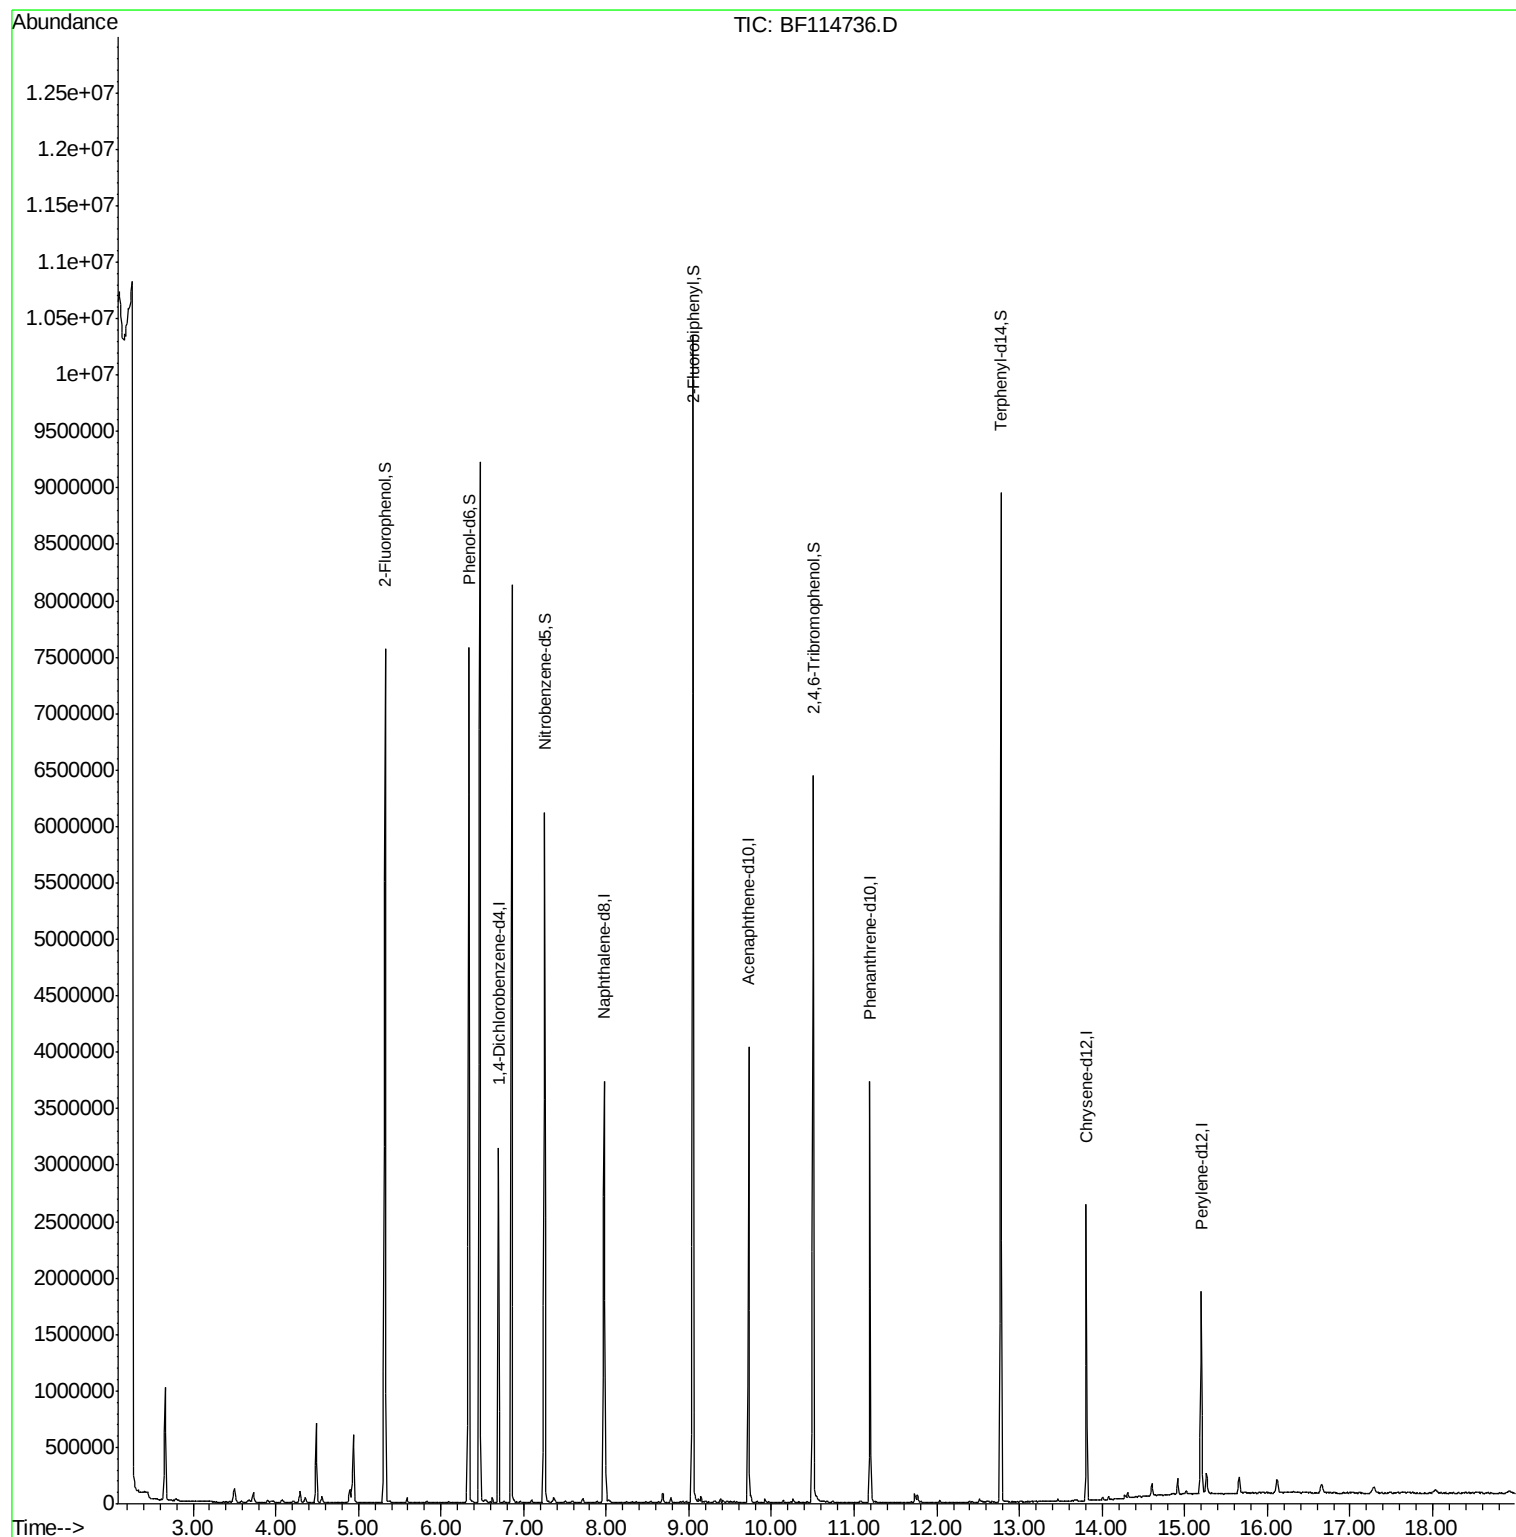

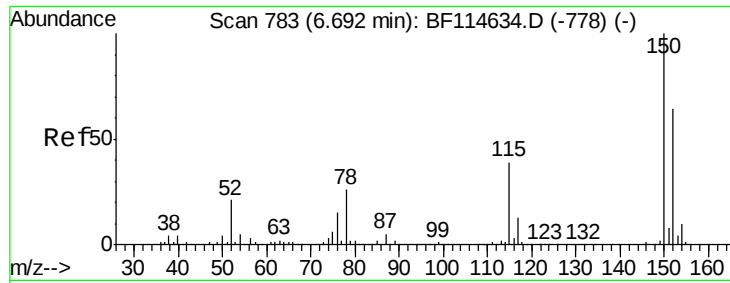


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 784
Delta R.T. 0.01 min
Lab File: BF114736.D
Acq: 1 Jun 2019 4:33

Instrument :
BNA_F
ClientSampleId :
TP-4-D

Tot Ion:152 Resp: 481093
Ion Ratio Lower Upper
152 100
150 151.9 124.4 186.6
115 57.9 48.7 73.1

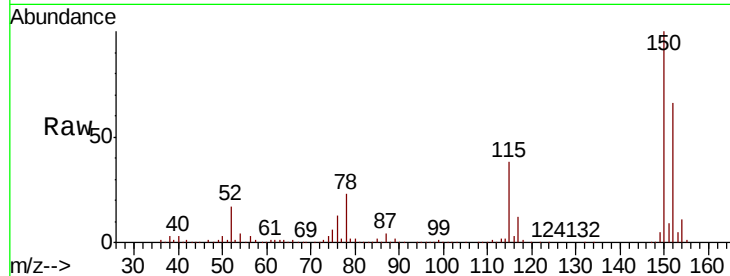


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

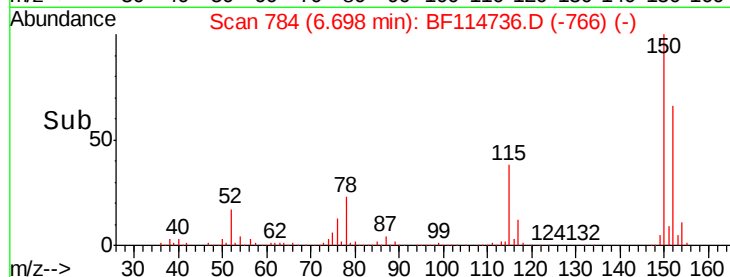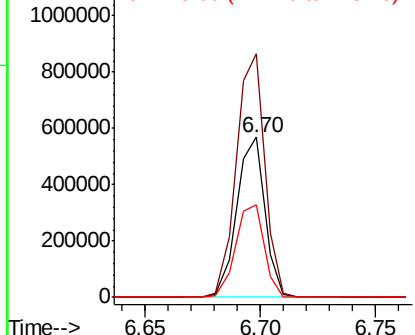



#5


2-Fluorophenol
Concen: 101.286 ng
RT: 5.33 min Scan# 551
Delta R.T. 0.04 min
Lab File: BF114736.D
Acq: 1 Jun 2019 4:33

Tgt Ion:112 Resp: 2775394
Ion Ratio Lower Upper
112 100
64 53.3 46.1 69.1
63 27.8 23.4 35.2



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

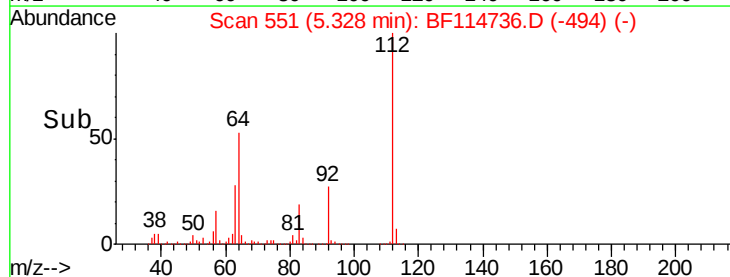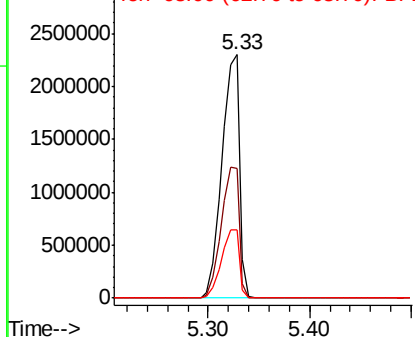

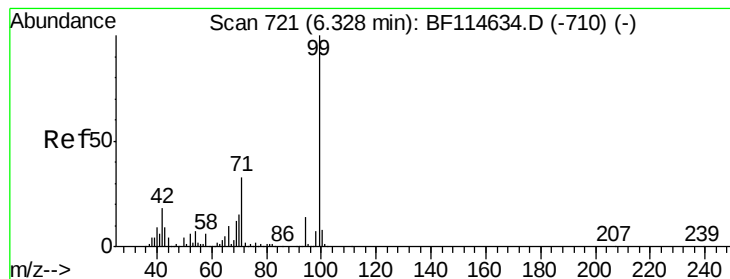

#7

Phenol-d6

Concen: 90.787 ng

RT: 6.34 min Scan# 723

Delta R.T. 0.01 min

Lab File: BF114736.D

Acq: 1 Jun 2019 4:33

Instrument :

BNA_F

ClientSampleId :

TP-4-D


Tot Ion: 99 Resp: 2997767

Ion Ratio Lower Upper




99 100

42 18.1 14.7 22.1

71 35.9 26.6 40.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

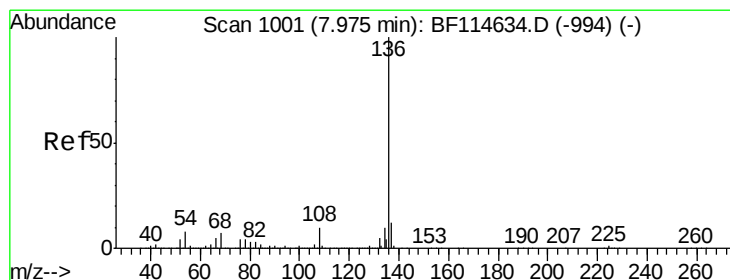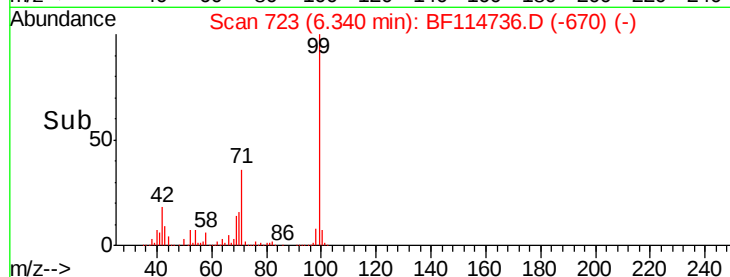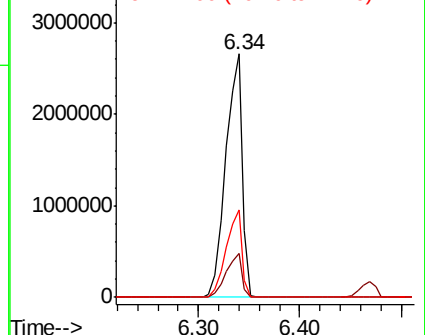

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1001

Delta R.T. 0.00 min

Lab File: BF114736.D

Acq: 1 Jun 2019 4:33

Tgt Ion: 136 Resp: 1780240


Ion Ratio Lower Upper

136 100



137 11.5 9.3 13.9


54 7.0 6.3 9.5

68 5.6 5.4 8.0



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

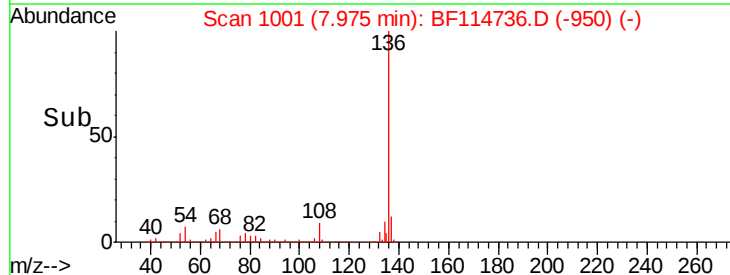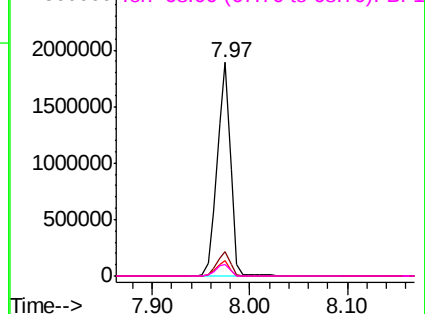


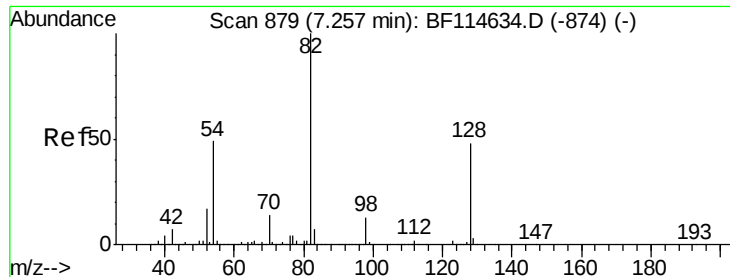




#23
Nitrobenzene-d5
Concen: 82.494 ng
RT: 7.26 min Scan# 879
Delta R.T. 0.00 min
Lab File: BF114736.D
Acq: 1 Jun 2019 4:33

Instrument :
BNA_F
ClientSampleID :
TP-4-D

Tot Ion: 82 Resp: 2353931
Ion Ratio Lower Upper
82 100
128 51.5 38.5 57.7
54 48.0 39.1 58.7

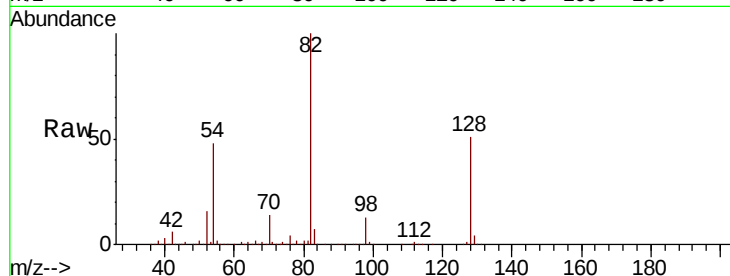


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

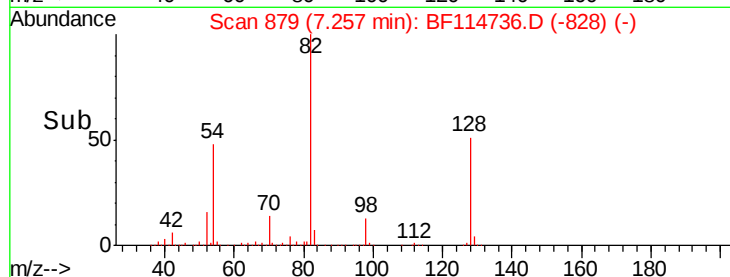
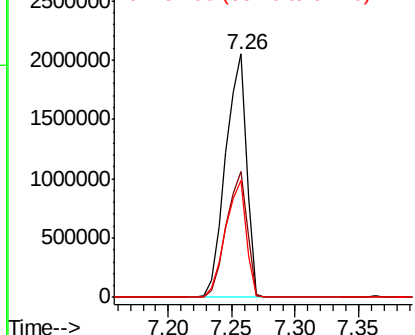



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.72 min Scan# 1298
Delta R.T. 0.00 min
Lab File: BF114736.D
Acq: 1 Jun 2019 4:33

Tgt Ion:164 Resp: 810846
Ion Ratio Lower Upper
164 100
162 102.8 81.4 122.2
160 46.7 36.6 54.8



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

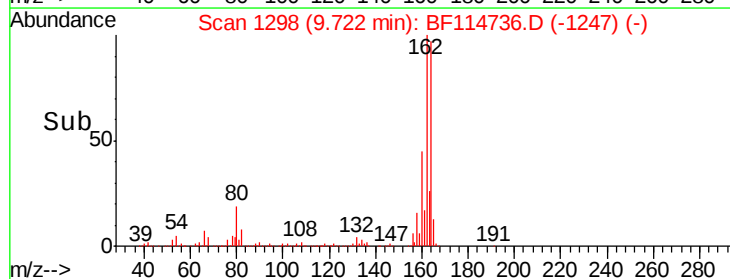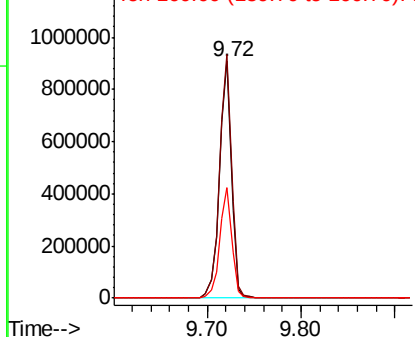


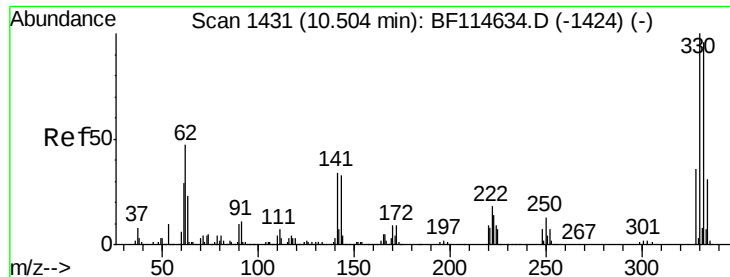




#42
 2,4,6-Tribromophenol
 Concen: 114.577 ng
 RT: 10.50 min Scan# 1431
 Delta R.T. 0.00 min
 Lab File: BF114736.D
 Acq: 1 Jun 2019 4:33

Instrument :
 BNA_F
 ClientSampleId :
 TP-4-D

Tot Ion:330 Resp: 885234
 Ion Ratio Lower Upper
 330 100
 332 96.5 75.8 113.8
 141 32.0 27.8 41.8

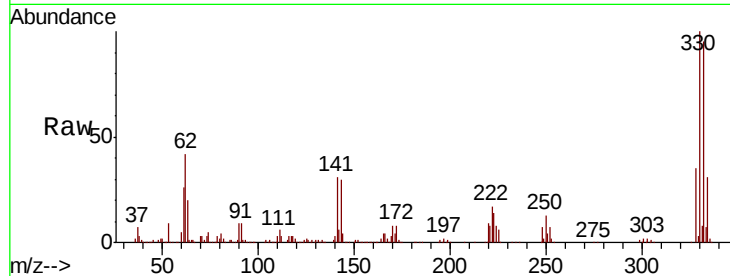


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

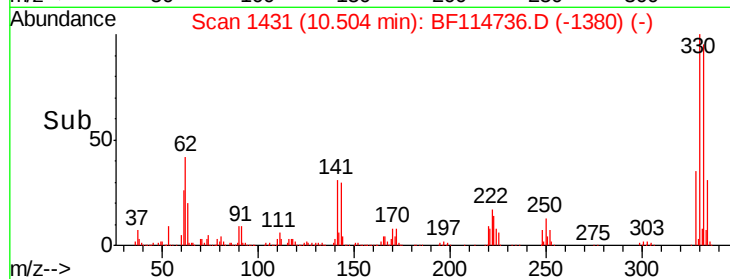
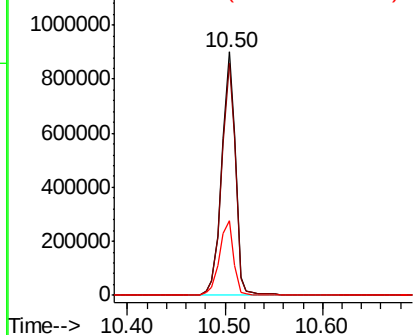



#45
 2-Fluorobiphenyl
 Concen: 93.281 ng
 RT: 9.05 min Scan# 1184
 Delta R.T. 0.00 min
 Lab File: BF114736.D
 Acq: 1 Jun 2019 4:33

Tgt Ion:172 Resp: 3959158
 Ion Ratio Lower Upper
 172 100
 171 39.9 30.6 45.8
 170 26.8 20.7 31.1



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

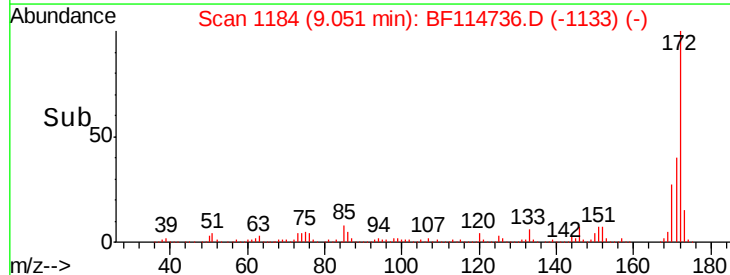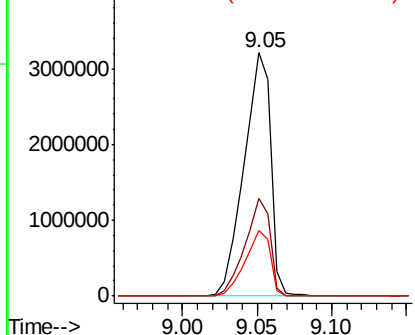

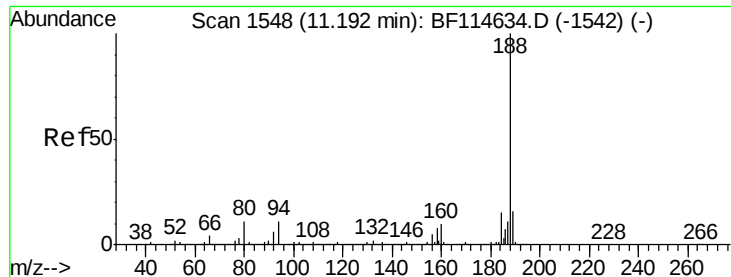

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.19 min Scan# 1548

Delta R.T. 0.00 min

Lab File: BF114736.D

Acq: 1 Jun 2019 4:33

Instrument :

BNA_F

ClientSampleId :

TP-4-D



Tot Ion:188 Resp: 1319986

Ion Ratio Lower Upper

188 100

94 9.9 8.6 13.0



80 10.5 9.0 13.6

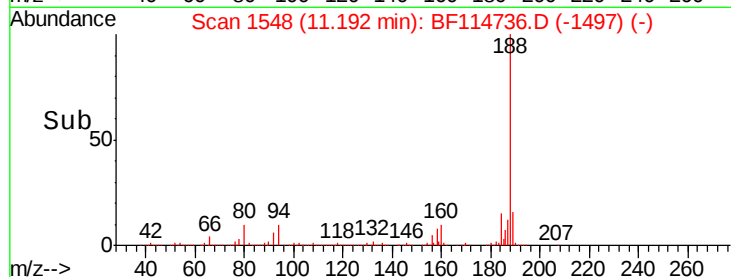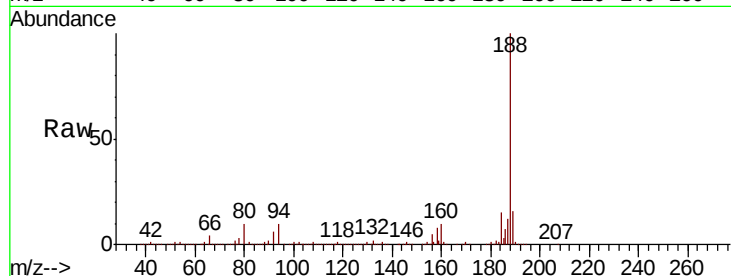

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

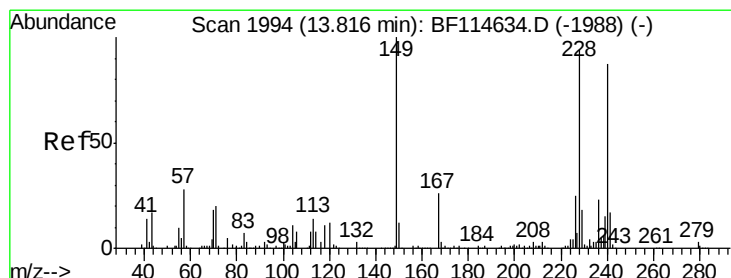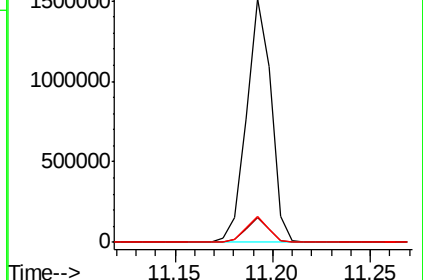

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.81 min Scan# 1993

Delta R.T. -0.01 min

Lab File: BF114736.D

Acq: 1 Jun 2019 4:33



Tgt Ion:240 Resp: 879377

Ion Ratio Lower Upper

240 100

120 13.0 11.2 16.8


236 27.1 21.2 31.8

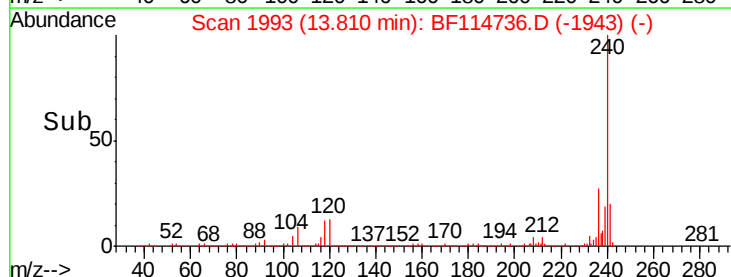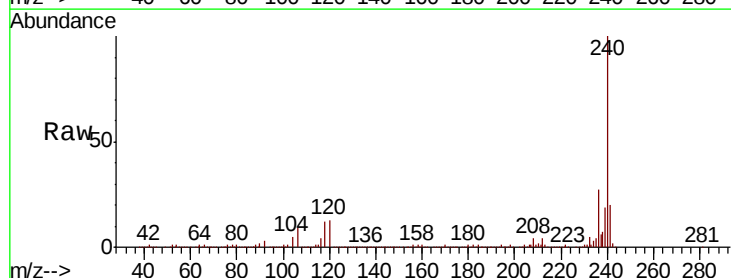


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

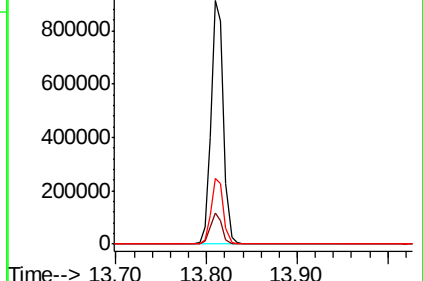

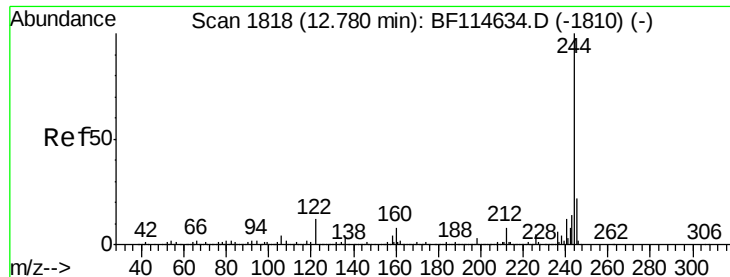

#79

Terphenyl-d14

Concen: 70.945 ng

RT: 12.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BF114736.D

Acq: 1 Jun 2019 4:33

Instrument :

BNA_F

ClientSampleId :

TP-4-D


Tot Ion:244 Resp: 3318210

Ion Ratio Lower Upper

244 100

212 7.4 6.1 9.1




122 12.1 9.8 14.8

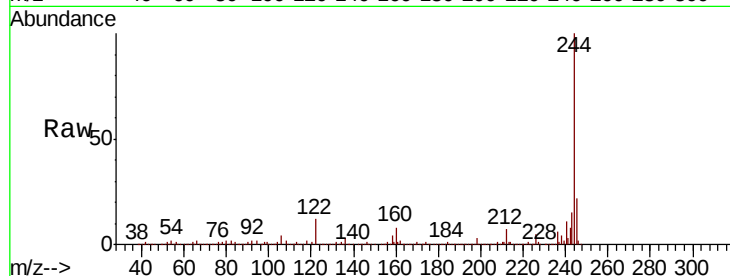

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

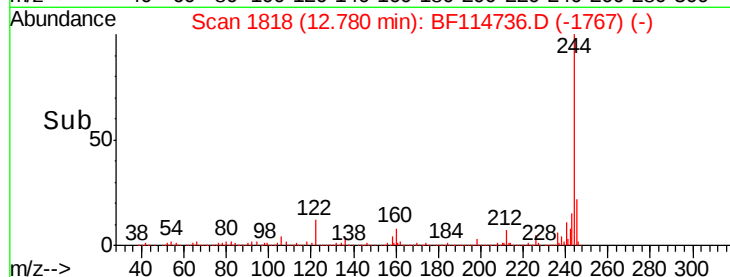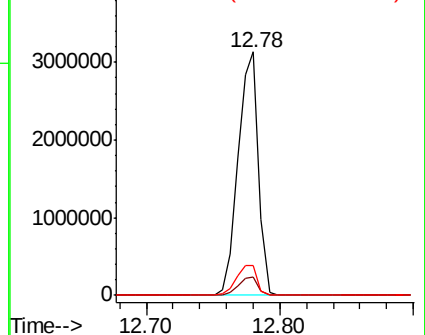

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.20 min Scan# 2229

Delta R.T. -0.01 min

Lab File: BF114736.D

Acq: 1 Jun 2019 4:33


Tgt Ion:264 Resp: 805865

Ion Ratio Lower Upper

264 100

260 24.6 19.7 29.5

265 21.8 18.1 27.1



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

