

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053119\
 Data File : BF114722.D
 Acq On : 31 May 2019 22:21
 Operator : HP/JU
 Sample : K3037-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-20190523

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.657	262	267	277	rVB2	59835	120006	1.05%	0.155%
2	5.304	542	547	550	rBV	4775913	4641889	40.45%	6.014%
3	6.322	716	720	723	rBV	3612751	2992203	26.07%	3.877%
4	6.463	739	744	747	rBV	8161768	8389498	73.10%	10.870%
5	6.692	779	783	787	rBV	2854781	2399290	20.91%	3.109%
6	6.851	806	810	813	rBV	7952101	7805948	68.02%	10.114%
7	7.257	873	879	882	rBV	6172113	6572050	57.27%	8.515%
8	7.975	996	1001	1004	rBV	3486845	3031580	26.42%	3.928%
9	9.051	1178	1184	1187	rBV	10382681	11476136	100.00%	14.869%
10	9.722	1291	1298	1306	rBV	3862444	3602502	31.39%	4.668%
11	10.504	1425	1431	1434	rBV	6970769	7051877	61.45%	9.137%
12	11.192	1544	1548	1552	rVB	4157518	3502227	30.52%	4.538%
13	12.780	1812	1818	1821	rBV	9989338	10553587	91.96%	13.674%
14	13.810	1989	1993	1997	rBV	2945680	2770863	24.14%	3.590%
15	15.198	2224	2229	2237	rBV	1911123	2272966	19.81%	2.945%


Sum of corrected areas: 77182622

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF053119\
Data File : BF114722.D
Acq On : 31 May 2019 22:21
Operator : HP/JU
Sample : K3037-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-20190523

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

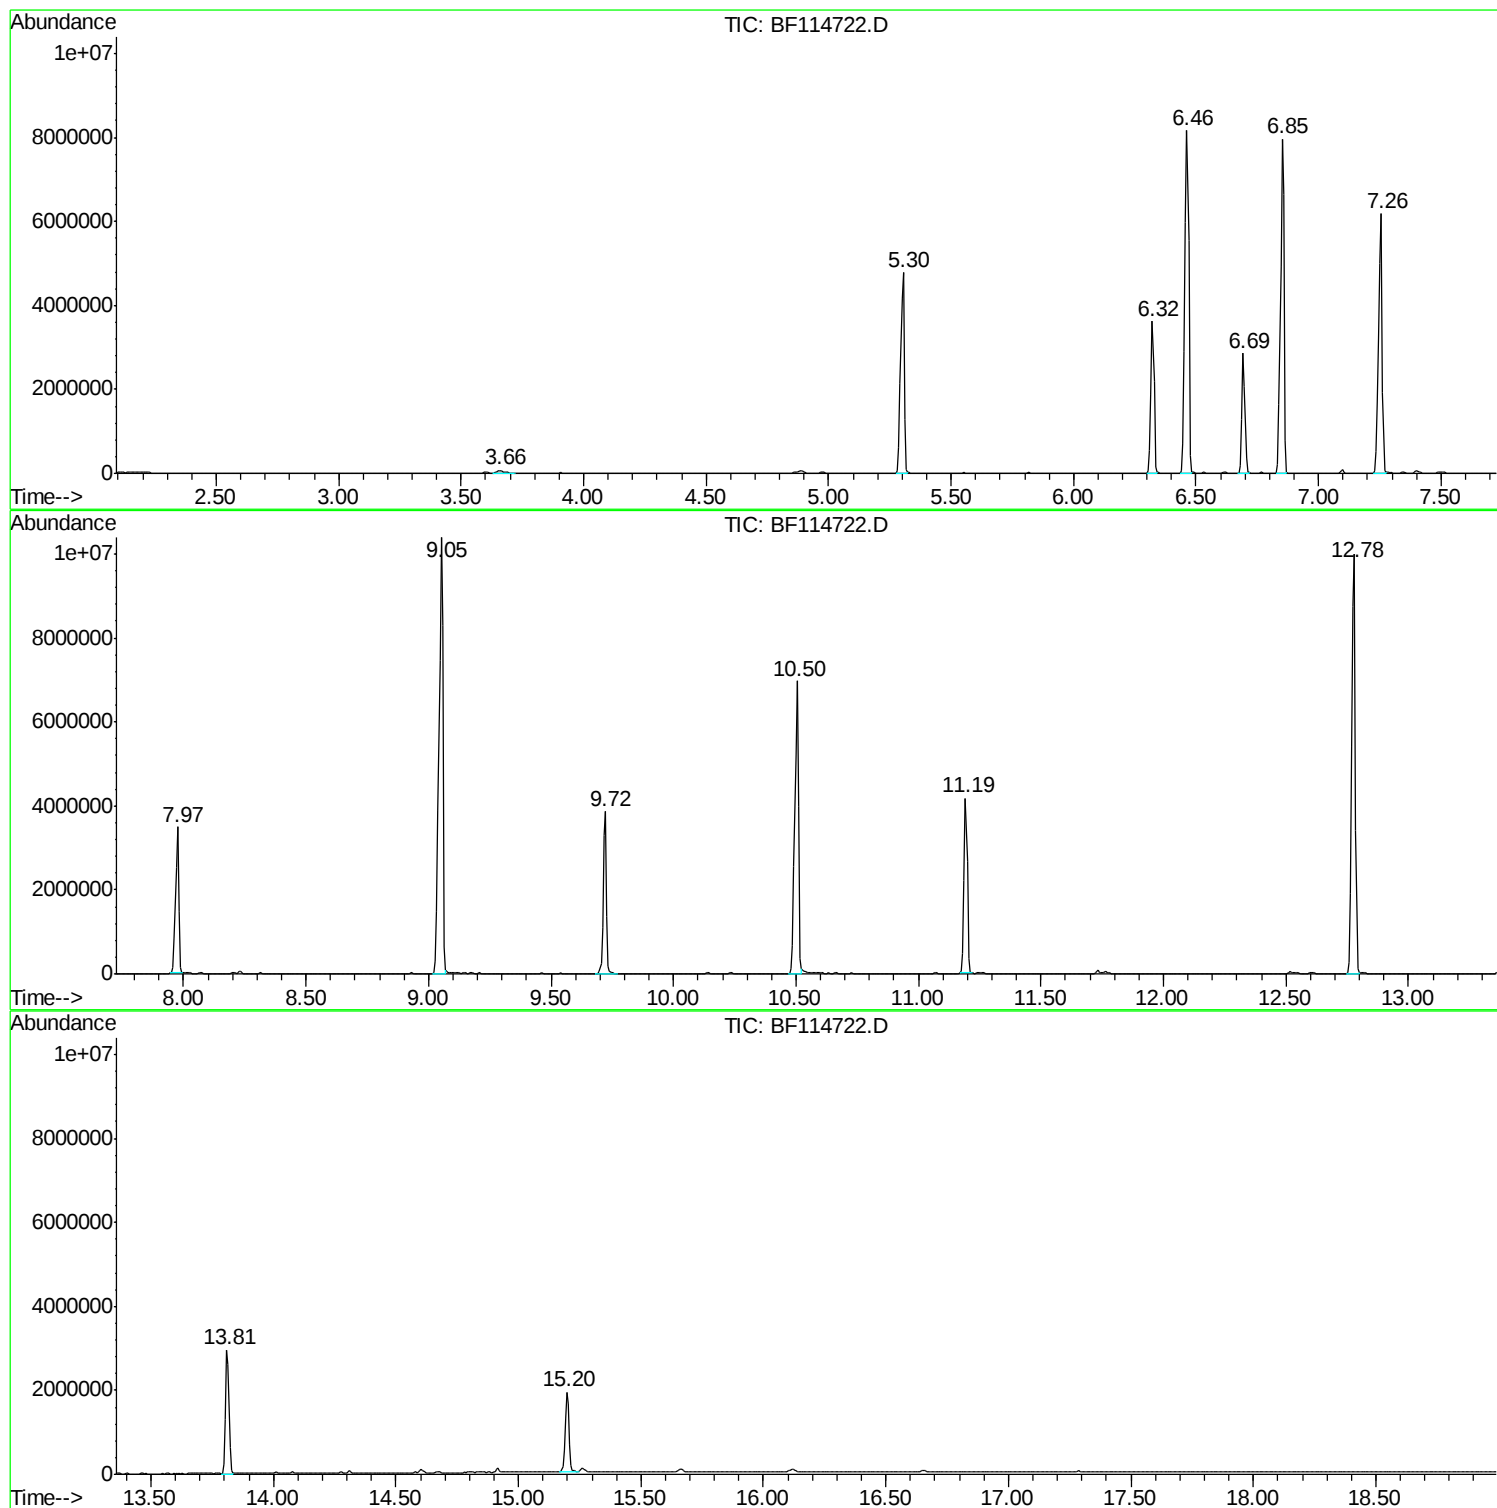

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF053119\
Data File : BF114722.D
Acq On : 31 May 2019 22:21
Operator : HP/JU
Sample : K3037-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-20190523









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	69.93 ng	8389500	1,4-Dichlorobenzene-d4	6.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

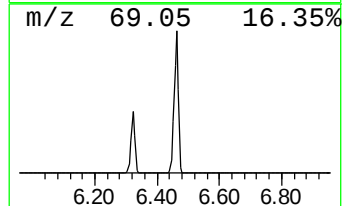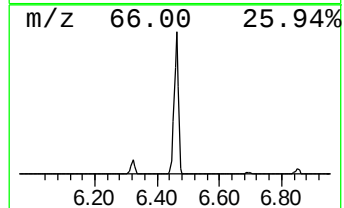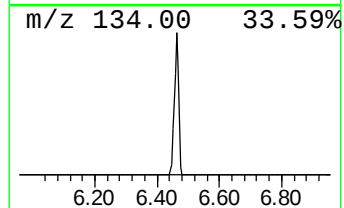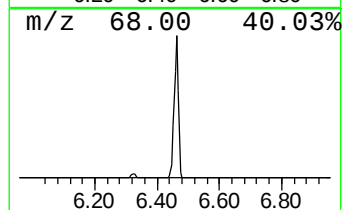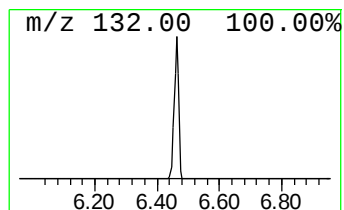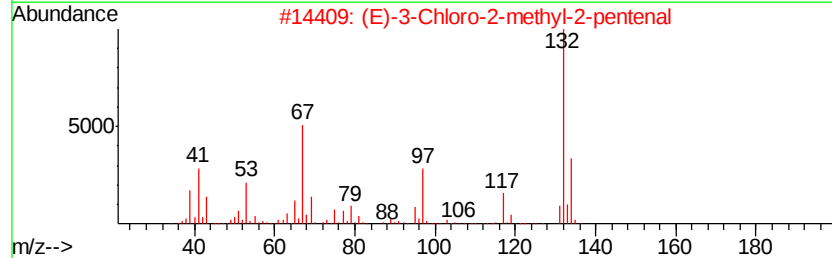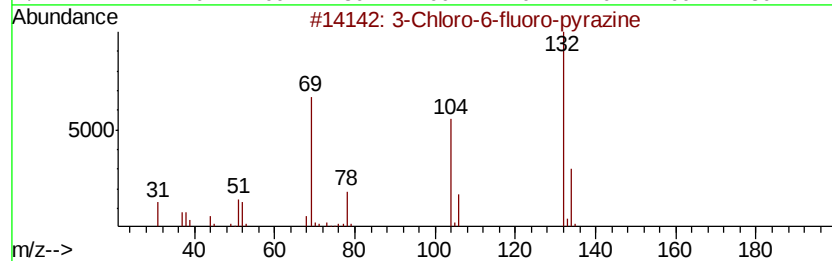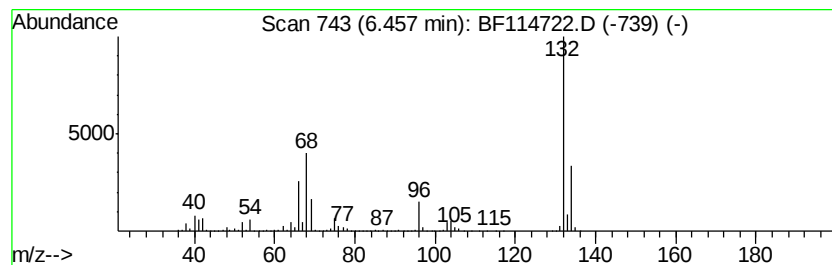

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053119\
Data File : BF114722.D
Acq On : 31 May 2019 22:21
Operator : HP/JU
Sample : K3037-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-20190523

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.46	6.46	69.9	ng	8389500	1	6.69	2399290	20.0