


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF053119\
 Data File : BF114716.D
 Acq On : 31 May 2019 19:41
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 19:08:51 2019

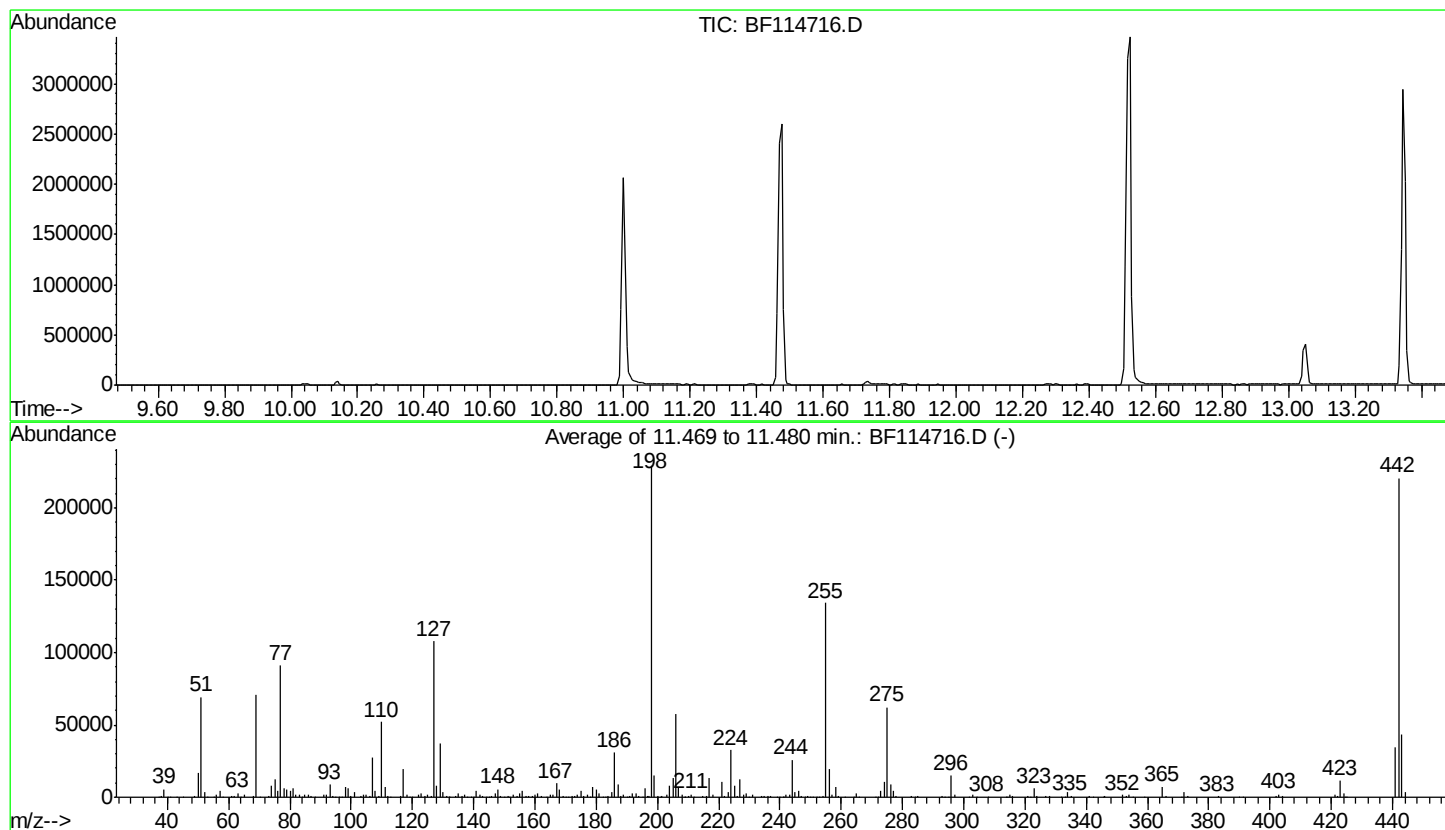

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	69185	PASS
68	69	0.00	2	1.7	1219	PASS
69	198	0.00	100	31.1	71193	PASS
70	69	0.00	2	0.6	444	PASS
127	198	10	80	46.9	107536	PASS
197	198	0.00	2	0.3	774	PASS
198	198	100	100	100.0	229202	PASS
199	198	5	9	6.5	14953	PASS
275	198	10	60	27.1	62064	PASS
365	198	1	100	3.2	7417	PASS
441	198	0.01	100	15.0	34298	PASS
442	198	50	100	96.2	220565	PASS
443	442	15	24	19.5	43018	PASS