

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060119\
 Data File : BF114762.D
 Acq On : 1 Jun 2019 17:32
 Operator : HP/JU
 Sample : K2639-05 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NB-07-053019-A

Manual Integrations
 APPROVED

mohammad
 6/3/2019 8:51:35 AM

Quant Time: Jun 03 04:16:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 29 19:08:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	343310	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	1249336	20.00	ng	0.00
39) Acenaphthene-d10	9.72	164	554666	20.00	ng	0.00
64) Phenanthrene-d10	11.19	188	976456	20.00	ng	0.00
76) Chrysene-d12	13.82	240	817552	20.00	ng	0.00
87) Perylene-d12	15.21	264	762993	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.29	112	385210	19.70	ng	0.00
7) Phenol-d6	6.32	99	477761	20.28	ng	0.00
23) Nitrobenzene-d5	7.25	82	258446	12.91	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	92249	17.45	ng	0.00
45) 2-Fluorobiphenyl	9.05	172	497942	1.06	ng	0.00
79) Terphenyl-d14	12.77	244	462244	10.63	ng	0.00

Target Compounds

						Qvalue
31) Naphthalene	8.00	128	685318	11.909	ng	96
37) 2-Methylnaphthalene	8.69	142	169420	4.431	ng	98
38) 1-Methylnaphthalene	8.78	142	102234	2.822	ng	96
52) Acenaphthene	9.75	154	108310	3.385	ng	99
55) Dibenzofuran	9.92	168	286053	6.280	ng	96
58) Fluorene	10.26	166	325704	5.983	ng	99
71) Phenanthrene	11.22	178	1549399	31.106	ng	97
72) Anthracene	11.27	178	506215	10.041	ng	97
73) Carbazole	11.42	167	203903	4.602	ng	# 95
75) Fluoranthene	12.40	202	1562624	30.297	ng	99
78) Pyrene	12.63	202	1374573	19.876	ng	97
81) Benzo(a)anthracene	13.81	228	856514	13.633	ng	100
83) Chrysene	13.84	228	740896	12.343	ng	95
86) Indeno(1,2,3-cd)pyrene	16.53	276	307850	5.121	ng	94
88) Benzo(b)fluoranthene	14.82	252	886050m	18.438	ng	
89) Benzo(k)fluoranthene	14.84	252	341454m	8.175	ng	
90) Benzo(a)pyrene	15.15	252	633465	15.005	ng	98
91) Dibenzo(a,h)anthracene	16.54	278	85050	2.280	ng	# 87
92) Benzo(a,h,i)perylene	16.93	276	275204	7.601	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060119\
Data File : BF114762.D
Acq On : 1 Jun 2019 17:32
Operator : HP/JU
Sample : K2639-05 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM

Quant Time: Jun 03 04:16:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 19:08:51 2019
Response via : Initial Calibration

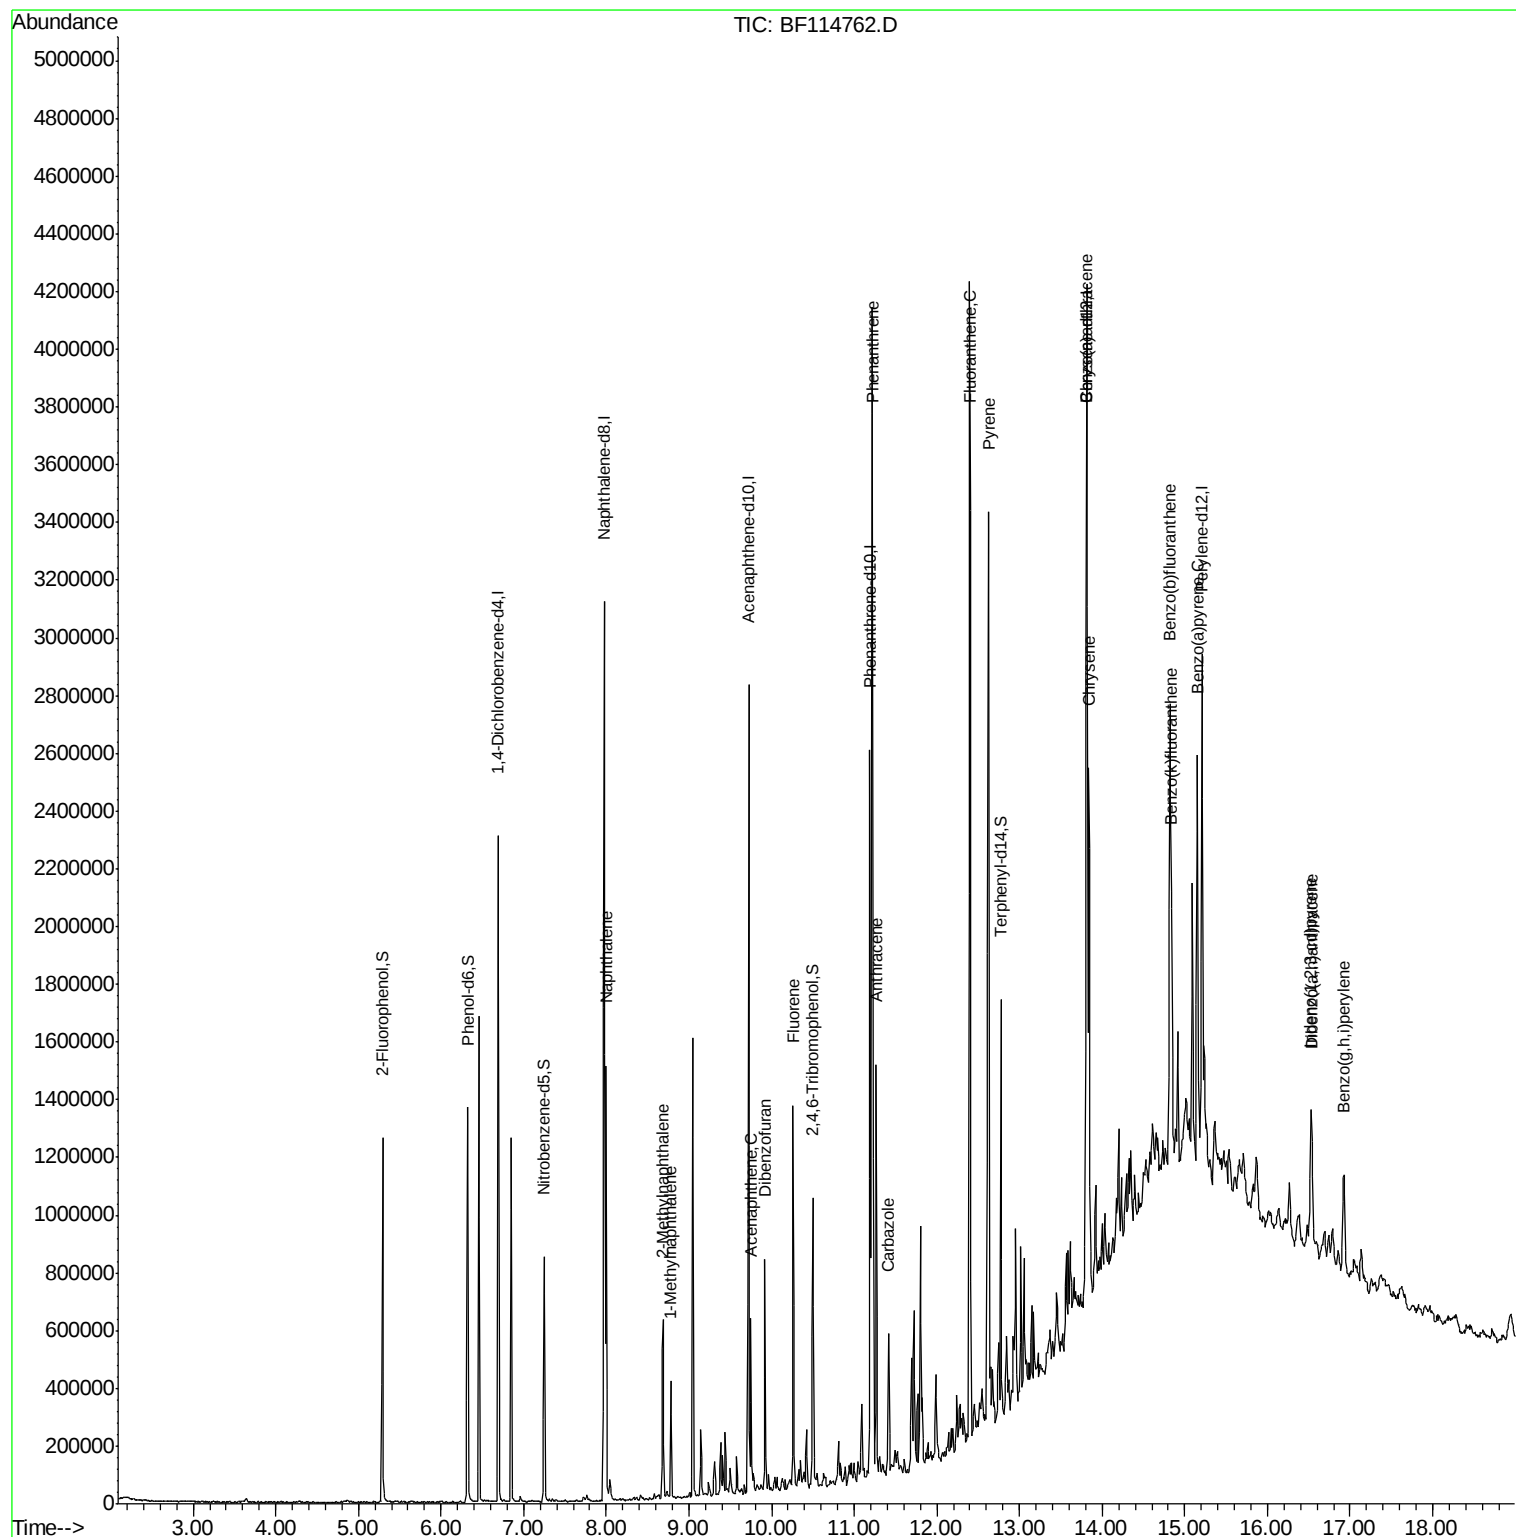



#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.69 min Scan# 783
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.5	124.4	186.6
115	60.9	48.7	73.1

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM



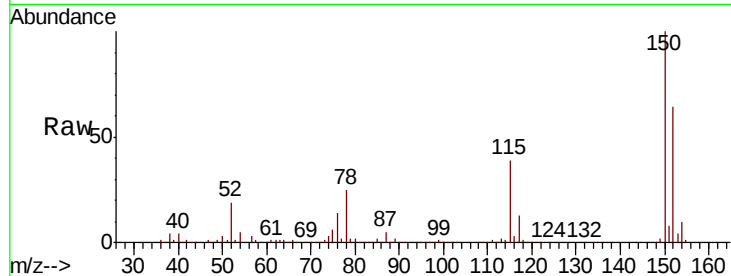


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

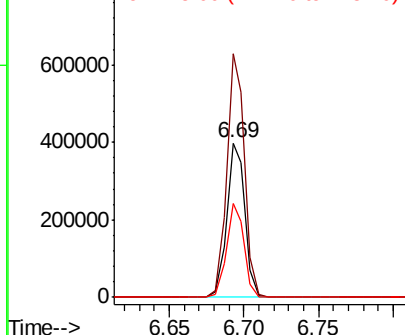

#5

2-Fluorophenol
Concen: 19.700 ng
RT: 5.29 min Scan# 545
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32




Tgt Ion	Ratio	Lower	Upper
112	100		
64	53.0	46.1	69.1
63	25.7	23.4	35.2


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

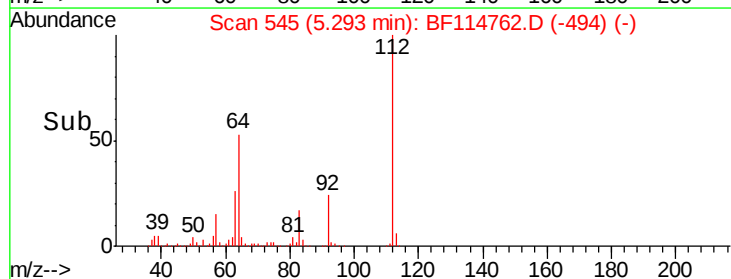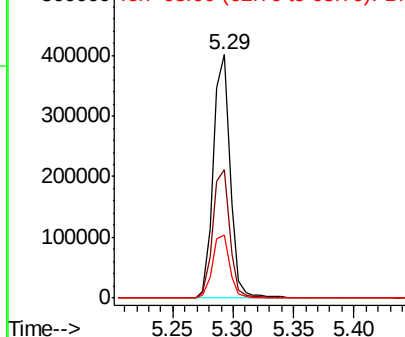



#7

Phenol-d6

Concen: 20.276 ng

RT: 6.32 min Scan# 720

Delta R.T. -0.01 min

Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Instrument :

BNA_F


ClientSampleId :

NB-07-053019-A




Tot Ion	Ion	Ratio	Resp	Lower	Upper
99	100		477761		
42	14.5	14.7	22.1#		
71	29.3	26.6	40.0		

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

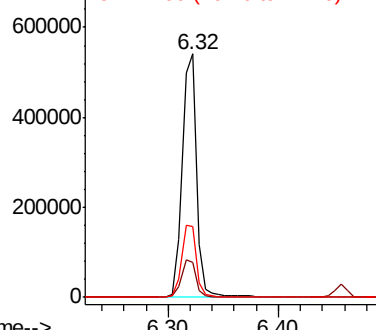

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1001




Delta R.T. 0.00 min


Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
136	100		1249336		
137	11.4	9.3	13.9		
54	7.0	6.3	9.5		
68	5.8	5.4	8.0		

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

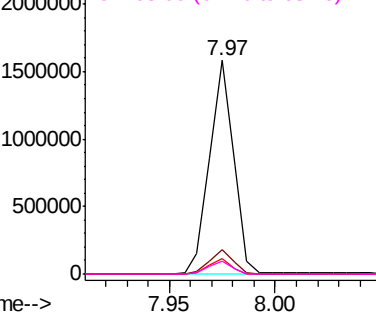

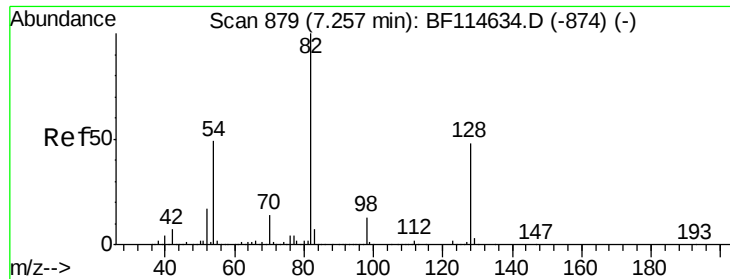





#23
Nitrobenzene-d5
Concen: 12.906 ng
RT: 7.25 min Scan# 877
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
82	100		
128	46.1	38.5	57.7
54	46.8	39.1	58.7




Manual Integrations
APPROVED


mohammad
6/3/2019 8:51:35 AM

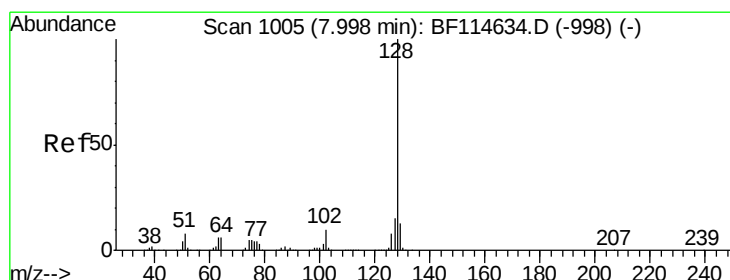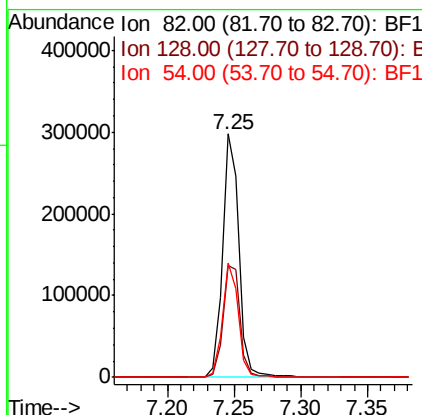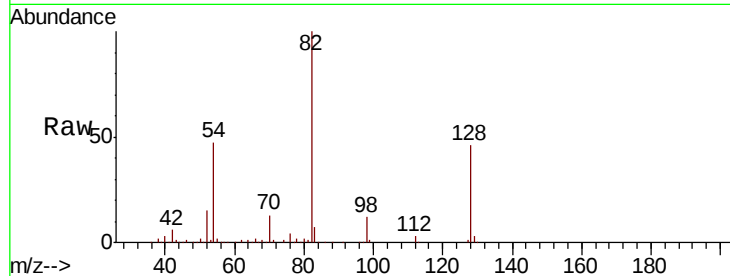

#31
Naphthalene
Concen: 11.909 ng
RT: 8.00 min Scan# 1005
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.0	10.2	15.2
127	13.2	11.9	17.9

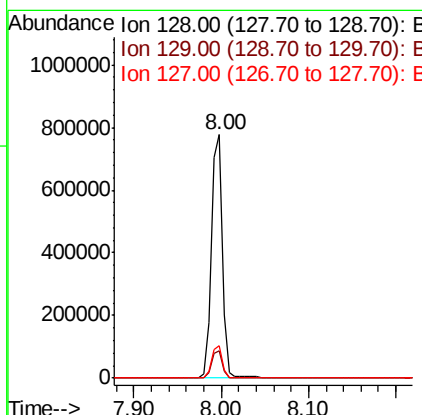




#37
2-Methylnaphthalene
Concen: 4.431 ng
RT: 8.69 min Scan# 1122
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
142	100		
141	88.5	70.3	105.5
115	31.0	28.0	42.0

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM






Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

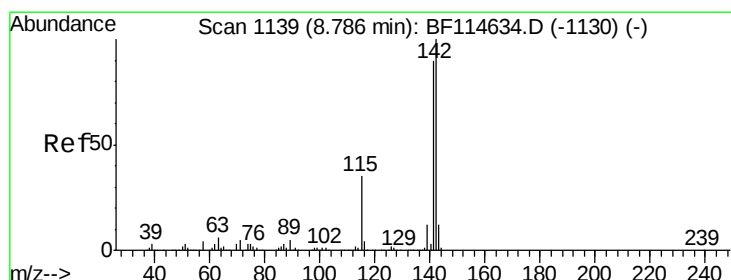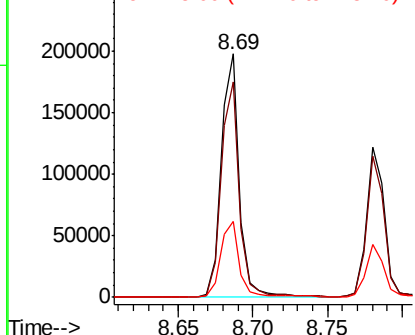

#38
1-Methylnaphthalene
Concen: 2.822 ng
RT: 8.78 min Scan# 1138
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32




Tgt Ion	Ratio	Lower	Upper
142	100		
141	94.1	72.3	108.5
116	4.0	3.0	4.4


Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

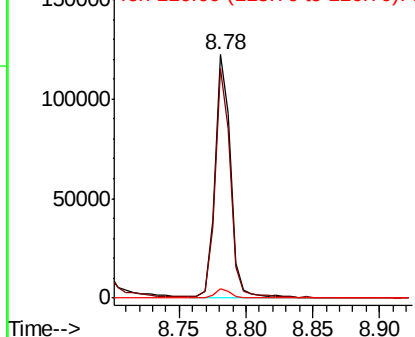

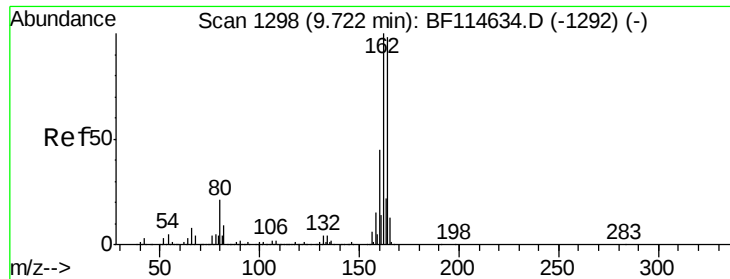





#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.72 min Scan# 1298
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Resp	Lower	Upper
164	100			
162	101.5	81.4	122.2	
160	45.6	36.6	54.8	




Manual Integrations
APPROVED


mohammad
6/3/2019 8:51:35 AM

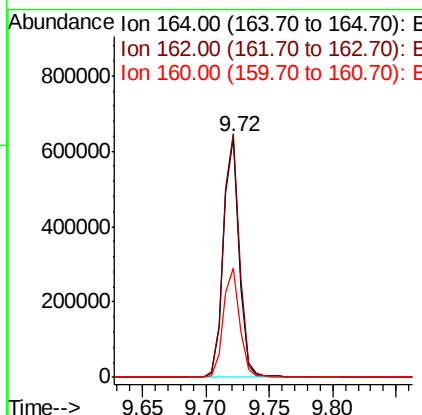

#42
2,4,6-Tribromophenol
Concen: 17.455 ng
RT: 10.50 min Scan# 1430
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Resp	Lower	Upper
330	100			
332	96.1	75.8	113.8	
141	35.0	27.8	41.8	

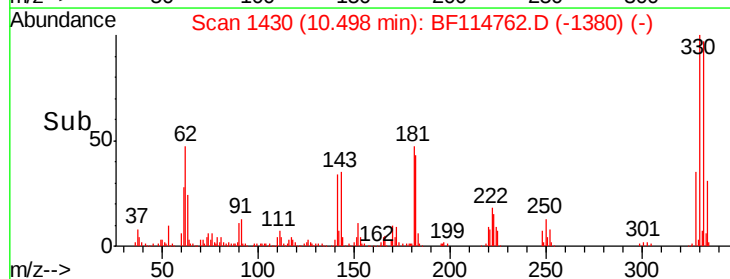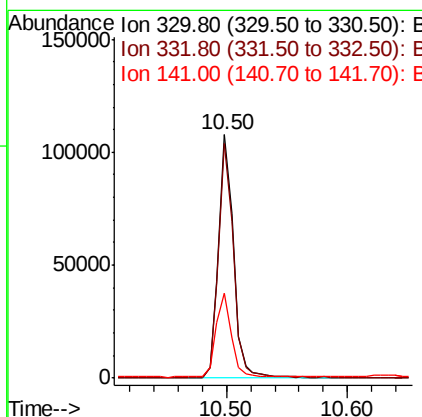




#45
2-Fluorobiphenyl
Concen: 1.062 ng
RT: 9.05 min Scan# 1183
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
172	100		
171	35.2	30.6	45.8
170	23.2	20.7	31.1

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM



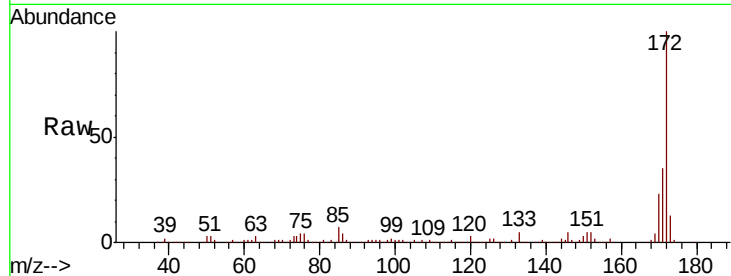


Abundance

Ion 172.00 (171.70 to 172.70): E


Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

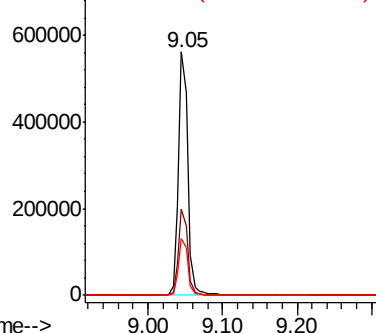

#52
Acenaphthene
Concen: 3.385 ng
RT: 9.75 min Scan# 1303
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Lower	Upper
154	100		
153	111.9	88.4	132.6
152	53.6	43.4	65.0






Abundance

Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

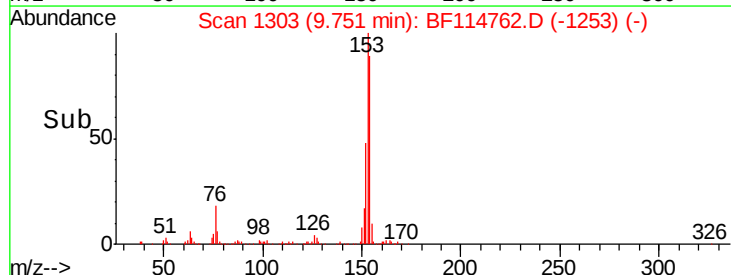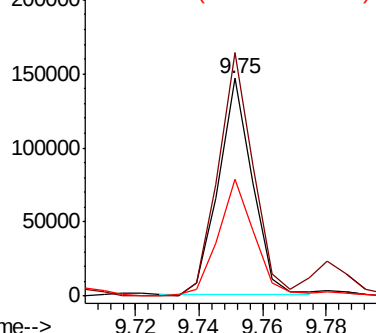







#55
Dibenzenofuran
Concen: 6.280 ng
RT: 9.92 min Scan# 1332
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Resp	Lower	Upper
168	100	286053		
139	37.4		32.6	48.8
169	14.2		11.8	17.8




Manual Integrations
APPROVED


mohammad
6/3/2019 8:51:35 AM

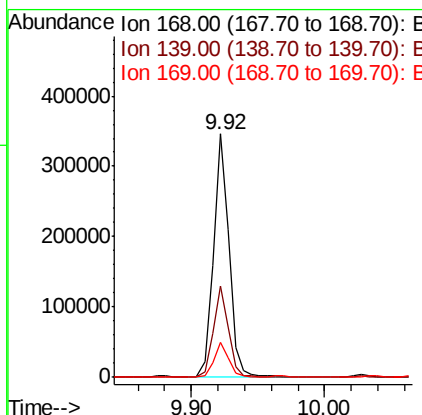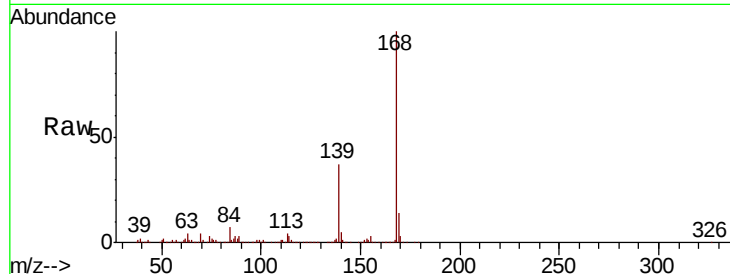

#58
Fluorene
Concen: 5.983 ng
RT: 10.26 min Scan# 1390
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Resp	Lower	Upper
166	100	325704		
165	98.4		77.6	116.4
167	13.5		11.2	16.8

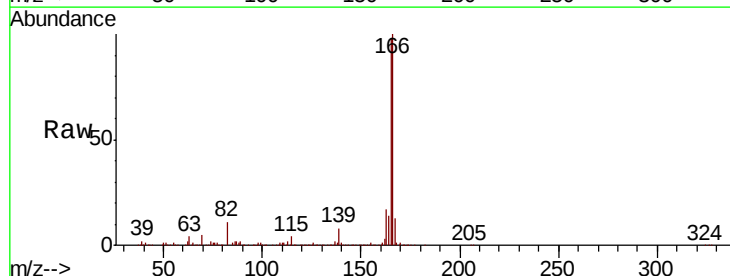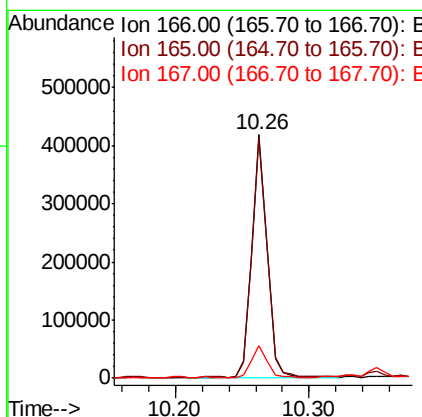

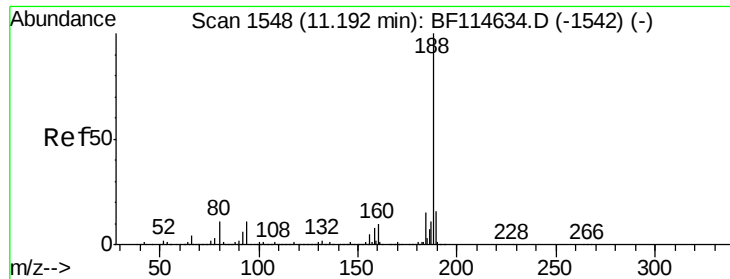


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1548
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A




Tot Ion	Ratio	Resp	Lower	Upper
188	100	976456		
94	10.3		8.6	13.0
80	11.0		9.0	13.6

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM

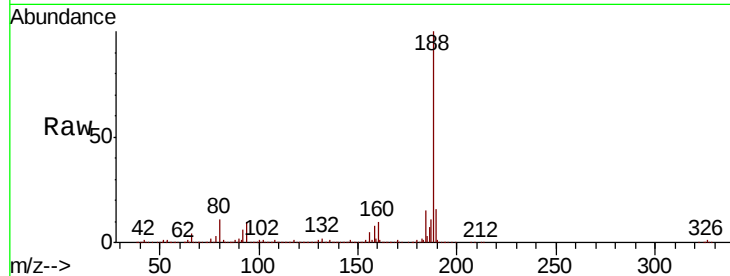


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


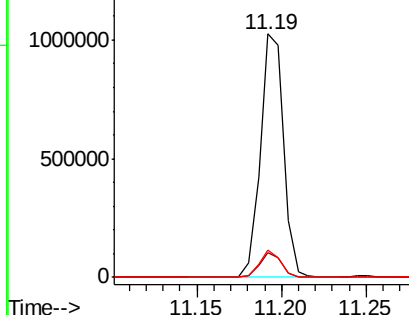



#71
Phenanthrene
Concen: 31.106 ng
RT: 11.22 min Scan# 1553
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	1549399		
176	20.2		17.2	25.8
179	16.0		13.9	20.9



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

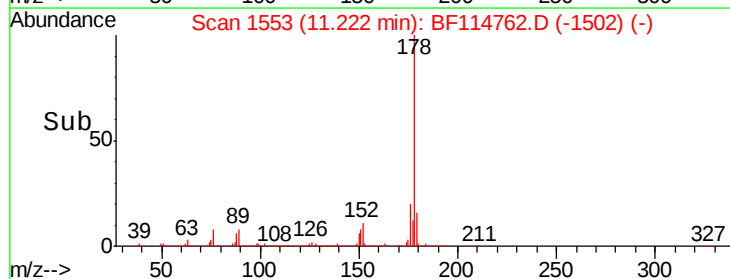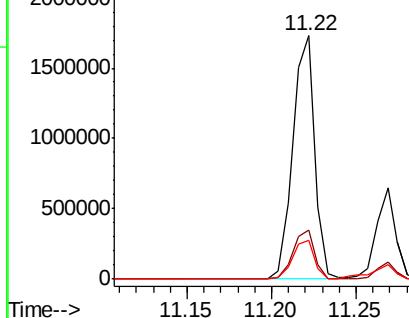



#72

Anthracene

Concen: 10.041 ng

RT: 11.27 min Scan# 1561

Delta R.T. -0.01 min

Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Instrument :

BNA_F


ClientSampleId :

NB-07-053019-A




Tot Ion:	178	Resp:	506215
Ion Ratio	Lower	Upper	
178	100		
176	18.9	16.6	24.8
179	15.5	13.4	20.0

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM

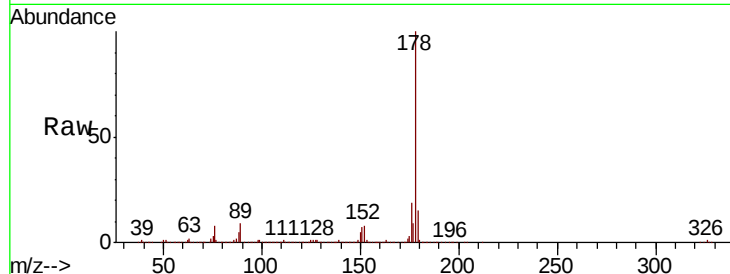

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

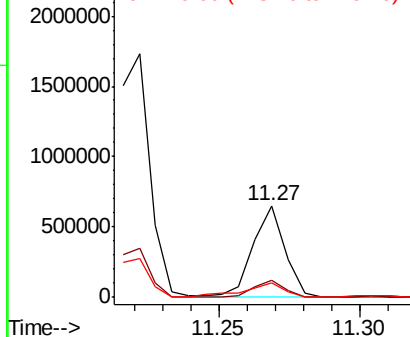

#73

Carbazole

Concen: 4.602 ng


RT: 11.42 min Scan# 1587

Delta R.T. 0.00 min



Lab File: BF114762.D


Acq: 1 Jun 2019 17:32

Tgt Ion:	167	Resp:	203903
Ion Ratio	Lower	Upper	
167	100		
166	21.3	18.7	28.1
139	11.8	11.8	17.8#



Abundance Ion 167.00 (166.70 to 167.70): E
Ion 166.00 (165.70 to 166.70): E
Ion 139.00 (138.70 to 139.70): E

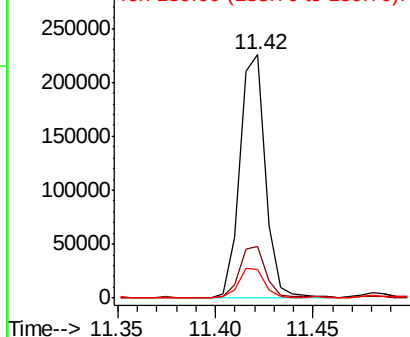

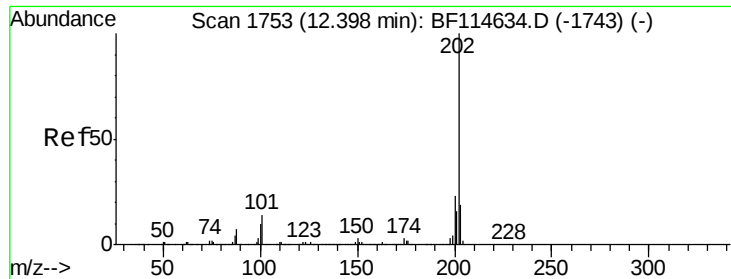





#75
 Fluoranthene
 Concen: 30.297 ng
 RT: 12.40 min Scan# 1753
 Delta R.T. 0.00 min
 Lab File: BF114762.D
 Acq: 1 Jun 2019 17:32

Instrument :
 BNA_F
 ClientSampleId :
 NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
202	100		
101	13.3	0.0	33.9
203	18.7	0.0	39.1




Manual Integrations
 APPROVED


mohammad
 6/3/2019 8:51:35 AM

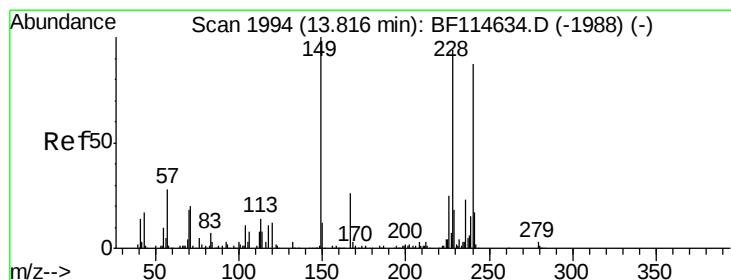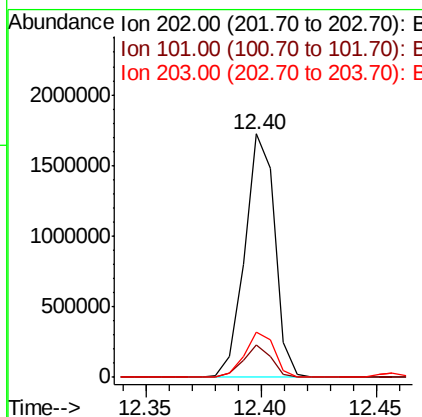

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.82 min Scan# 1994
 Delta R.T. 0.00 min
 Lab File: BF114762.D
 Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Lower	Upper
240	100		
120	13.3	11.2	16.8
236	26.8	21.2	31.8

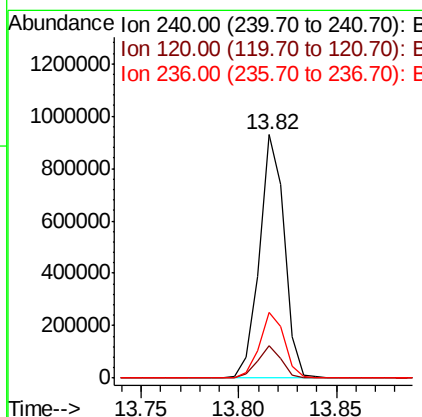

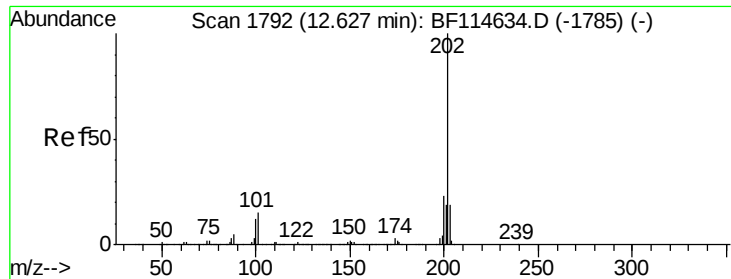


#78
Pvrene
Concen: 19.876 ng
RT: 12.63 min Scan# 1792
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
202	100		
200	21.9	18.6	28.0
203	18.1	15.4	23.2

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM



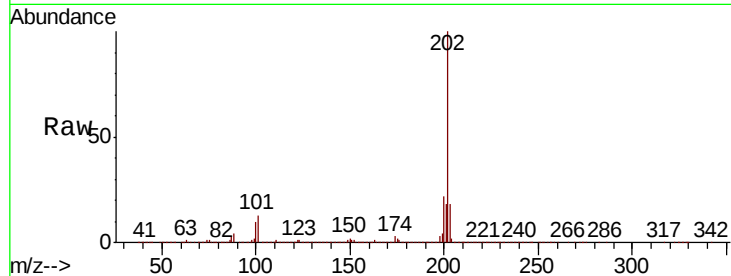


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

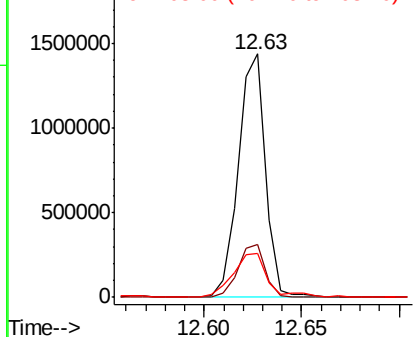

#79
Terphenyl-d14
Concen: 10.630 ng
RT: 12.77 min Scan# 1817
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32




Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.3	6.1	9.1
122	10.7	9.8	14.8


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

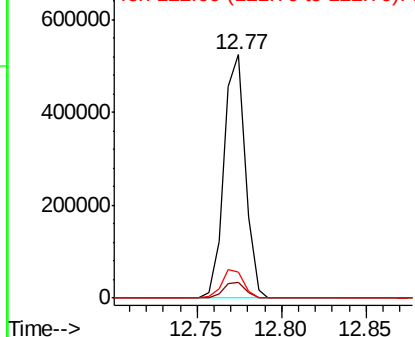



#81

Benzo(a)anthracene

Concen: 13.633 ng

RT: 13.81 min Scan# 1993

Delta R.T. 0.00 min

Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Instrument :

BNA_F


ClientSampleId :

NB-07-053019-A




Tot Ion:	228	Resp:	856514
Ion	Ratio	Lower	Upper
228	100		
226	29.2	23.0	34.6
229	21.3	17.0	25.4

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM

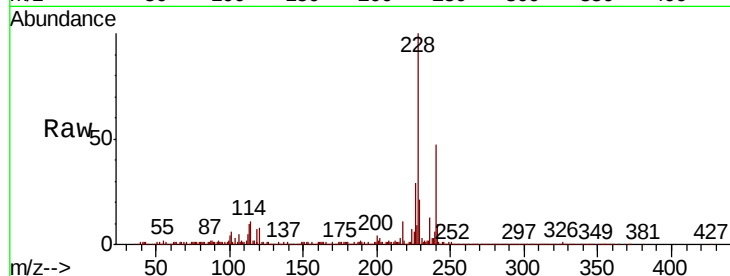

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

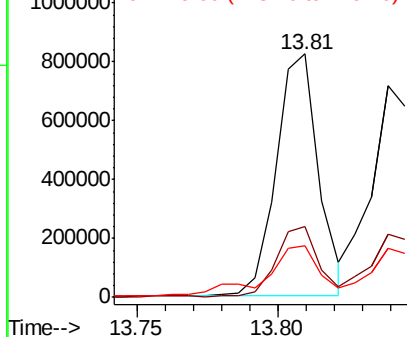

#83

Chrysene

Concen: 12.343 ng

RT: 13.84 min Scan# 1998




Delta R.T. -0.01 min


Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Tgt Ion:	228	Resp:	740896
Ion	Ratio	Lower	Upper
228	100		
226	29.7	26.4	39.6
229	23.2	17.1	25.7

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

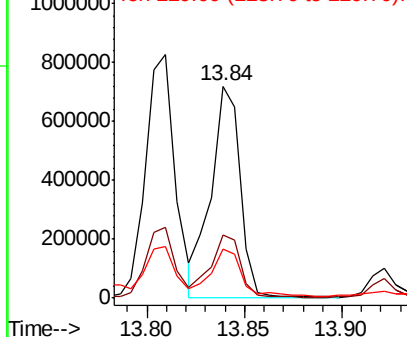

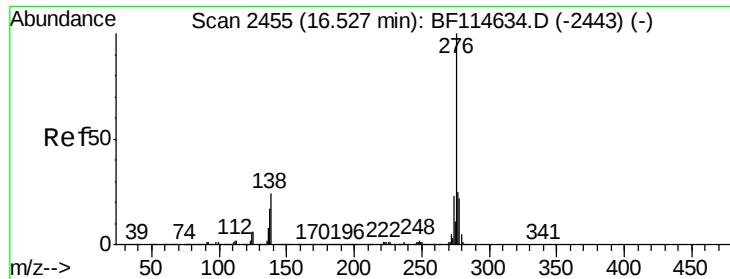


#86
Indeno(1,2,3-cd)pyrene
Concen: 5.121 ng
RT: 16.53 min Scan# 2456
Delta R.T. 0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Lower	Upper
276	100		
138	24.2	23.0	34.6
277	24.2	20.5	30.7

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM



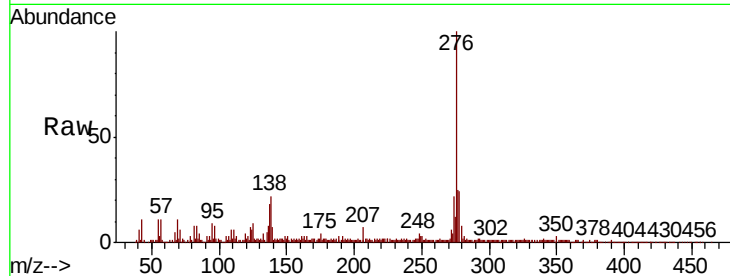


Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

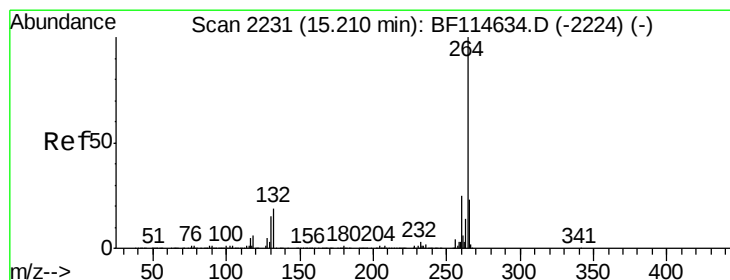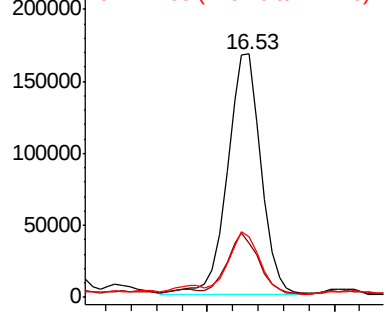

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.21 min Scan# 2231
Delta R.T. 0.00 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32




Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.7	29.5
265	22.3	18.1	27.1


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

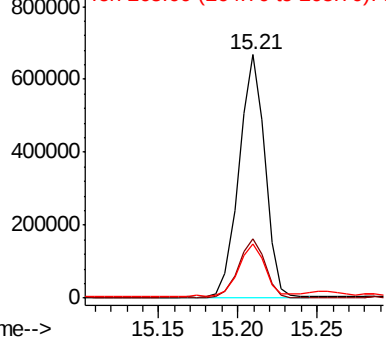

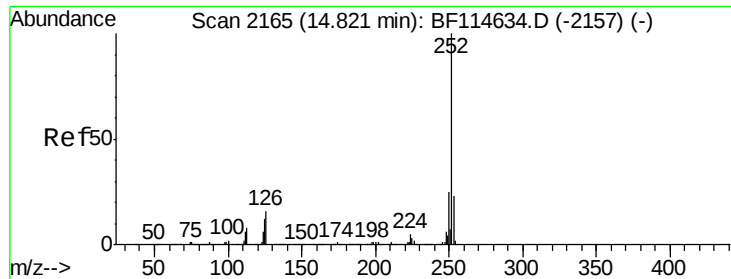

#88

Benzo(b)fluoranthene

Concen: 18.438 ng m

RT: 14.82 min Scan# 2165

Delta R.T. 0.00 min

Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Instrument :

BNA_F





ClientSampleId :

NB-07-053019-A

Tot Ion:	252	Resp:	886050
Ion Ratio	Lower	Upper	
252	100		
253	23.4	18.7	28.1
125	12.9	9.4	14.2

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM

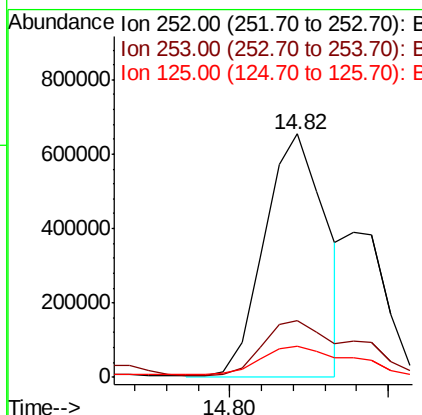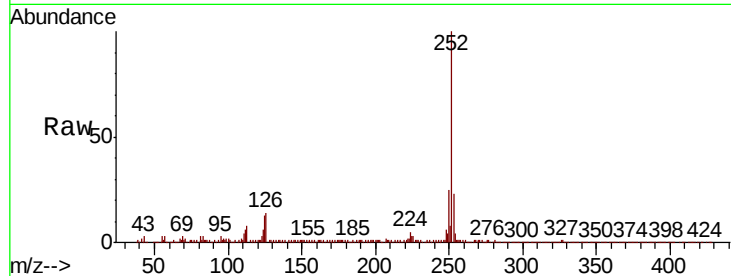

#89

Benzo(k)fluoranthene

Concen: 8.175 ng m




RT: 14.84 min Scan# 2168


Delta R.T. -0.01 min

Lab File: BF114762.D

Acq: 1 Jun 2019 17:32

Tgt Ion:	252	Resp:	341454
Ion Ratio	Lower	Upper	
252	100		
253	24.7	18.9	28.3
125	13.6	9.5	14.3

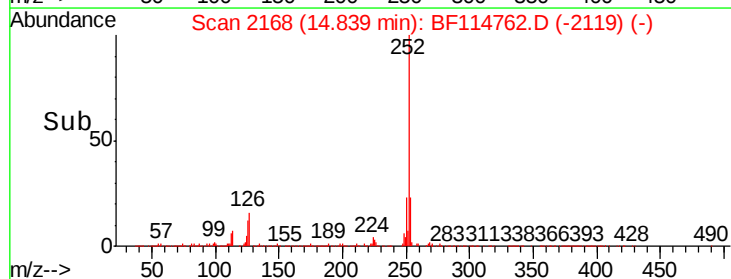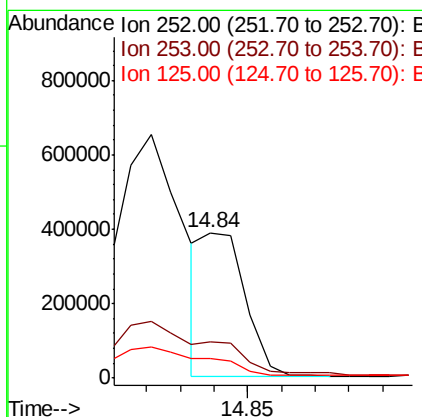

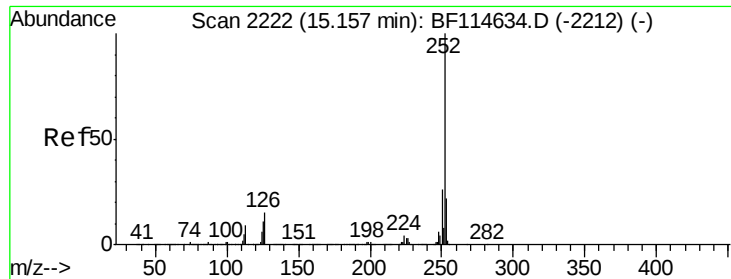


#90
Benzo(a)pyrene
Concen: 15.005 ng
RT: 15.15 min Scan# 2221
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Instrument :
BNA_F
ClientSampleId :
NB-07-053019-A

Tot Ion	Ratio	Resp Lower	Upper
252	100		
253	22.8	18.0	27.0
125	12.9	9.2	13.8

Manual Integrations
APPROVED

mohammad
6/3/2019 8:51:35 AM






Abundance

Ion 252.00 (251.70 to 252.70): E


Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

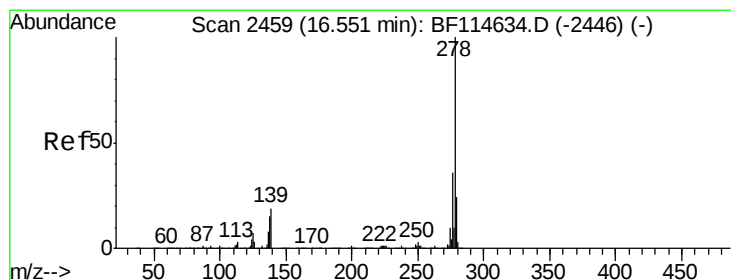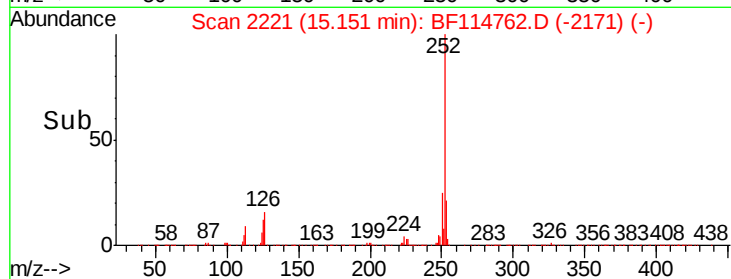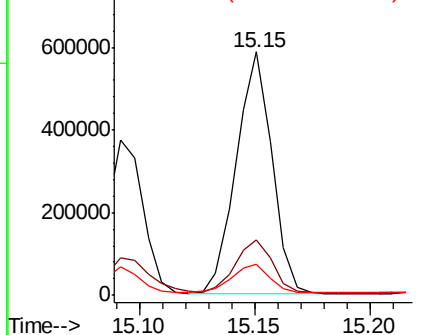

#91
Dibenzo(a,h)anthracene
Concen: 2.280 ng
RT: 16.54 min Scan# 2457
Delta R.T. -0.01 min
Lab File: BF114762.D
Acq: 1 Jun 2019 17:32

Tgt Ion	Ratio	Resp Lower	Upper
278	100		
139	25.8	14.9	22.3#
279	29.5	19.5	29.3#


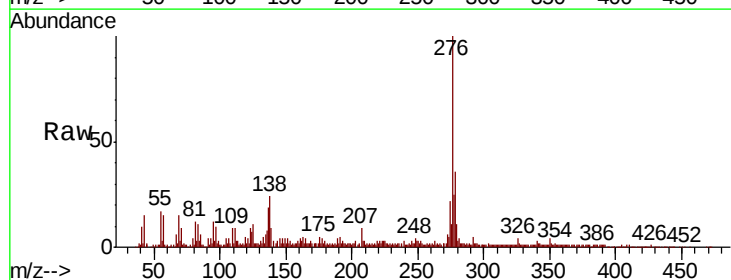



Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

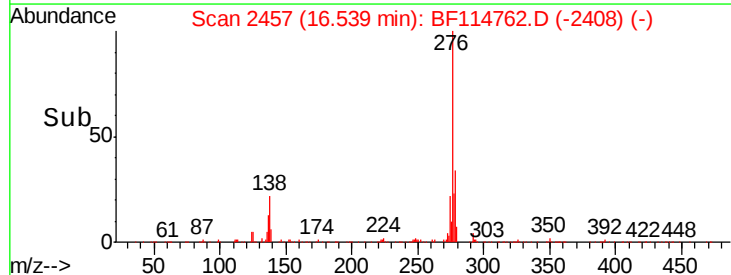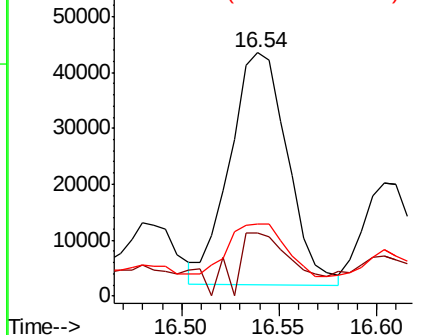

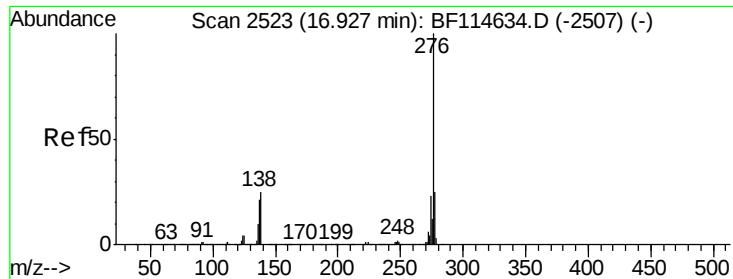

#92
 Benzo(a,h,i)perylene
 Concen: 7.601 ng
 RT: 16.93 min Scan# 2523
 Delta R.T. 0.00 min
 Lab File: BF114762.D
 Acq: 1 Jun 2019 17:32

Instrument :
 BNA_F
 ClientSampleId :
 NB-07-053019-A

Tot Ion:	276	Resp:	275204
Ion Ratio	Lower	Upper	
276	100		
277	24.0	19.7	29.5
138	22.7	19.8	29.8

Manual Integrations
 APPROVED

mohammad
 6/3/2019 8:51:35 AM

