


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060119\
 Data File : BF114740.D
 Acq On : 1 Jun 2019 7:16
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 19:08:51 2019

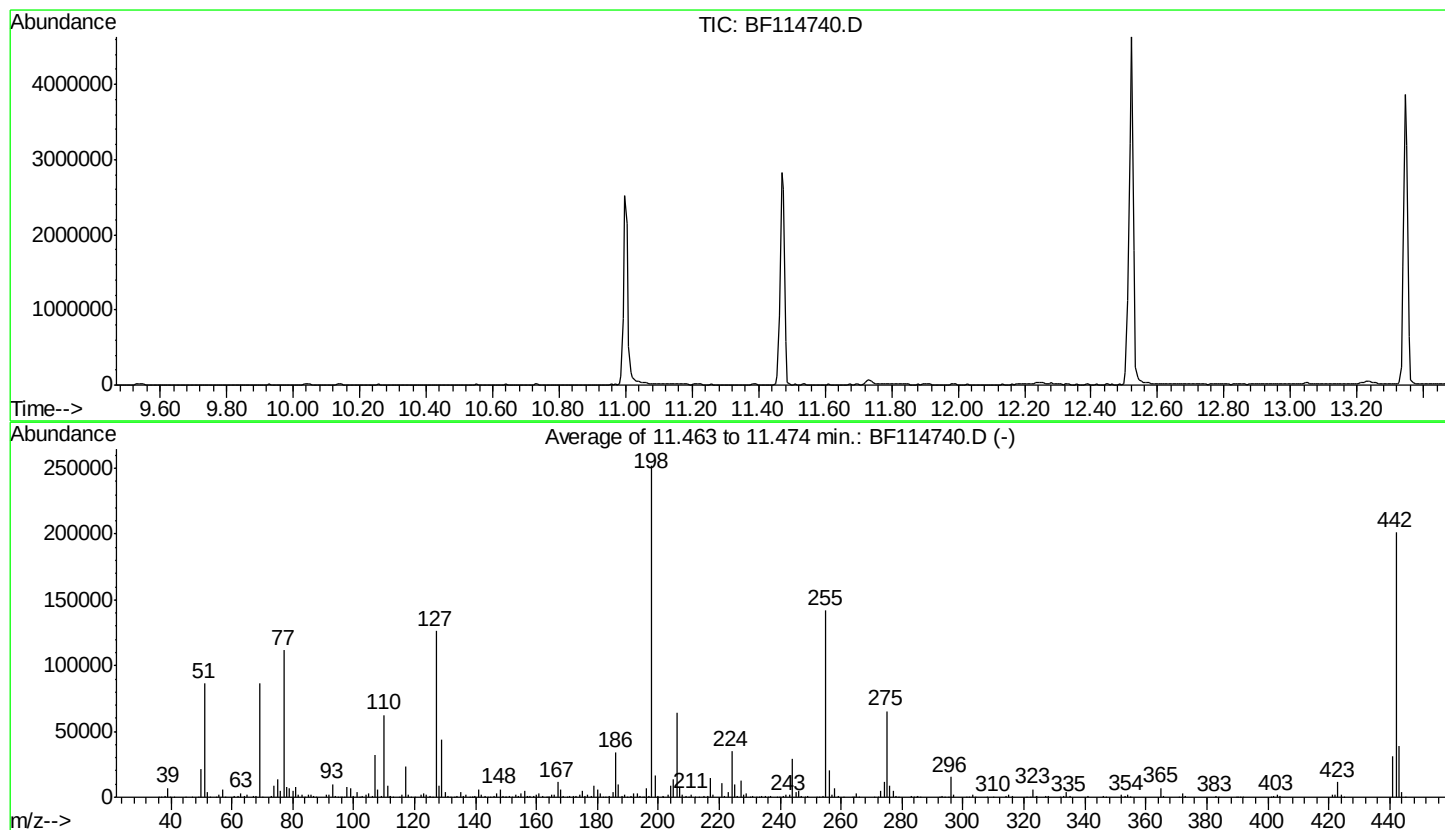

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	86549	PASS
68	69	0.00	2	1.7	1497	PASS
69	198	0.00	100	34.5	86828	PASS
70	69	0.00	2	0.5	462	PASS
127	198	10	80	50.1	126168	PASS
197	198	0.00	2	0.5	1348	PASS
198	198	100	100	100.0	252013	PASS
199	198	5	9	6.6	16558	PASS
275	198	10	60	25.9	65370	PASS
365	198	1	100	2.8	6986	PASS
441	198	0.01	100	12.5	31414	PASS
442	198	50	100	79.8	201149	PASS
443	442	15	24	19.3	38866	PASS