


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060119\
 Data File : BF114764.D
 Acq On : 1 Jun 2019 18:52
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 19:08:51 2019

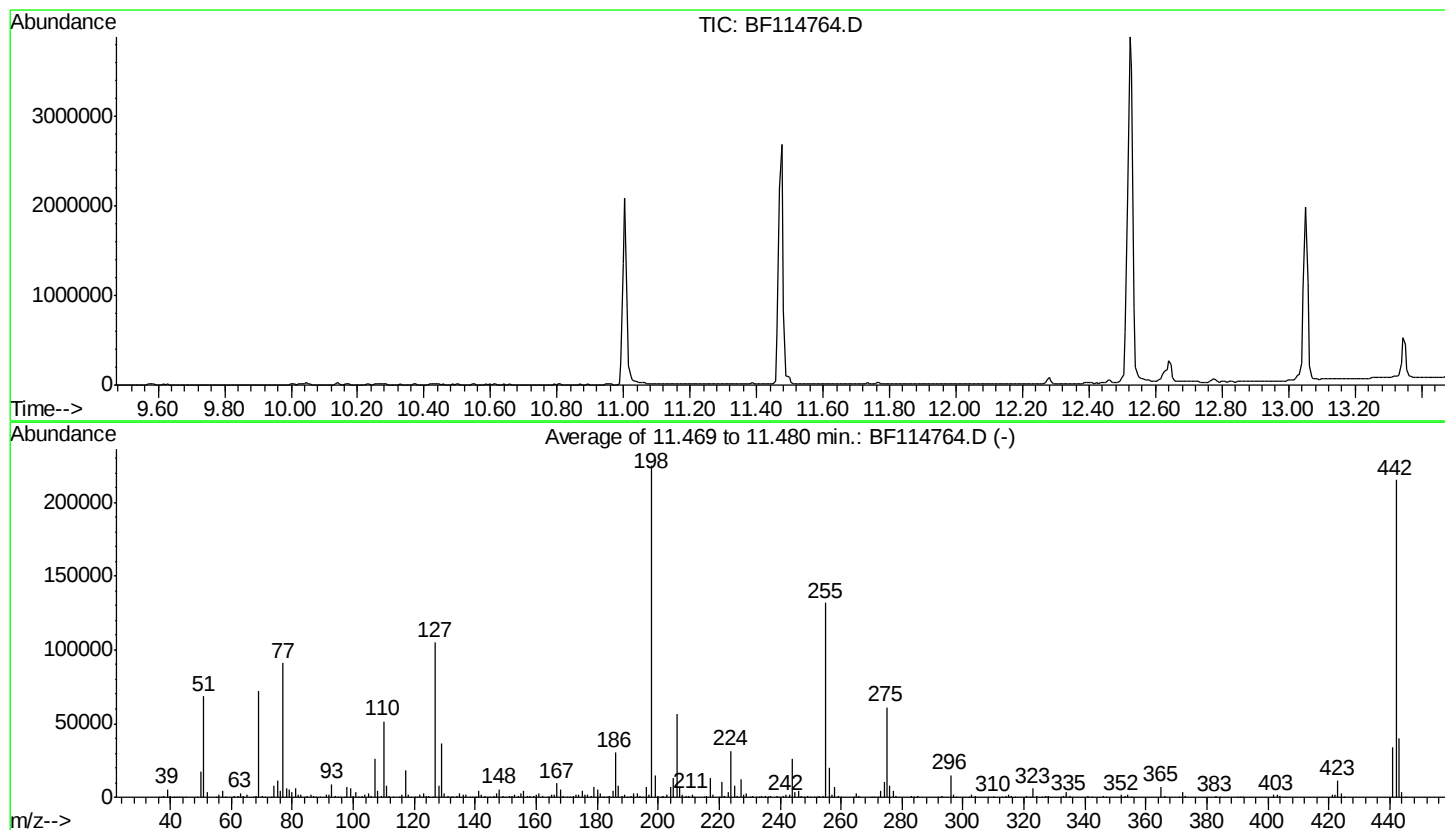

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	68583	PASS
68	69	0.00	2	1.7	1244	PASS
69	198	0.00	100	32.0	72130	PASS
70	69	0.00	2	0.7	522	PASS
127	198	10	80	46.6	104989	PASS
197	198	0.00	2	0.7	1605	PASS
198	198	100	100	100.0	225168	PASS
199	198	5	9	6.8	15237	PASS
275	198	10	60	27.2	61277	PASS
365	198	1	100	3.2	7250	PASS
441	198	0.01	100	14.9	33629	PASS
442	198	50	100	95.6	215317	PASS
443	442	15	24	18.5	39890	PASS