
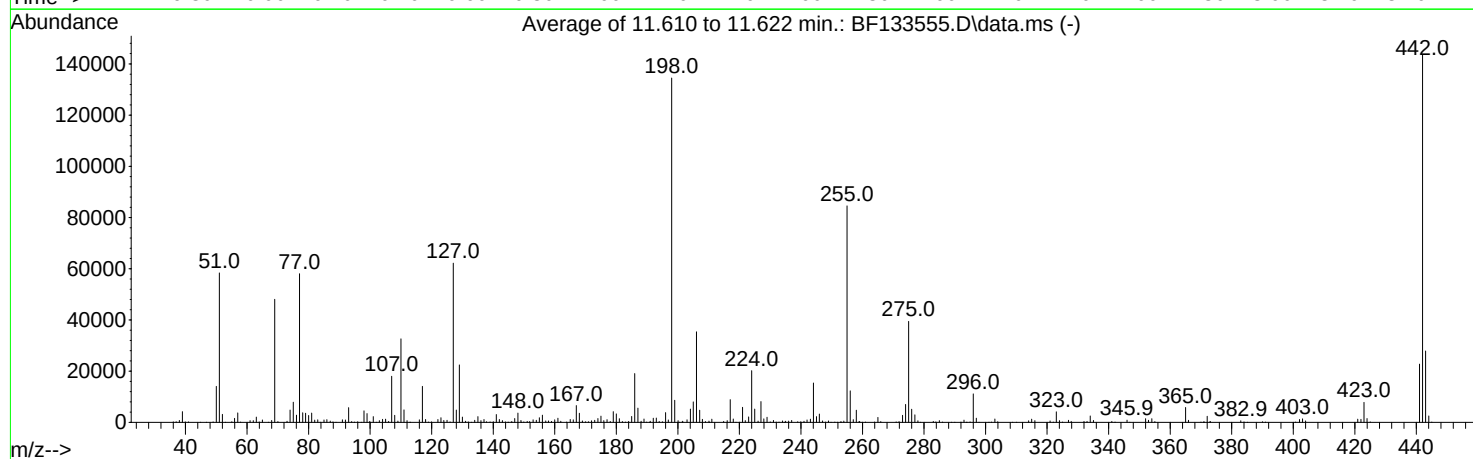


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060223\
Data File : BF133555.D
Acq On : 02 Jun 2023 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 02 17:05:55 2023

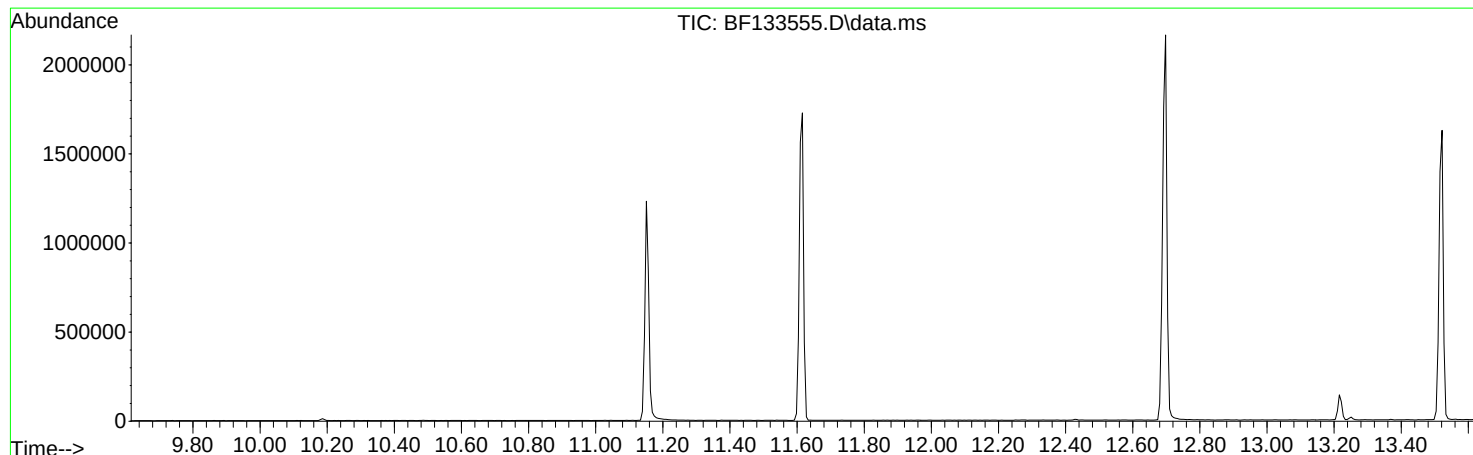

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	58338	PASS
68	69	0.00	2	1.5	743	PASS
69	198	0.00	100	35.7	48024	PASS
70	69	0.00	2	0.7	325	PASS
127	198	10	80	46.2	62158	PASS
197	198	0.00	2	0.7	944	PASS
198	198	100	100	100.0	134501	PASS
199	198	5	9	6.4	8610	PASS
275	198	10	60	29.3	39461	PASS
365	198	1	100	4.3	5788	PASS
441	198	0.01	100	16.9	22750	PASS
442	442	50	100	100.0	143661	PASS
443	442	15	24	19.4	27859	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/2/2023	BNA_F	<u>BF133555.D</u>
Compound Name	Response	Retention Time
DDT	268901	13.521
DDD	25461	13.216
DDE	318	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25779	294680	8.75

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060223\
Data File : BF133555.D
Acq On : 02 Jun 2023 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 13:17:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 30 12:58:40 2023
Response via : Initial Calibration

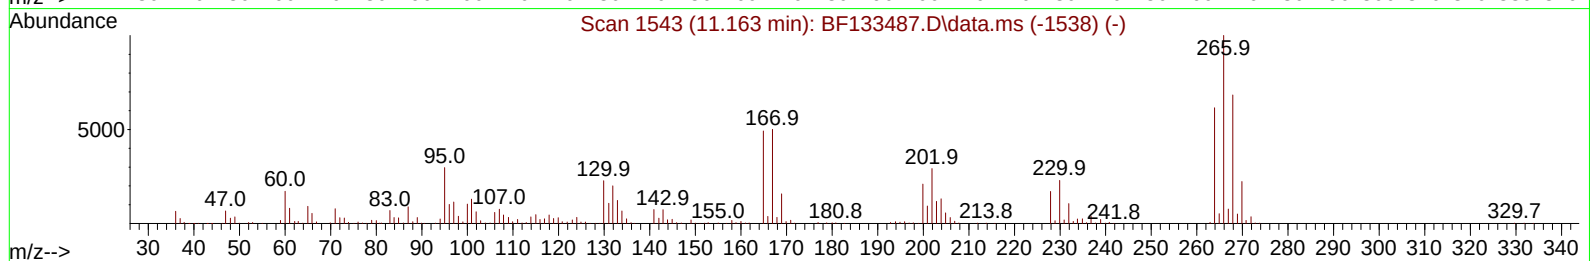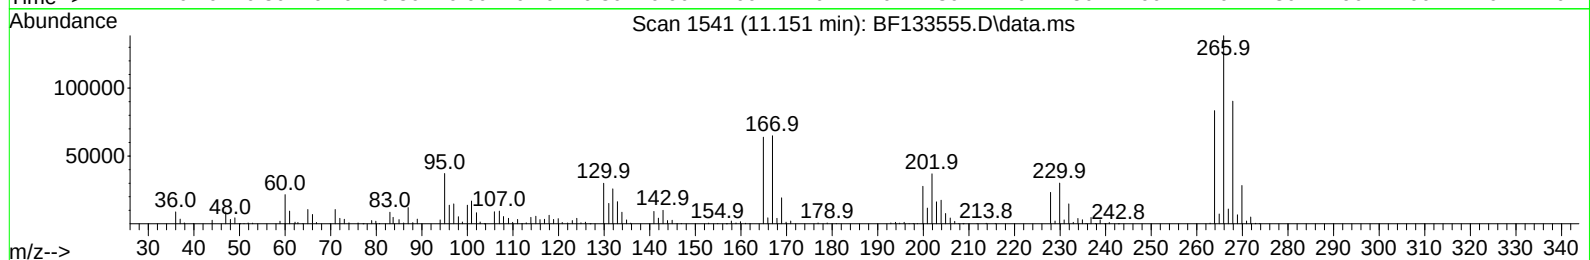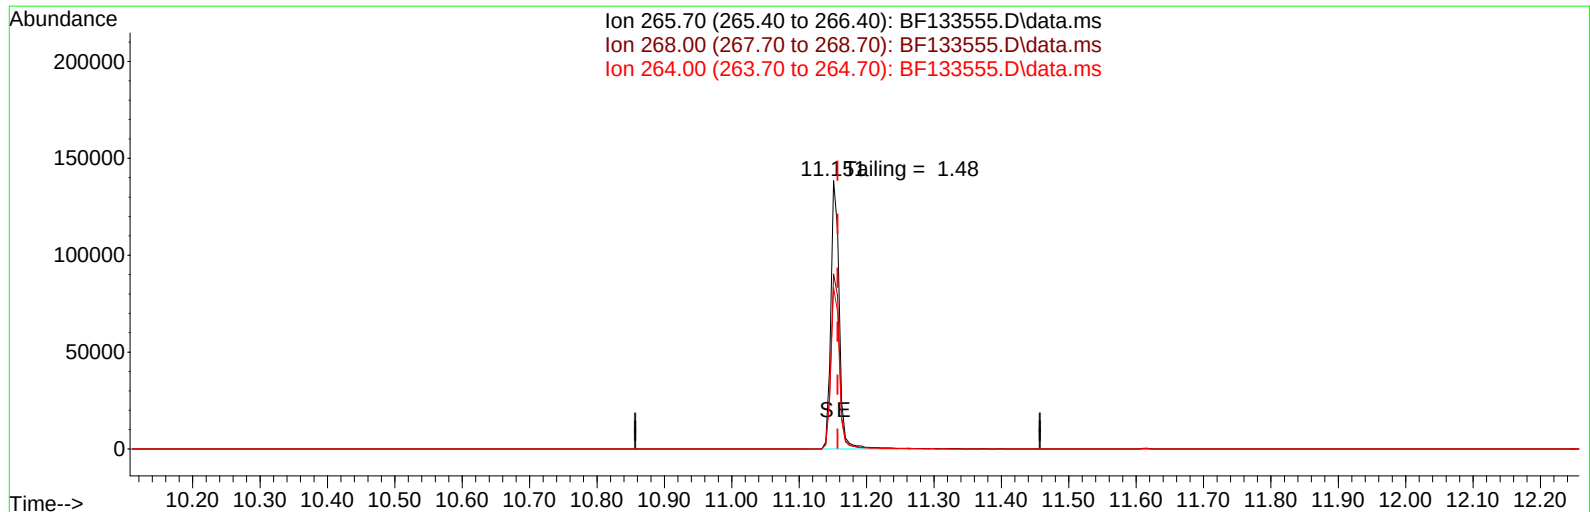

TIC: BF133555.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.006) 32683.40 ng




response 120454

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	65.26
264.00	61.50	60.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060223\
 Data File : BF133555.D
 Acq On : 02 Jun 2023 11:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 02 13:17:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 12:58:40 2023
 Response via : Initial Calibration

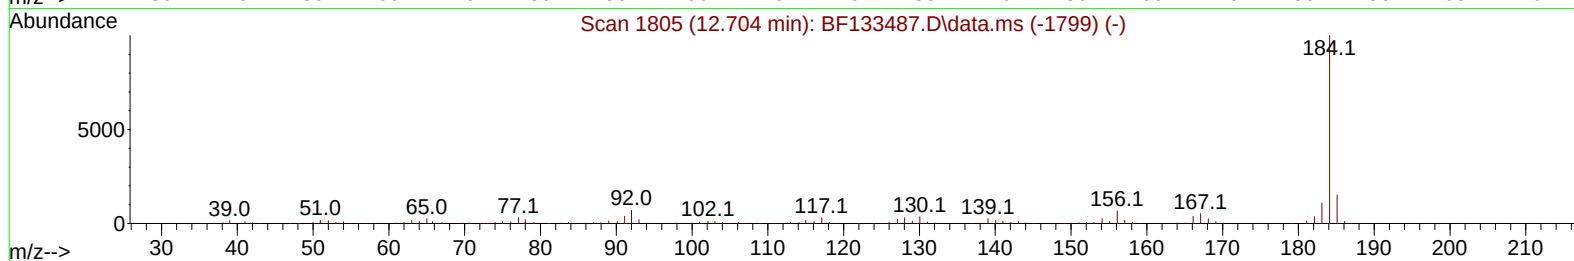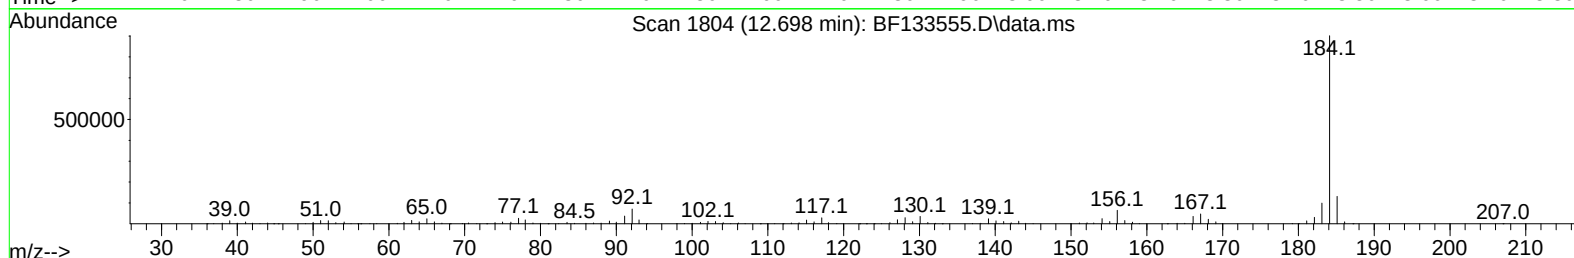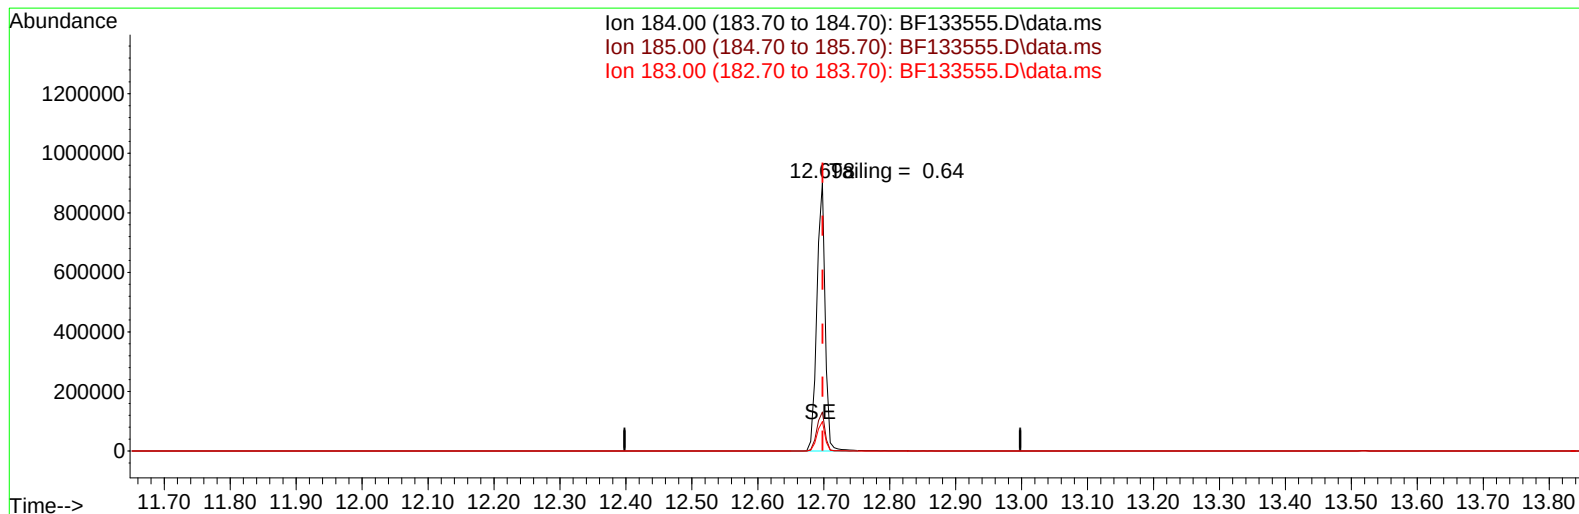

TIC: BF133555.D\data.ms

(77) Benzidine

12.698min (-0.000) 0.00 ng

response 785953

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.57
183.00	10.90	10.99
0.00	0.00	0.00