

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060419\
 Data File : BF114801.D
 Acq On : 4 Jun 2019 19:54
 Operator : HP/JU
 Sample : K3135-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROLL-OFF-COMP

Quant Time: Jun 05 04:45:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF060419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 04 16:57:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	229317	20.00	ng	0.00
21) Naphthalene-d8	7.94	136	877729	20.00	ng	-0.01
39) Acenaphthene-d10	9.69	164	450296	20.00	ng	-0.01
64) Phenanthrene-d10	11.16	188	910636	20.00	ng	0.00
76) Chrysene-d12	13.78	240	763466	20.00	ng	-0.01
87) Perylene-d12	15.16	264	808486	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.27	112	1558505	118.76	ng	0.00
7) Phenol-d6	6.30	99	1724753	108.01	ng	0.00
23) Nitrobenzene-d5	7.22	82	1270529	89.11	ng	-0.01
42) 2,4,6-Tribromophenol	10.47	330	646496	133.23	ng	0.00
45) 2-Fluorobiphenyl	9.02	172	2425957	100.92	ng	0.00
79) Terphenyl-d14	12.74	244	2999537	76.41	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060419\
Data File : BF114801.D
Acq On : 4 Jun 2019 19:54
Operator : HP/JU
Sample : K3135-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP

Quant Time: Jun 05 04:45:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF060419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 04 16:57:15 2019
Response via : Initial Calibration

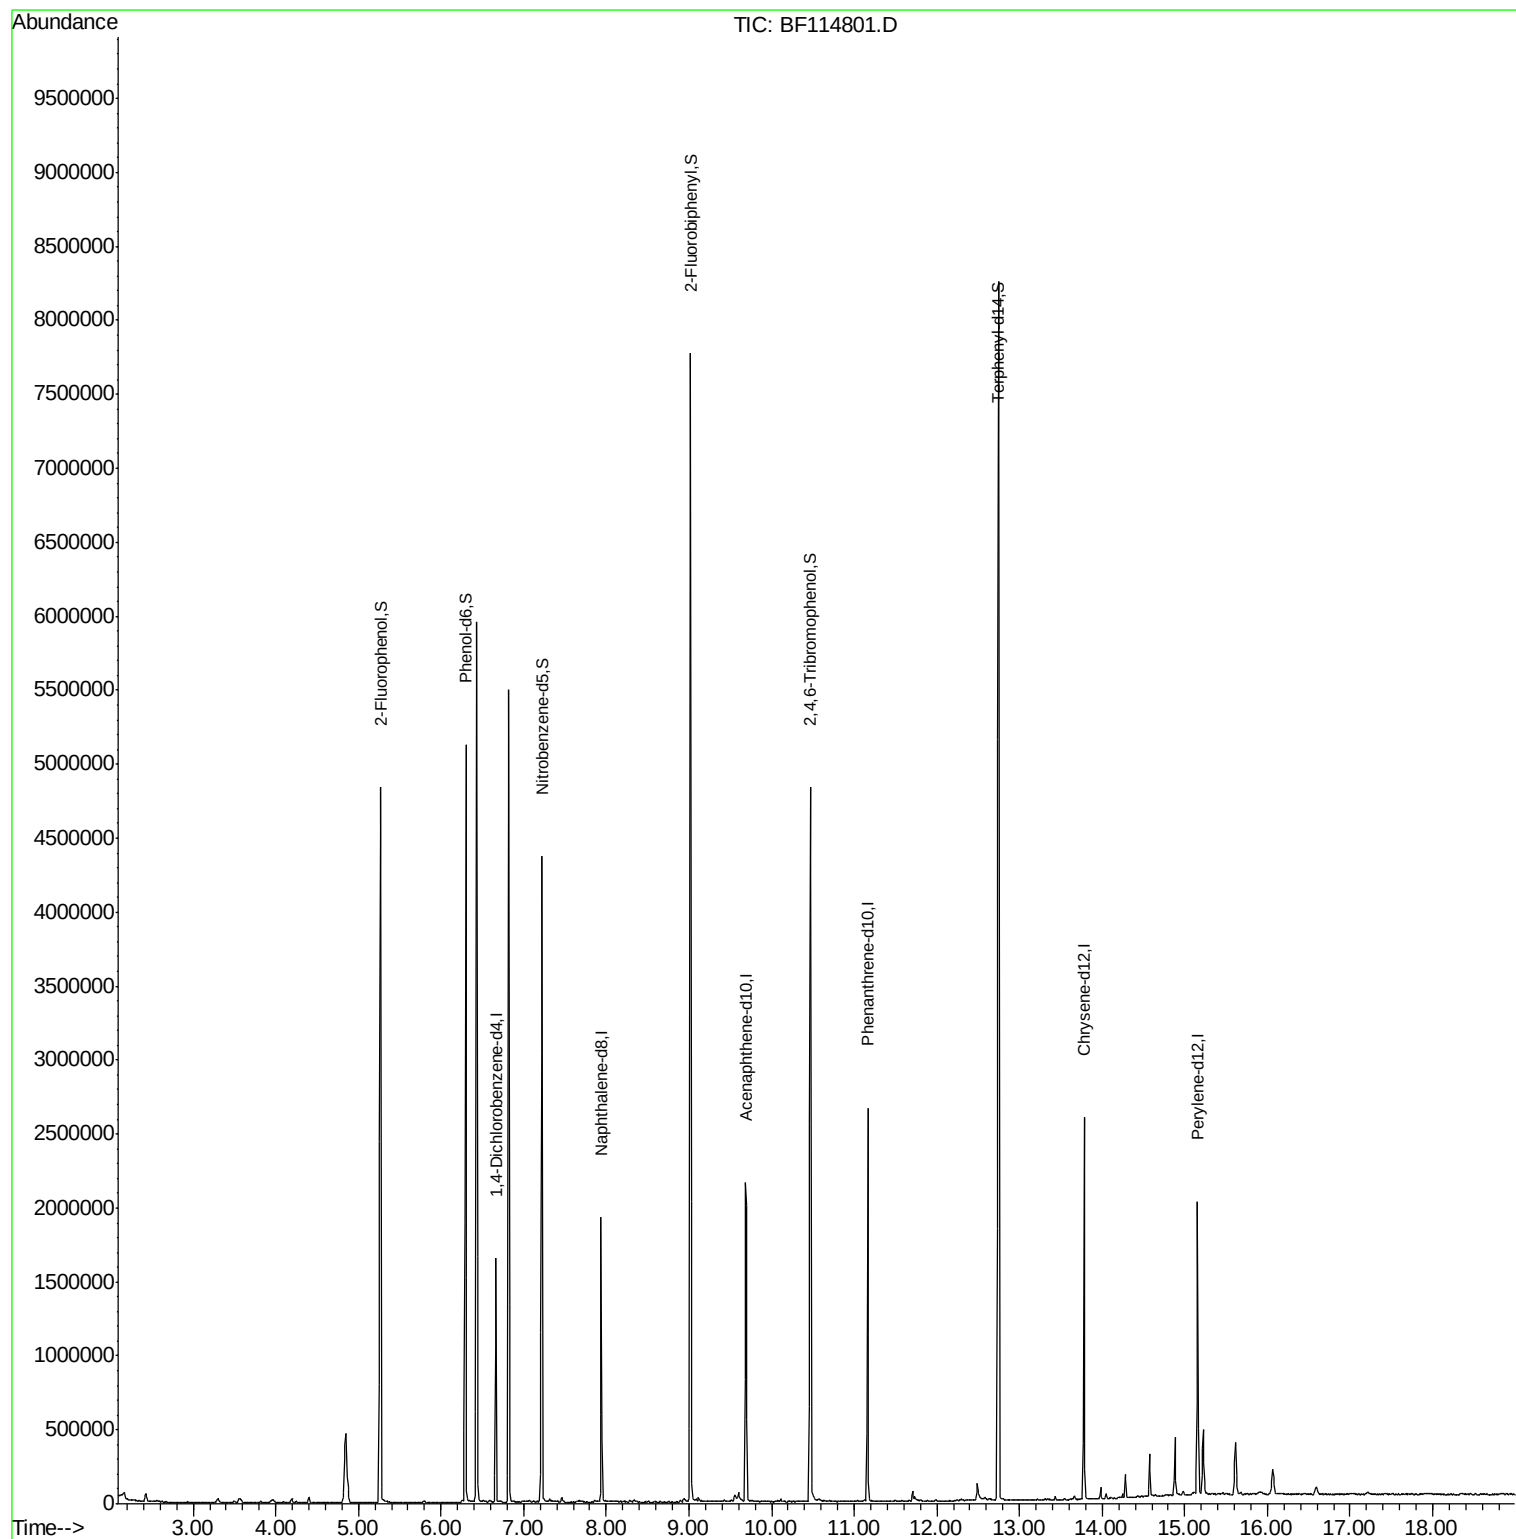

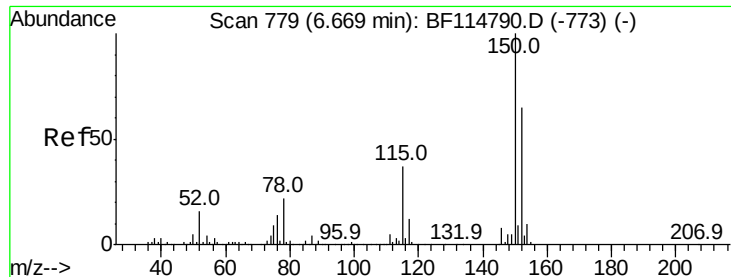


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.66 min Scan# 778
Delta R.T. -0.01 min
Lab File: BF114801.D
Acq: 4 Jun 2019 19:54

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP

Tot Ion:152 Resp: 229317
Ion Ratio Lower Upper
152 100
150 157.7 124.0 186.0
115 59.0 46.3 69.5

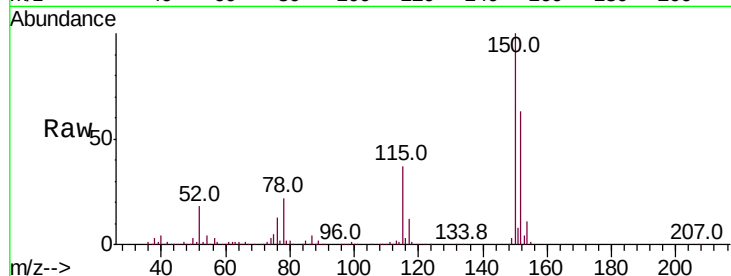


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

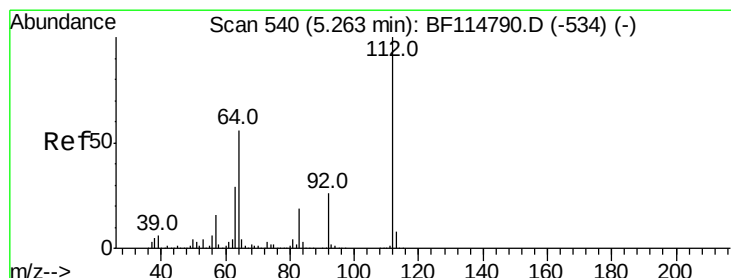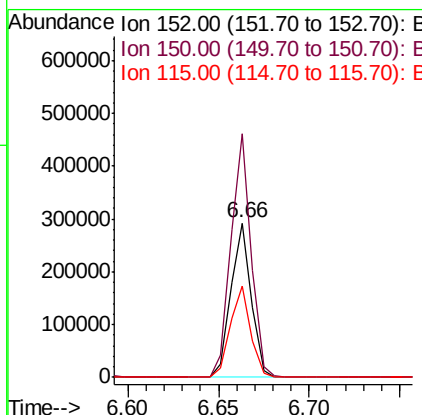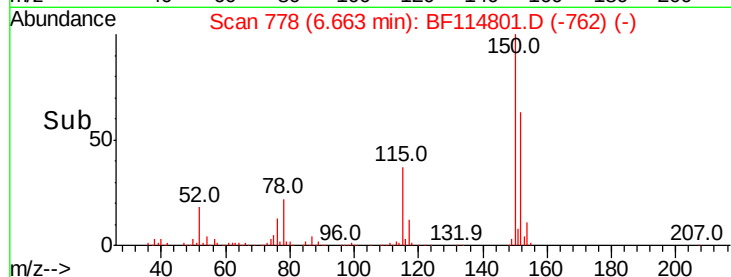



#5


2-Fluorophenol
Concen: 118.755 ng
RT: 5.27 min Scan# 541
Delta R.T. 0.01 min
Lab File: BF114801.D
Acq: 4 Jun 2019 19:54

Tgt Ion:112 Resp: 1558505
Ion Ratio Lower Upper
112 100
64 51.5 44.6 66.8
63 26.1 23.0 34.4

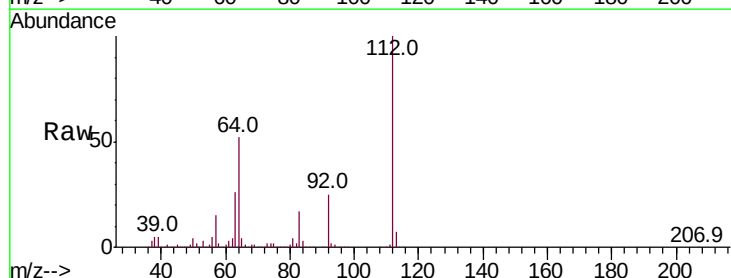

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

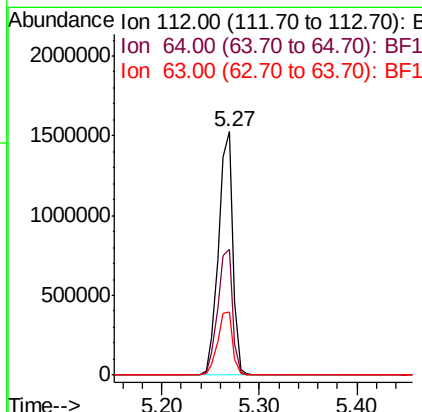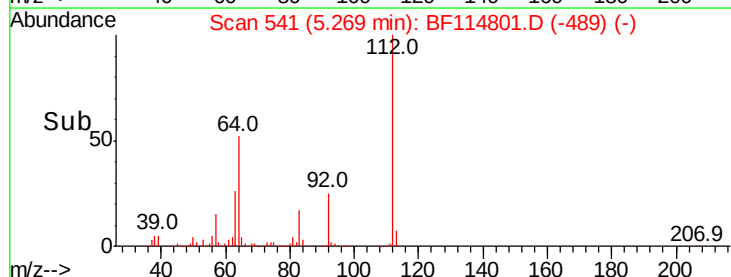

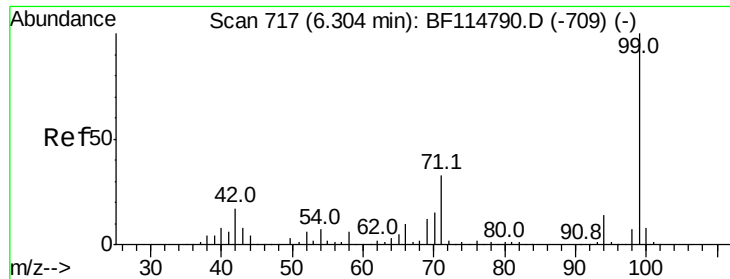

#7

Phenol-d6

Concen: 108.007 ng

RT: 6.30 min Scan# 716

Delta R.T. -0.01 min

Lab File: BF114801.D

Acq: 4 Jun 2019 19:54

Instrument :

BNA_F

ClientSampleId :

ROLL-OFF-COMP


Tot Ion: 99 Resp: 1724753

Ion Ratio Lower Upper




99 100

42 16.6 13.3 19.9

71 32.9 26.3 39.5

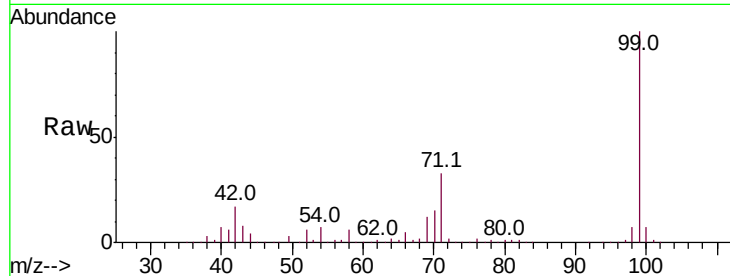

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

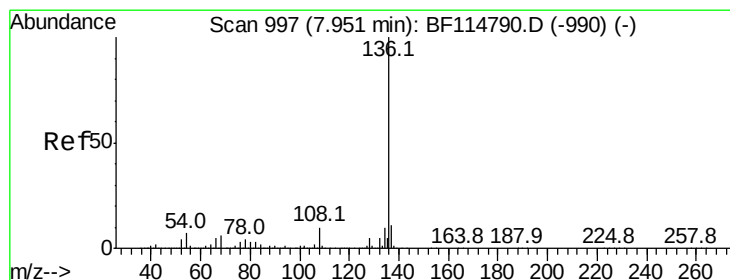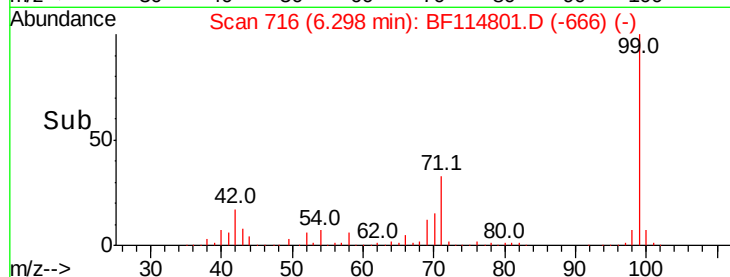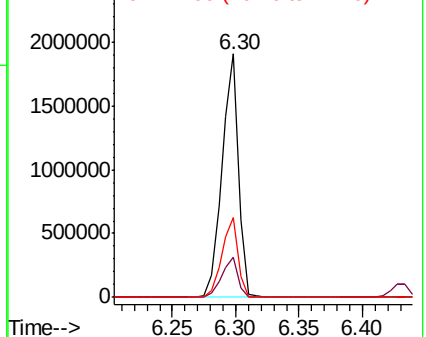

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.94 min Scan# 995

Delta R.T. -0.01 min

Lab File: BF114801.D

Acq: 4 Jun 2019 19:54

Tgt Ion: 136 Resp: 877729


Ion Ratio Lower Upper

136 100



137 11.4 9.1 13.7


54 7.2 5.4 8.0

68 6.0 4.6 6.8

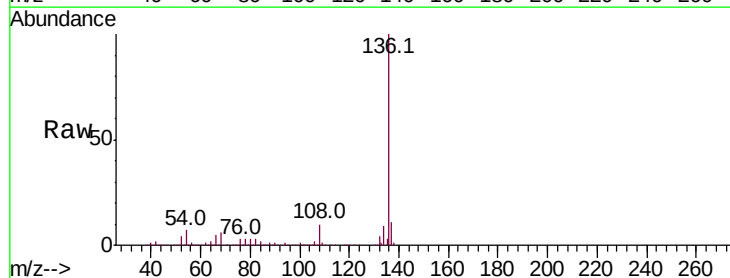

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

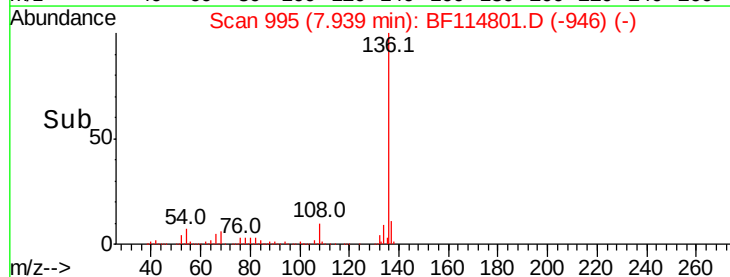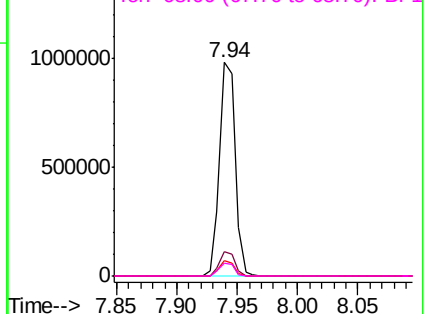


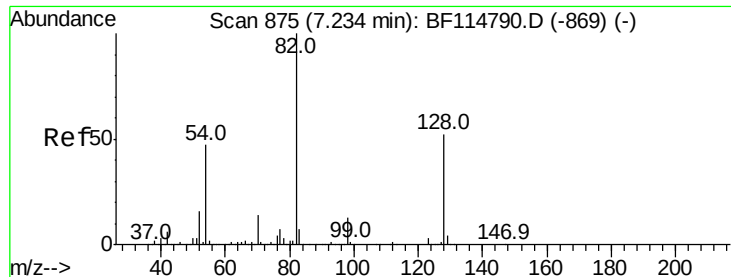




#23
Nitrobenzene-d5
Concen: 89.107 ng
RT: 7.22 min Scan# 873
Delta R.T. -0.01 min
Lab File: BF114801.D
Acq: 4 Jun 2019 19:54

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP

Tot Ion: 82 Resp: 1270529
Ion Ratio Lower Upper
82 100
128 51.2 41.8 62.6
54 46.5 37.9 56.9

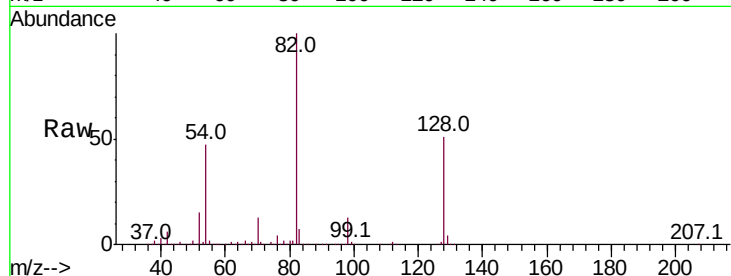


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

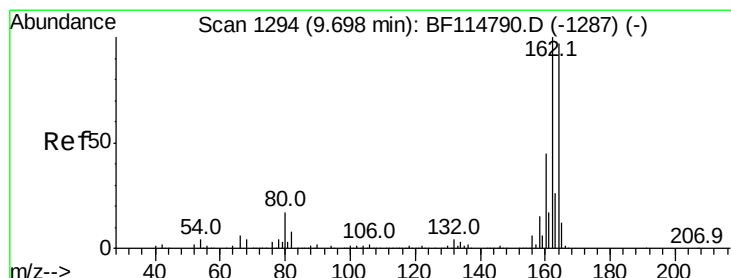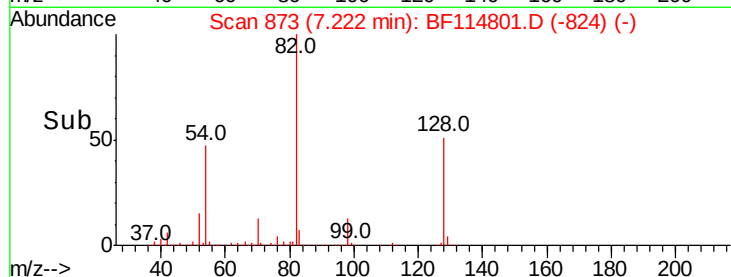
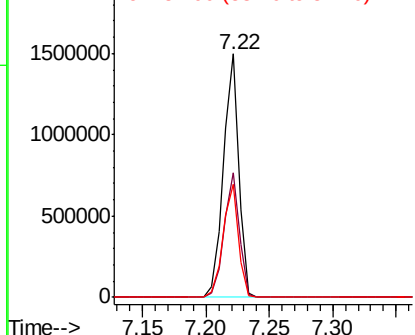



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.69 min Scan# 1292
Delta R.T. -0.01 min
Lab File: BF114801.D
Acq: 4 Jun 2019 19:54

Tgt Ion:164 Resp: 450296
Ion Ratio Lower Upper
164 100
162 101.2 82.3 123.5
160 44.2 36.7 55.1

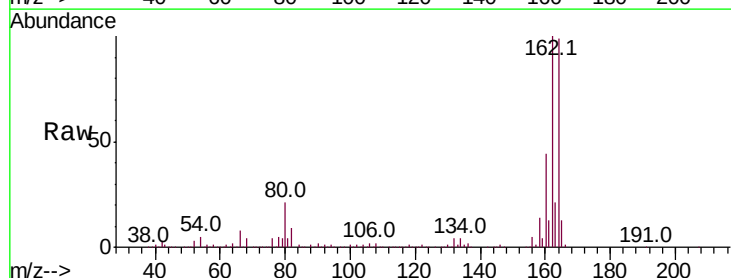

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

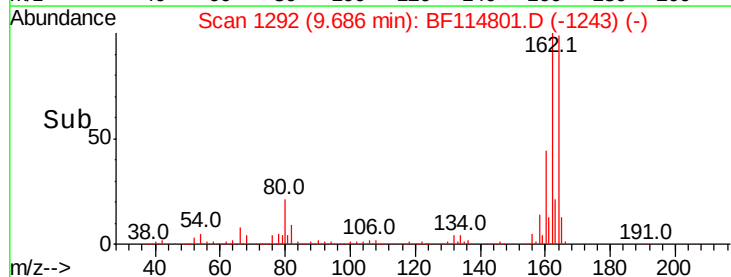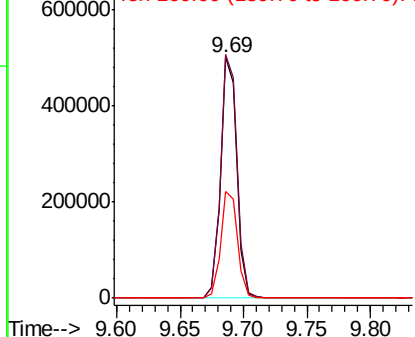

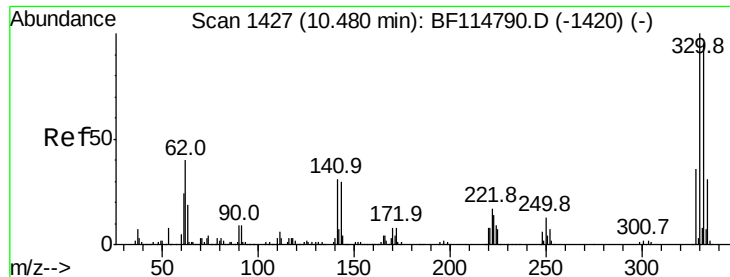

#42

2,4,6-Tribromophenol

Concen: 133.225 ng

RT: 10.47 min Scan# 1426

Delta R.T. -0.01 min

Lab File: BF114801.D

Acq: 4 Jun 2019 19:54

Instrument :

BNA_F

ClientSampleId :

ROLL-OFF-COMP


Tot Ion:330 Resp: 646496

Ion Ratio Lower Upper

330 100

332 97.2 77.3 115.9




141 33.6 26.2 39.4

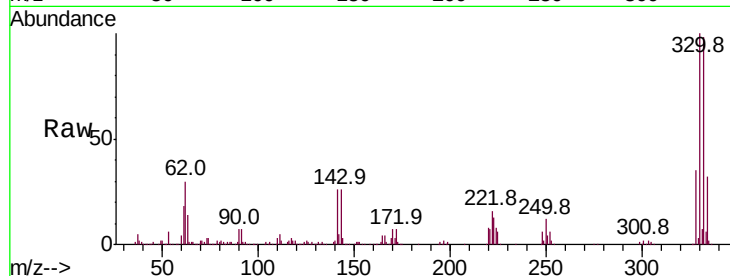

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

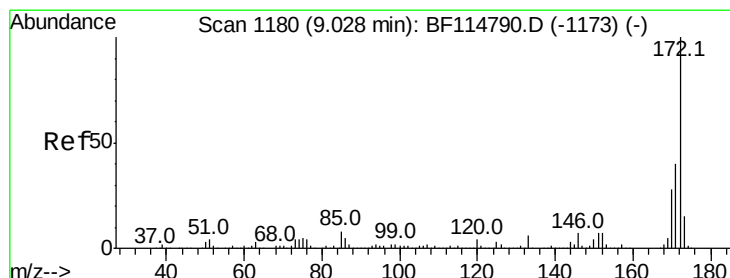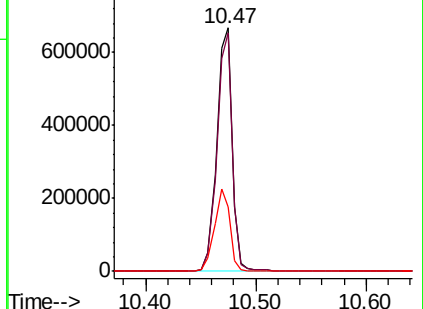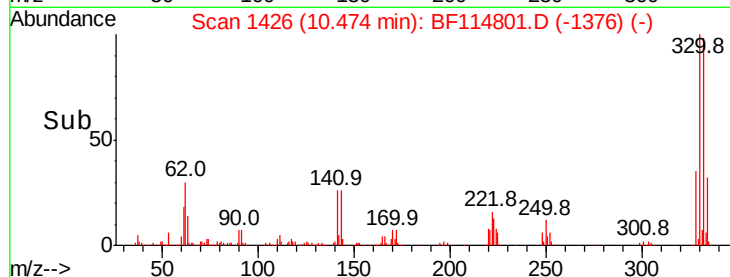

#45

2-Fluorobiphenyl

Concen: 100.922 ng

RT: 9.02 min Scan# 1179

Delta R.T. -0.01 min

Lab File: BF114801.D

Acq: 4 Jun 2019 19:54


Tgt Ion:172 Resp: 2425957

Ion Ratio Lower Upper

172 100

171 38.3 32.3 48.5



170 25.9 22.4 33.6

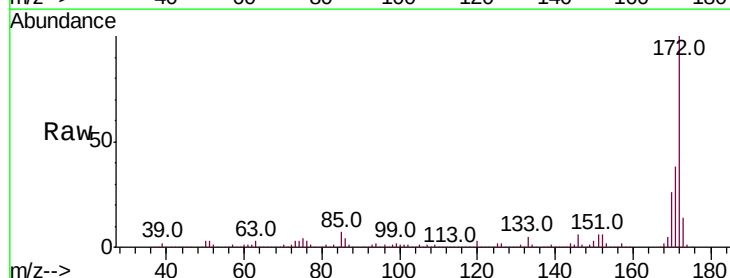


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



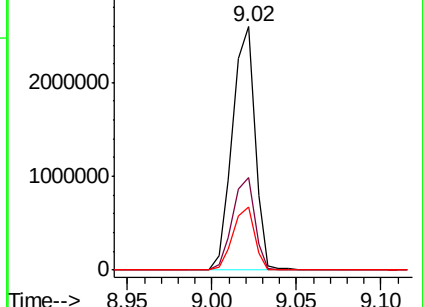
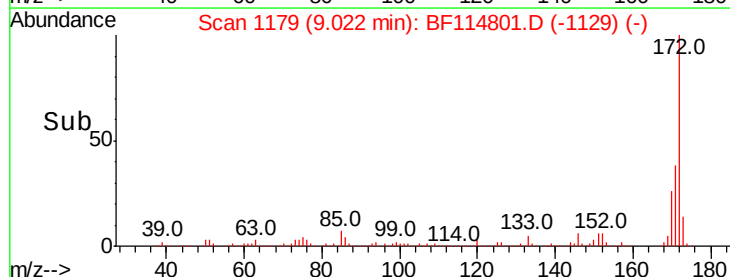


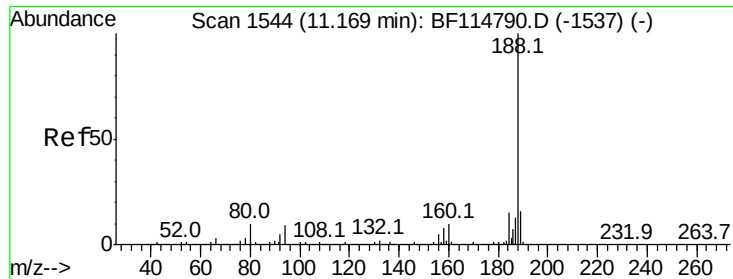

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.16 min Scan# 1543
Delta R.T. -0.01 min
Lab File: BF114801.D
Acq: 4 Jun 2019 19:54




Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP


Tot Ion:188 Resp: 910636
Ion Ratio Lower Upper
188 100
94 9.5 7.6 11.4
80 9.8 8.3 12.5

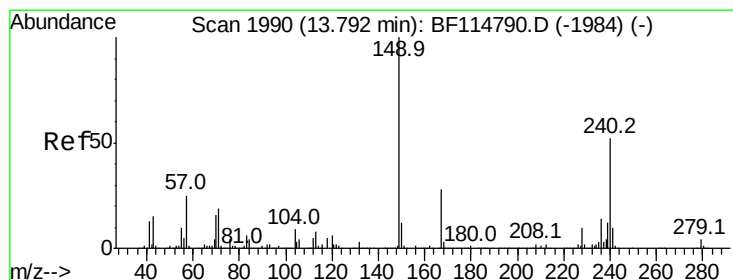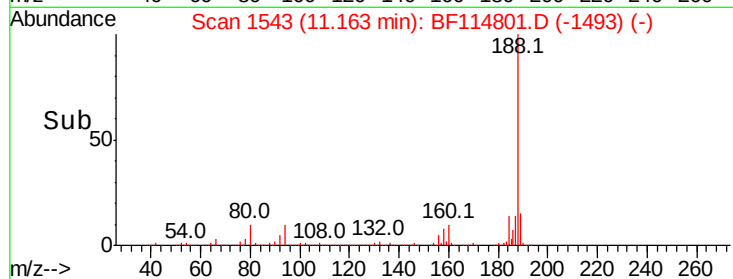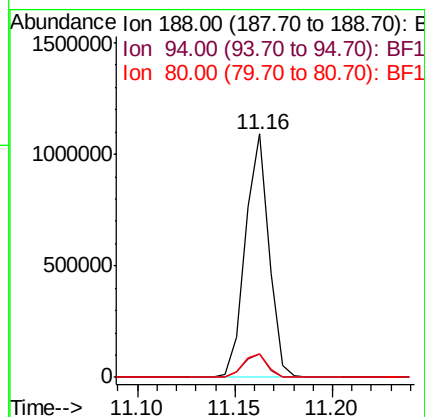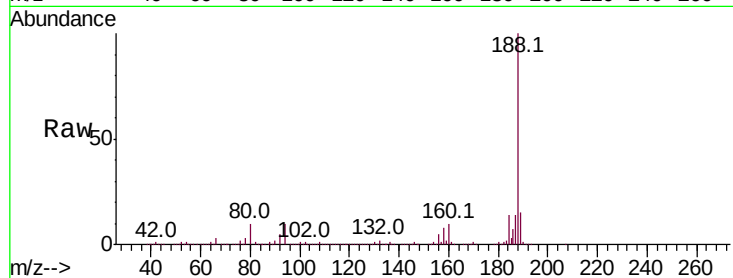

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.78 min Scan# 1988
Delta R.T. -0.01 min
Lab File: BF114801.D
Acq: 4 Jun 2019 19:54

Tgt Ion:240 Resp: 763466
Ion Ratio Lower Upper
240 100
120 12.1 9.0 13.4
236 26.9 21.4 32.0

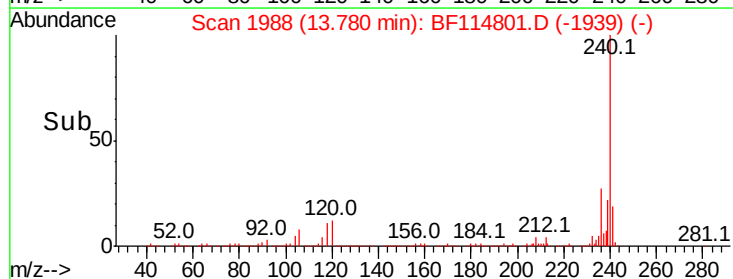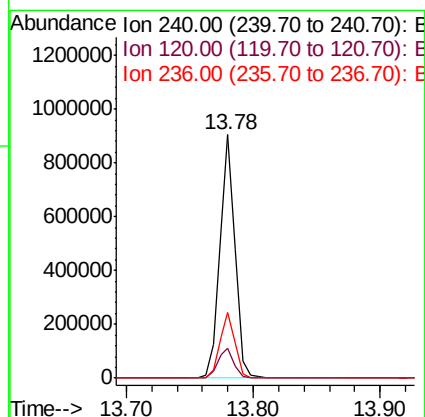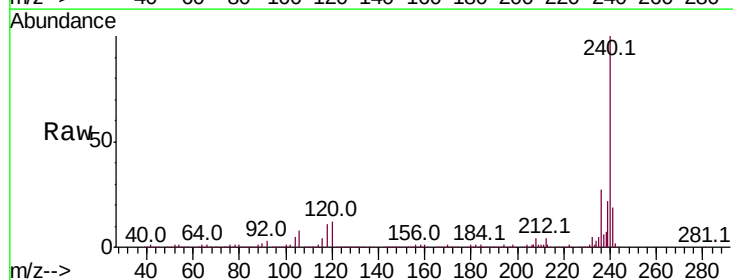

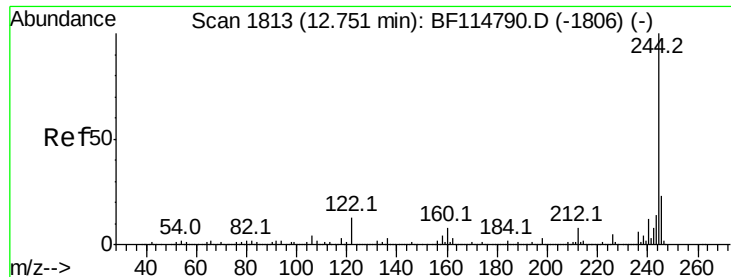


#79
 Terphenyl-d14
 Concen: 76.406 ng
 RT: 12.74 min Scan# 1812
 Delta R.T. -0.01 min
 Lab File: BF114801.D
 Acq: 4 Jun 2019 19:54




Instrument :
 BNA_F
 ClientSampleId :
 ROLL-OFF-COMP

Tot Ion:244 Resp: 2999537

Ion	Ratio	Lower	Upper
244	100		
212	7.5	6.5	9.7
122	13.5	10.5	15.7

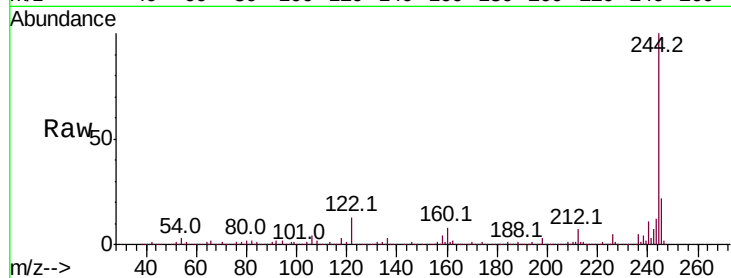


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

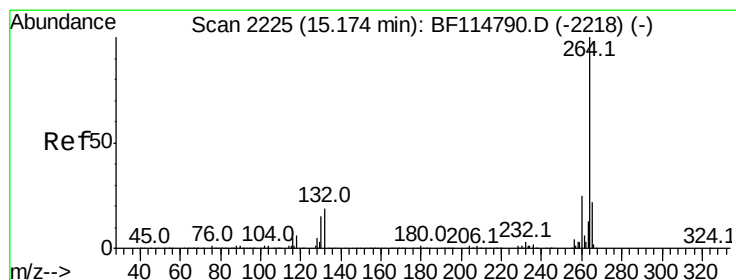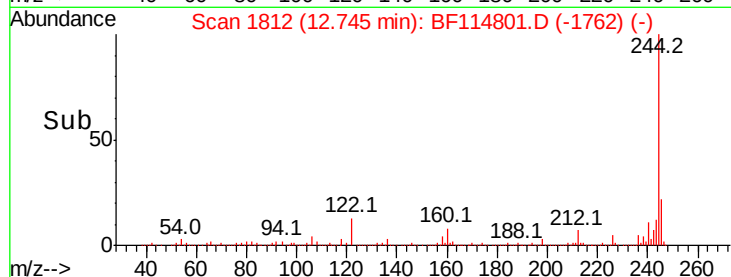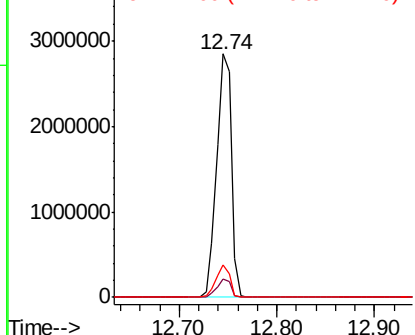

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.16 min Scan# 2222
 Delta R.T. -0.02 min
 Lab File: BF114801.D
 Acq: 4 Jun 2019 19:54

Tgt Ion:264 Resp: 808486

Ion	Ratio	Lower	Upper
264	100		
260	24.3	20.1	30.1
265	21.8	17.7	26.5

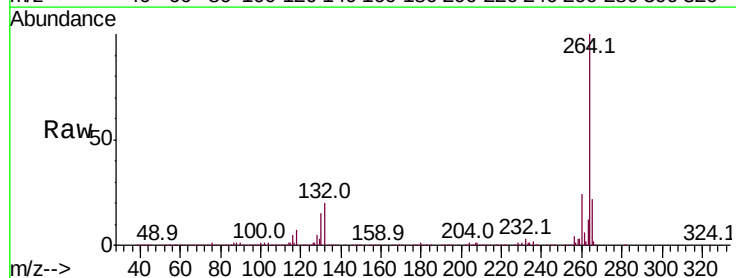

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

