

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133565.D
Acq On : 05 Jun 2023 14:55
Operator : CG\JU
Sample : PB153176BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153176BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	564	568	572	rBV	490837	408879	25.57%	4.036%
2	6.440	737	740	744	rBV	512504	405172	25.34%	4.000%
3	6.828	803	806	810	rBV	1263144	998921	62.47%	9.860%
4	7.387	897	901	904	rBV	321502	233499	14.60%	2.305%
5	8.110	1021	1024	1028	rBV	1501796	1319869	82.54%	13.029%
6	9.187	1204	1207	1210	rBV	732818	535850	33.51%	5.289%
7	9.869	1319	1323	1326	rBV	1876652	1460939	91.36%	14.421%
8	10.651	1453	1456	1463	rBV	329817	258715	16.18%	2.554%
9	11.357	1572	1576	1579	rBV	1982632	1599026	100.00%	15.784%
10	12.939	1842	1845	1849	rBV	658363	568639	35.56%	5.613%
11	13.998	2021	2025	2031	rBV	1425369	1228825	76.85%	12.130%
12	15.457	2266	2273	2284	rBV	923412	1112229	69.56%	10.979%




Sum of corrected areas: 10130563

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133565.D
Acq On : 05 Jun 2023 14:55
Operator : CG\JU
Sample : PB153176BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153176BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

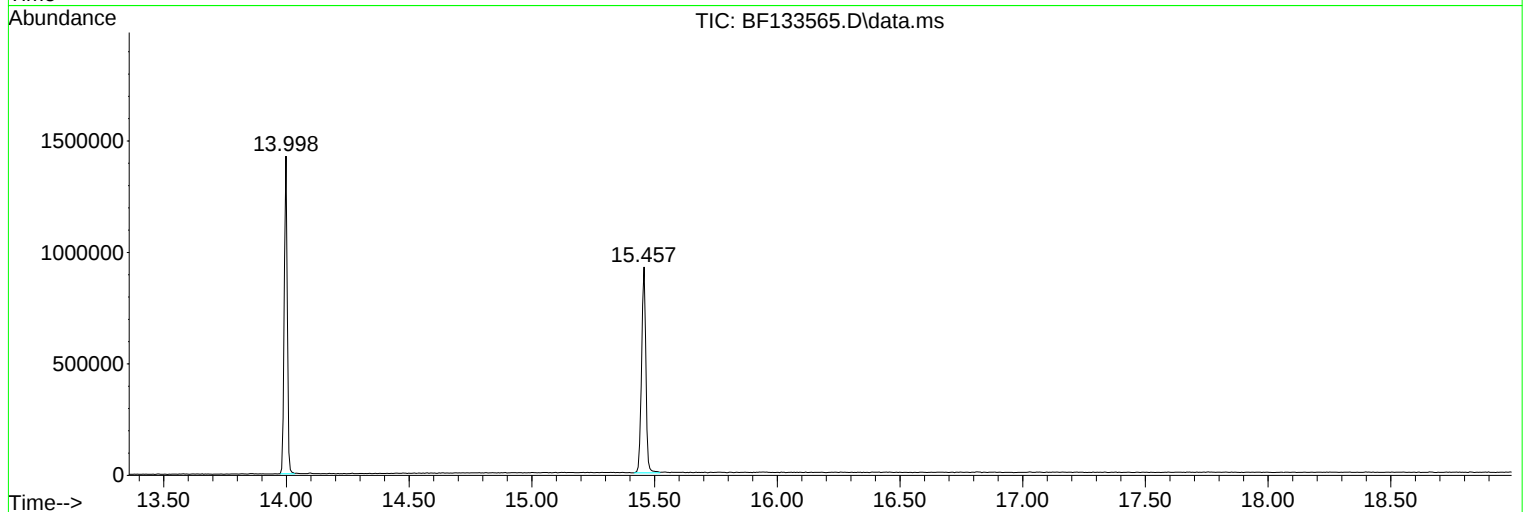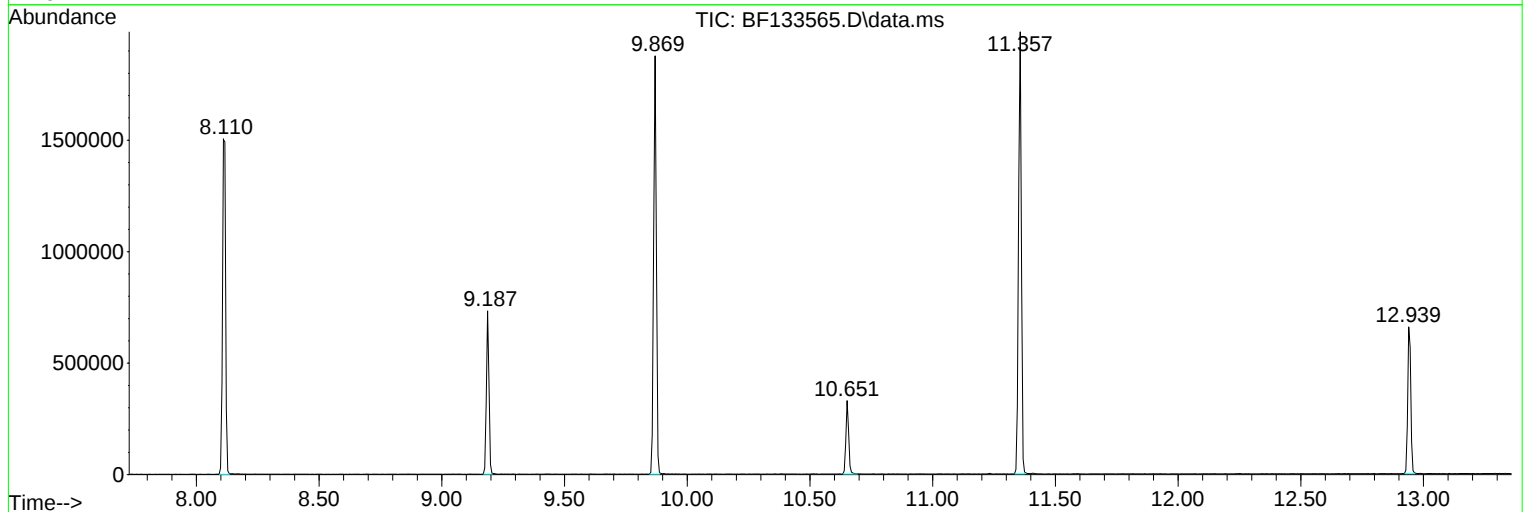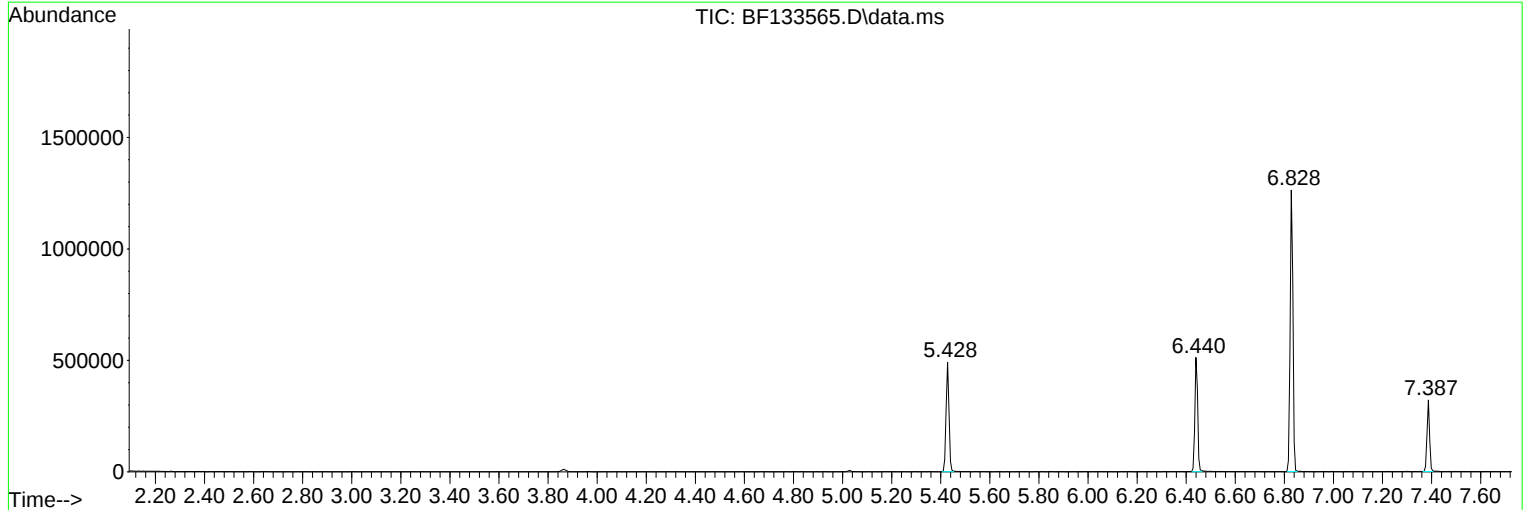

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133565.D
Acq On : 05 Jun 2023 14:55
Operator : CG\JU
Sample : PB153176BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153176BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133565.D
Acq On : 05 Jun 2023 14:55
Operator : CG\JU
Sample : PB153176BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153176BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------