

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060523\  
 Data File : BF133574.D  
 Acq On : 05 Jun 2023 19:41  
 Operator : CG\JU  
 Sample : 02987-01  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 BLAST-WALL-23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133574.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.210       | 17            | 21          | 28           | rVB      | 43490          | 56954         | 1.77%           | 0.275%        |
| 2         | 4.416       | 392           | 396         | 403          | rVB      | 119703         | 134051        | 4.16%           | 0.648%        |
| 3         | 5.045       | 498           | 503         | 511          | rVB      | 269863         | 330253        | 10.26%          | 1.596%        |
| 4         | 5.445       | 566           | 571         | 574          | rBV      | 2812466        | 2711953       | 84.23%          | 13.105%       |
| 5         | 6.457       | 738           | 743         | 746          | rBV      | 2747149        | 2891912       | 89.82%          | 13.975%       |
| 6         | 6.834       | 803           | 807         | 810          | rBV      | 989002         | 765488        | 23.78%          | 3.699%        |
| 7         | 7.398       | 898           | 903         | 906          | rBV      | 1976102        | 1831072       | 56.87%          | 8.848%        |
| 8         | 8.116       | 1021          | 1025        | 1028         | rBV      | 1239314        | 949630        | 29.50%          | 4.589%        |
| 9         | 8.828       | 1143          | 1146        | 1149         | rBV      | 88746          | 66043         | 2.05%           | 0.319%        |
| 10        | 9.192       | 1204          | 1208        | 1211         | rBV      | 3899579        | 3219573       | 100.00%         | 15.558%       |
| 11        | 9.869       | 1320          | 1323        | 1327         | rBV      | 1156972        | 918482        | 28.53%          | 4.438%        |
| 12        | 10.586      | 1441          | 1445        | 1448         | rBV      | 124121         | 107713        | 3.35%           | 0.521%        |
| 13        | 10.657      | 1453          | 1457        | 1460         | rBV      | 1718283        | 1466213       | 45.54%          | 7.085%        |
| 14        | 10.775      | 1472          | 1477        | 1486         | rVB3     | 29198          | 40755         | 1.27%           | 0.197%        |
| 15        | 11.357      | 1572          | 1576        | 1579         | rBV      | 1077477        | 861908        | 26.77%          | 4.165%        |
| 16        | 11.886      | 1663          | 1666        | 1670         | rBV      | 57069          | 59783         | 1.86%           | 0.289%        |
| 17        | 12.951      | 1842          | 1847        | 1850         | rBV      | 3236636        | 2891685       | 89.82%          | 13.974%       |
| 18        | 13.904      | 2003          | 2009        | 2019         | rBV6     | 48093          | 170006        | 5.28%           | 0.822%        |
| 19        | 13.998      | 2021          | 2025        | 2029         | rVB      | 771685         | 680552        | 21.14%          | 3.289%        |
| 20        | 14.857      | 2169          | 2171        | 2176         | rVB      | 44818          | 47741         | 1.48%           | 0.231%        |
| 21        | 15.457      | 2269          | 2273        | 2278         | rBV      | 409263         | 491912        | 15.28%          | 2.377%        |




Sum of corrected areas: 20693679

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060523\  
Data File : BF133574.D  
Acq On : 05 Jun 2023 19:41  
Operator : CG\JU  
Sample : 02987-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
BLAST-WALL-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF052523.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

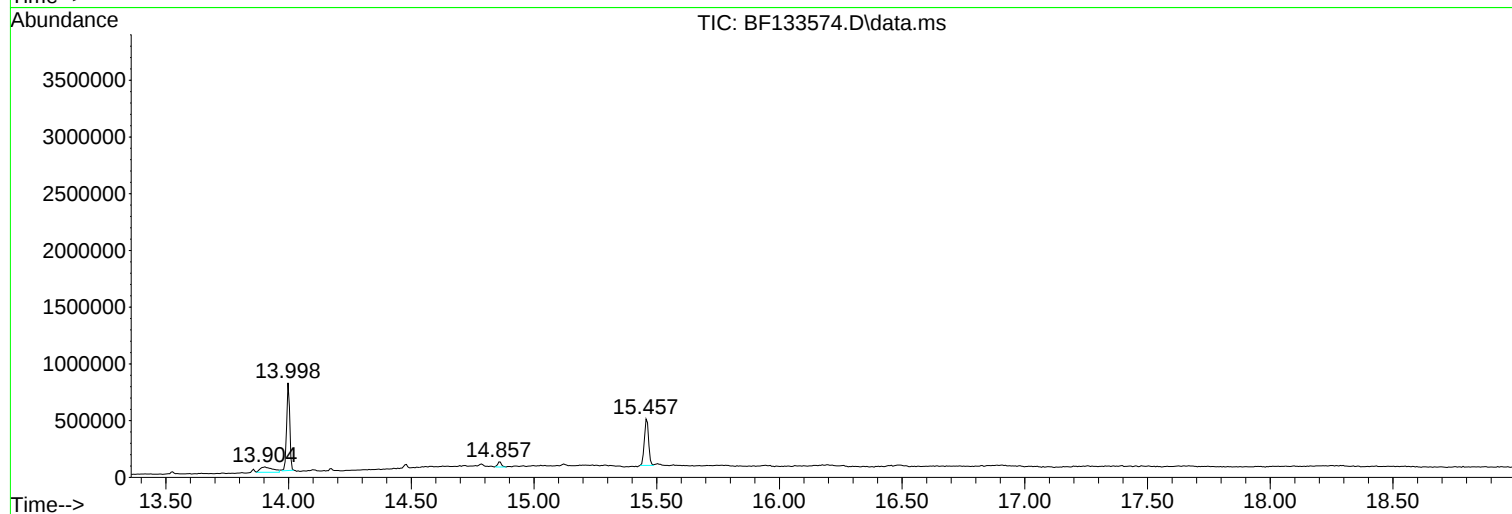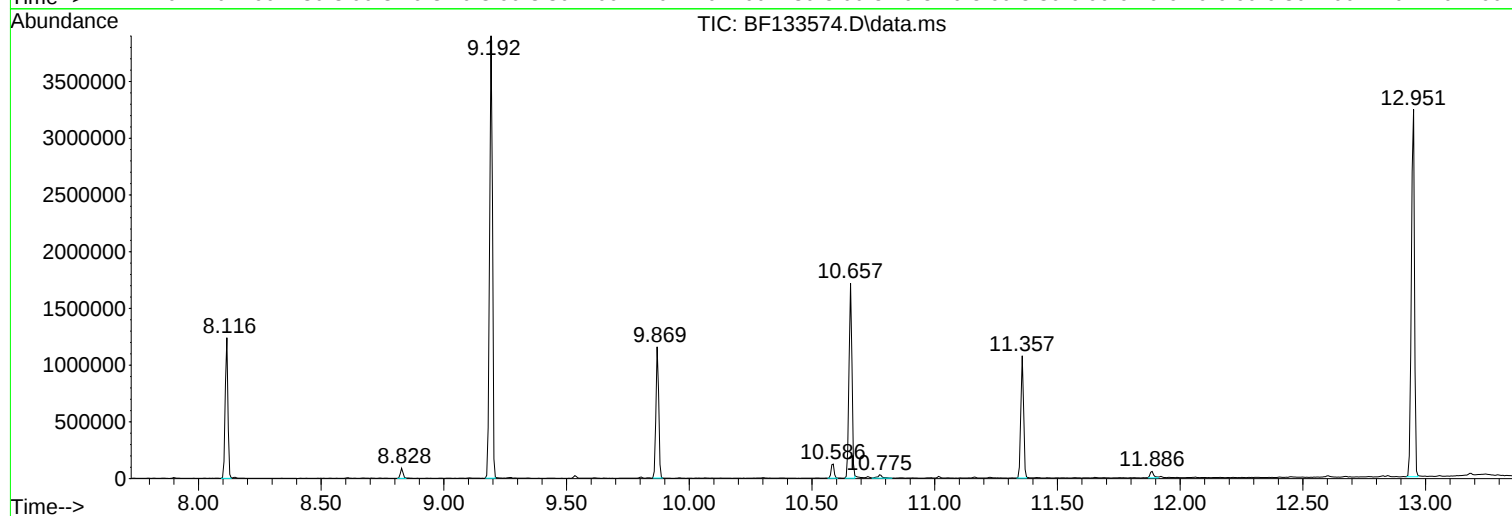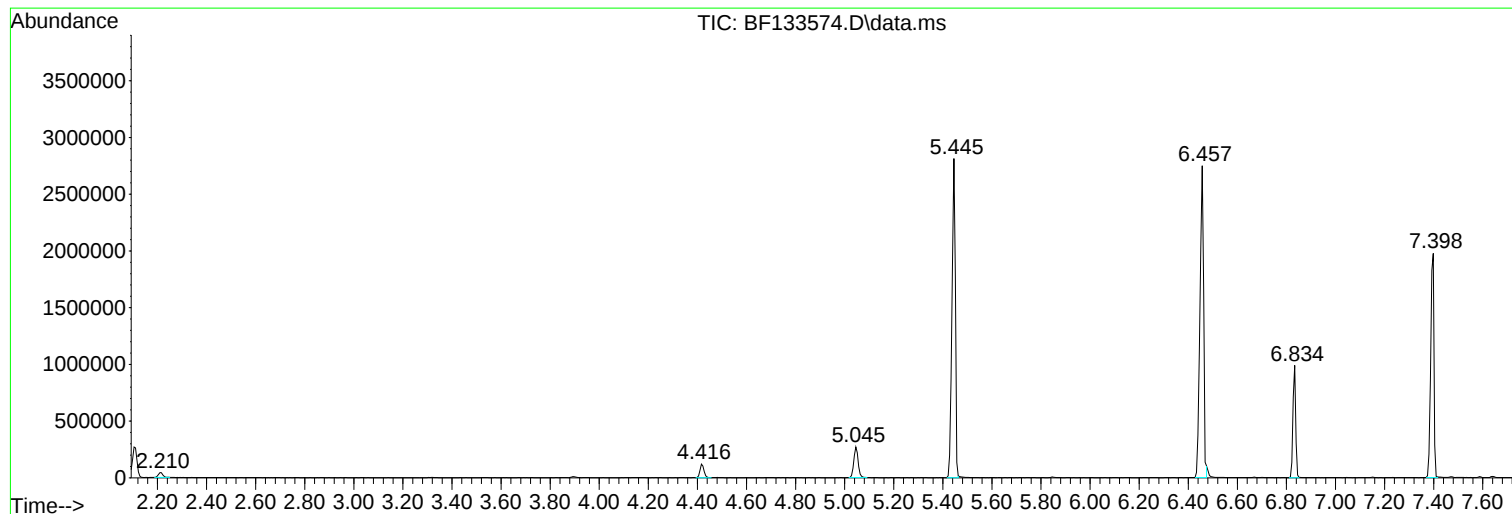

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060523\  
Data File : BF133574.D  
Acq On : 05 Jun 2023 19:41  
Operator : CG\JU  
Sample : 02987-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
BLAST-WALL-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF052523.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060523\  
Data File : BF133574.D  
Acq On : 05 Jun 2023 19:41  
Operator : CG\JU  
Sample : 02987-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
BLAST-WALL-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF052523.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|