

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
 Data File : BF133583.D
 Acq On : 06 Jun 2023 00:23
 Operator : CG\JU
 Sample : 02983-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	8	14	25	rBV2	35190	50225	2.06%	0.273%
2	3.875	299	304	309	rVB	45856	61549	2.53%	0.335%
3	5.040	498	502	508	rBV	94135	104476	4.29%	0.569%
4	5.439	563	570	574	rBV	2241759	2333973	95.92%	12.708%
5	5.675	607	610	614	rBV	60235	54587	2.24%	0.297%
6	6.357	723	726	729	rBV	59635	48807	2.01%	0.266%
7	6.386	729	731	735	rBV	36504	31150	1.28%	0.170%
8	6.457	736	743	746	rBV	2304641	2362319	97.09%	12.862%
9	6.657	774	777	782	rBV2	63786	82046	3.37%	0.447%
10	6.834	803	807	810	rBV	1071574	823505	33.85%	4.484%
11	7.151	857	861	864	rBV	50309	46608	1.92%	0.254%
12	7.369	895	898	899	rBV	36191	29355	1.21%	0.160%
13	7.392	899	902	906	rVV	1467158	1375337	56.53%	7.488%
14	7.428	906	908	913	rVB	35987	30981	1.27%	0.169%
15	8.116	1020	1025	1028	rBV	1316998	1032265	42.43%	5.620%
16	8.710	1123	1126	1129	rBV	35575	32492	1.34%	0.177%
17	8.828	1144	1146	1149	rVB	51122	37853	1.56%	0.206%
18	9.192	1204	1208	1211	rBV	3045320	2433133	100.00%	13.248%
19	9.275	1219	1222	1224	rBV	44748	41872	1.72%	0.228%
20	9.592	1272	1276	1278	rBV4	23507	30173	1.24%	0.164%
21	9.875	1320	1324	1327	rVB	1091769	959456	39.43%	5.224%
22	10.251	1385	1388	1390	rBV	87652	68154	2.80%	0.371%
23	10.527	1433	1435	1438	rVB	41592	32016	1.32%	0.174%
24	10.586	1442	1445	1448	rBV	184334	141186	5.80%	0.769%
25	10.663	1454	1458	1461	rBV	1393081	1335430	54.89%	7.271%
26	10.780	1476	1478	1487	rVB3	45263	75026	3.08%	0.408%
27	11.363	1573	1577	1580	rBV	1053018	939724	38.62%	5.117%
28	11.657	1625	1627	1631	rBV	37781	34292	1.41%	0.187%
29	11.886	1663	1666	1670	rBV	248723	249076	10.24%	1.356%
30	12.574	1781	1783	1786	rVB	76659	55015	2.26%	0.300%
31	12.804	1820	1822	1824	rVB	64096	42616	1.75%	0.232%
32	12.951	1843	1847	1850	rBV	2388634	2030407	83.45%	11.055%
33	13.857	1999	2001	2004	rBV	72526	52371	2.15%	0.285%
34	14.004	2022	2026	2029	rBV	754923	648064	26.63%	3.529%
35	14.480	2105	2107	2109	rVB	85869	60625	2.49%	0.330%
36	15.127	2214	2217	2220	rBV	142938	150053	6.17%	0.817%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133583.D
Acq On : 06 Jun 2023 00:23
Operator : CG\JU
Sample : 02983-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC18

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.468	2271	2275	2279	rVB	386800	450030	18.50%	2.450%
----	--------	------	------	------	-----	--------	--------	--------	--------




Sum of corrected areas: 18366247

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133583.D
Acq On : 06 Jun 2023 00:23
Operator : CG\JU
Sample : 02983-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

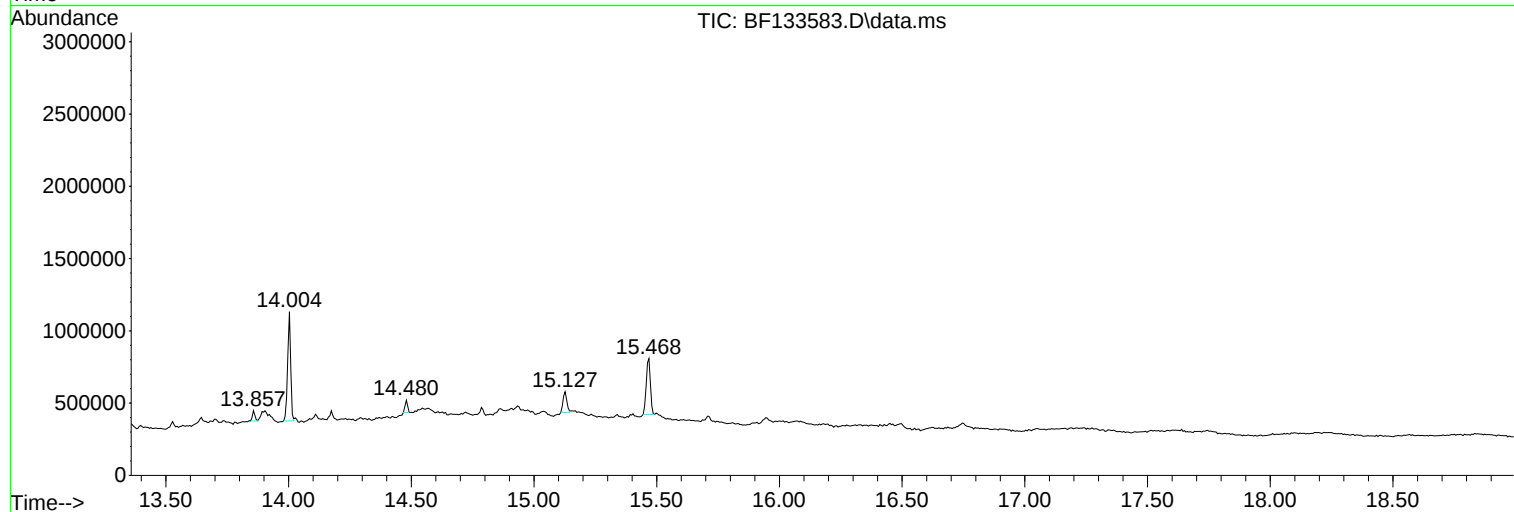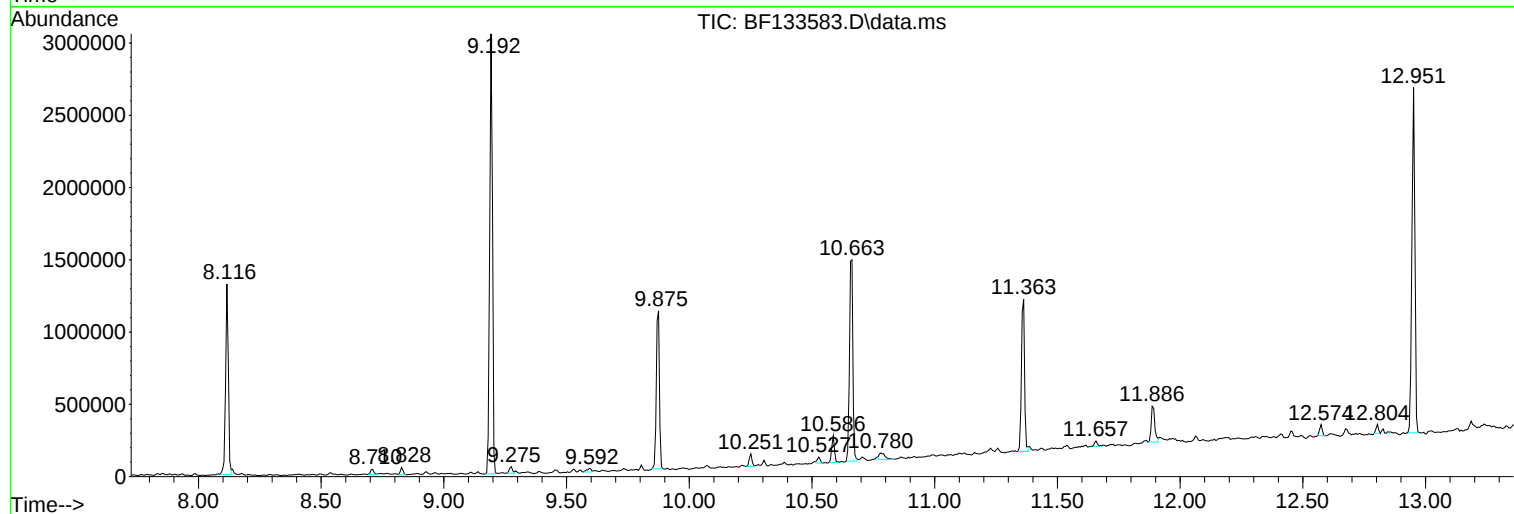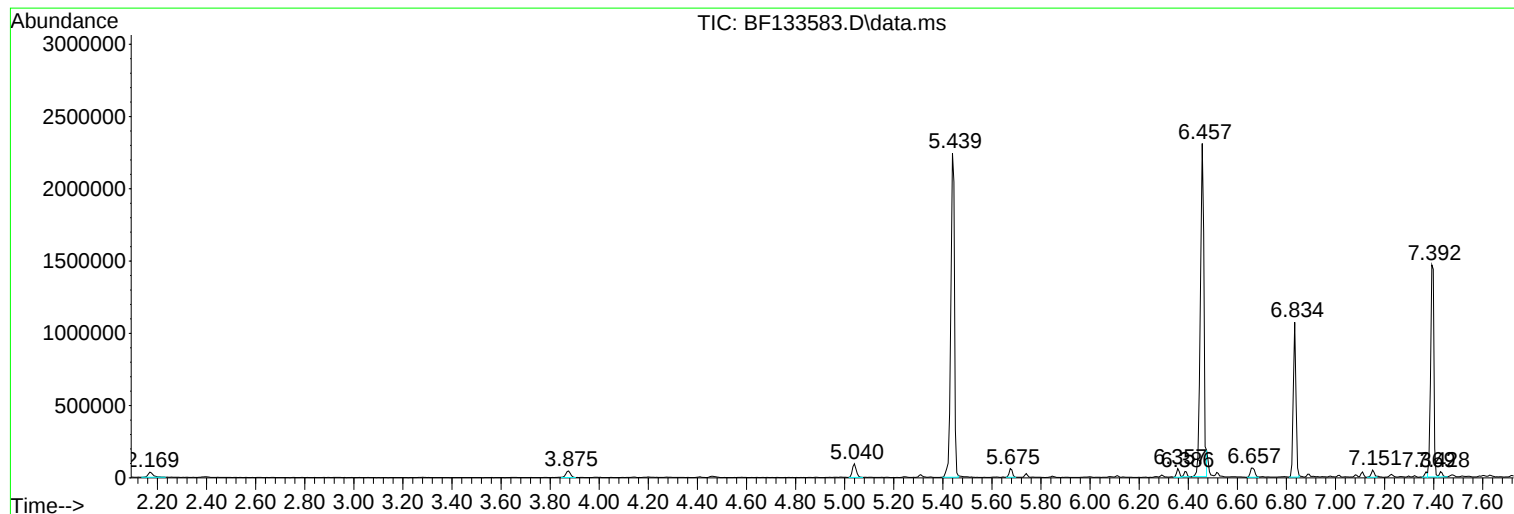

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133583.D
Acq On : 06 Jun 2023 00:23
Operator : CG\JU
Sample : 02983-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133583.D
Acq On : 06 Jun 2023 00:23
Operator : CG\JU
Sample : 02983-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------