


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133563.D
Acq On : 05 Jun 2023 12:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 05 17:49:53 2023

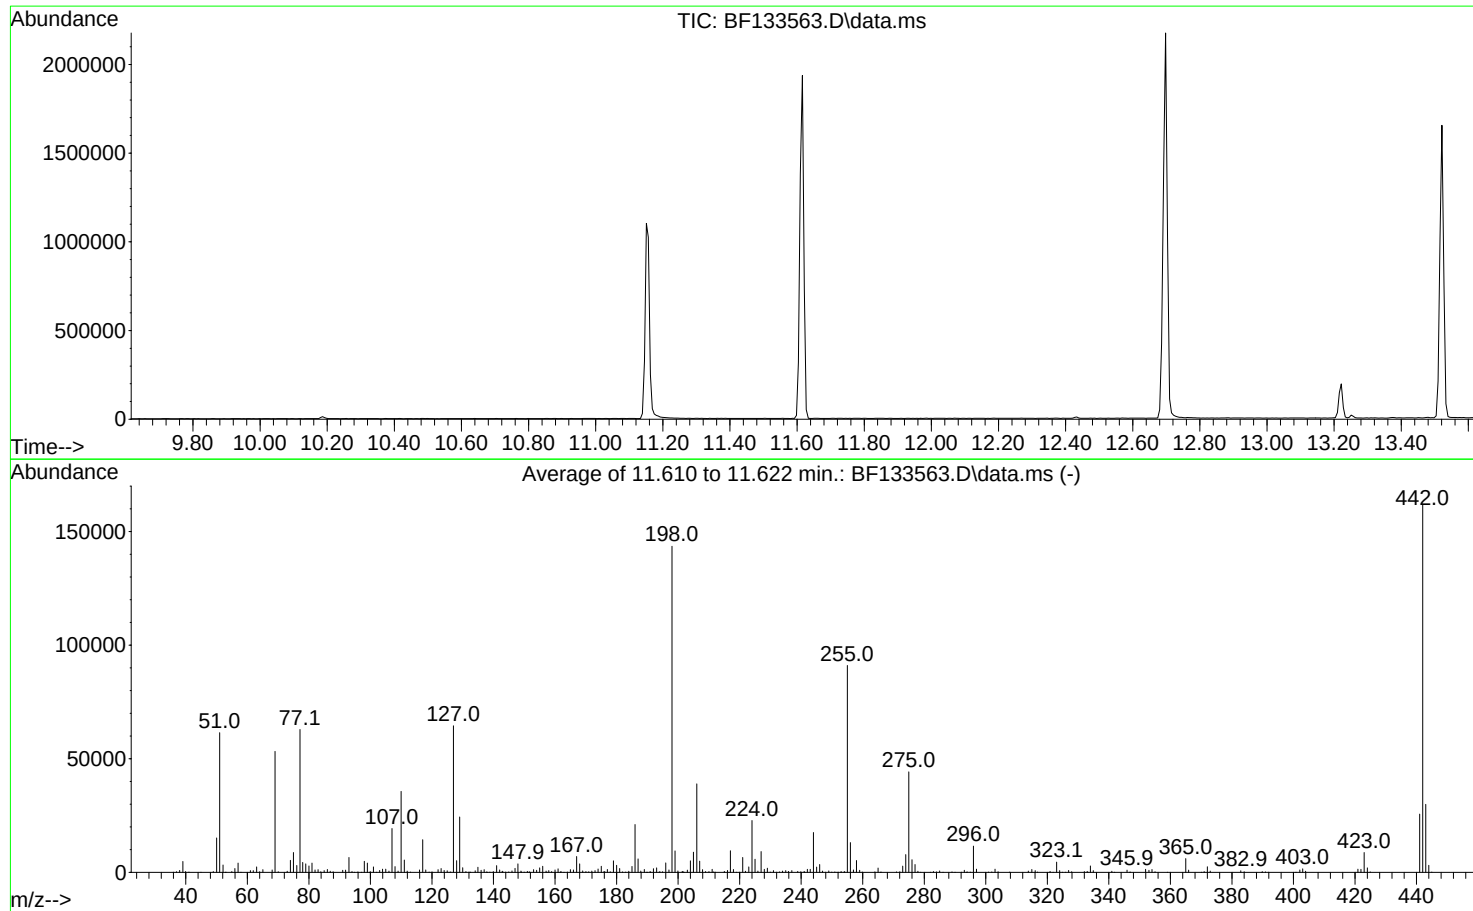

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	61517	PASS
68	69	0.00	2	1.9	1027	PASS
69	198	0.00	100	37.1	53269	PASS
70	69	0.00	2	0.6	319	PASS
127	198	10	80	45.0	64552	PASS
197	198	0.00	2	0.7	1028	PASS
198	198	100	100	100.0	143565	PASS
199	198	5	9	6.6	9479	PASS
275	198	10	60	30.8	44264	PASS
365	198	1	100	4.2	6078	PASS
441	198	0.01	100	17.9	25665	PASS
442	442	50	100	100.0	161941	PASS
443	442	15	24	18.5	29928	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/5/2023	BNA_F	<u>BF133563.D</u>
Compound Name	Response	Retention Time
DDT	256206	13.521
DDD	33706	13.221
DDE	306	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34012	290218	11.72

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133563.D
Acq On : 05 Jun 2023 12:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 05 12:43:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:05:55 2023
Response via : Initial Calibration

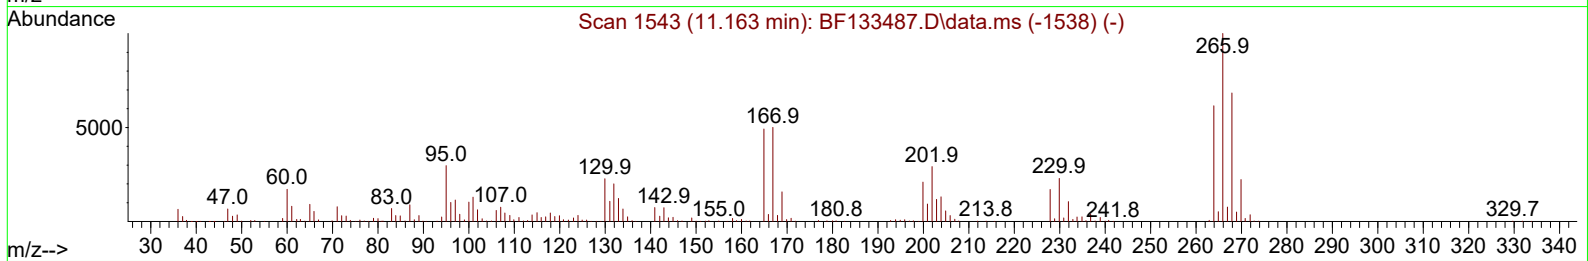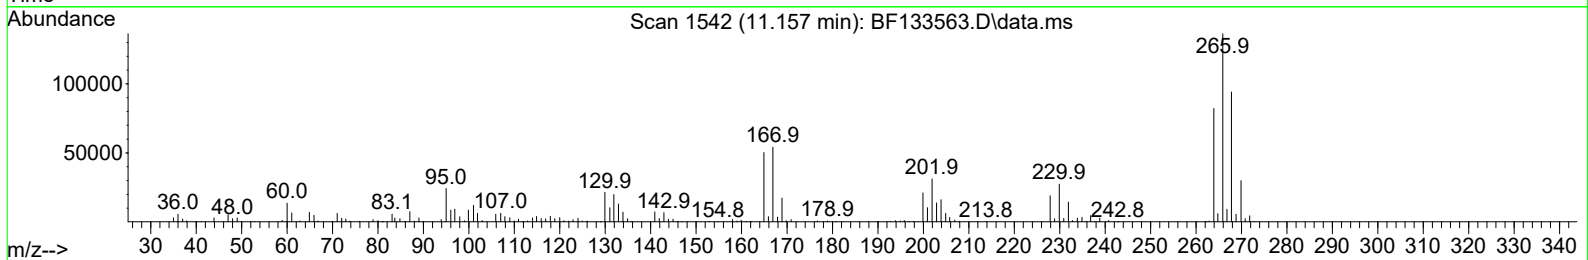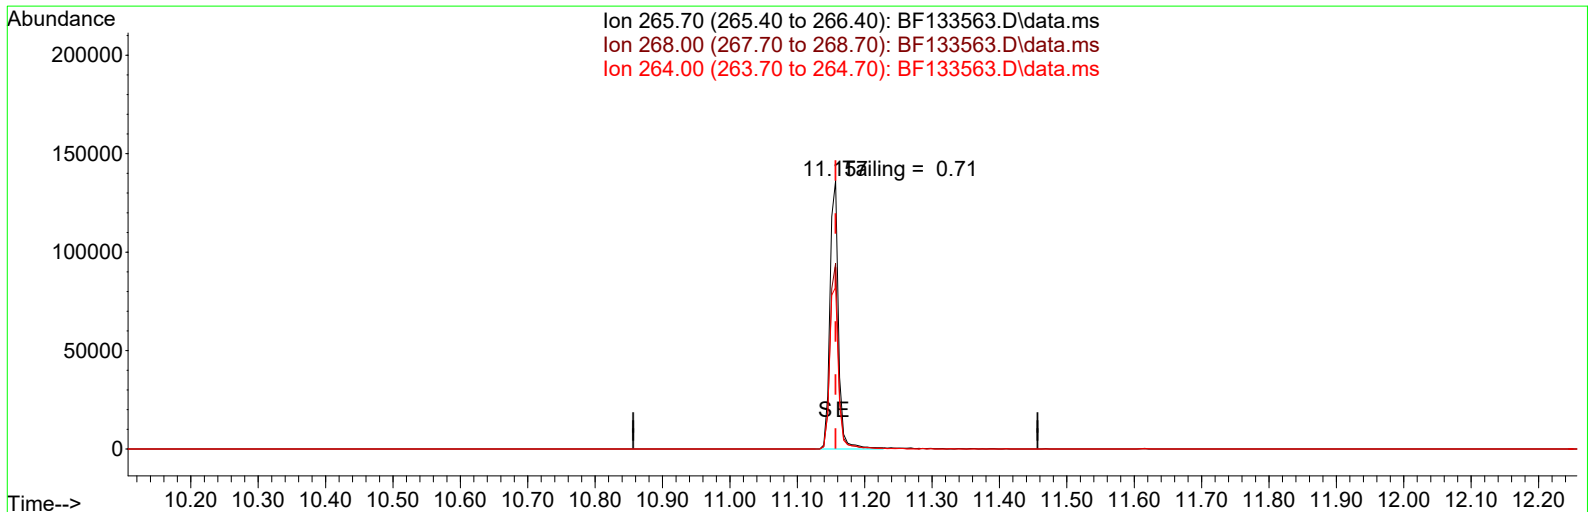

TIC: BF133563.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.000) 26717.10 ng




response 120997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	69.10
264.00	61.50	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060523\
Data File : BF133563.D
Acq On : 05 Jun 2023 12:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 05 12:43:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:05:55 2023
Response via : Initial Calibration

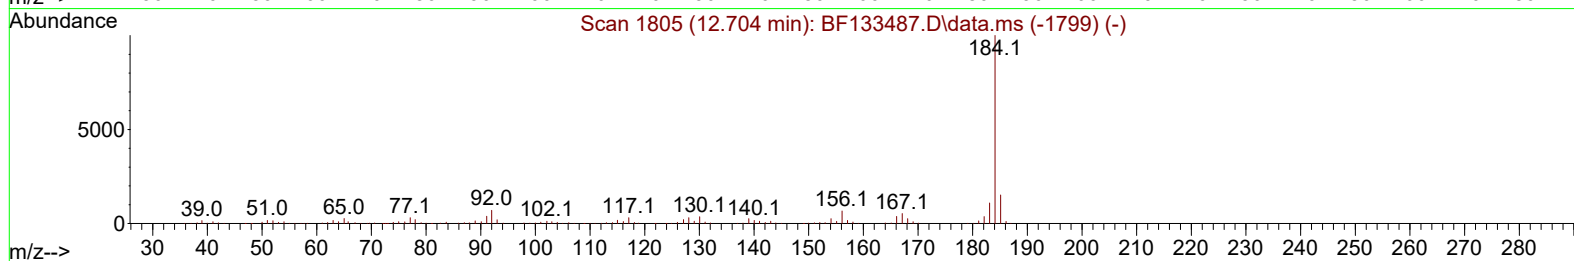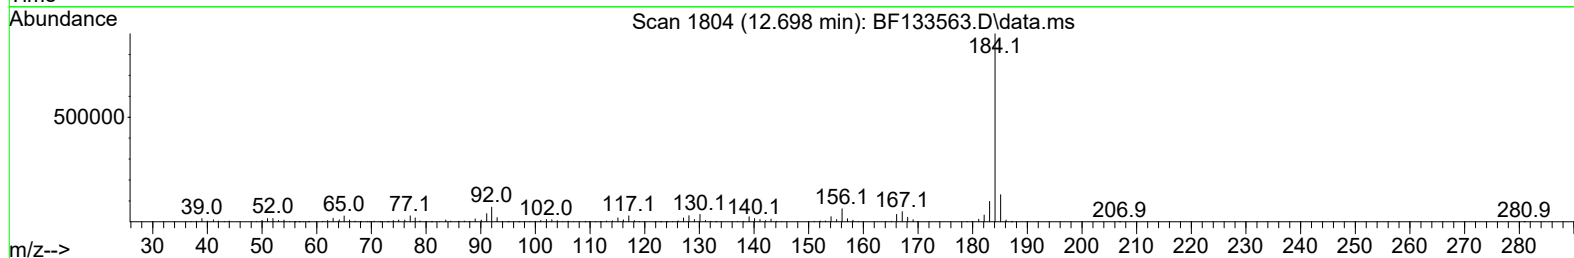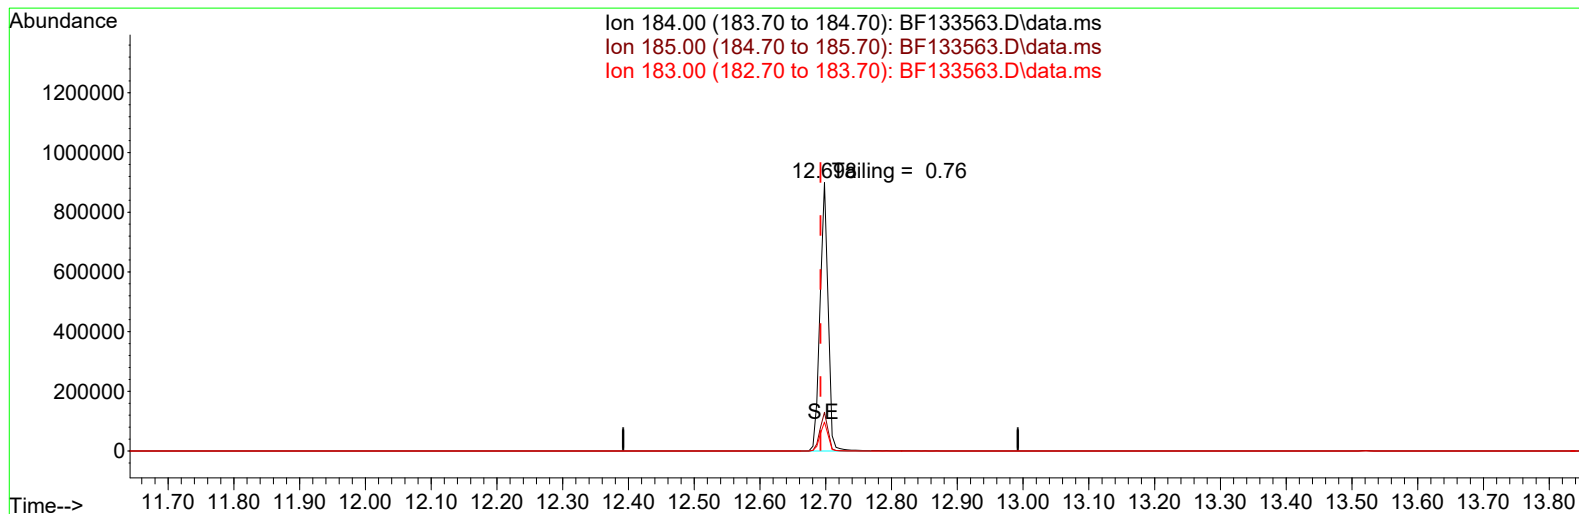

TIC: BF133563.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 778086

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.42
183.00	10.90	10.81
0.00	0.00	0.00