

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060616\
 Data File : BF087755.D
 Acq On : 6 Jun 2016 16:44
 Operator : UM/SJ
 Sample : H3267-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 STA-TA-1261+50(0-4)

Quant Time: Jun 07 01:13:55 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	131866	20.00	ng	-0.01
21) Naphthalene-d8	8.14	136	519166	20.00	ng	-0.01
38) Acenaphthene-d10	9.88	164	211779	20.00	ng	-0.02
63) Phenanthrene-d10	11.37	188	354347	20.00	ng	-0.01
75) Chrysene-d12	14.01	240	255946	20.00	ng	-0.01
86) Perylene-d12	15.43	264	228488	20.00	ng	-0.01

System Monitoring Compounds

5) 2-Fluorophenol	5.46	112	1035984	126.98	ng	0.01
7) Phenol-d6	6.49	99	1116264	109.10	ng	0.00
23) Nitrobenzene-d5	7.42	82	667576	74.40	ng	-0.01
41) 2,4,6-Tribromophenol	10.67	330	241086	113.41	ng	-0.01
44) 2-Fluorobiphenyl	9.22	172	1268524	95.97	ng	-0.01
78) Terphenyl-d14	12.96	244	792138	75.52	ng	-0.01

Target Compounds


						Qvalue
19) n-Nitroso-di-n-propylamine	7.42	70	90235	14.12	ng	# 74
48) Acenaphthylene	9.75	152	149922	7.03	ng	99
49) Dimethylphthalate	9.61	163	193613	12.58	ng	98
64) 4,6-Dinitro-2-methylphenol	10.67	198	320	2.17	ng	# 1
66) 4-Bromophenyl-phenylether	10.67	248	13528	3.85	ng	# 1
70) Phenanthrene	11.39	178	138912	7.23	ng	98
71) Anthracene	11.44	178	116132	6.03	ng	99
72) Carbazole	11.60	167	49901	2.74	ng	98
74) Fluoranthene	12.58	202	784257	41.48	ng	99
77) Pyrene	12.81	202	820022	44.99	ng	99
80) Benzo(a)anthracene	14.03	228	423823	28.69	ng	96
82) Chrysene	14.03	228	423930	28.83	ng	98
83) Bis(2-ethylhexyl)phthalate	14.00	149	38435	4.16	ng	# 97
85) Indeno(1,2,3-cd)pyrene	16.82	276	207396	17.07	ng	# 100
87) Benzo(b)fluoranthene	15.03	252	792648	53.33	ng	# 94
88) Benzo(k)fluoranthene	15.03	252	792648	64.10	ng	99
89) Benzo(a)pyrene	15.37	252	309951	24.81	ng	97
90) Dibenzo(a,h)anthracene	16.83	278	52134	4.90	ng	96
91) Benzo(g,h,i)perylene	17.23	276	174963	16.31	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060616\
Data File : BF087755.D
Acq On : 6 Jun 2016 16:44
Operator : UM/SJ
Sample : H3267-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STA-TA-1261+50(0-4)

Quant Time: Jun 07 01:13:55 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

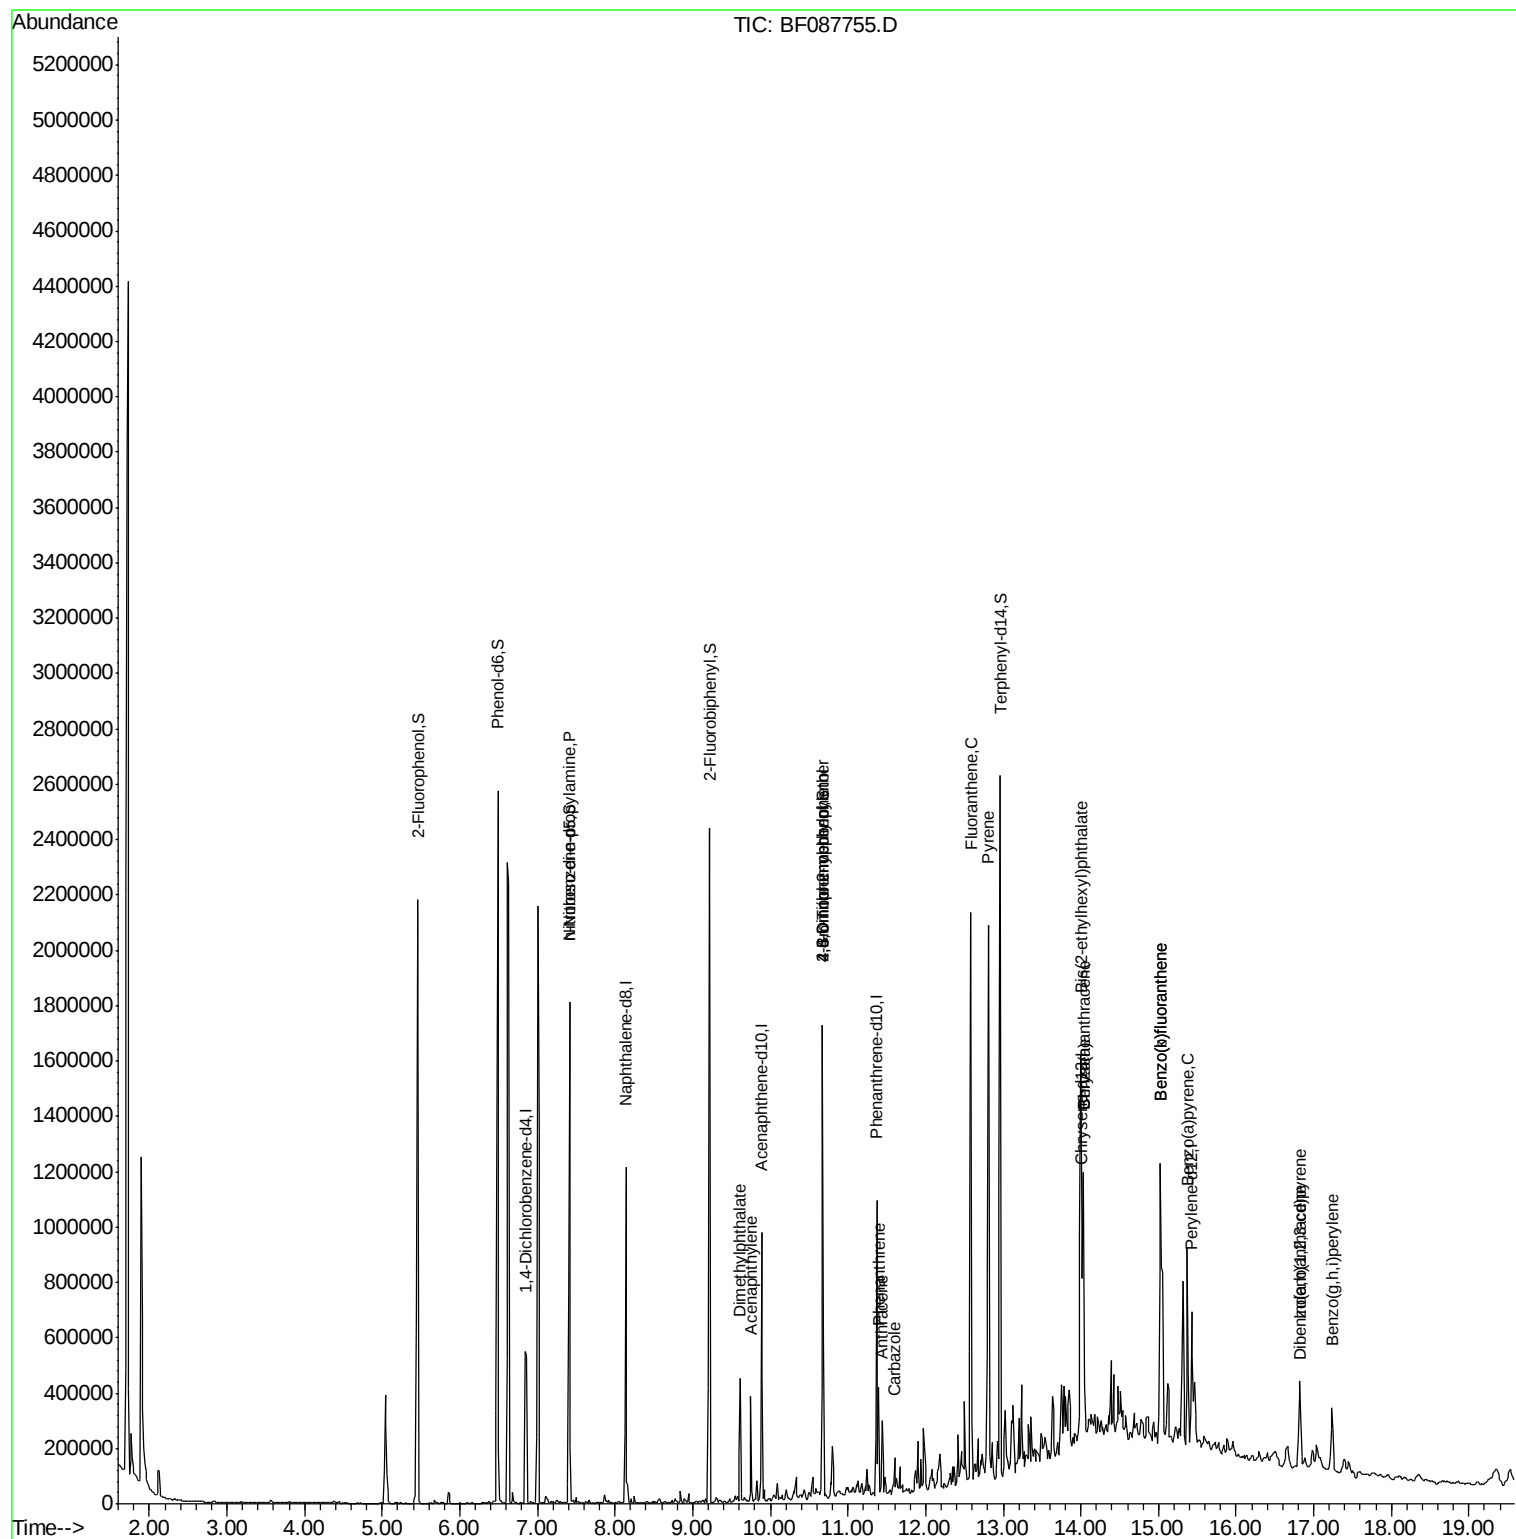

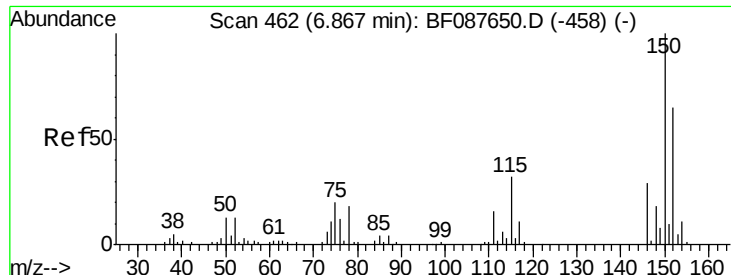


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.86 min Scan# 461
Delta R.T. -0.01 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Instrument :
BNA_F
ClientSampleId :
STA-TA-1261+50(0-4)

Tgt Ion:152 Resp: 131866
Ion Ratio Lower Upper
152 100
150 149.1 123.8 185.6
115 48.2 39.6 59.4

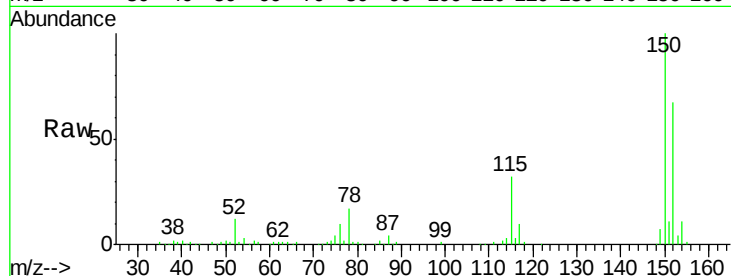


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

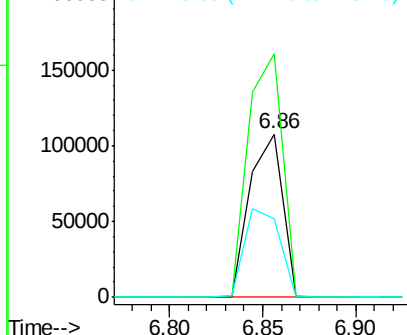



#5


2-Fluorophenol
Concen: 126.98 ng
RT: 5.46 min Scan# 339
Delta R.T. 0.01 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Tgt Ion:112 Resp: 1035984
Ion Ratio Lower Upper
112 100
64 47.7 42.2 63.2
63 24.5 21.8 32.8



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

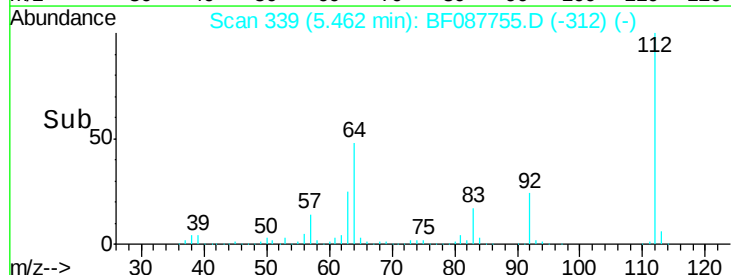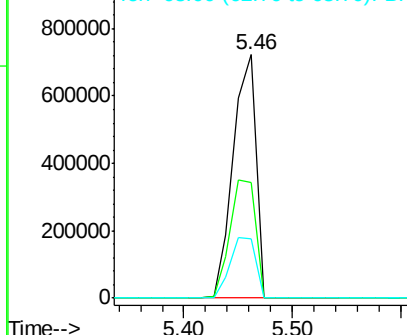

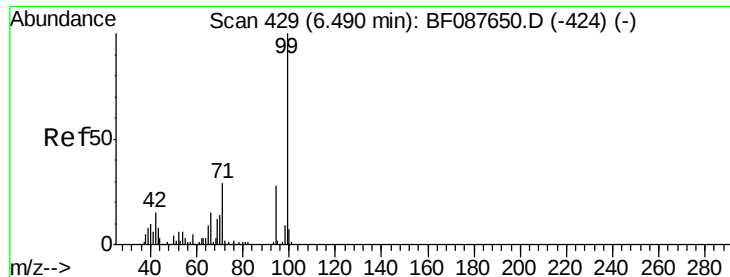

#7

Phenol-d6

Concen: 109.10 ng

RT: 6.49 min Scan# 429

Delta R.T. 0.00 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)





Tgt Ion: 99 Resp: 1116264

Ion Ratio Lower Upper

99 100

42 17.9 12.2 18.2

71 35.2 23.4 35.0#

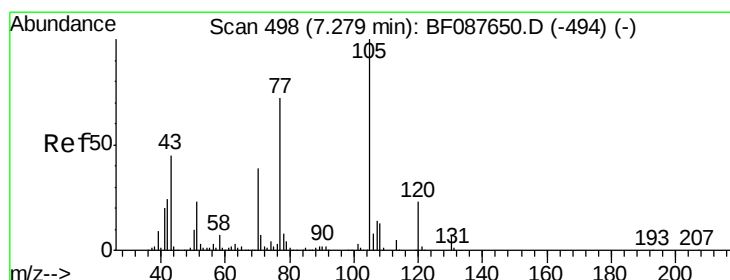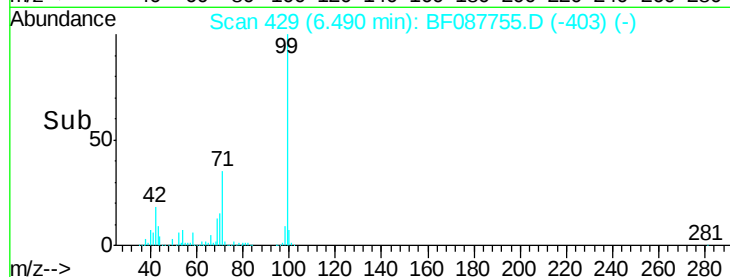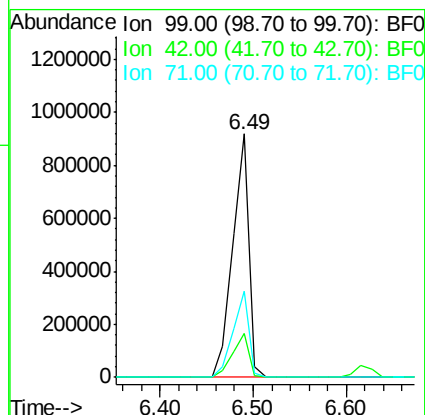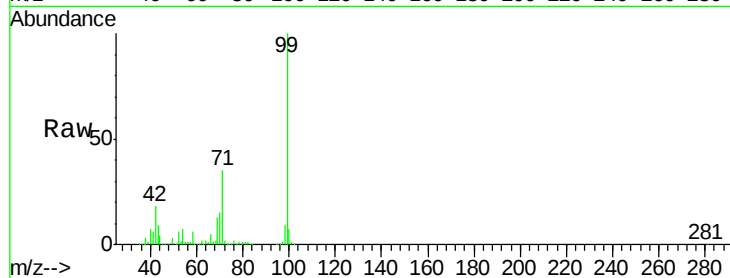

#19

n-Nitroso-di-n-propylamine

Concen: 14.12 ng

RT: 7.42 min Scan# 510

Delta R.T. 0.14 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Tgt Ion: 70 Resp: 90235




Ion Ratio Lower Upper


70 100

42 44.8 49.6 74.4#

101 0.0 7.1 10.7#

130 2.5 15.4 23.2#

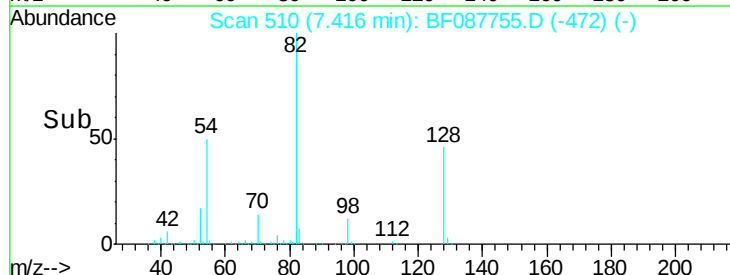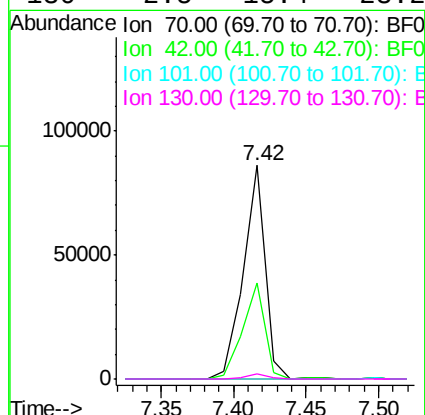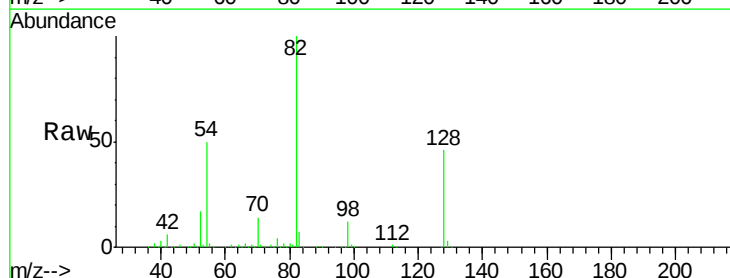



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 573

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)

Tgt Ion:136 Resp: 519166


Ion Ratio Lower Upper

136 100

137 11.1 9.1 13.7

54 7.2 6.6 10.0

68 5.7 5.1 7.7



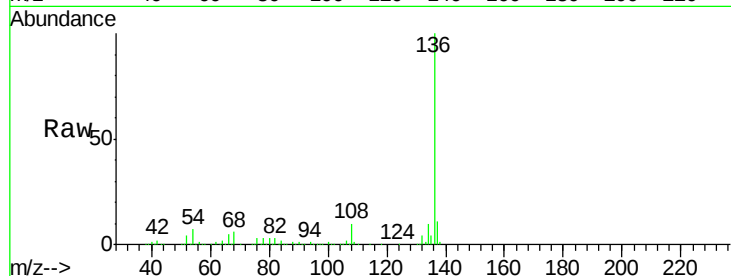


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

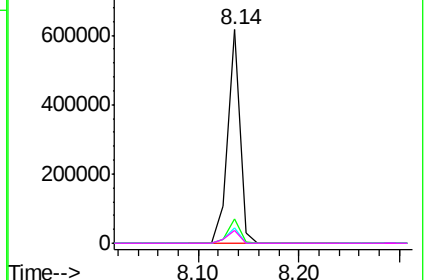

#23

Nitrobenzene-d5

Concen: 74.40 ng

RT: 7.42 min Scan# 510

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44


Tgt Ion: 82 Resp: 667576

Ion Ratio Lower Upper

82 100

128 46.5 35.9 53.9



54 50.2 40.9 61.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

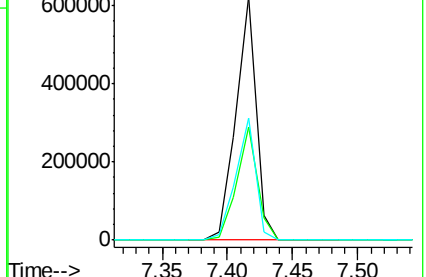


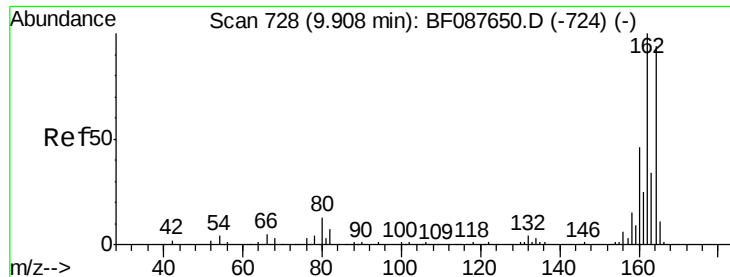




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.88 min Scan# 726
 Delta R.T. -0.02 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Instrument :
 BNA_F
 ClientSampleId :
 STA-TA-1261+50(0-4)

Tgt Ion:164 Resp: 211779
 Ion Ratio Lower Upper
 164 100
 162 104.2 85.4 128.2
 160 46.2 39.5 59.3

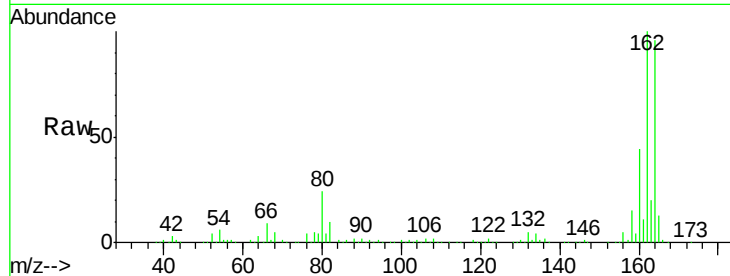


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

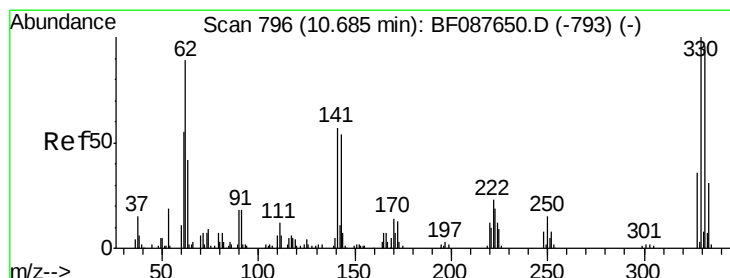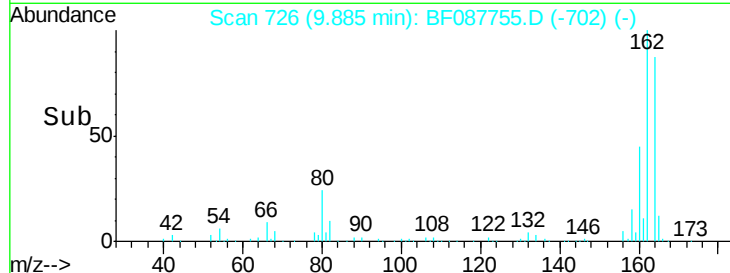
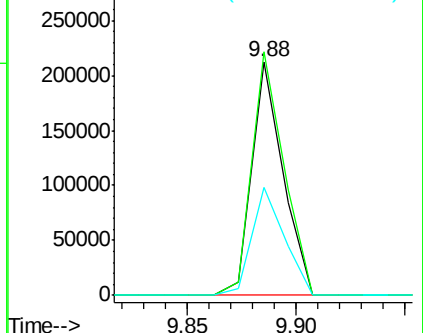



#41
 2,4,6-Tribromophenol
 Concen: 113.41 ng
 RT: 10.67 min Scan# 795
 Delta R.T. -0.01 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Tgt Ion:330 Resp: 241086
 Ion Ratio Lower Upper
 330 100
 332 97.6 0.0 0.0#
 141 33.8 0.0 0.0#

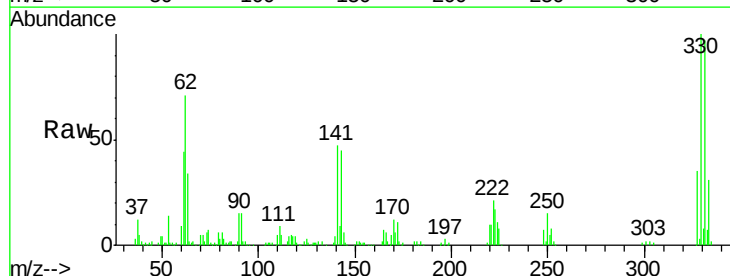

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



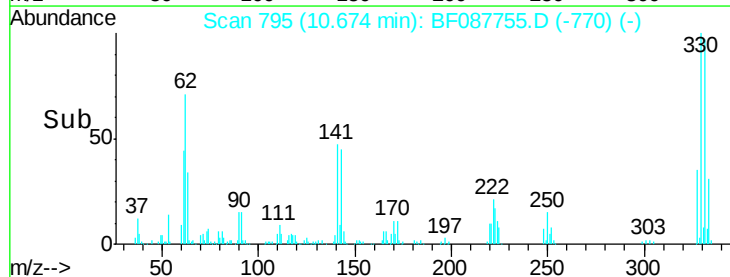
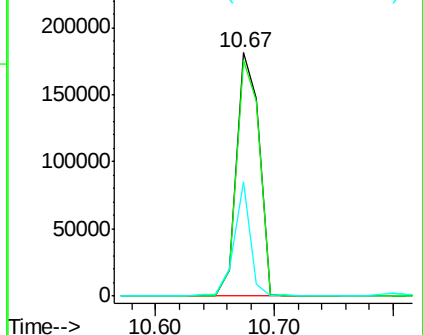


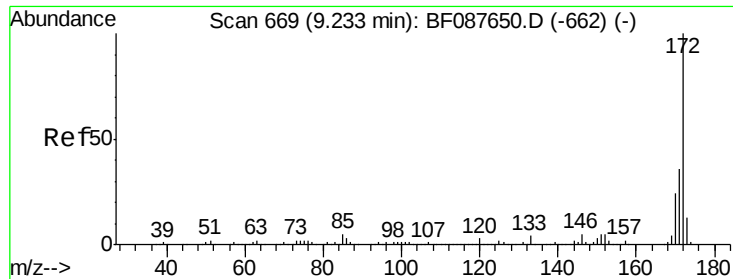

#44
 2-Fluorobiphenyl
 Concen: 95.97 ng
 RT: 9.22 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44




Instrument :
 BNA_F
 ClientSampleId :
 STA-TA-1261+50(0-4)


Tgt Ion:172 Resp: 1268524
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.6 43.0
 170 24.1 19.2 28.8

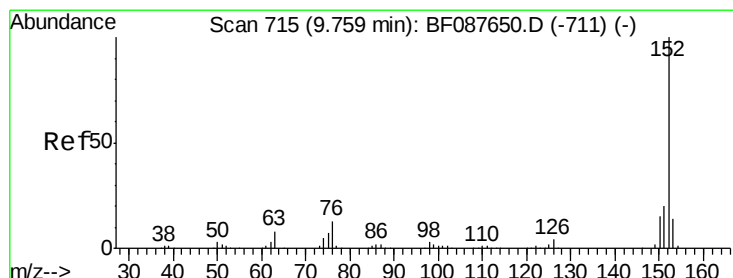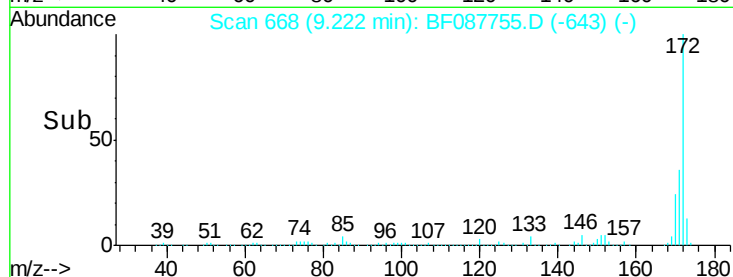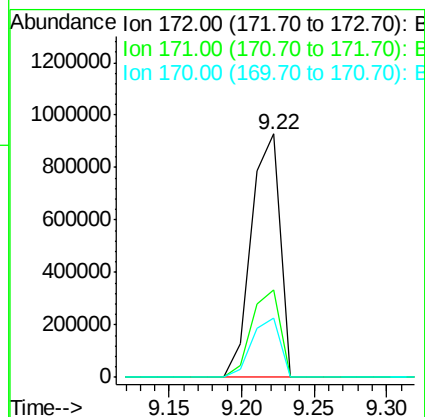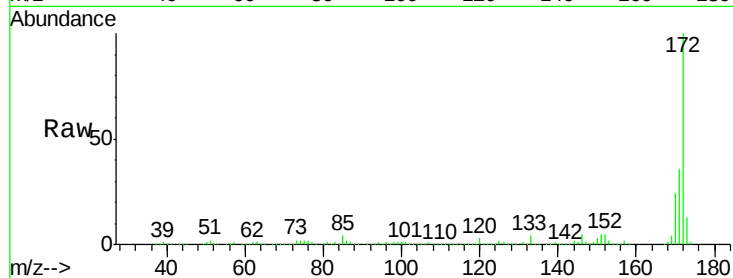

#48
 Acenaphthylene
 Concen: 7.03 ng
 RT: 9.75 min Scan# 714
 Delta R.T. -0.01 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Tgt Ion:152 Resp: 149922
 Ion Ratio Lower Upper
 152 100
 151 20.1 16.2 24.4
 153 13.2 11.0 16.6

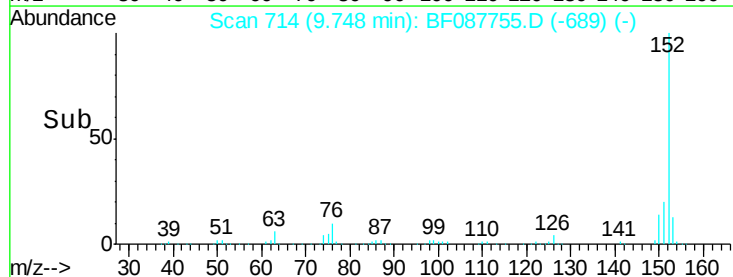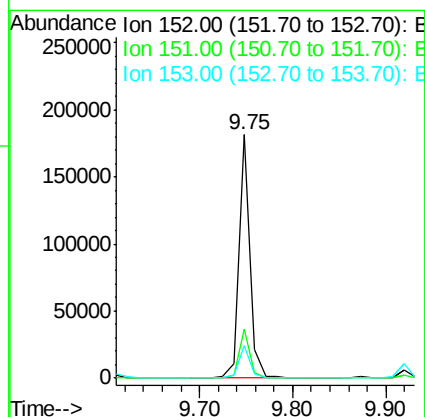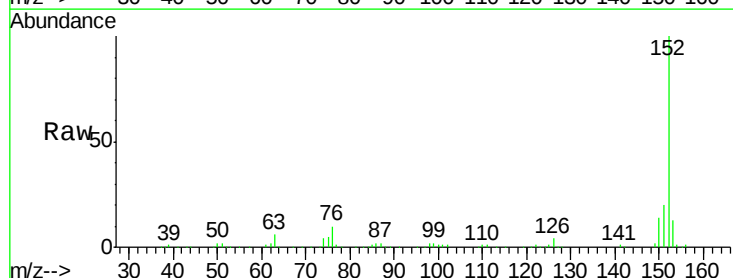


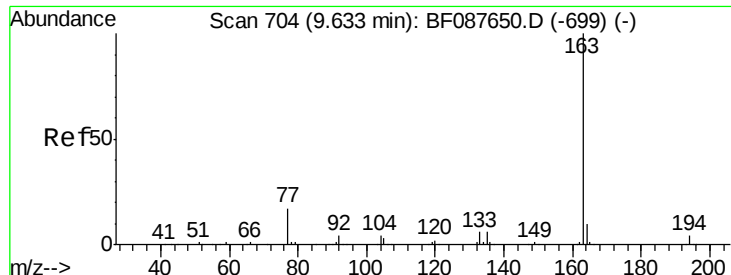




#49
Dimethylphthalate
Concen: 12.58 ng
RT: 9.61 min Scan# 702
Delta R.T. -0.02 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Instrument :
BNA_F
ClientSampleId :
STA-TA-1261+50(0-4)

Tgt Ion:163 Resp: 193613
Ion Ratio Lower Upper
163 100
194 3.6 2.8 4.2
164 9.6 8.3 12.5

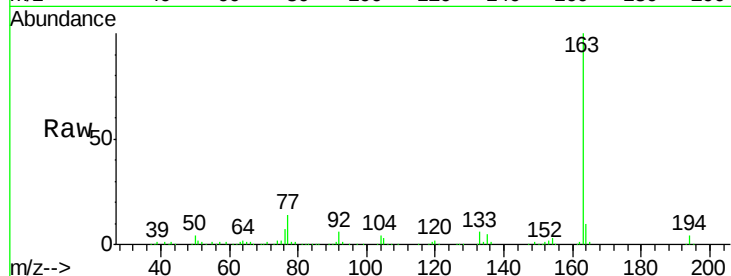


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

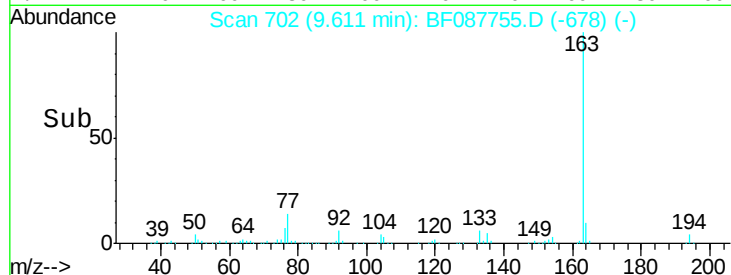
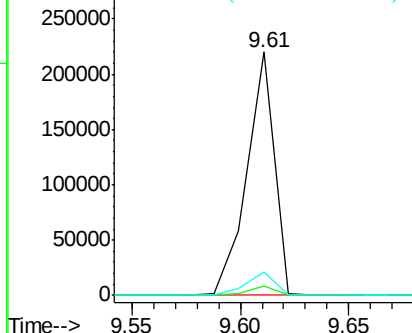



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.37 min Scan# 856
Delta R.T. -0.01 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Tgt Ion:188 Resp: 354347
Ion Ratio Lower Upper
188 100
94 9.5 9.0 13.6
80 10.0 10.0 15.0#

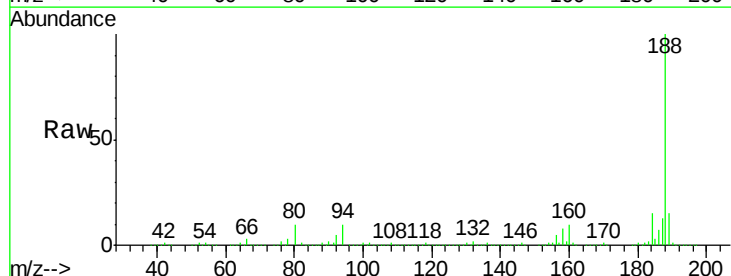

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

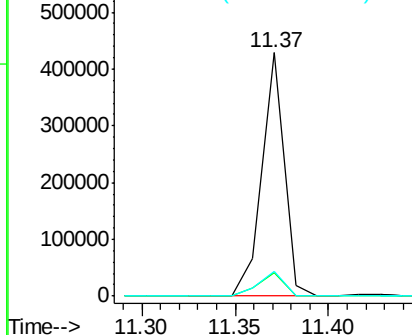


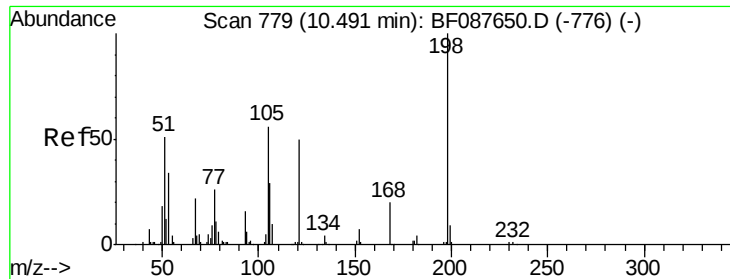




#64
 4,6-Dinitro-2-methylphenol
 Concen: 2.17 ng
 RT: 10.67 min Scan# 795
 Delta R.T. 0.18 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Instrument :
 BNA_F
 ClientSampleId :
 STA-TA-1261+50(0-4)

Tgt Ion:198 Resp: 320
 Ion Ratio Lower Upper
 198 100
 51 298.5 39.6 79.6#
 105 291.0 36.6 76.6#

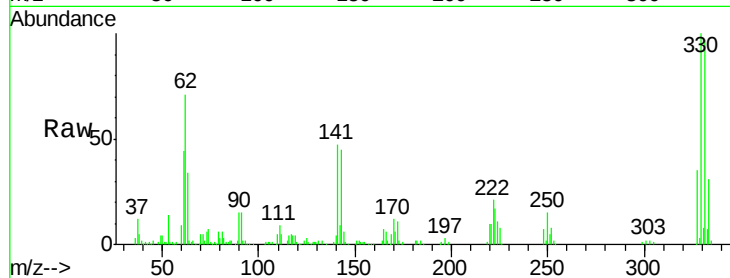


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF0
 Ion 105.00 (104.70 to 105.70): E

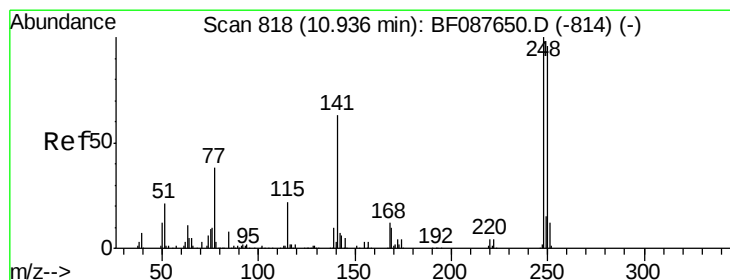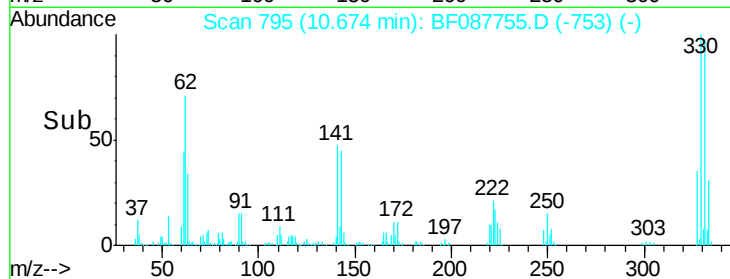
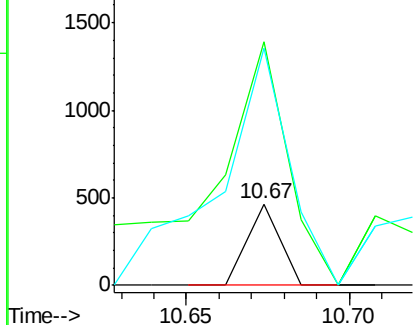



#66
 4-Bromophenyl-phenylether
 Concen: 3.85 ng
 RT: 10.67 min Scan# 795
 Delta R.T. -0.26 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Tgt Ion:248 Resp: 13528
 Ion Ratio Lower Upper
 248 100
 250 198.9 77.1 115.7#
 141 643.4 50.6 76.0#

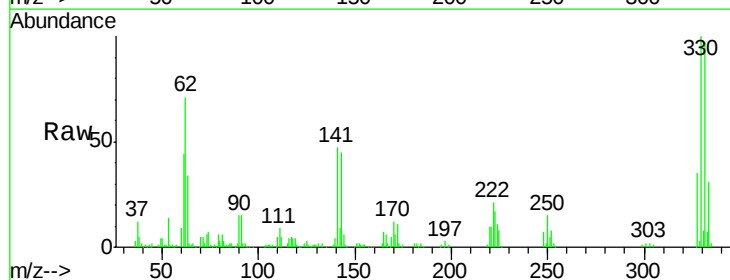

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

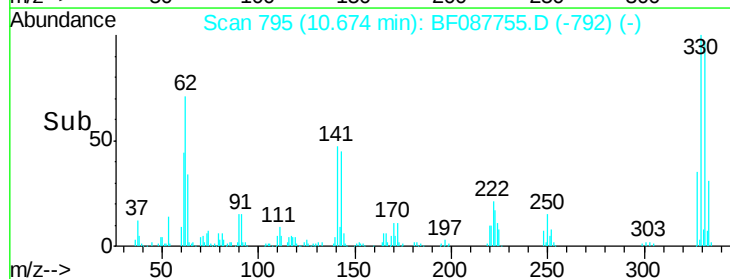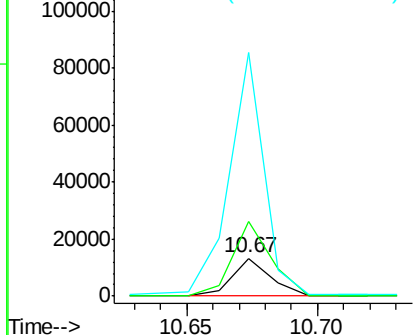







#70
Phenanthrene
Concen: 7.23 ng
RT: 11.39 min Scan# 858
Delta R.T. -0.01 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Instrument :
BNA_F
ClientSampleId :
STA-TA-1261+50(0-4)

Tgt Ion:178 Resp: 138912
Ion Ratio Lower Upper
178 100
176 18.4 15.8 23.6
179 15.4 13.0 19.4




Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

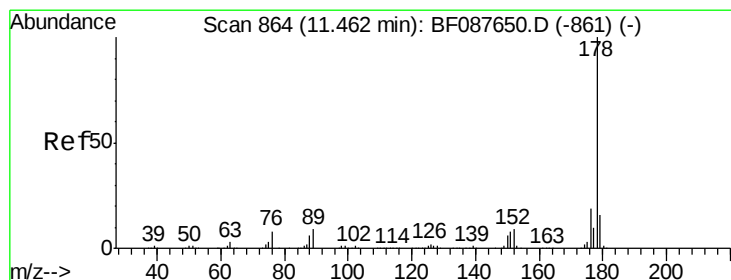
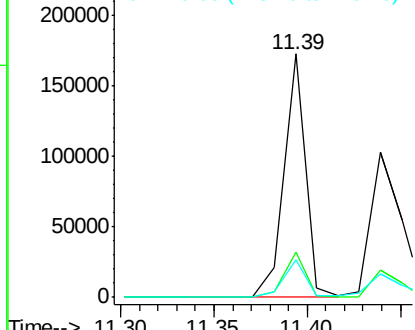



#71
Anthracene
Concen: 6.03 ng
RT: 11.44 min Scan# 862
Delta R.T. -0.02 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Tgt Ion:178 Resp: 116132
Ion Ratio Lower Upper
178 100
176 18.6 15.6 23.4
179 16.3 12.8 19.2



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

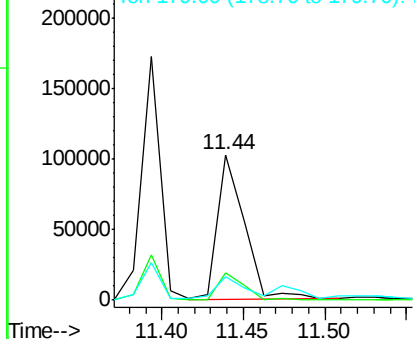



#72

Carbazole

Concen: 2.74 ng

RT: 11.60 min Scan# 876

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)


Tgt Ion:167 Resp: 49901

Ion Ratio Lower Upper

167 100

166 21.6 17.8 26.6




139 12.5 11.2 16.8



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

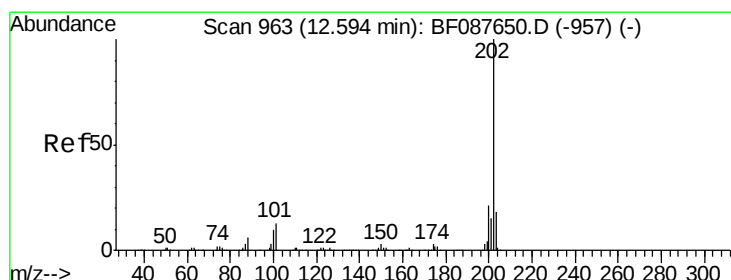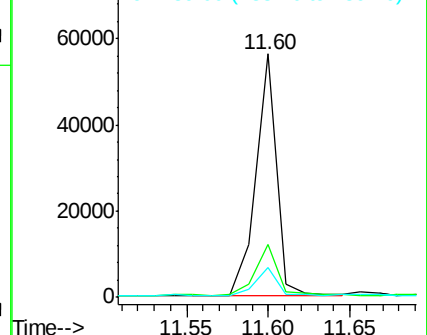

#74

Fluoranthene

Concen: 41.48 ng

RT: 12.58 min Scan# 962

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44


Tgt Ion:202 Resp: 784257

Ion Ratio Lower Upper

202 100

101 13.7 0.0 33.1



203 18.2 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

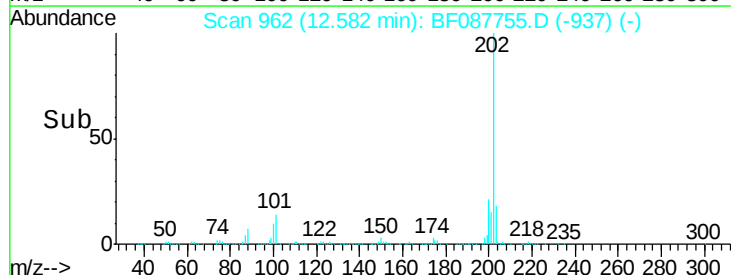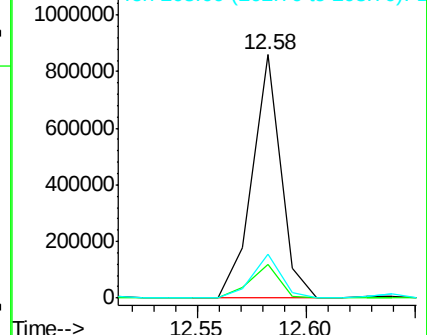

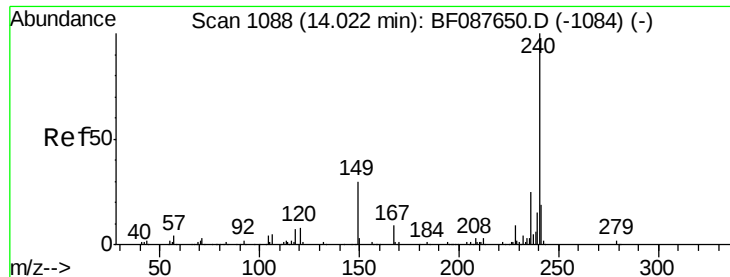

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1087

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)


Tgt Ion:240 Resp: 255946

Ion Ratio Lower Upper

240 100

120 7.6 6.8 10.2




236 25.4 20.2 30.2

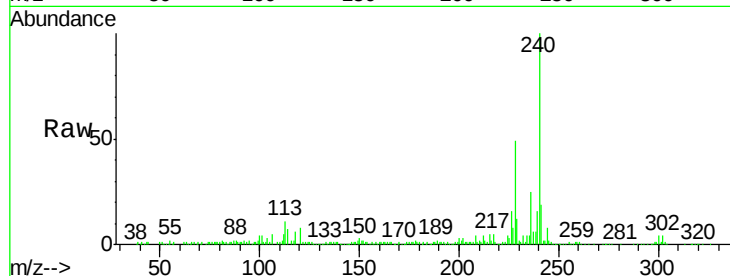

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

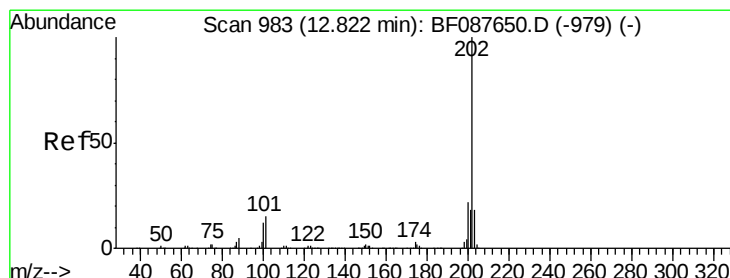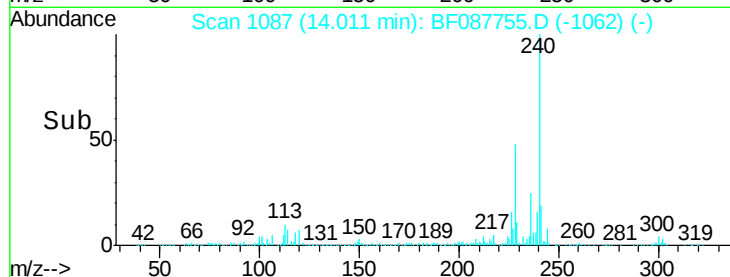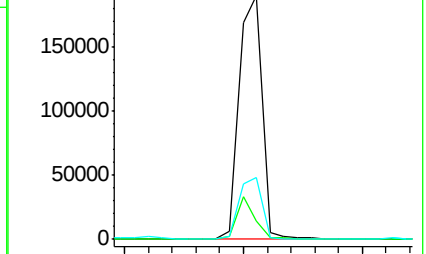

#77

Pyrene

Concen: 44.99 ng

RT: 12.81 min Scan# 982

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44


Tgt Ion:202 Resp: 820022

Ion Ratio Lower Upper

202 100

200 21.7 17.4 26.2



203 18.4 14.5 21.7

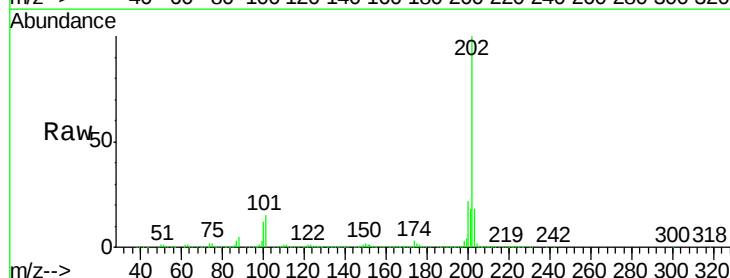


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



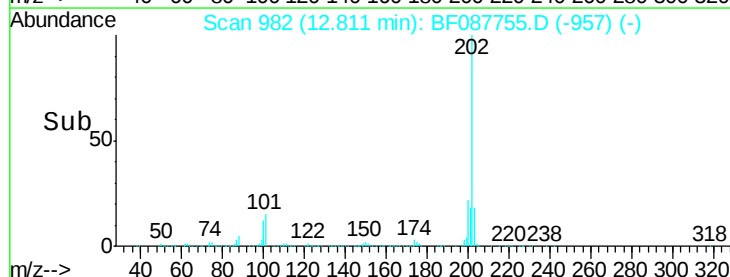
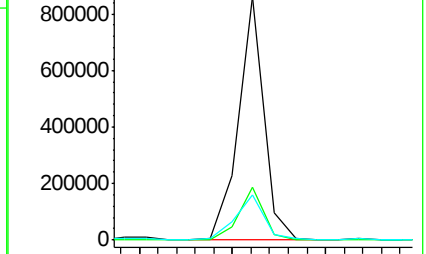


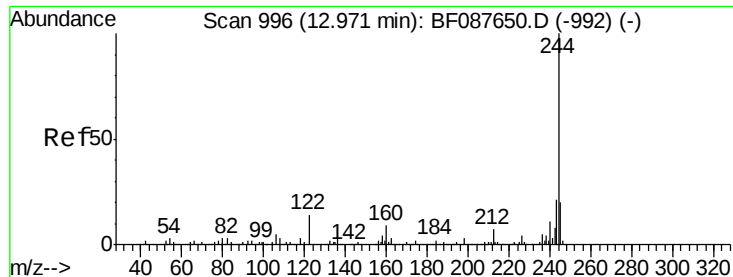

#78
 Terphenyl-d14
 Concen: 75.52 ng
 RT: 12.96 min Scan# 995
 Delta R.T. -0.01 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44




Instrument :
 BNA_F
 ClientSampleId :
 STA-TA-1261+50(0-4)


Tgt Ion:244 Resp: 792138
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.0 9.0
 122 11.9 11.2 16.8

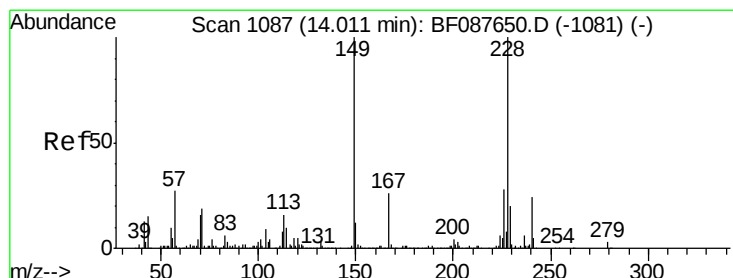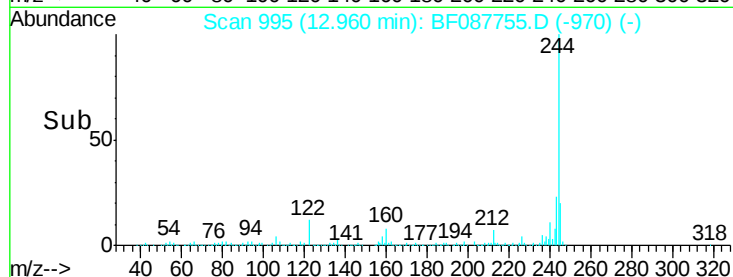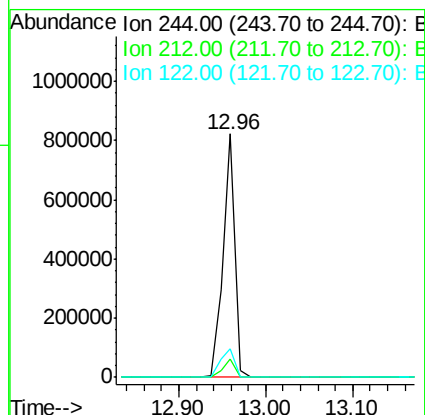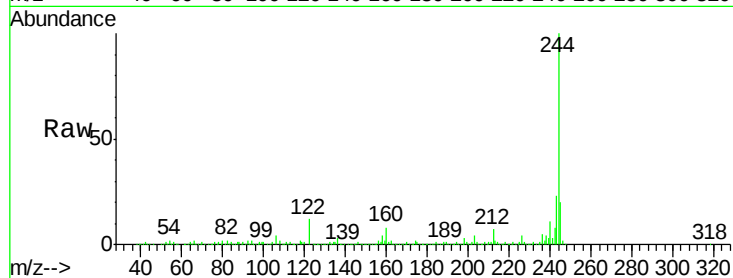

#80
 Benzo(a)anthracene
 Concen: 28.69 ng
 RT: 14.03 min Scan# 1089
 Delta R.T. 0.02 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Tgt Ion:228 Resp: 423823
 Ion Ratio Lower Upper
 228 100
 226 30.5 22.3 33.5
 229 21.5 16.0 24.0

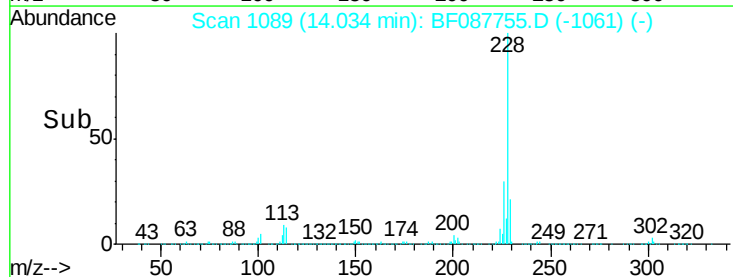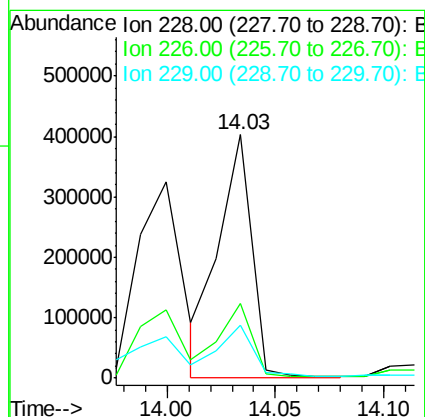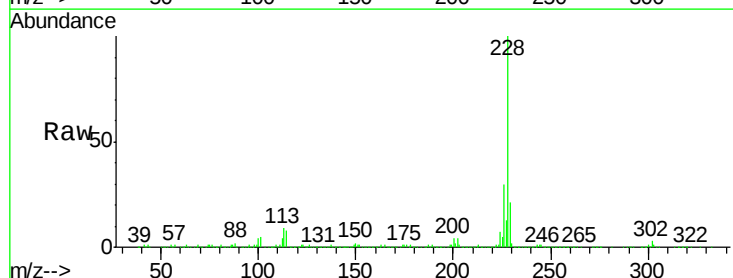



#82

Chrysene

Concen: 28.83 ng

RT: 14.03 min Scan# 1089

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)


Tgt Ion:228 Resp: 423930

Ion Ratio Lower Upper

228 100

226 30.5 25.4 38.2




229 21.5 16.3 24.5

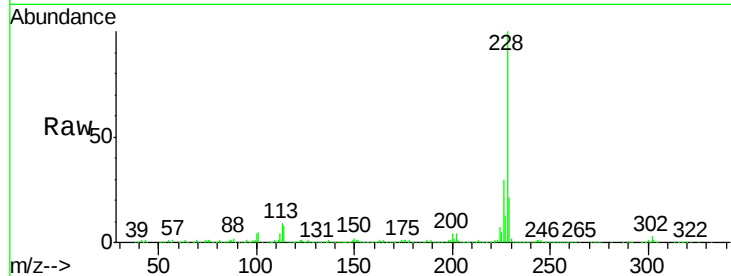

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

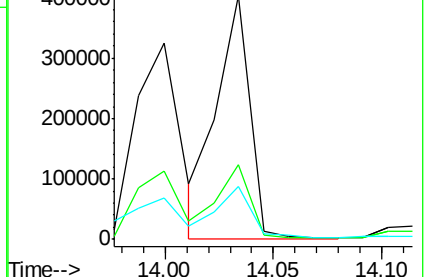

#83

Bis(2-ethylhexyl)phthalate

Concen: 4.16 ng

RT: 14.00 min Scan# 1086

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44


Tgt Ion:149 Resp: 38435

Ion Ratio Lower Upper

149 100

167 24.2 20.5 30.7



279 4.1 2.0 3.0#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

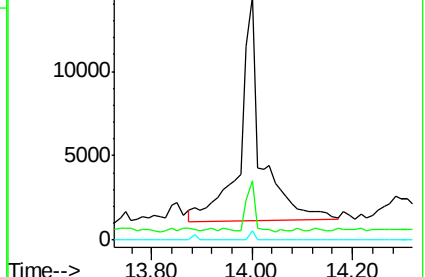





#85
 Indeno(1,2,3-cd)pyrene
 Concen: 17.07 ng
 RT: 16.82 min Scan# 1333
 Delta R.T. -0.01 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44

Instrument :
 BNA_F
 ClientSampleId :
 STA-TA-1261+50(0-4)



Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.6	0.0	0.0#
277	25.1	0.0	0.0#

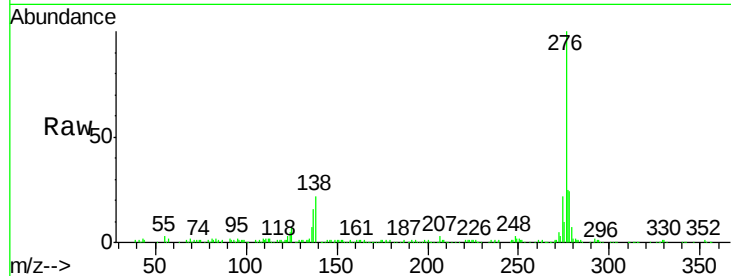

Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

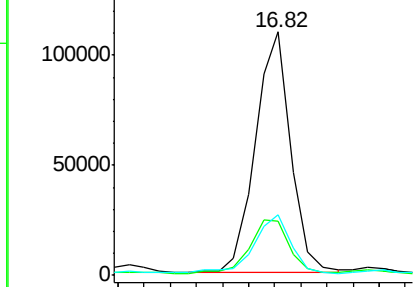


Time--> 16.70 16.80 16.90

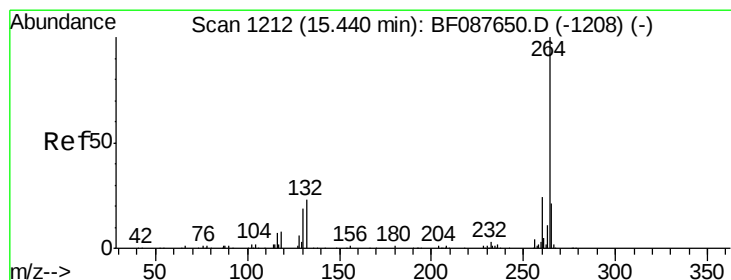


#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.43 min Scan# 1211
 Delta R.T. -0.01 min
 Lab File: BF087755.D
 Acq: 6 Jun 2016 16:44


Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.2	28.8
265	23.6	16.9	25.3




Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

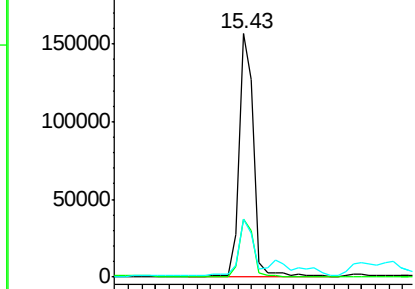

Time--> 15.30 15.40 15.50 15.60





#87

Benzo(b)fluoranthene

Concen: 53.33 ng

RT: 15.03 min Scan# 1176

Delta R.T. -0.01 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44





Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)

Tgt Ion:	252	Resp:	792648
Ion Ratio	Lower	Upper	
252	100		
253	22.9	17.4	26.2
125	13.8	7.1	10.7#

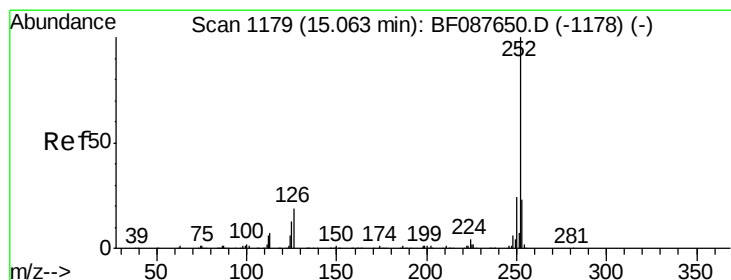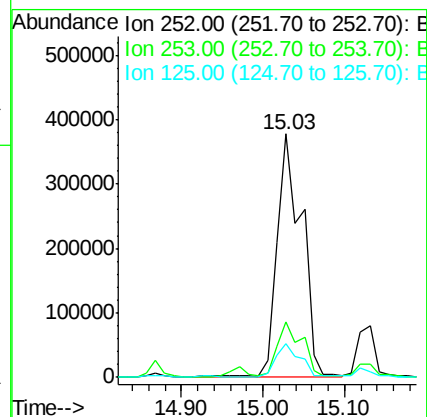

#88

Benzo(k)fluoranthene

Concen: 64.10 ng




RT: 15.03 min Scan# 1176


Delta R.T. -0.03 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Tgt Ion:	252	Resp:	792648
Ion Ratio	Lower	Upper	
252	100		
253	22.9	18.0	27.0
125	13.8	11.2	16.8



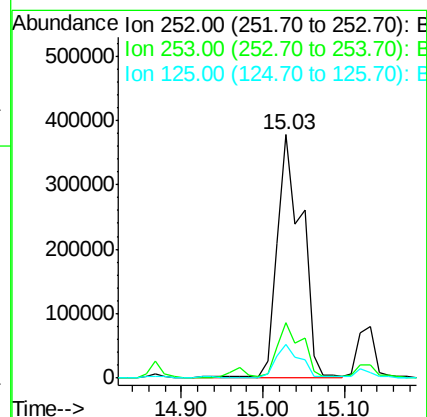
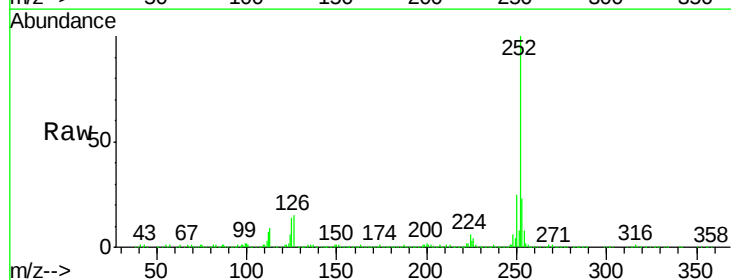




#89
Benzo(a)pyrene
Concen: 24.81 ng
RT: 15.37 min Scan# 1206
Delta R.T. -0.01 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44




Instrument :
BNA_F
ClientSampleId :
STA-TA-1261+50(0-4)


Tgt Ion: 252 Resp: 309951
Ion Ratio Lower Upper
252 100
253 24.2 17.9 26.9
125 14.7 12.5 18.7

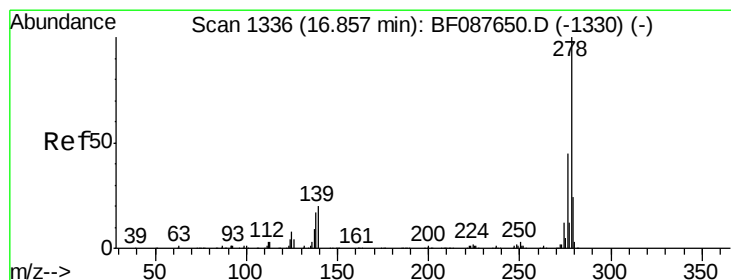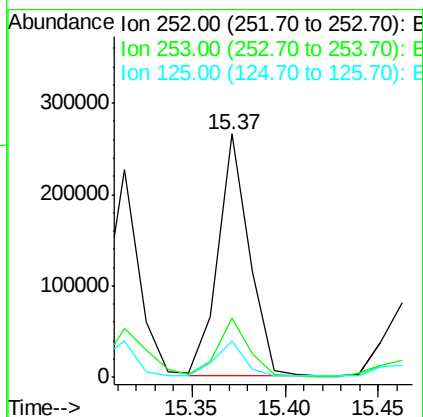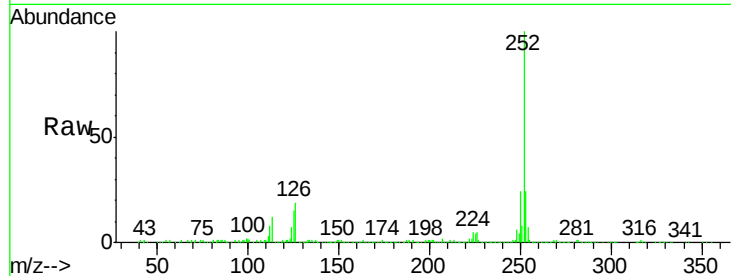

#90
Dibenzo(a,h)anthracene
Concen: 4.90 ng
RT: 16.83 min Scan# 1334
Delta R.T. -0.02 min
Lab File: BF087755.D
Acq: 6 Jun 2016 16:44

Tgt Ion: 278 Resp: 52134
Ion Ratio Lower Upper
278 100
139 17.8 15.7 23.5
279 26.5 19.4 29.2

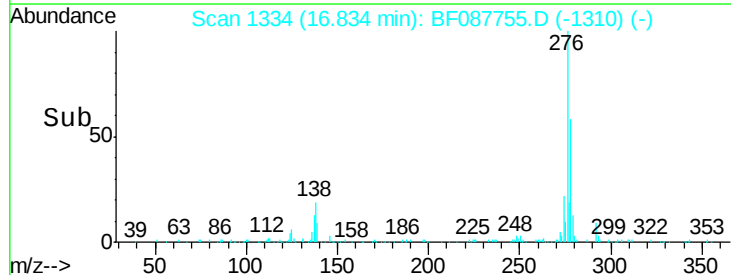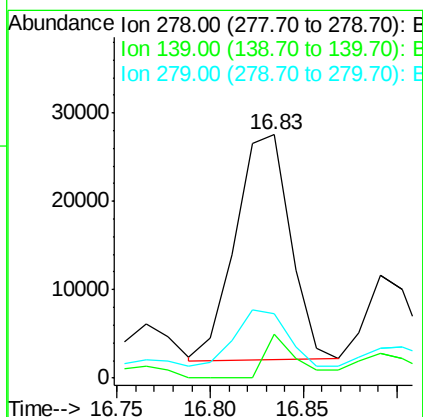



#91

Benzo(g,h,i)perylene

Concen: 16.31 ng

RT: 17.23 min Scan# 1369

Delta R.T. -0.02 min

Lab File: BF087755.D

Acq: 6 Jun 2016 16:44

Instrument :

BNA_F

ClientSampleId :

STA-TA-1261+50(0-4)

Tgt Ion: 276 Resp: 174963

Ion Ratio Lower Upper

276 100

277 22.9 18.9 28.3

138 24.6 21.4 32.2

