
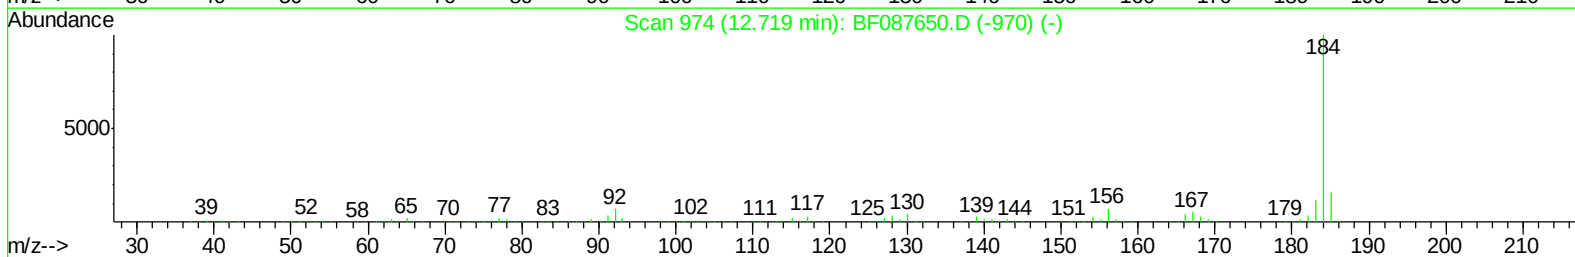
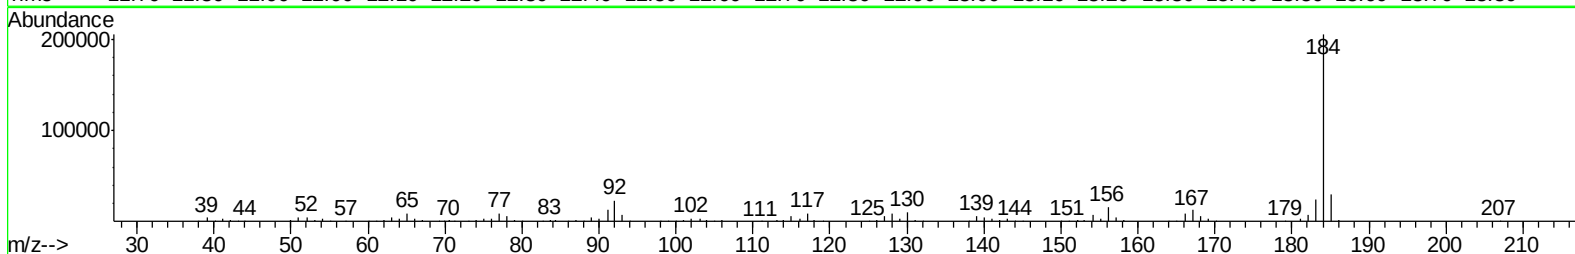


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060616\
Data File : BF087743.D
Acq On : 6 Jun 2016 10:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:24:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

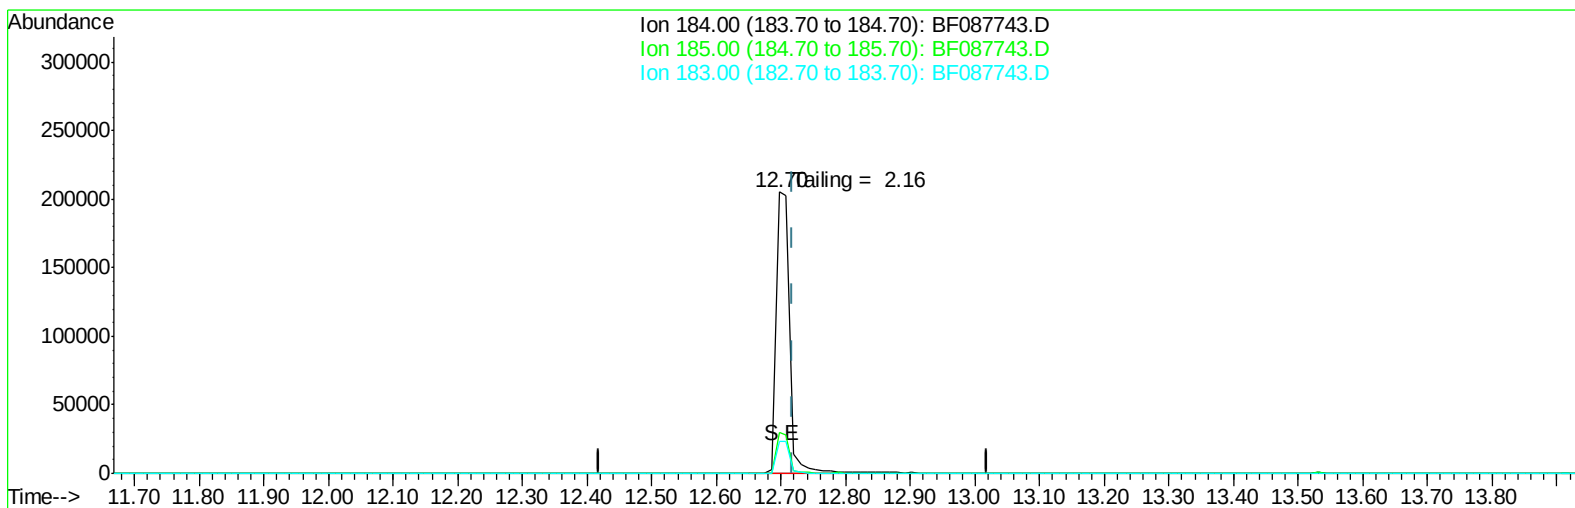

TIC: BF087743.D

(76) Benzidine




12.696min (-0.023) 25315.21ng

response 308454

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.67
183.00	11.60	11.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060616\
Data File : BF087743.D
Acq On : 6 Jun 2016 10:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:24:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

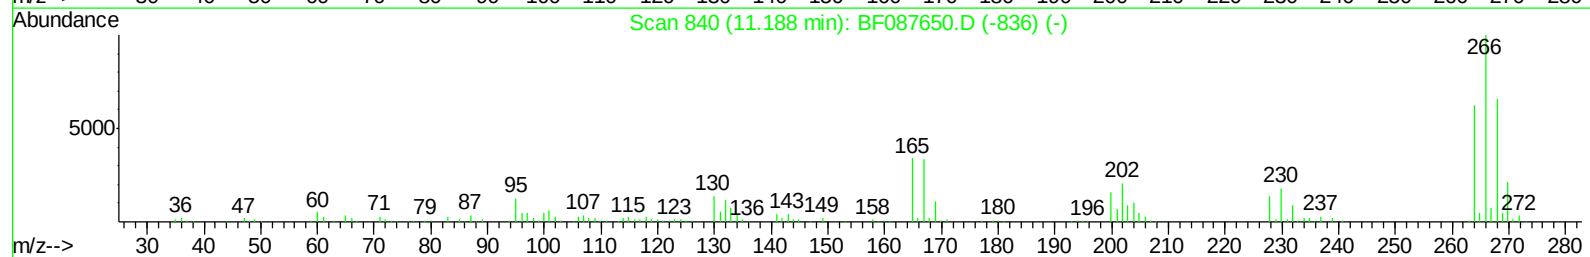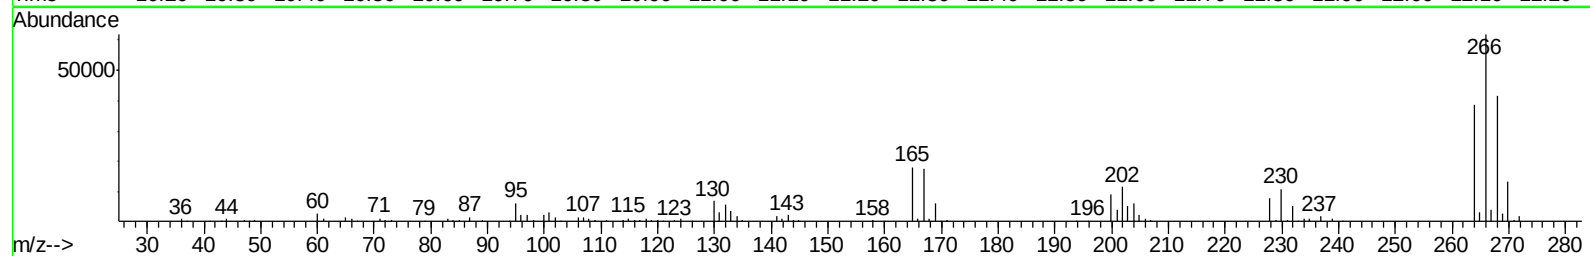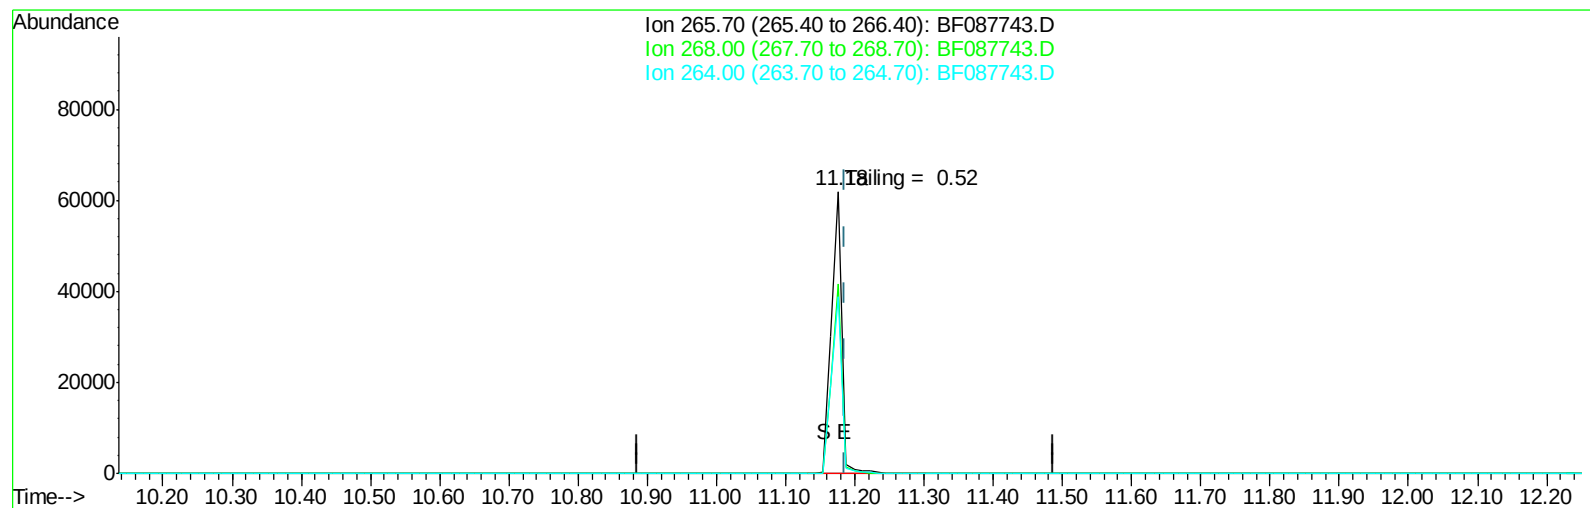

TIC: BF087743.D

(69) Pentachlorophenol (C)

11.176min (-0.011) 38020.02ng

response 66132

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	67.47
264.00	62.00	62.70
0.00	0.00	0.00