

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060616\
 Data File : BF087763.D
 Acq On : 6 Jun 2016 20:49
 Operator : UM/SJ
 Sample : H3356-07 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 U5-B3(0-12)C

Quant Time: Jun 07 02:02:56 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	112856	20.00	ng	-0.02
21) Naphthalene-d8	8.14	136	460075	20.00	ng	-0.01
38) Acenaphthene-d10	9.88	164	173223	20.00	ng	-0.02
63) Phenanthrene-d10	11.37	188	302536	20.00	ng	-0.01
75) Chrysene-d12	14.00	240	253162	20.00	ng	-0.02
86) Perylene-d12	15.43	264	186211	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	151224	21.66	ng	-0.01
7) Phenol-d6	6.47	99	165823	18.94	ng	-0.02
23) Nitrobenzene-d5	7.40	82	87469	11.00	ng	-0.02
41) 2,4,6-Tribromophenol	10.67	330	31177	17.93	ng	-0.01
44) 2-Fluorobiphenyl	9.21	172	206680	14.65	ng	-0.02
78) Terphenyl-d14	12.95	244	139807	13.48	ng	-0.02
Target Compounds						Qvalue
49) Dimethylphthalate	9.61	163	32990	2.62	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060616\
Data File : BF087763.D
Acq On : 6 Jun 2016 20:49
Operator : UM/SJ
Sample : H3356-07 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
U5-B3(0-12)C

Quant Time: Jun 07 02:02:56 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

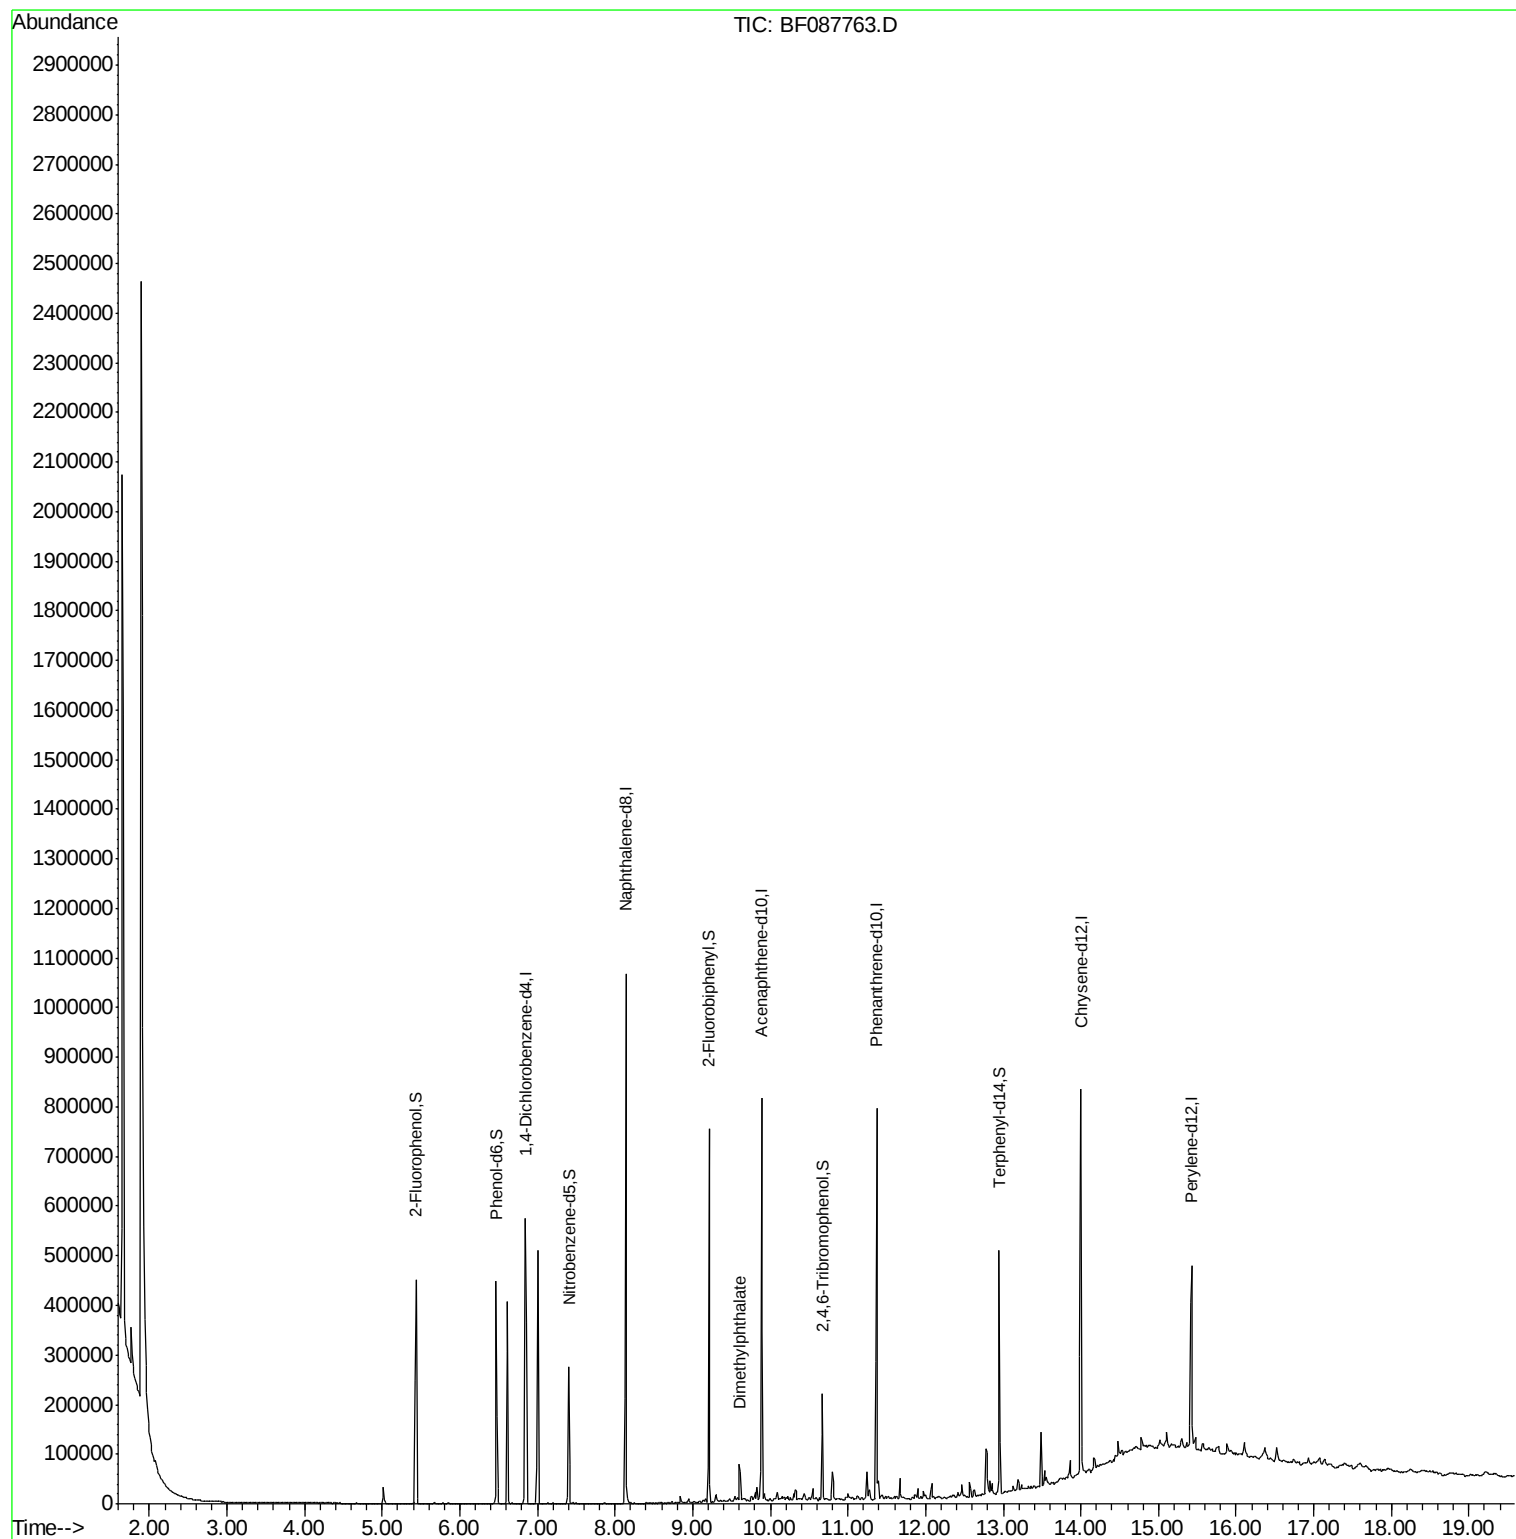

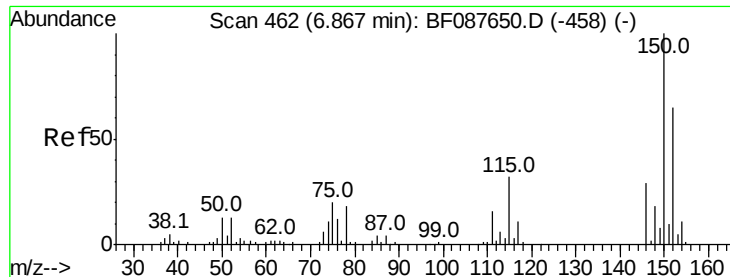

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.84 min Scan# 460

Delta R.T. -0.02 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49

Instrument :

BNA_F

ClientSampleId :

U5-B3(0-12)C


Tot Ion:152 Resp: 112856

Ion Ratio Lower Upper

152 100

150 158.7 123.8 185.6




115 69.1 39.6 59.4#

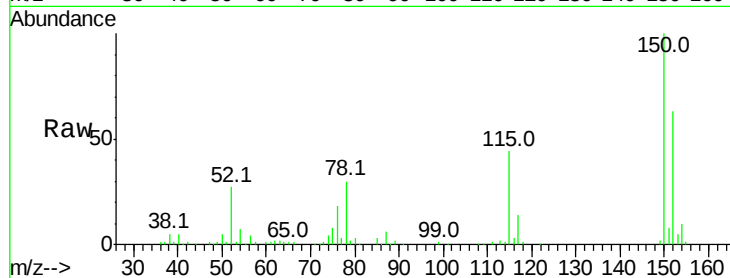

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

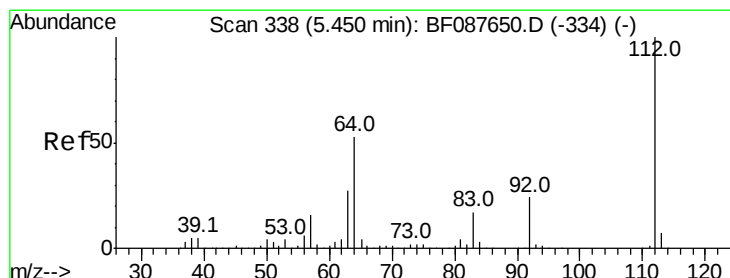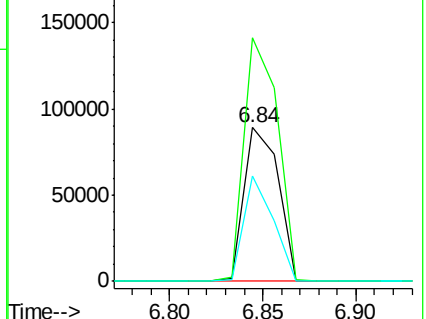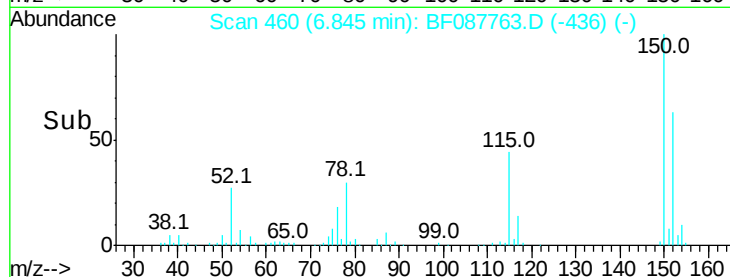

#5

2-Fluorophenol

Concen: 21.66 ng

RT: 5.44 min Scan# 337

Delta R.T. -0.01 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49


Tgt Ion:112 Resp: 151224

Ion Ratio Lower Upper

112 100

64 47.9 42.2 63.2



63 24.0 21.8 32.8

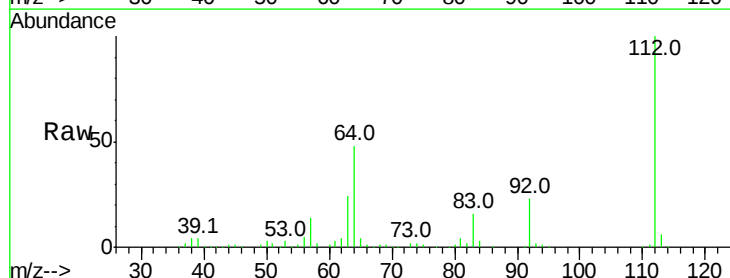


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

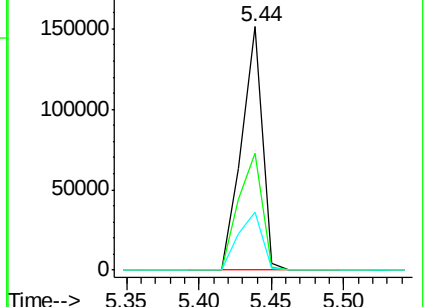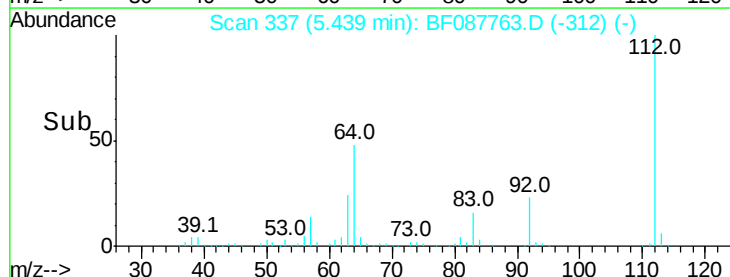

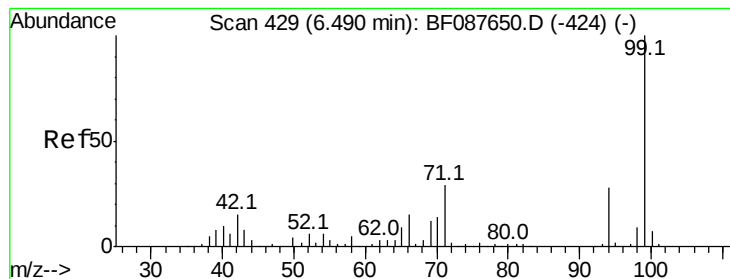

#7

Phenol-d6

Concen: 18.94 ng

RT: 6.47 min Scan# 427

Delta R.T. -0.02 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49

Instrument :


BNA_F

ClientSampleId :

U5-B3(0-12)C

Tot Ion: 99 Resp: 165823




Ion	Ratio	Lower	Upper
99	100		
42	19.5	12.2	18.2#
71	34.5	23.4	35.0

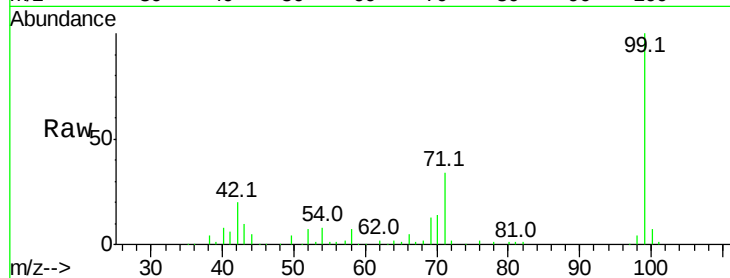

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

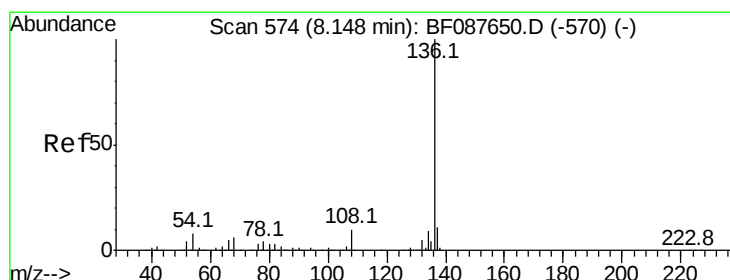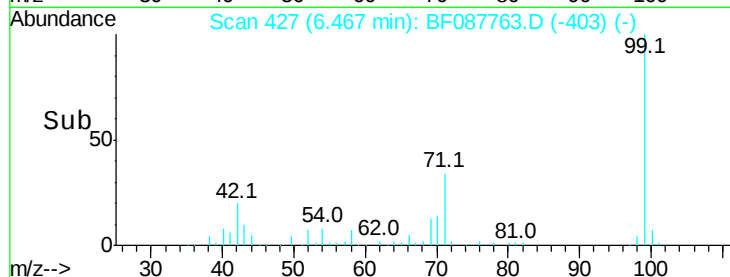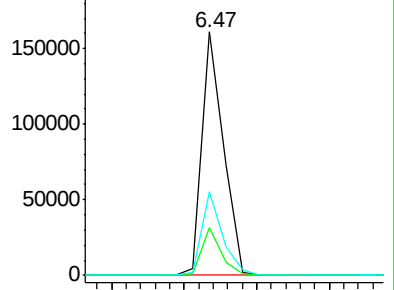

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 573


Delta R.T. -0.01 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49

Tgt Ion: 136 Resp: 460075

Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.1	13.7
54	6.8	6.6	10.0
68	5.5	5.1	7.7


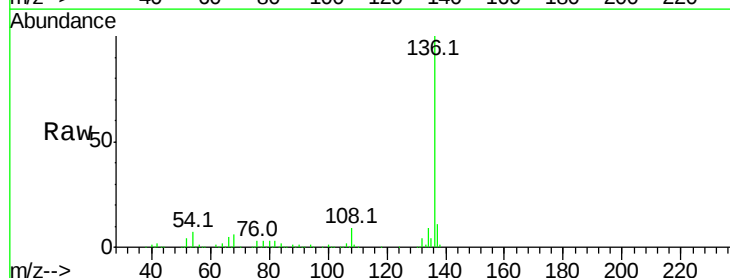



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

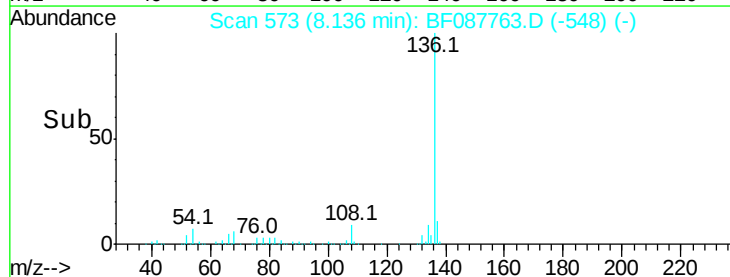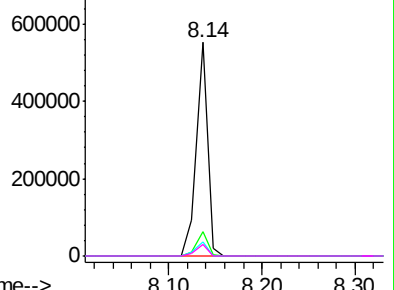

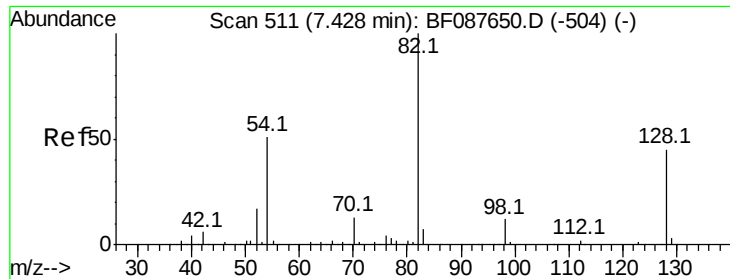

#23

Nitrobenzene-d5

Concen: 11.00 ng

RT: 7.40 min Scan# 509

Delta R.T. -0.02 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49

Instrument :

BNA_F

ClientSampleId :

U5-B3(0-12)C


Tot Ion: 82 Resp: 87469

Ion Ratio Lower Upper

82 100

128 40.4 35.9 53.9




54 52.2 40.9 61.3

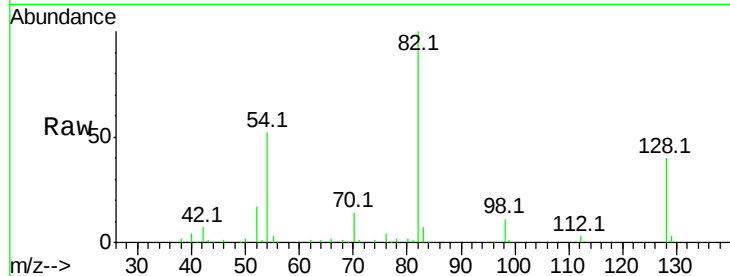

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

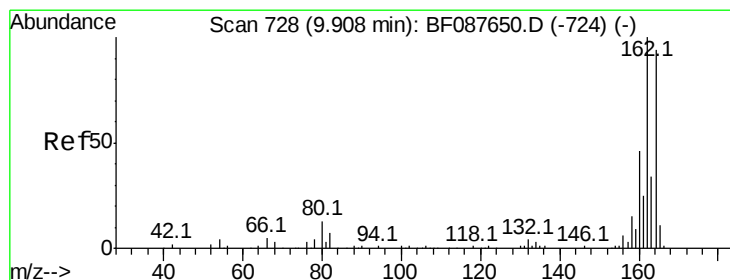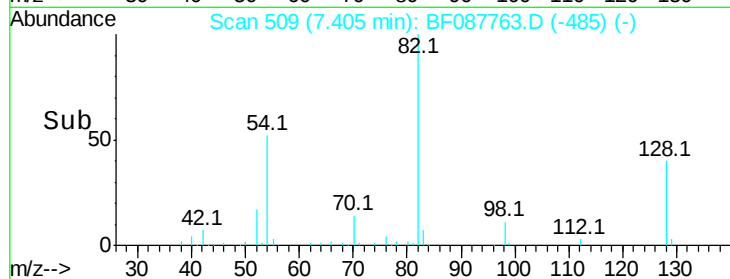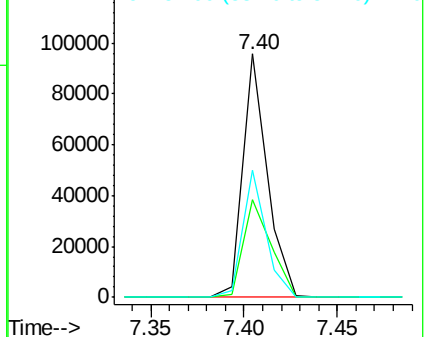

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.88 min Scan# 726

Delta R.T. -0.02 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49


Tgt Ion: 164 Resp: 173223

Ion Ratio Lower Upper

164 100

162 103.6 85.4 128.2



160 46.4 39.5 59.3

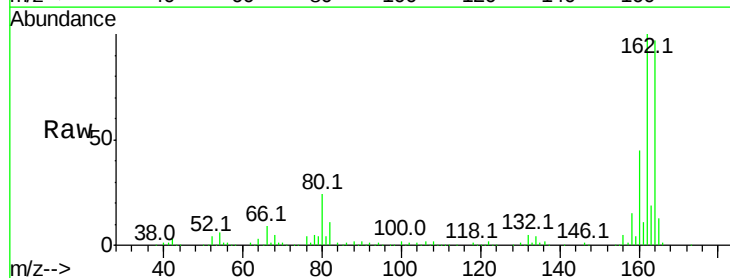


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

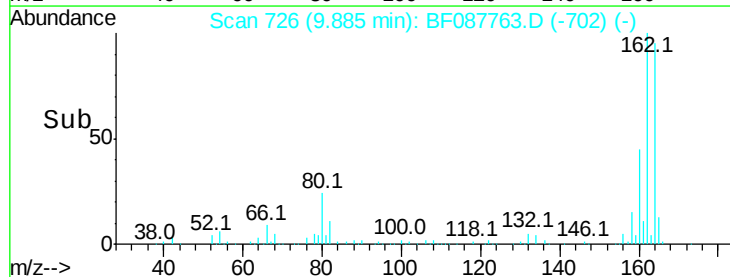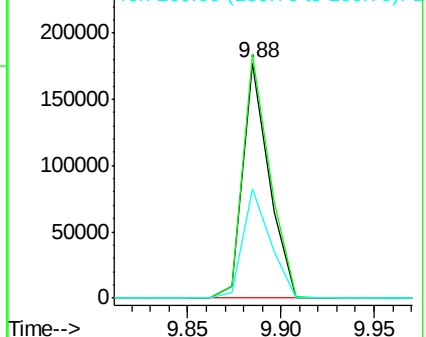


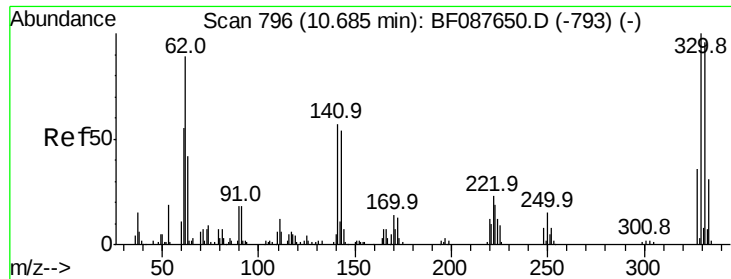




#41
 2,4,6-Tribromophenol
 Concen: 17.93 ng
 RT: 10.67 min Scan# 795
 Delta R.T. -0.01 min
 Lab File: BF087763.D
 Acq: 6 Jun 2016 20:49

Instrument :
 BNA_F
 ClientSampleId :
 U5-B3(0-12)C

Tot Ion:330 Resp: 31177
 Ion Ratio Lower Upper
 330 100
 332 99.2 0.0 0.0#
 141 34.4 0.0 0.0#

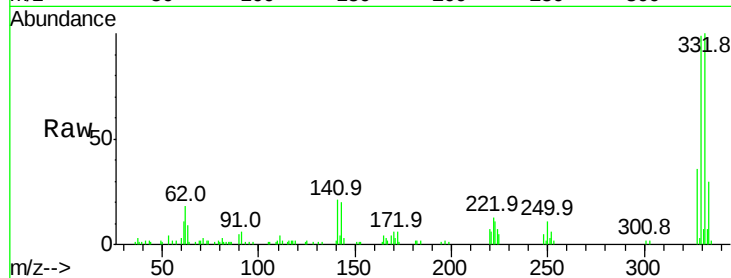


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

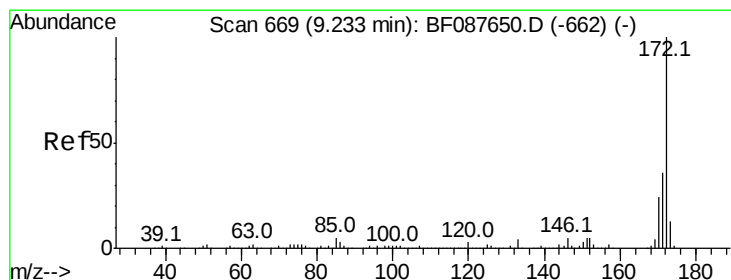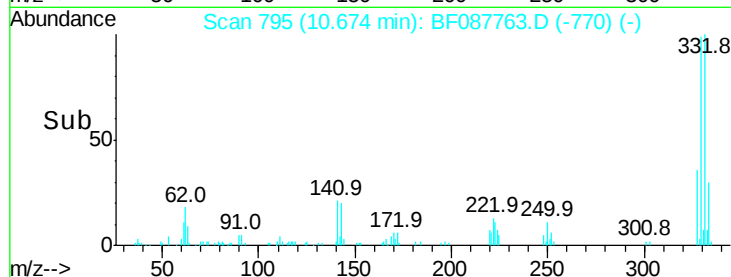
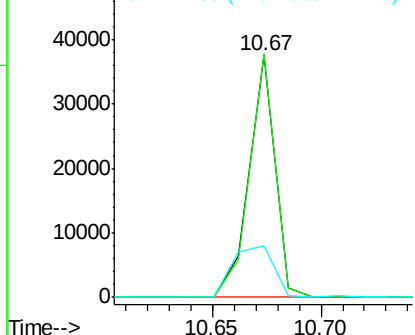



#44
 2-Fluorobiphenyl
 Concen: 14.65 ng
 RT: 9.21 min Scan# 667
 Delta R.T. -0.02 min
 Lab File: BF087763.D
 Acq: 6 Jun 2016 20:49

Tgt Ion:172 Resp: 206680
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.6 43.0
 170 23.1 19.2 28.8

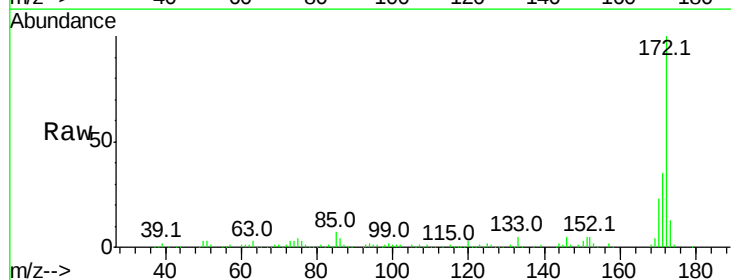

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

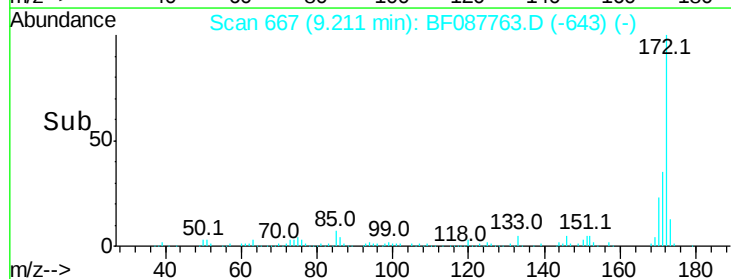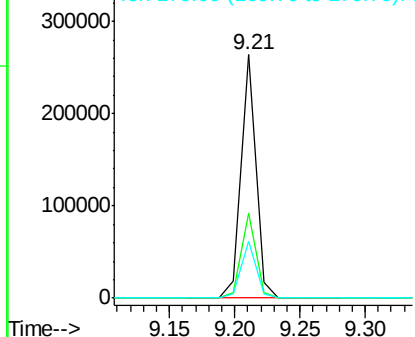

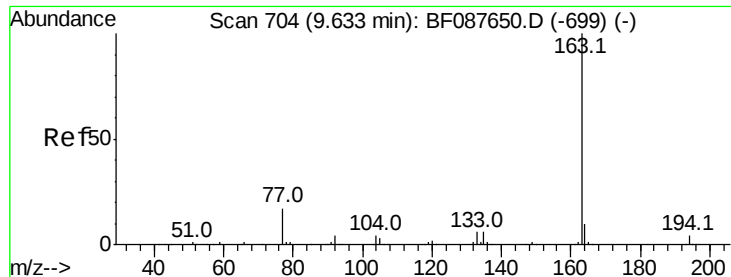

#49

Dimethylphthalate

Concen: 2.62 ng

RT: 9.61 min Scan# 702

Delta R.T. -0.02 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49

Instrument :

BNA_F

ClientSampleId :

U5-B3(0-12)C


Tot Ion:163 Resp: 32990

Ion Ratio Lower Upper

163 100

194 4.6 2.8 4.2#




164 9.4 8.3 12.5

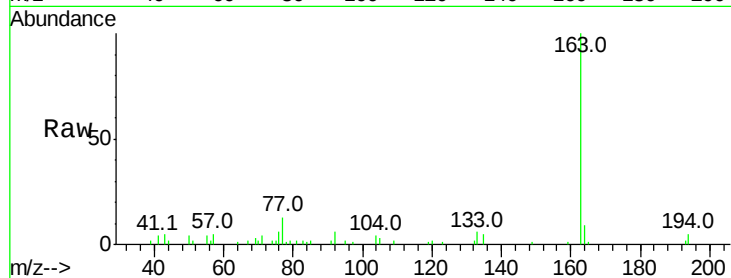

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

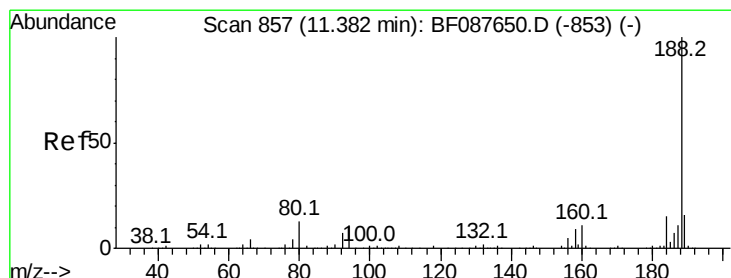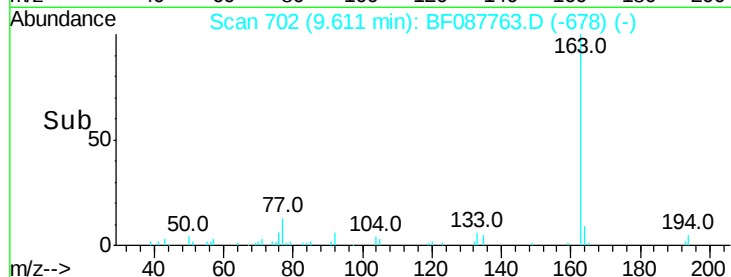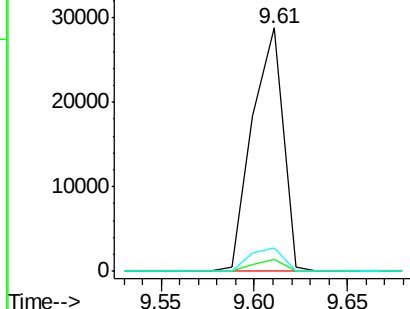

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.37 min Scan# 856

Delta R.T. -0.01 min

Lab File: BF087763.D

Acq: 6 Jun 2016 20:49


Tgt Ion:188 Resp: 302536

Ion Ratio Lower Upper

188 100

94 7.9 9.0 13.6#



80 8.1 10.0 15.0#

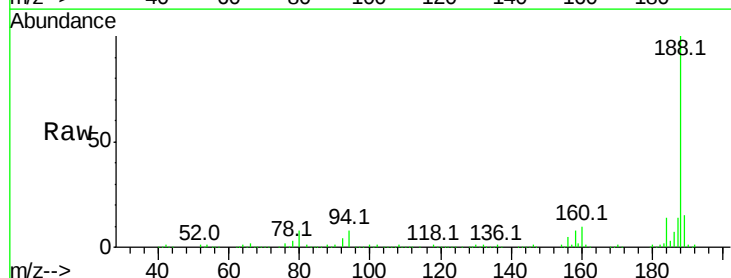


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



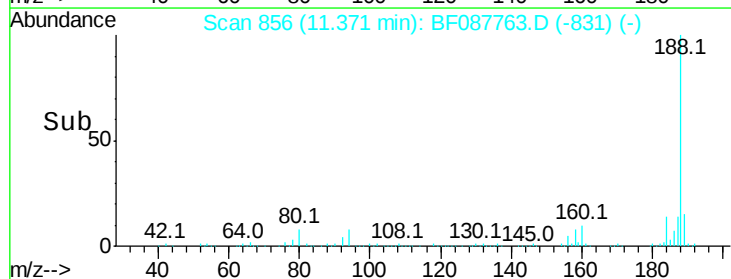
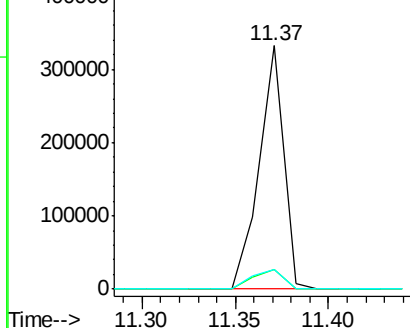


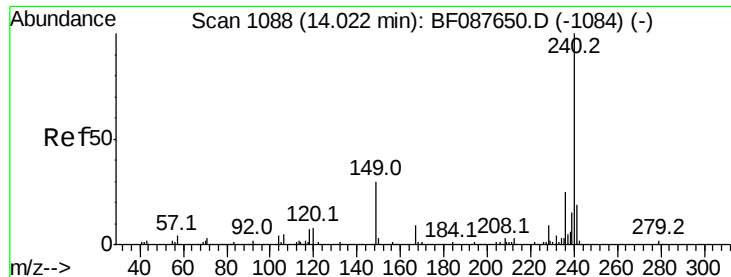

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.00 min Scan# 1086
Delta R.T. -0.02 min
Lab File: BF087763.D
Acq: 6 Jun 2016 20:49




Instrument :
BNA_F
ClientSampleId :
U5-B3(0-12)C


Tot Ion:240 Resp: 253162
Ion Ratio Lower Upper
240 100
120 12.0 6.8 10.2#
236 25.8 20.2 30.2

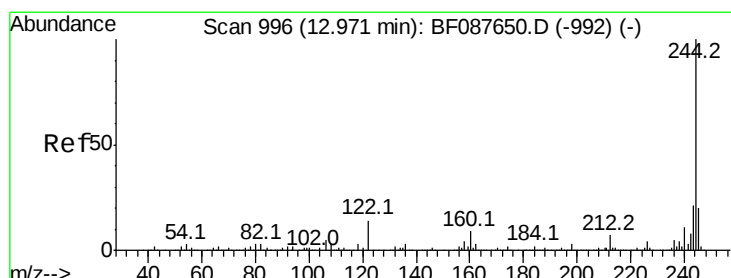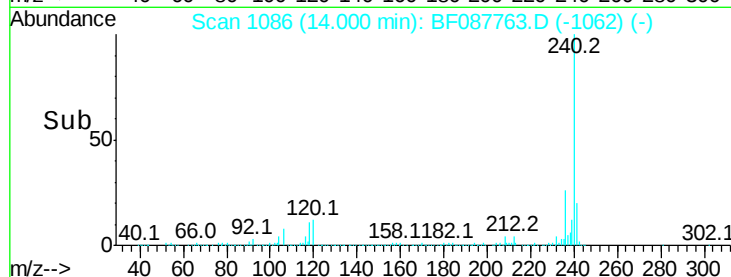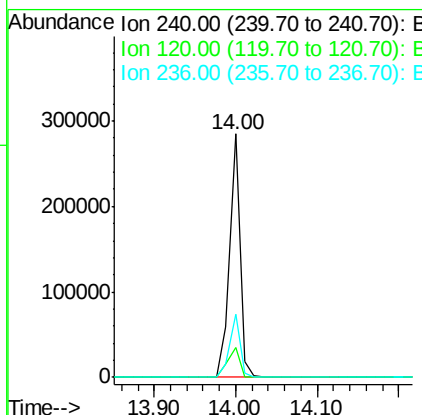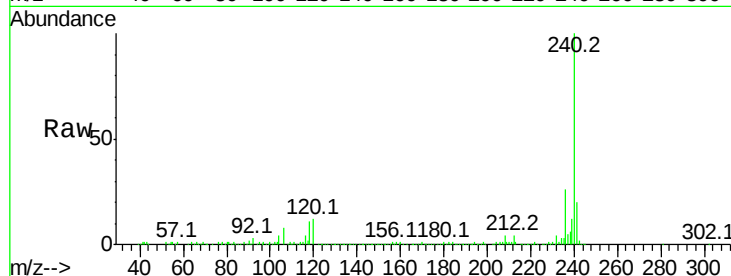

#78
Terphenyl-d14
Concen: 13.48 ng
RT: 12.95 min Scan# 994
Delta R.T. -0.02 min
Lab File: BF087763.D
Acq: 6 Jun 2016 20:49

Tgt Ion:244 Resp: 139807
Ion Ratio Lower Upper
244 100
212 6.8 6.0 9.0
122 14.8 11.2 16.8

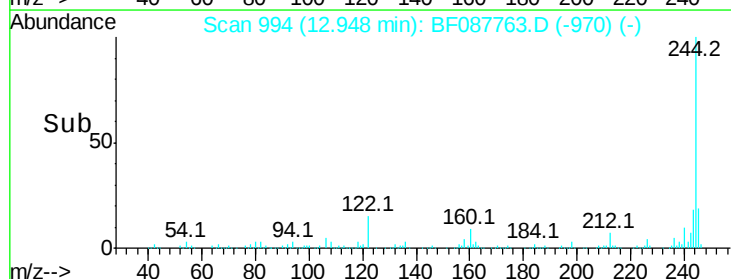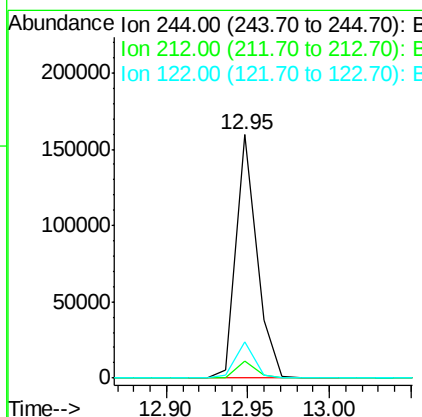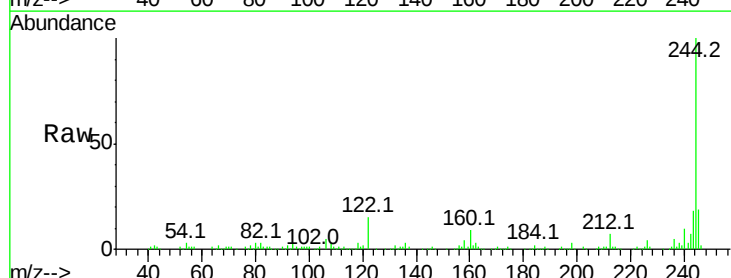


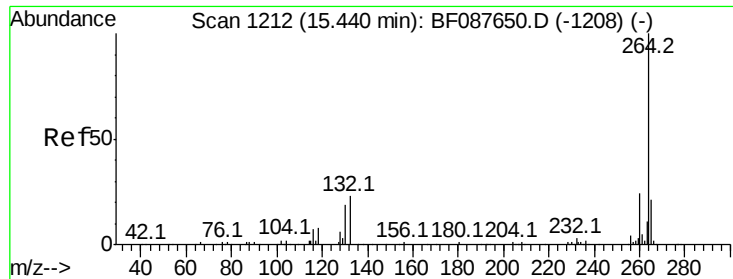

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.43 min Scan# 1211
Delta R.T. -0.01 min
Lab File: BF087763.D
Acq: 6 Jun 2016 20:49

Instrument :
BNA_F
ClientSampleId :
U5-B3(0-12)C

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	21.5	16.9	25.3

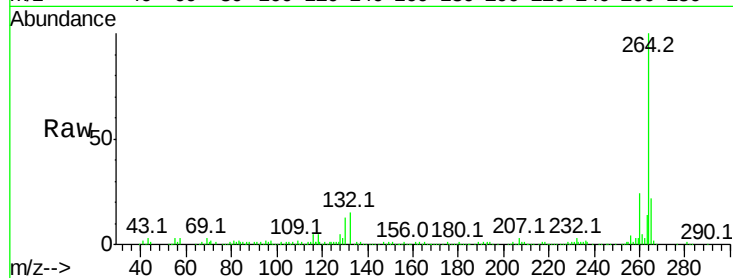

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

