


Data Path : Z:\HPCHEM1\BNA F\Data\BF060616\
 Data File : BF087743.D
 Acq On : 6 Jun 2016 10:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 04 11:07:28 2016

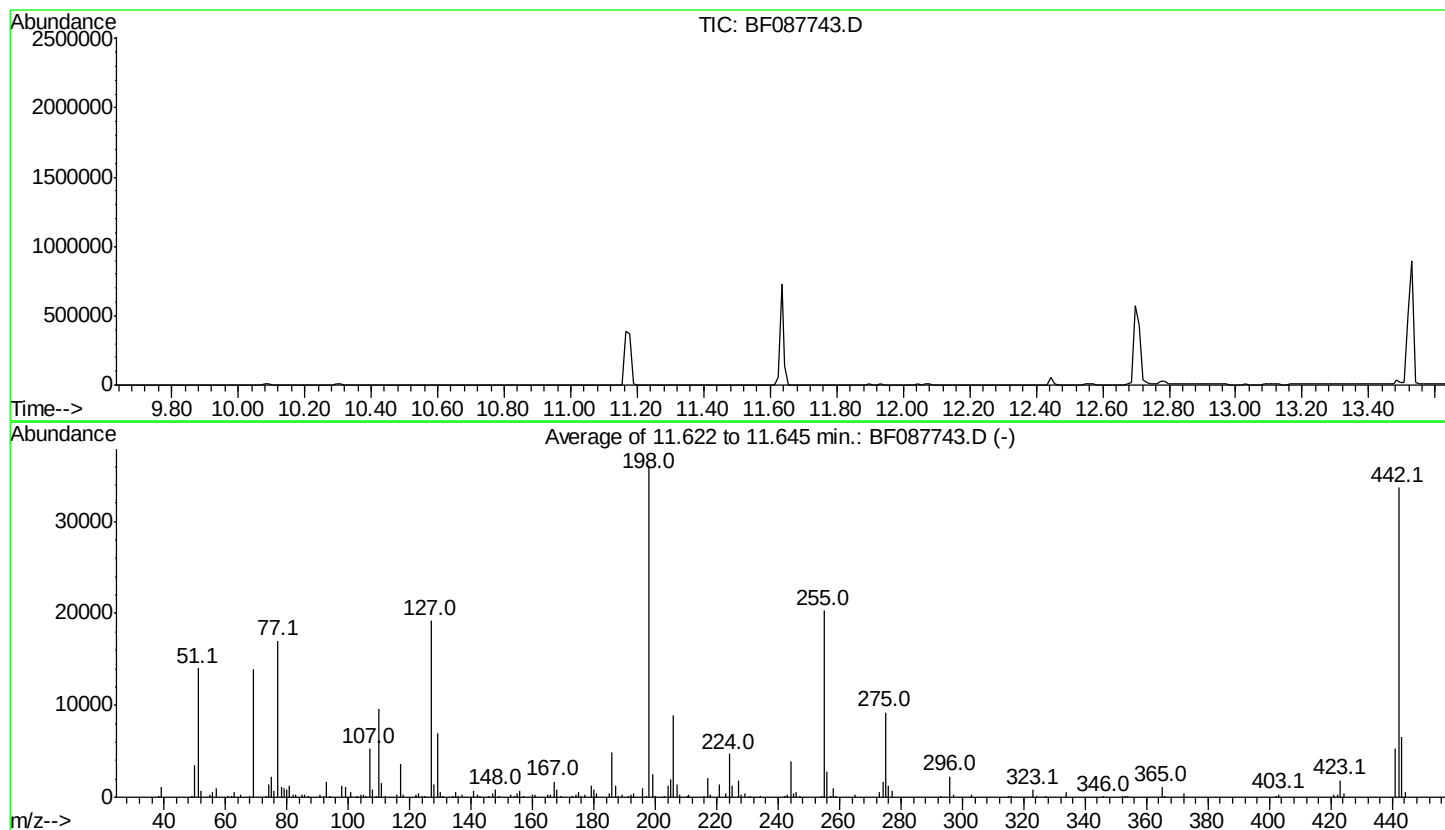

AutoFind: Scans 878, 879, 880; Background Corrected with Scan 875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	14010	PASS
68	69	0.00	2	1.5	209	PASS
69	198	0.00	100	38.5	13909	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	19190	PASS
197	198	0.00	2	0.5	174	PASS
198	198	100	100	100.0	36088	PASS
199	198	5	9	6.8	2450	PASS
275	198	10	60	25.6	9237	PASS
365	198	1	100	3.3	1184	PASS
441	442	0.01	24	15.6	5249	PASS
442	198	50	100	93.3	33687	PASS
443	442	15	24	19.3	6486	PASS