

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060619\
 Data File : BF114869.D
 Acq On : 6 Jun 2019 18:30
 Operator : HP/JU
 Sample : K3211-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RBR-200052

Quant Time: Jun 07 02:19:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF060419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 04 16:57:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	458587	20.00	ng	0.00
21) Naphthalene-d8	7.95	136	1785464	20.00	ng	0.00
39) Acenaphthene-d10	9.70	164	922713	20.00	ng	0.00
64) Phenanthrene-d10	11.17	188	1726520	20.00	ng	0.00
76) Chrysene-d12	13.79	240	1086749	20.00	ng	0.00
87) Perylene-d12	15.17	264	958708	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	3261839	124.29	ng	0.02
7) Phenol-d6	6.32	99	4066208	127.33	ng	0.01
23) Nitrobenzene-d5	7.23	82	2640855	91.05	ng	0.00
42) 2,4,6-Tribromophenol	10.49	330	1248904	125.60	ng	0.00
45) 2-Fluorobiphenyl	9.03	172	4277735	86.85	ng	0.00
79) Terphenyl-d14	12.76	244	4134006	73.98	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.42	163	1035199	15.361	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060619\
Data File : BF114869.D
Acq On : 6 Jun 2019 18:30
Operator : HP/JU
Sample : K3211-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RBR-200052

Quant Time: Jun 07 02:19:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF060419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 04 16:57:15 2019
Response via : Initial Calibration

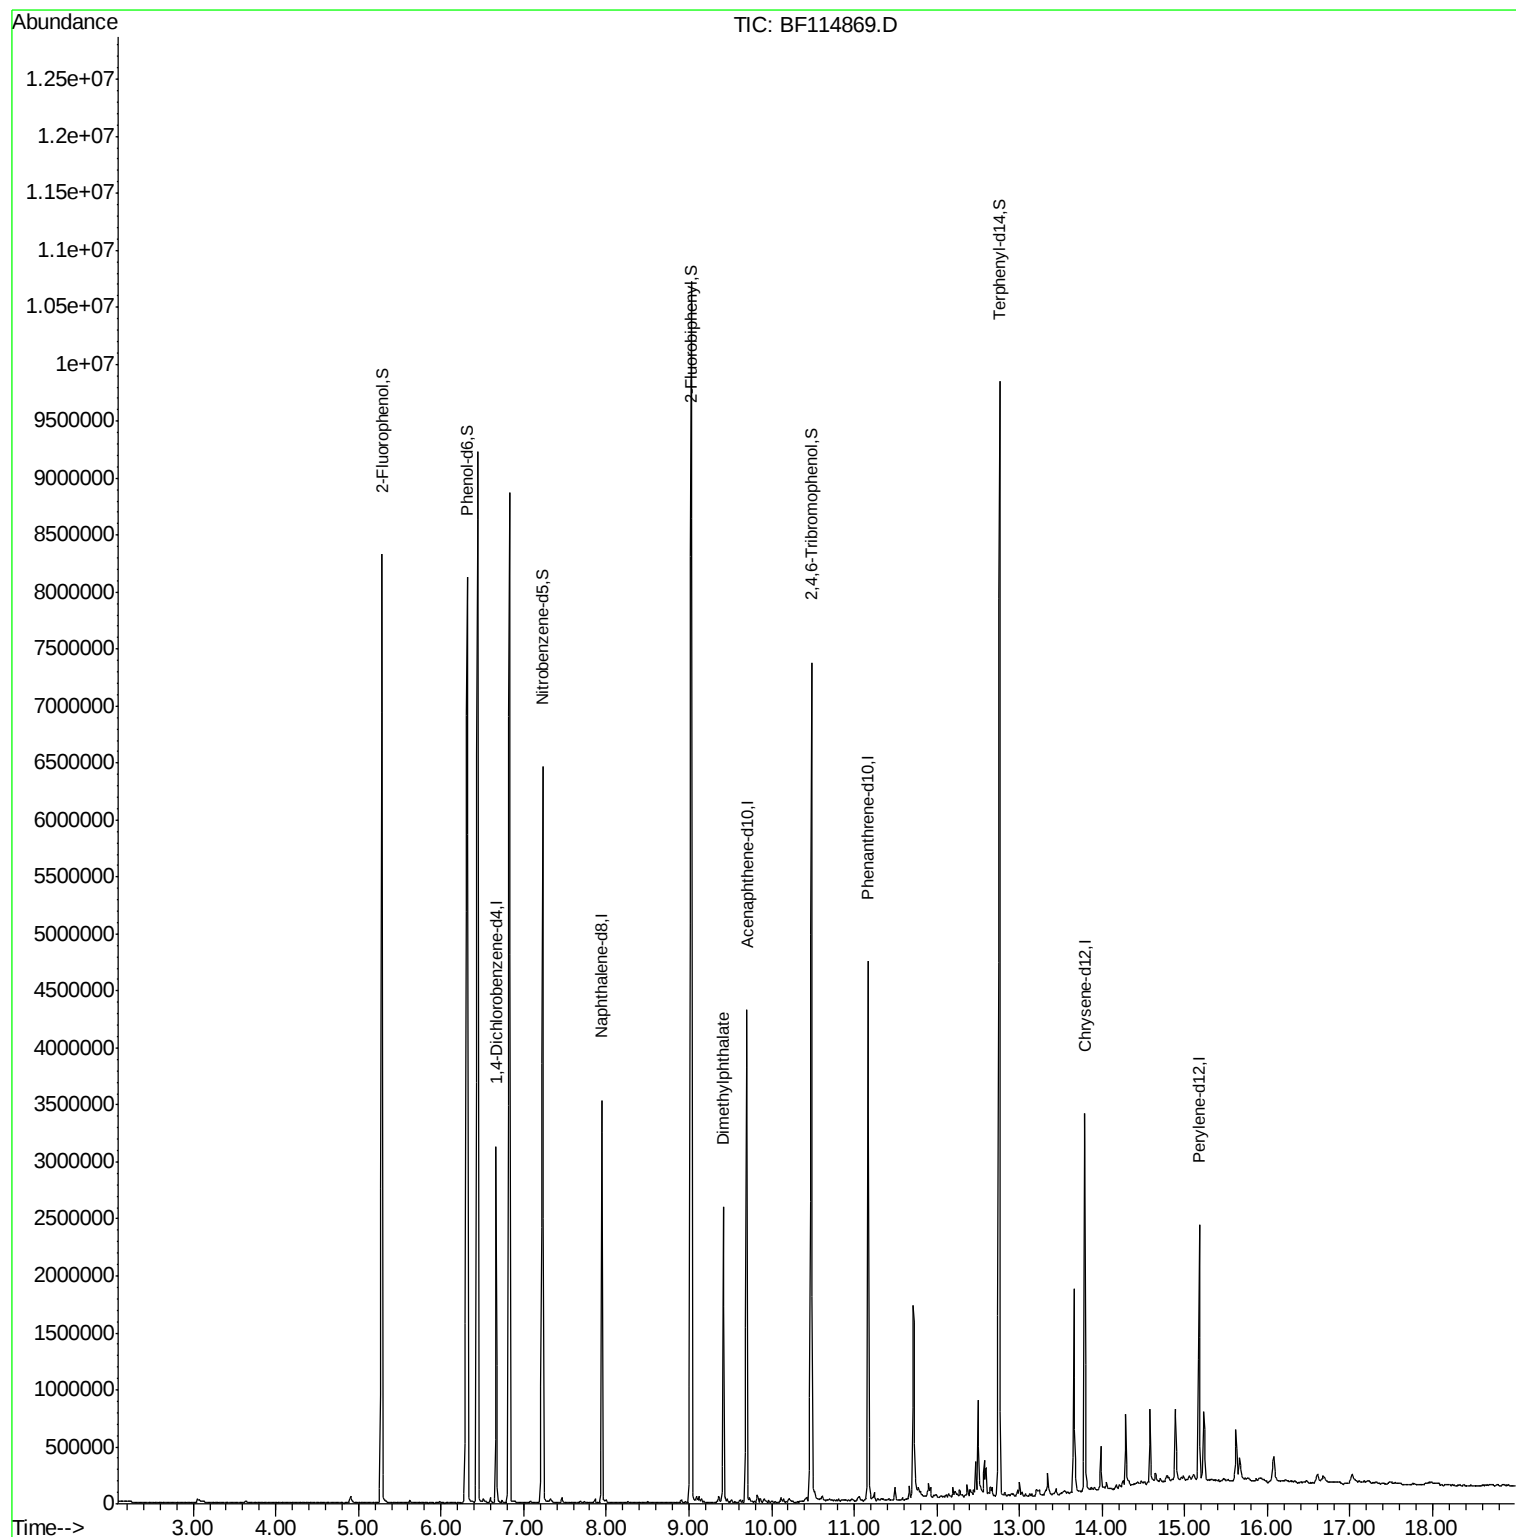

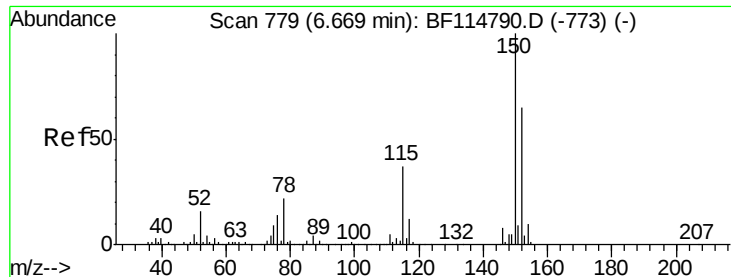


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.67 min Scan# 779
Delta R.T. 0.00 min
Lab File: BF114869.D
Acq: 6 Jun 2019 18:30

Instrument :
BNA_F
ClientSampleId :
RBR-200052

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.2	124.0	186.0
115	58.0	46.3	69.5



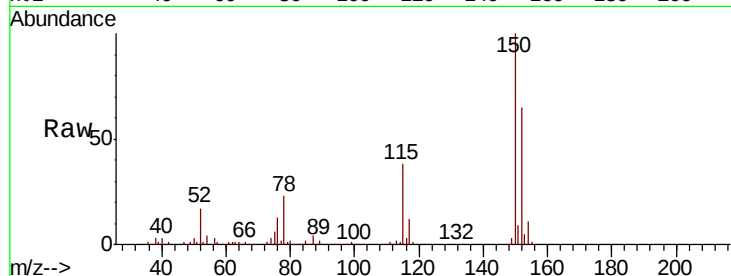


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

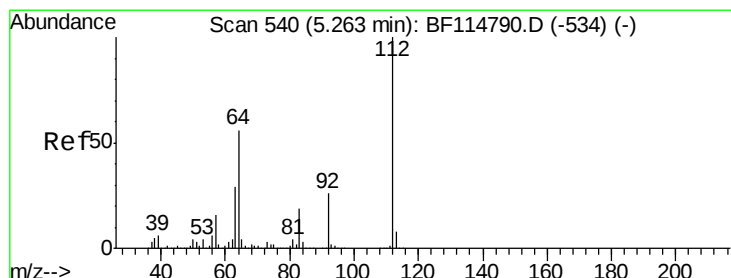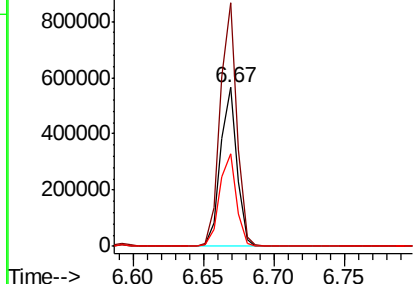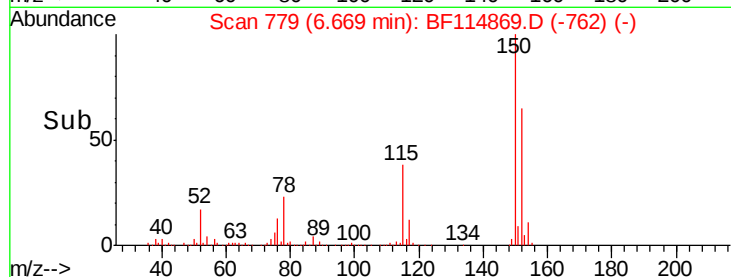

#5

2-Fluorophenol
Concen: 124.286 ng
RT: 5.29 min Scan# 544
Delta R.T. 0.02 min
Lab File: BF114869.D
Acq: 6 Jun 2019 18:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.8	44.6	66.8
63	29.9	23.0	34.4


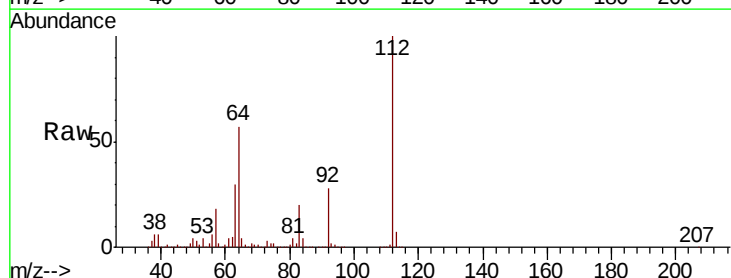



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

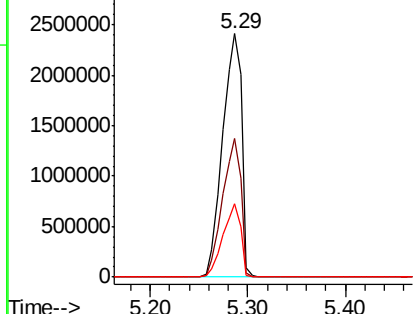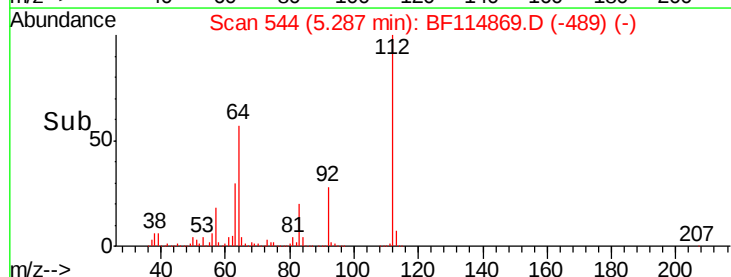

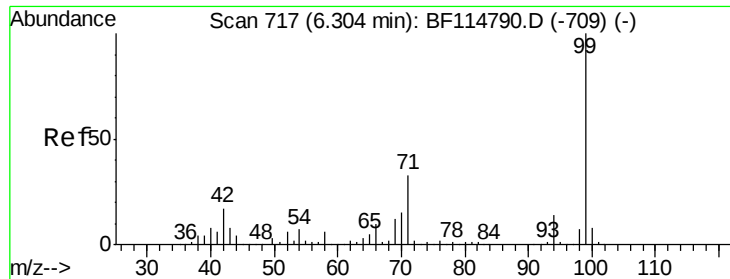

#7

Phenol-d6

Concen: 127.329 ng

RT: 6.32 min Scan# 719

Delta R.T. 0.01 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30

Instrument :

BNA_F

ClientSampleId :

RBR-200052


Tot Ion: 99 Resp: 4066208

Ion Ratio Lower Upper




99 100

42 18.4 13.3 19.9

71 36.9 26.3 39.5



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

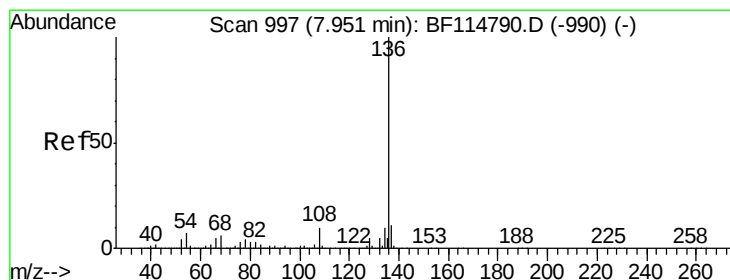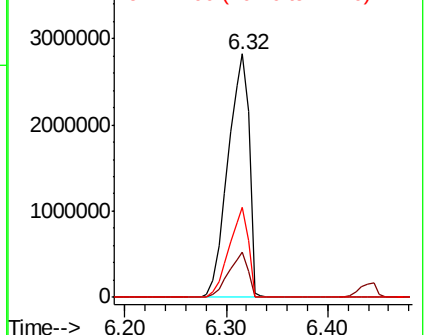

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.95 min Scan# 996

Delta R.T. -0.01 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30

Tgt Ion:136 Resp: 1785464


Ion Ratio Lower Upper

136 100



137 11.8 9.1 13.7


54 7.4 5.4 8.0

68 6.3 4.6 6.8



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1




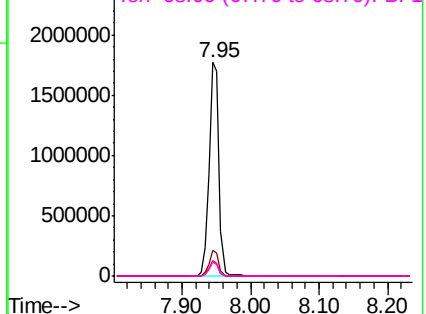


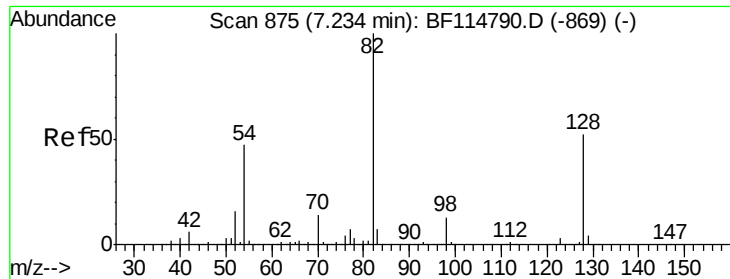

#23
Nitrobenzene-d5
Concen: 91.050 ng
RT: 7.23 min Scan# 875
Delta R.T. -0.00 min
Lab File: BF114869.D
Acq: 6 Jun 2019 18:30




Instrument :
BNA_F
ClientSampleId :
RBR-200052


Tot Ion: 82 Resp: 2640855
Ion Ratio Lower Upper
82 100
128 52.7 41.8 62.6
54 47.2 37.9 56.9

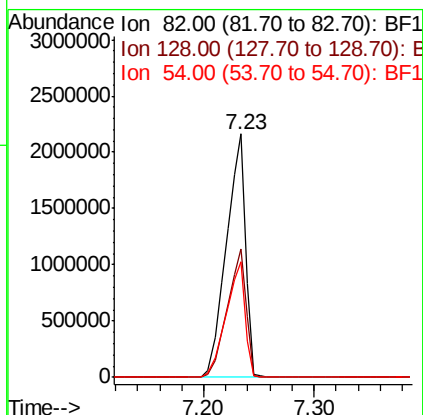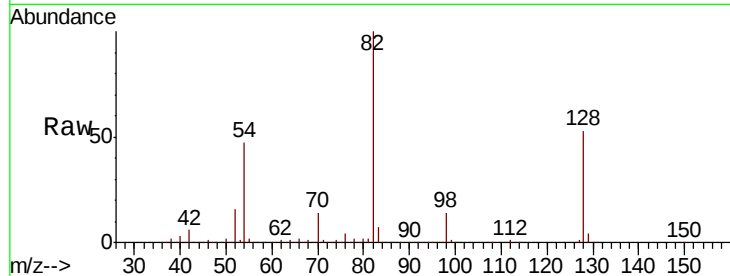

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.70 min Scan# 1294
Delta R.T. 0.00 min
Lab File: BF114869.D
Acq: 6 Jun 2019 18:30

Tgt Ion:164 Resp: 922713
Ion Ratio Lower Upper
164 100
162 102.1 82.3 123.5
160 46.7 36.7 55.1

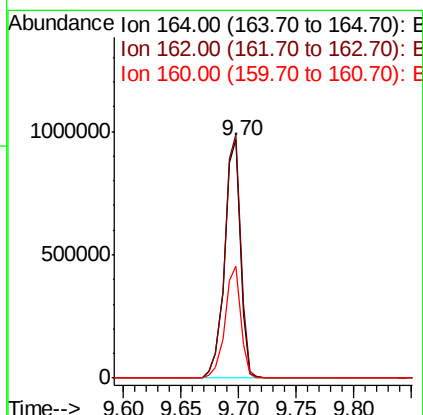



#42

2,4,6-Tribromophenol

Concen: 125.598 ng

RT: 10.49 min Scan# 1428

Delta R.T. 0.01 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30

Instrument :

BNA_F

ClientSampleId :

RBR-200052


Tot Ion:330 Resp: 1248904

Ion Ratio Lower Upper




330 100

332 95.8 77.3 115.9

141 31.1 26.2 39.4

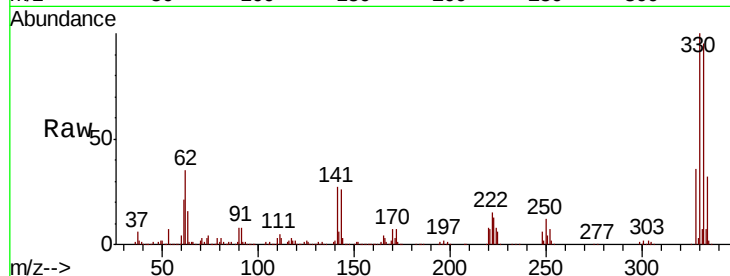

Abundance Ion 329.80 (329.50 to 330.50): E
1500000 Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

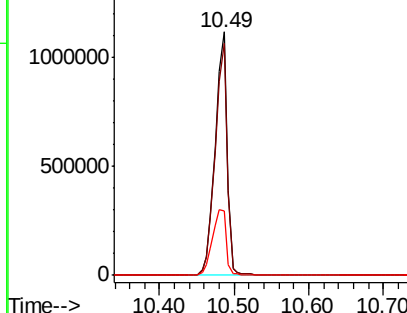

#45

2-Fluorobiphenyl

Concen: 86.846 ng

RT: 9.03 min Scan# 1180

Delta R.T. -0.00 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30


Tgt Ion:172 Resp: 4277735

Ion Ratio Lower Upper



172 100


171 40.2 32.3 48.5

170 27.3 22.4 33.6



Abundance Ion 172.00 (171.70 to 172.70): E
4000000 Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

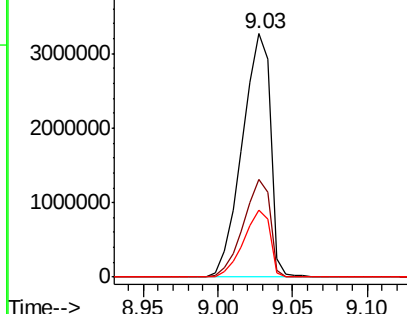

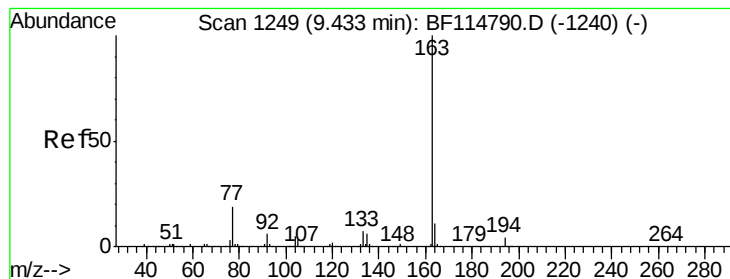

#50

Dimethylphthalate

Concen: 15.361 ng

RT: 9.42 min Scan# 1246

Delta R.T. -0.02 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30

Instrument :

BNA_F

ClientSampleId :

RBR-200052


Tot Ion:163 Resp: 1035199

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.2




164 10.9 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

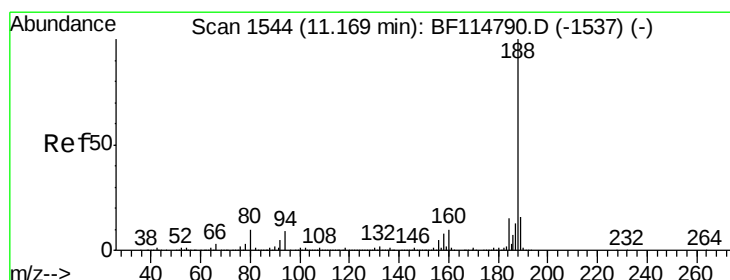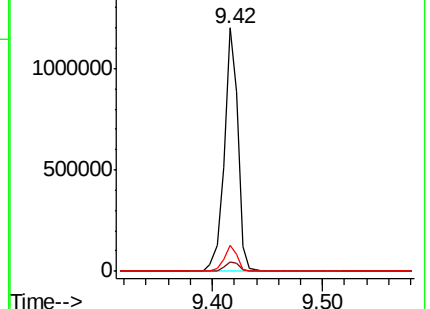

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.17 min Scan# 1544

Delta R.T. 0.00 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30


Tgt Ion:188 Resp: 1726520

Ion Ratio Lower Upper

188 100

94 10.5 7.6 11.4



80 11.2 8.3 12.5




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

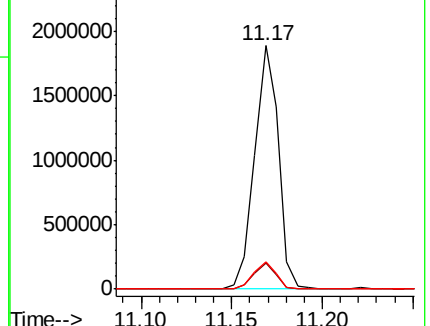



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.79 min Scan# 1990

Delta R.T. 0.00 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30

Instrument :

BNA_F

ClientSampleId :

RBR-200052


Tot Ion:240 Resp: 1086749

Ion Ratio Lower Upper

240 100

120 11.9 9.0 13.4




236 27.8 21.4 32.0

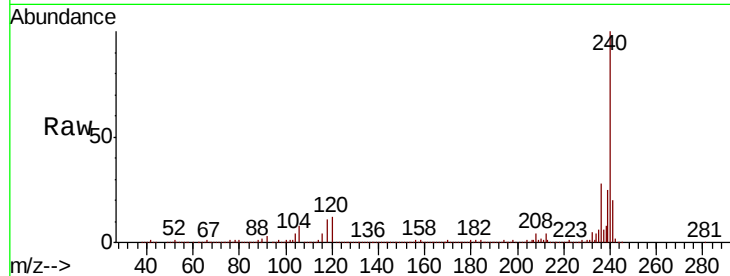

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

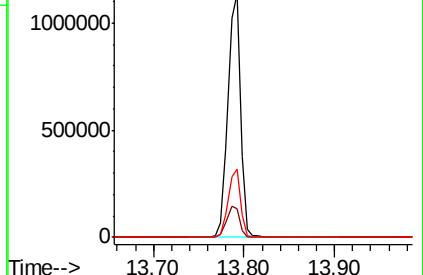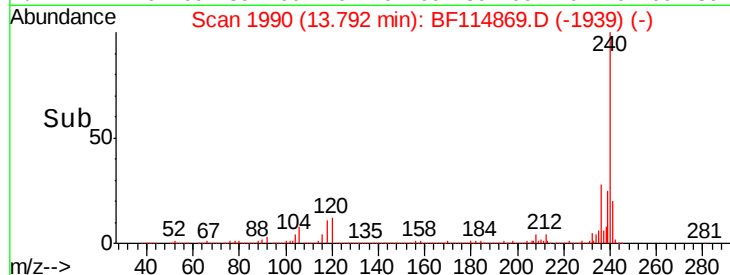

#79

Terphenyl-d14

Concen: 73.979 ng

RT: 12.76 min Scan# 1814

Delta R.T. 0.01 min

Lab File: BF114869.D

Acq: 6 Jun 2019 18:30


Tgt Ion:244 Resp: 4134006

Ion Ratio Lower Upper

244 100

212 7.9 6.5 9.7



122 12.7 10.5 15.7






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

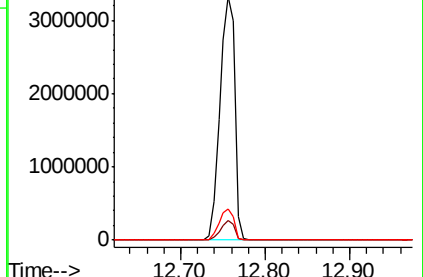

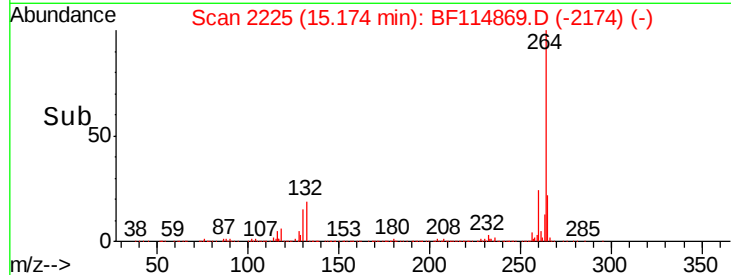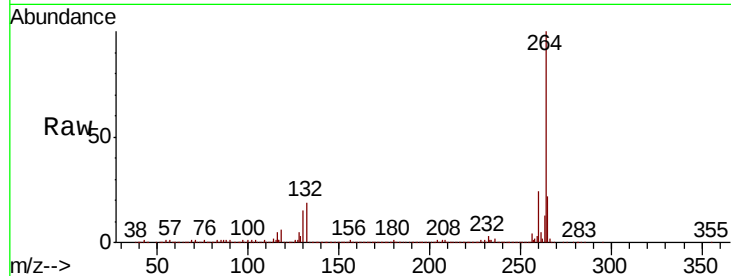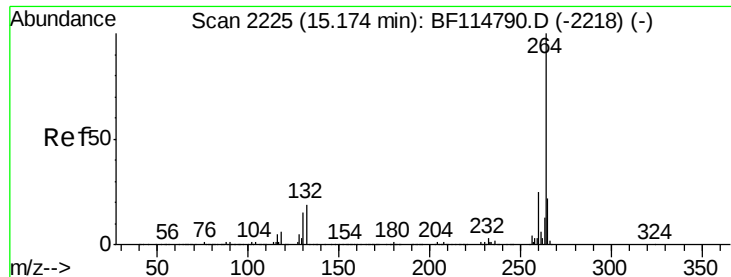

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.17 min Scan# 2225
Delta R.T. 0.00 min
Lab File: BF114869.D
Acq: 6 Jun 2019 18:30

Instrument :
BNA_F
ClientSampleId :
RBR-200052

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	20.1	30.1
265	22.1	17.7	26.5

