


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060619\
 Data File : BF114847.D
 Acq On : 6 Jun 2019 8:12
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 04 16:57:15 2019

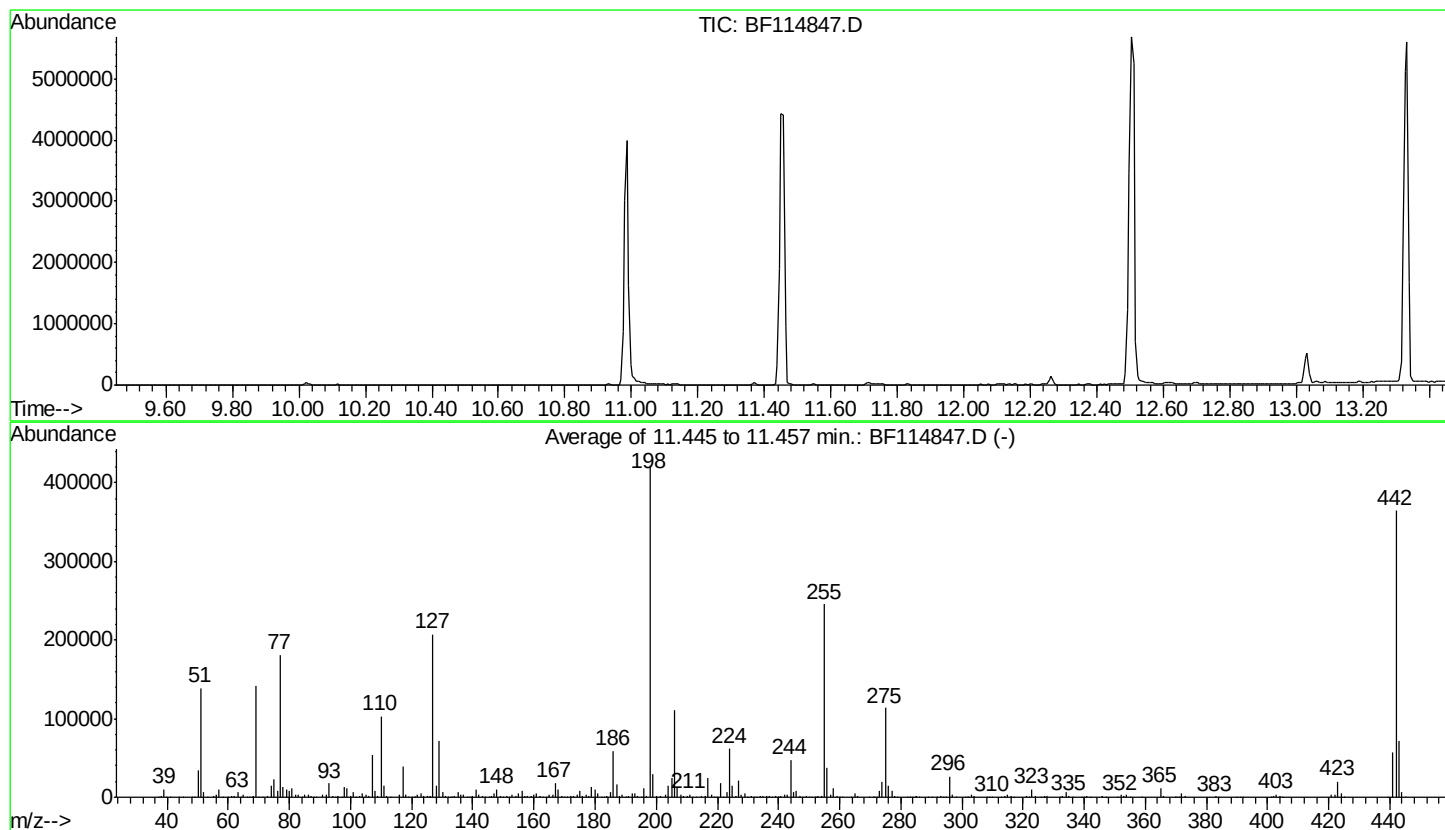

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	138488	PASS
68	69	0.00	2	1.3	1887	PASS
69	198	0.00	100	33.7	142341	PASS
70	69	0.00	2	0.6	829	PASS
127	198	10	80	49.1	207213	PASS
197	198	0.00	2	0.5	2004	PASS
198	198	100	100	100.0	421952	PASS
199	198	5	9	6.9	28994	PASS
275	198	10	60	27.0	113949	PASS
365	198	1	100	2.9	12062	PASS
441	198	0.01	100	13.4	56743	PASS
442	198	50	100	86.4	364533	PASS
443	442	15	24	19.5	70933	PASS