

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
 Data File : BF133587.D
 Acq On : 06 Jun 2023 12:38
 Operator : CG\JU
 Sample : PB153153BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153153BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.081	502	509	515	rBV	49640	69693	1.40%	0.230%
2	5.457	567	573	576	rBV	3680474	4000067	80.33%	13.205%
3	6.463	738	744	747	rBV	3302029	4079819	81.94%	13.468%
4	6.834	803	807	810	rBV	1104904	860576	17.28%	2.841%
5	7.398	897	903	906	rBV	2566983	2648924	53.20%	8.745%
6	8.116	1020	1025	1028	rBV	1387351	1125078	22.60%	3.714%
7	9.198	1203	1209	1212	rBV	4993359	4434602	89.06%	14.639%
8	9.875	1320	1324	1327	rVB	1524060	1219361	24.49%	4.025%
9	10.663	1453	1458	1462	rBV	2947261	3049698	61.25%	10.068%
10	11.363	1573	1577	1580	rBV	1590518	1362841	27.37%	4.499%
11	12.957	1843	1848	1851	rBV	4870486	4979251	100.00%	16.437%
12	14.004	2022	2026	2030	rBV	1352654	1240506	24.91%	4.095%
13	15.468	2269	2275	2279	rBV	1019030	1221865	24.54%	4.034%




Sum of corrected areas: 30292281

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133587.D
Acq On : 06 Jun 2023 12:38
Operator : CG\JU
Sample : PB153153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153153BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

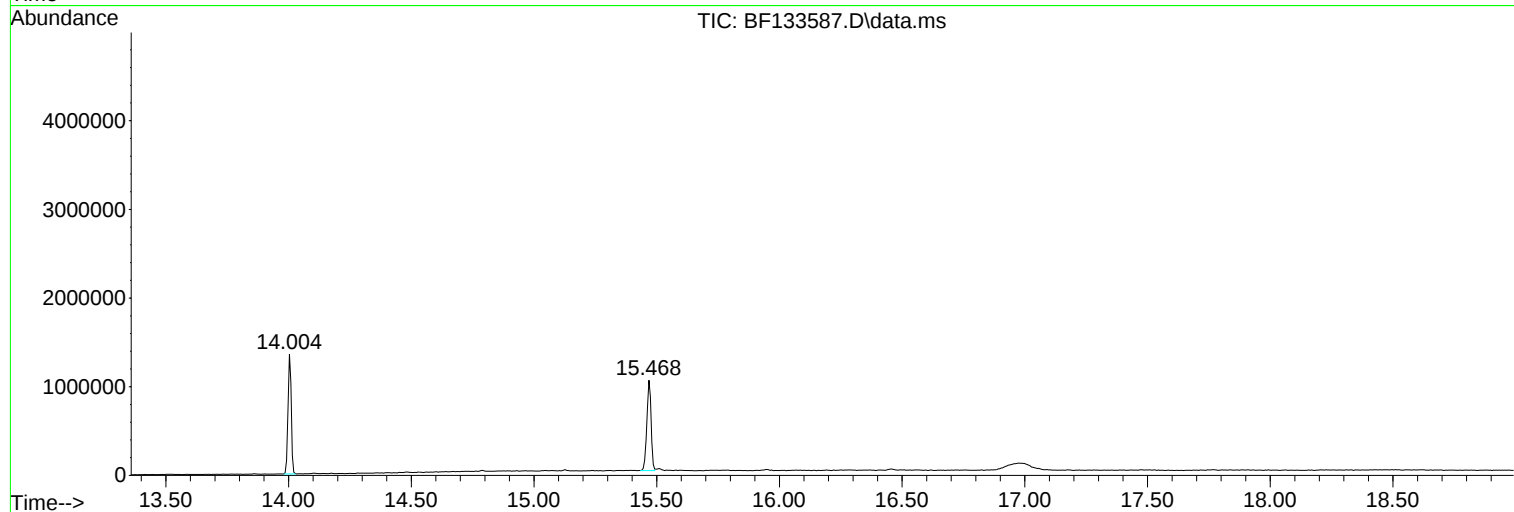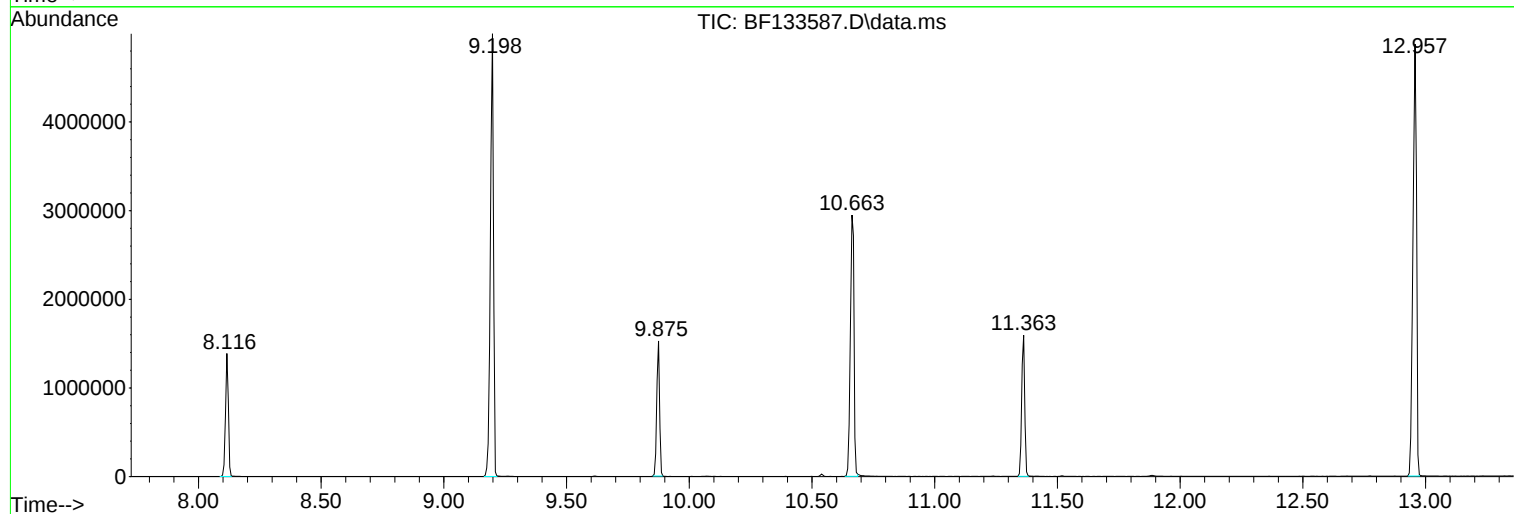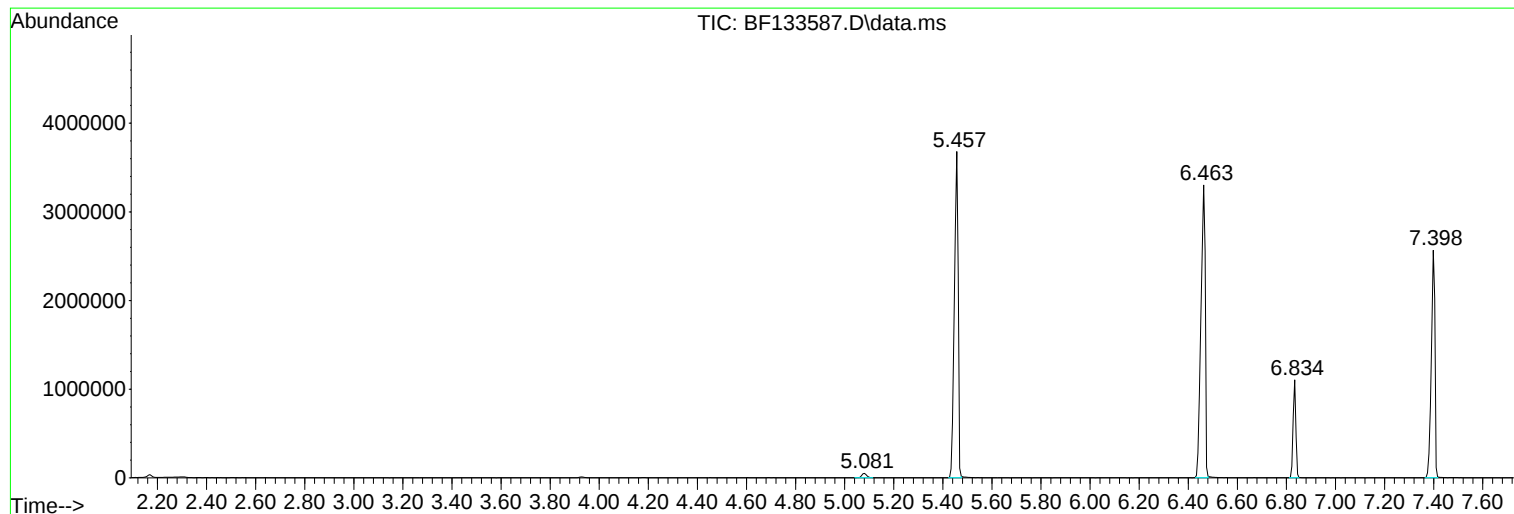

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133587.D
Acq On : 06 Jun 2023 12:38
Operator : CG\JU
Sample : PB153153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153153BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133587.D
Acq On : 06 Jun 2023 12:38
Operator : CG\JU
Sample : PB153153BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153153BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------