

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
 Data File : BF133606.D
 Acq On : 07 Jun 2023 00:36
 Operator : CG\JU
 Sample : PB153188BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153188BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	504	508	514	rVB	43079	56755	1.58%	0.265%
2	5.457	567	573	576	rBV	3401157	3468999	96.60%	16.189%
3	6.469	739	745	759	rBV	3098029	3538679	98.54%	16.515%
4	6.834	804	807	811	rBV	959574	754314	21.00%	3.520%
5	7.404	898	904	907	rBV	2253218	2148986	59.84%	10.029%
6	8.122	1022	1026	1029	rBV	1064851	930829	25.92%	4.344%
7	9.198	1205	1209	1212	rBV	4226308	3591159	100.00%	16.759%
8	9.875	1320	1324	1327	rBV	1119167	856911	23.86%	3.999%
9	10.663	1454	1458	1462	rBV	1953822	1711968	47.67%	7.990%
10	11.363	1573	1577	1581	rBV	989230	769933	21.44%	3.593%
11	12.957	1843	1848	1851	rBV	3109619	2762321	76.92%	12.891%
12	14.010	2023	2027	2030	rBV	500355	459076	12.78%	2.142%
13	15.474	2271	2276	2280	rBV	297307	377698	10.52%	1.763%




Sum of corrected areas: 21427628

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133606.D
Acq On : 07 Jun 2023 00:36
Operator : CG\JU
Sample : PB153188BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

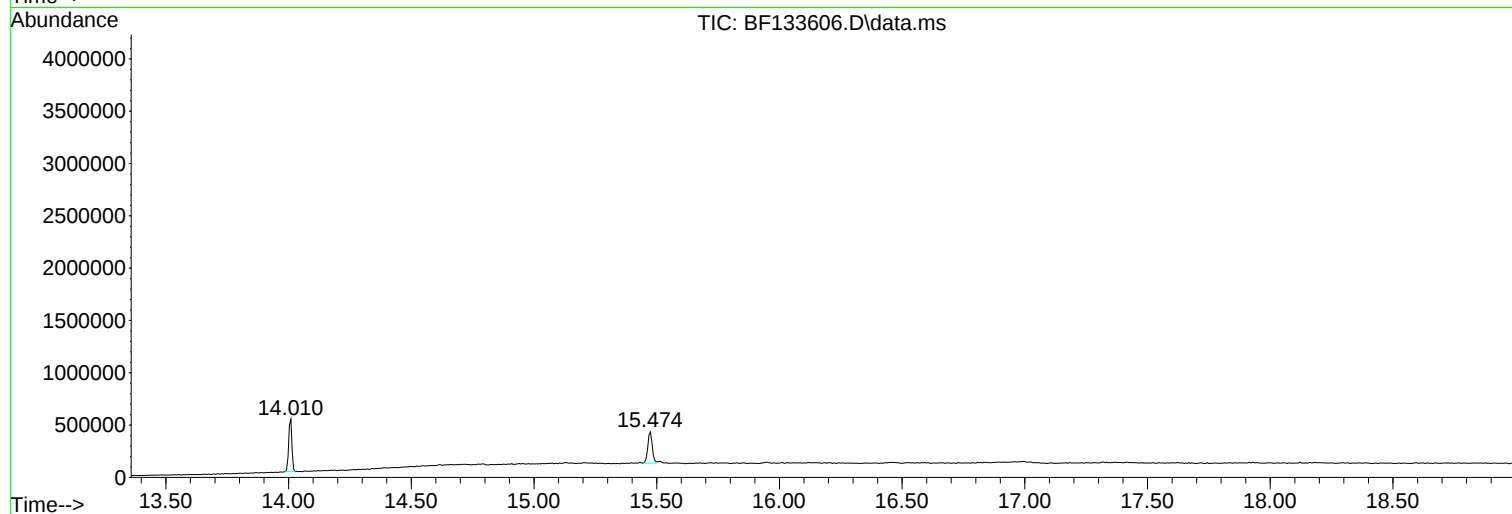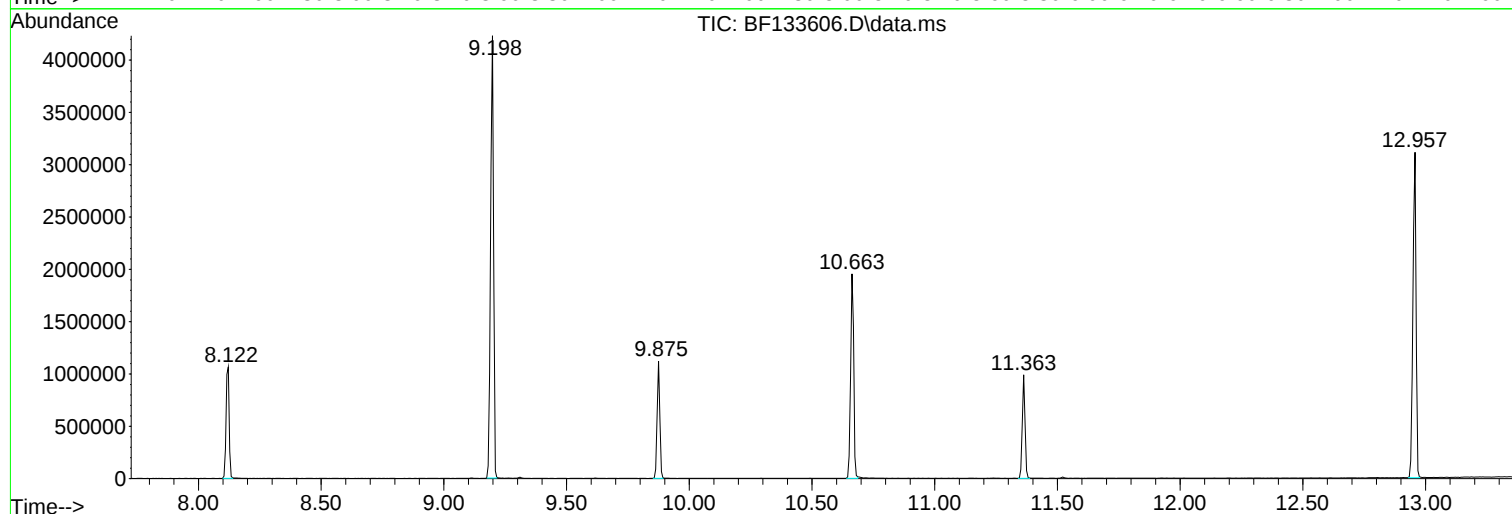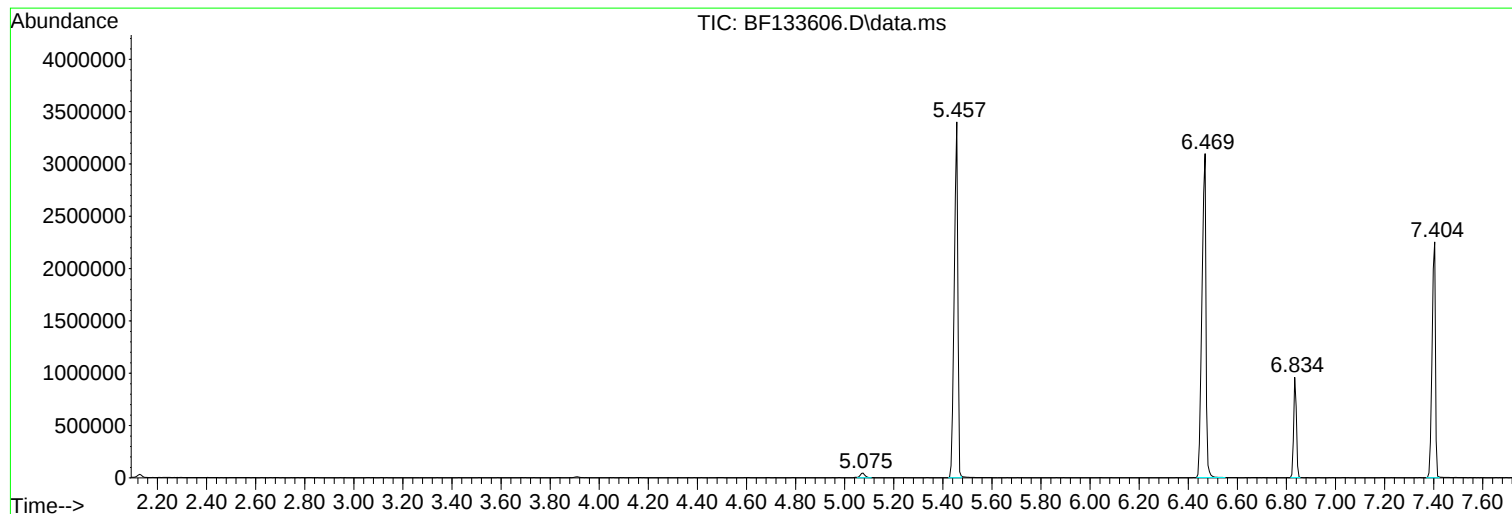

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133606.D
Acq On : 07 Jun 2023 00:36
Operator : CG\JU
Sample : PB153188BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133606.D
Acq On : 07 Jun 2023 00:36
Operator : CG\JU
Sample : PB153188BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------