


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
 Data File : BF133585.D
 Acq On : 06 Jun 2023 09:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 14:05:12 2023

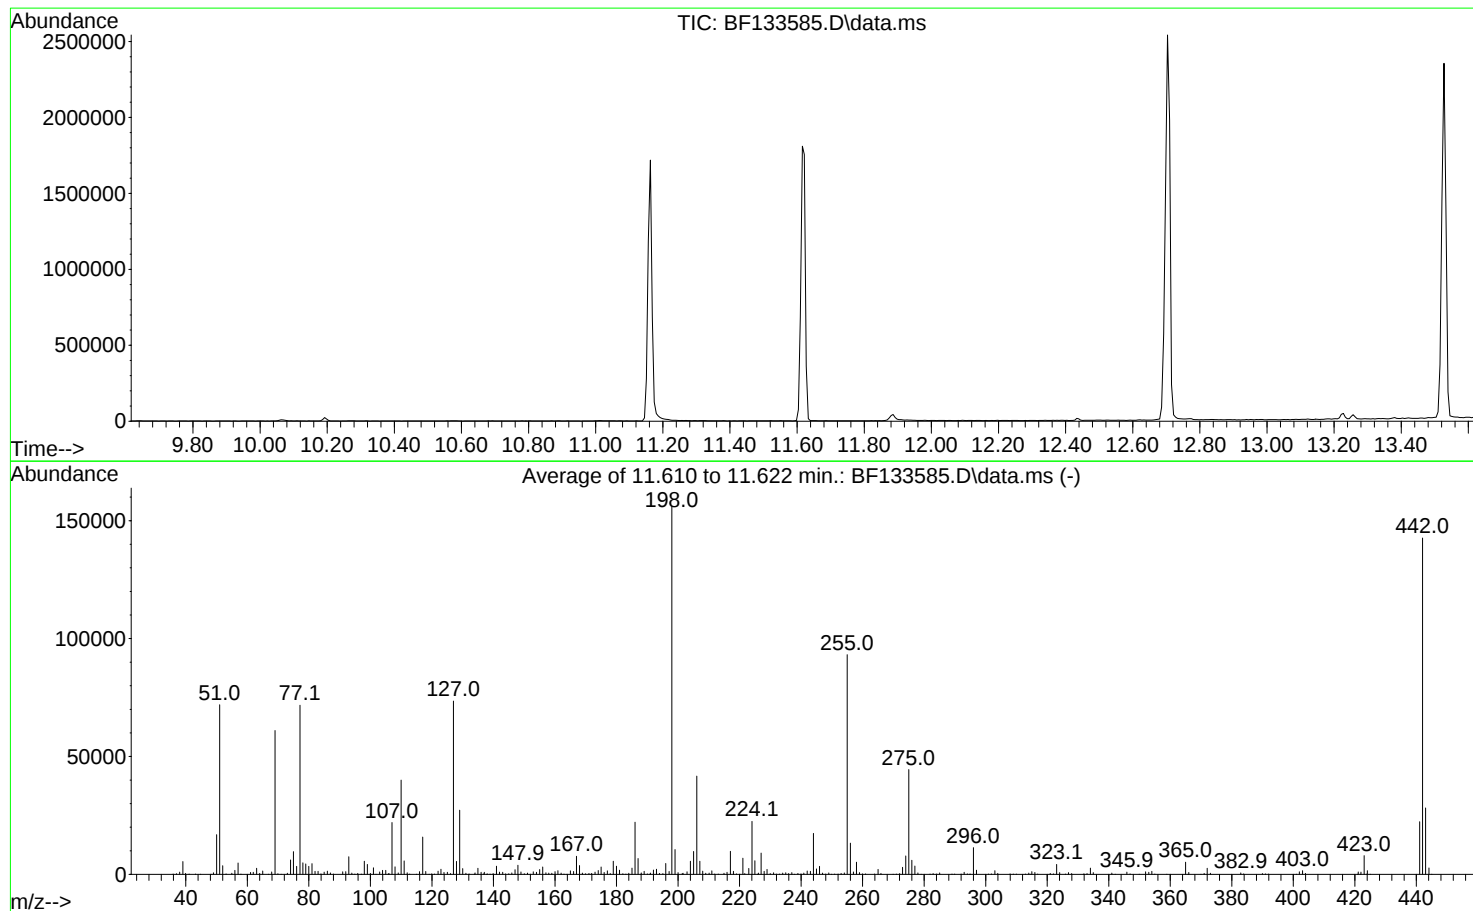

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	71941	PASS
68	69	0.00	2	1.7	1025	PASS
69	198	0.00	100	39.1	61045	PASS
70	69	0.00	2	0.4	259	PASS
127	198	10	80	47.1	73477	PASS
197	198	0.00	2	0.8	1227	PASS
198	198	100	100	100.0	156019	PASS
199	198	5	9	6.8	10549	PASS
275	198	10	60	28.5	44437	PASS
365	198	1	100	3.3	5160	PASS
441	198	0.01	100	14.3	22300	PASS
442	442	50	100	100.0	142627	PASS
443	442	15	24	19.7	28165	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_F	<u>BF133585.D</u>
Compound Name	Response	Retention Time
DDT	392172	13.527
DDD	11219	13.227
DDE	186	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11405	403577	2.83

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133585.D
Acq On : 06 Jun 2023 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 06 09:41:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 17:49:53 2023
Response via : Initial Calibration

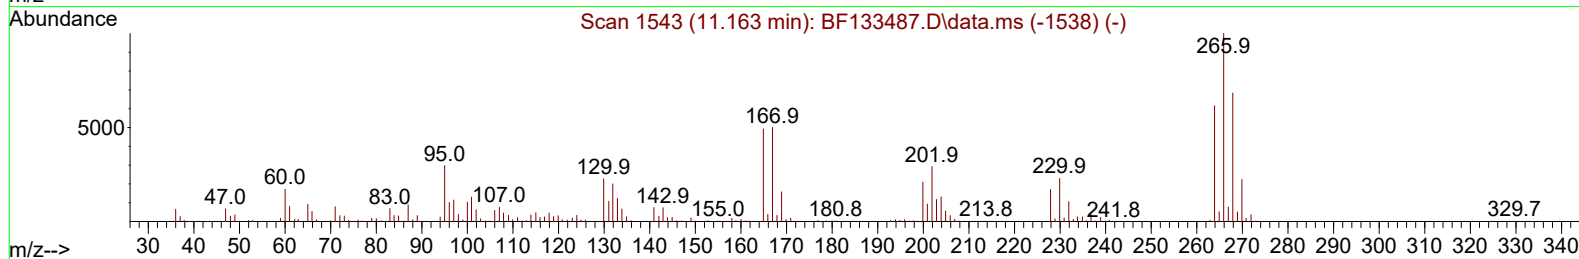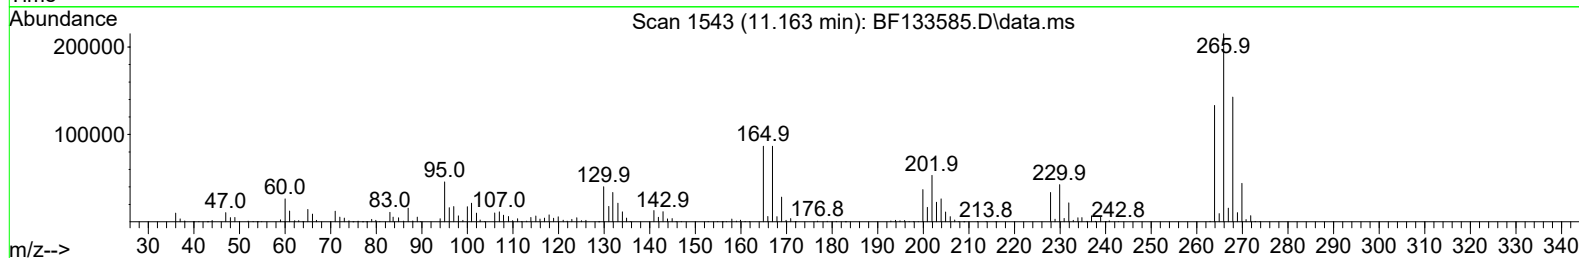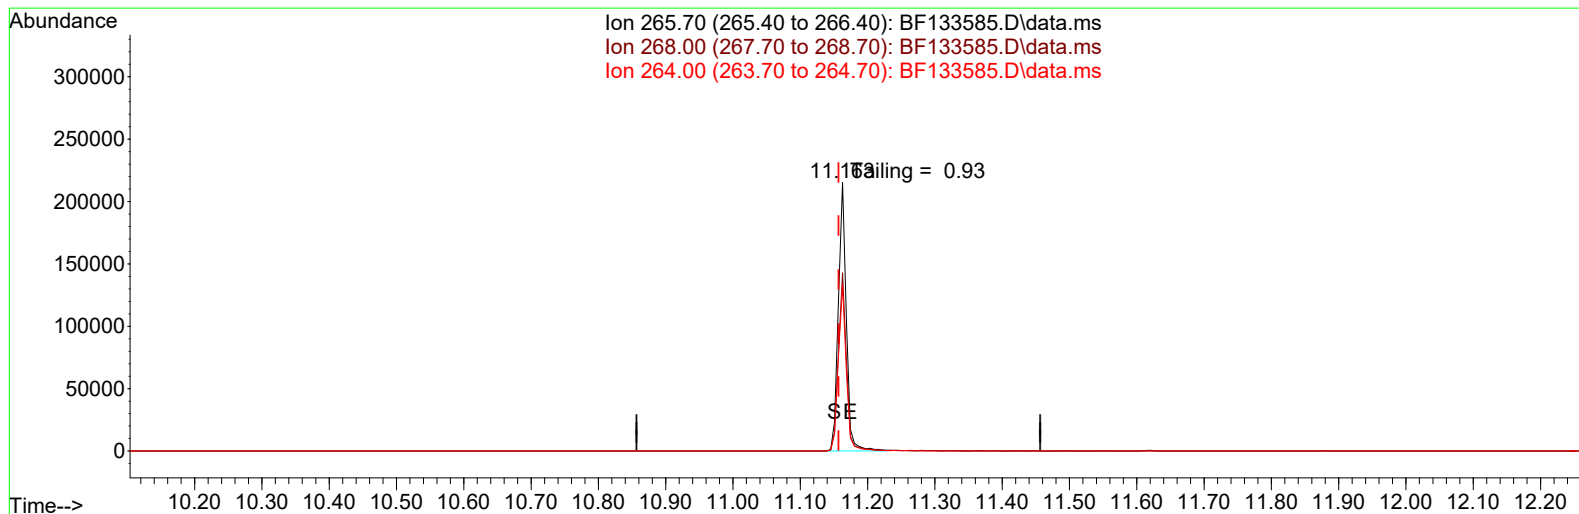

TIC: BF133585.D\data.ms

(70) Pentachlorophenol (C)

11.163min (+ 0.006) 32357.47 ng




response 178342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	66.36
264.00	61.50	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133585.D
Acq On : 06 Jun 2023 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 06 09:41:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 17:49:53 2023
Response via : Initial Calibration

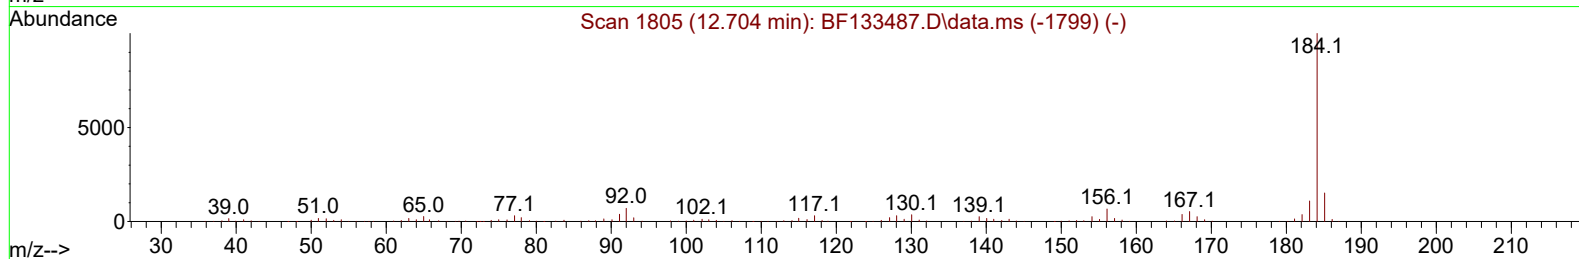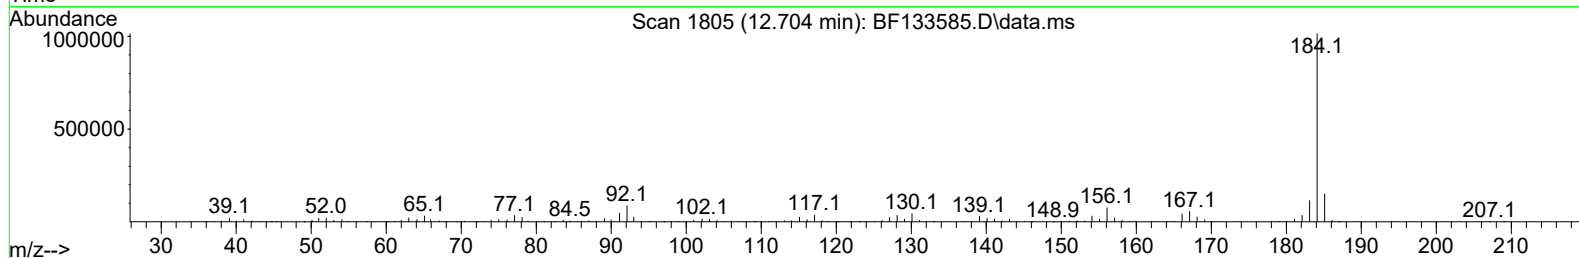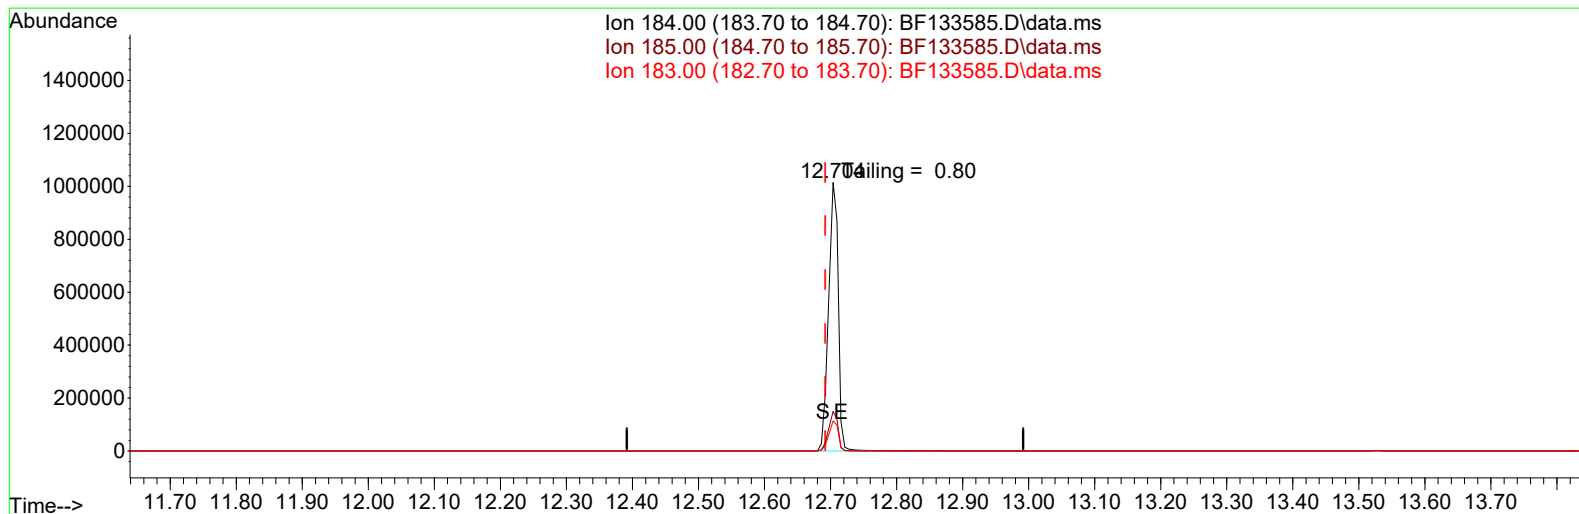

TIC: BF133585.D\data.ms

(77) Benzidine

12.704min (+ 0.012) 505894.81 ng

response 1020939

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.76
183.00	10.90	11.22
0.00	0.00	0.00