


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
 Data File : BF133604.D
 Acq On : 06 Jun 2023 23:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 14:05:12 2023

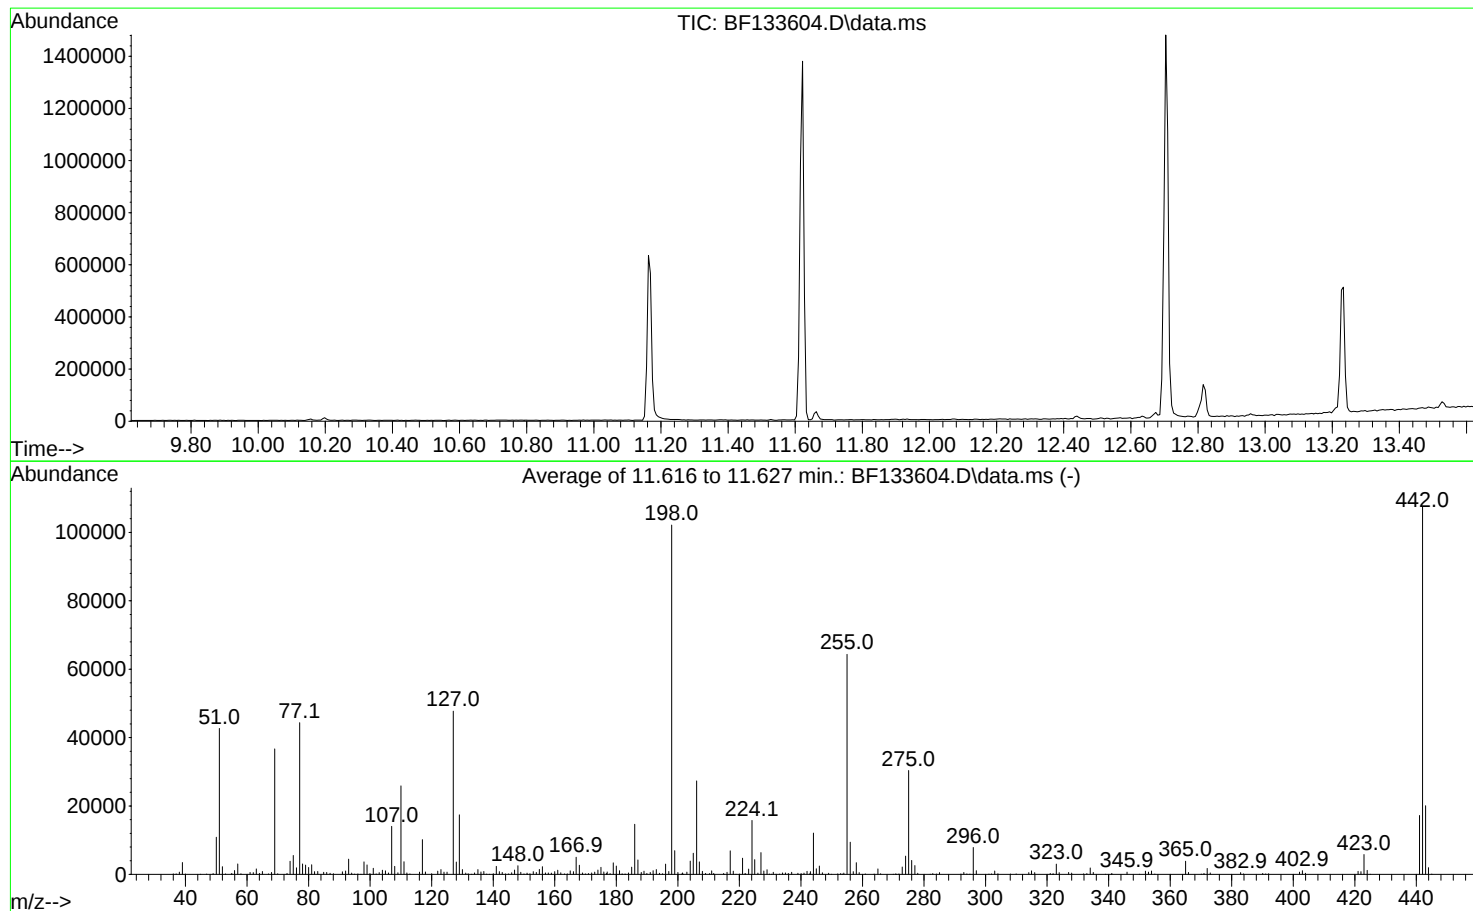

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	42670	PASS
68	69	0.00	2	1.6	574	PASS
69	198	0.00	100	35.9	36664	PASS
70	69	0.00	2	0.5	196	PASS
127	198	10	80	46.7	47702	PASS
197	198	0.00	2	0.8	852	PASS
198	198	100	100	100.0	102112	PASS
199	198	5	9	6.8	6927	PASS
275	198	10	60	29.7	30347	PASS
365	198	1	100	3.8	3860	PASS
441	198	0.01	100	16.9	17223	PASS
442	442	50	100	100.0	107565	PASS
443	442	15	24	18.7	20092	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_F	<u>BF133604.D</u>
Compound Name	Response	Retention Time
DDT	3322	13.527
DDD	90483	13.233
DDE	0	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
90483	93805	96.46

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133604.D
Acq On : 06 Jun 2023 23:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 07:46:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 14:05:12 2023
Response via : Initial Calibration

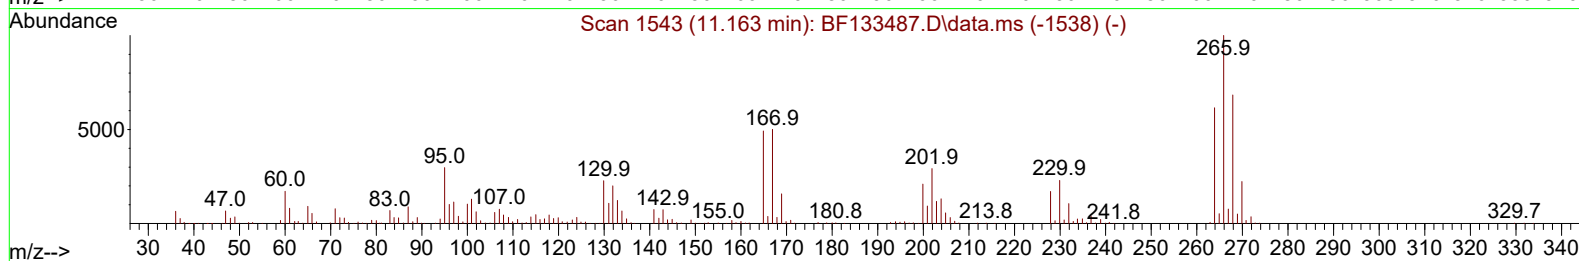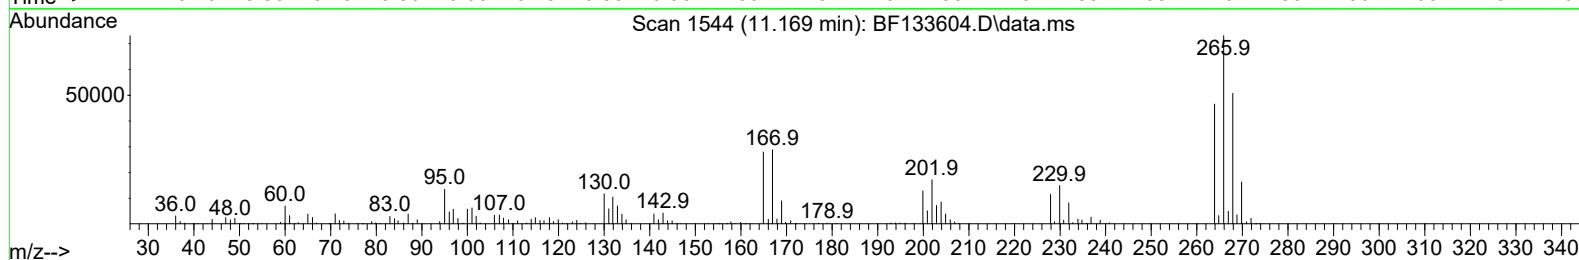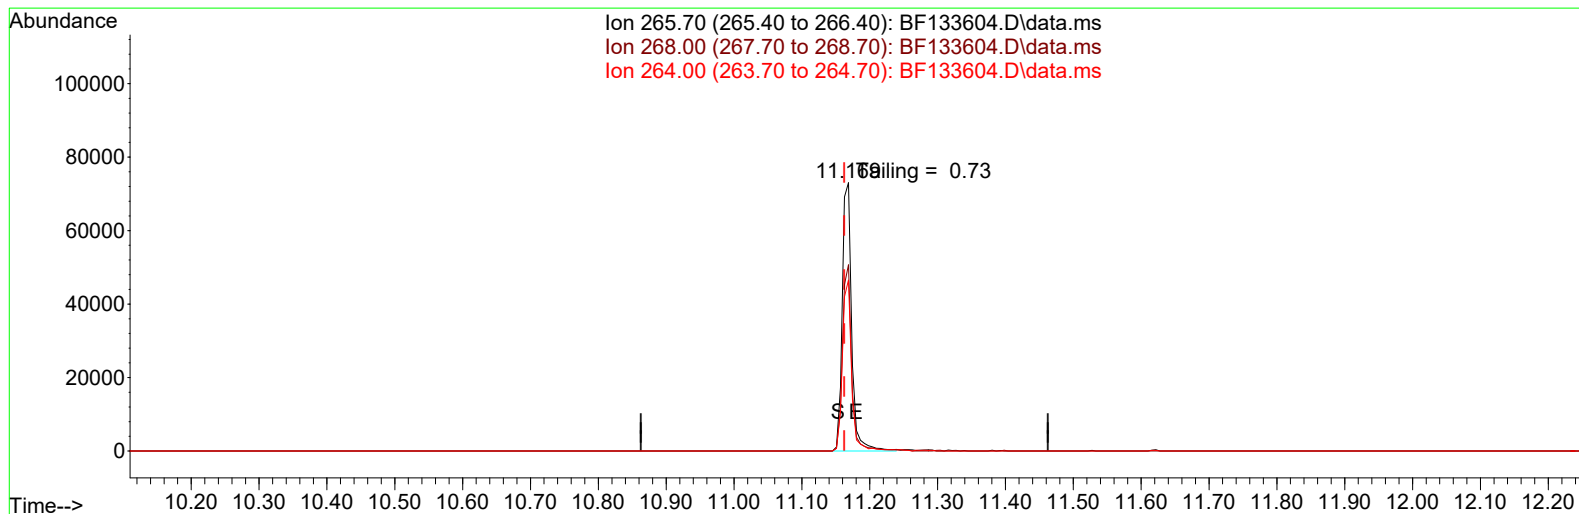

TIC: BF133604.D\data.ms

(70) Pentachlorophenol (C)

11.169min (+ 0.006) 30862.43 ng




response 70705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	69.39
264.00	61.50	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060623\
Data File : BF133604.D
Acq On : 06 Jun 2023 23:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 07:46:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 14:05:12 2023
Response via : Initial Calibration

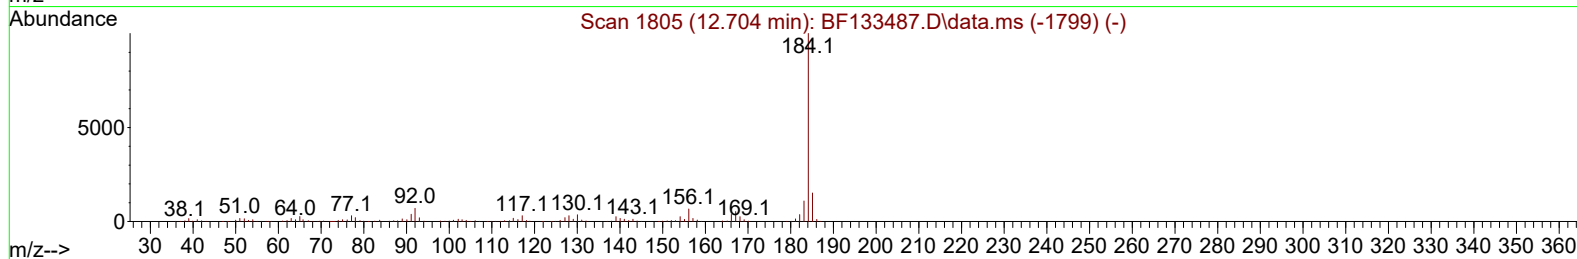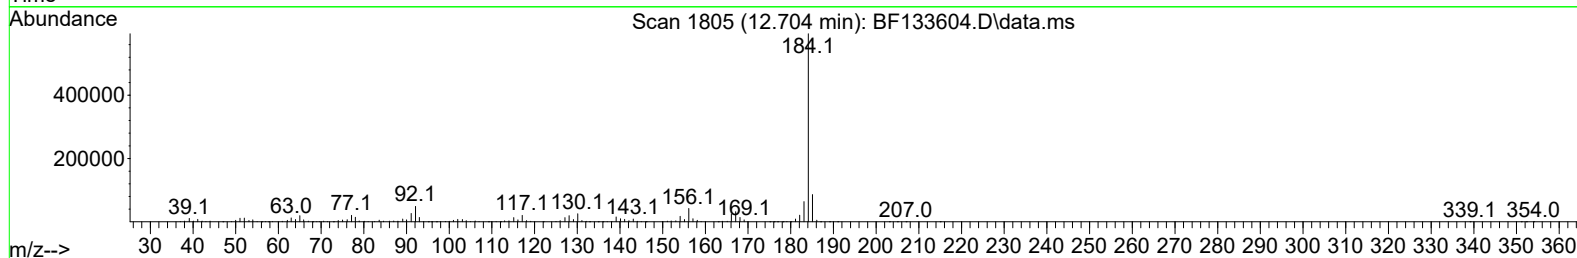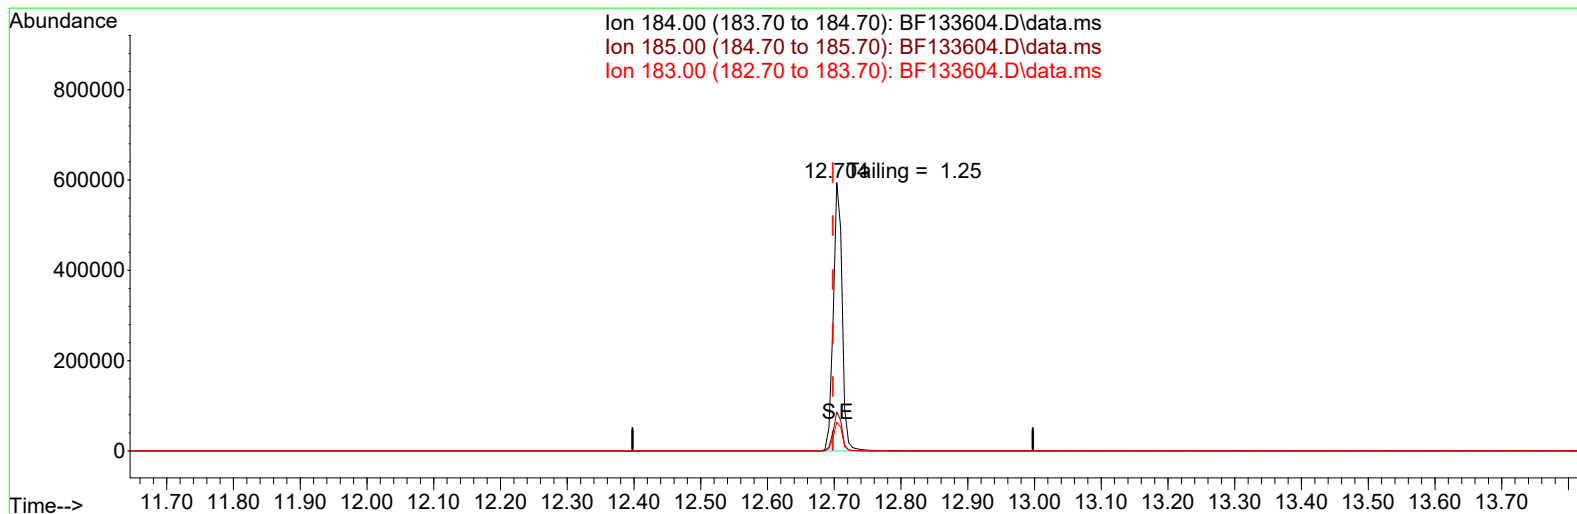

TIC: BF133604.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 29107.96 ng

response 553370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.54
183.00	10.90	10.76
0.00	0.00	0.00