

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
 Data File : BF142674.D
 Acq On : 07 Jun 2025 06:35
 Operator : RC/JU
 Sample : Q2227-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP07-MHH-WC

Quant Time: Jun 09 01:02:28 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 20 16:26:47 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.893	152	127322	20.000	ng	-0.01
21) Naphthalene-d8	8.175	136	485551	20.000	ng	-0.01
39) Acenaphthene-d10	9.933	164	232600	20.000	ng	-0.01
64) Phenanthrene-d10	11.422	188	313857	20.000	ng	-0.01
76) Chrysene-d12	14.063	240	258549	20.000	ng	-0.01
86) Perylene-d12	15.557	264	270848	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	514287	68.052	ng	0.00
7) Phenol-d6	6.516	99	639693	70.318	ng	-0.02
23) Nitrobenzene-d5	7.451	82	371998	41.776	ng	-0.02
42) 2,4,6-Tribromophenol	10.722	330	148605	57.564	ng	-0.02
45) 2-Fluorobiphenyl	9.251	172	786562	45.377	ng	-0.02
79) Terphenyl-d14	13.004	244	551285	29.138	ng	-0.01
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.451	70	50135	8.892	ng	# 76
25) Isophorone	7.451	82	358226	24.062	ng	# 63
51) 2,6-Dinitrotoluene	9.933	165	29875	9.019	ng	# 27
57) 2,4-Dinitrotoluene	9.933	165	29875	6.906	ng	# 28
63) Azobenzene	10.645	77	37688	2.799	ng	# 1
67) 4-Bromophenyl-phenylether	10.722	248	9119	2.457	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
Data File : BF142674.D
Acq On : 07 Jun 2025 06:35
Operator : RC/JU
Sample : Q2227-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC

Quant Time: Jun 09 01:02:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration



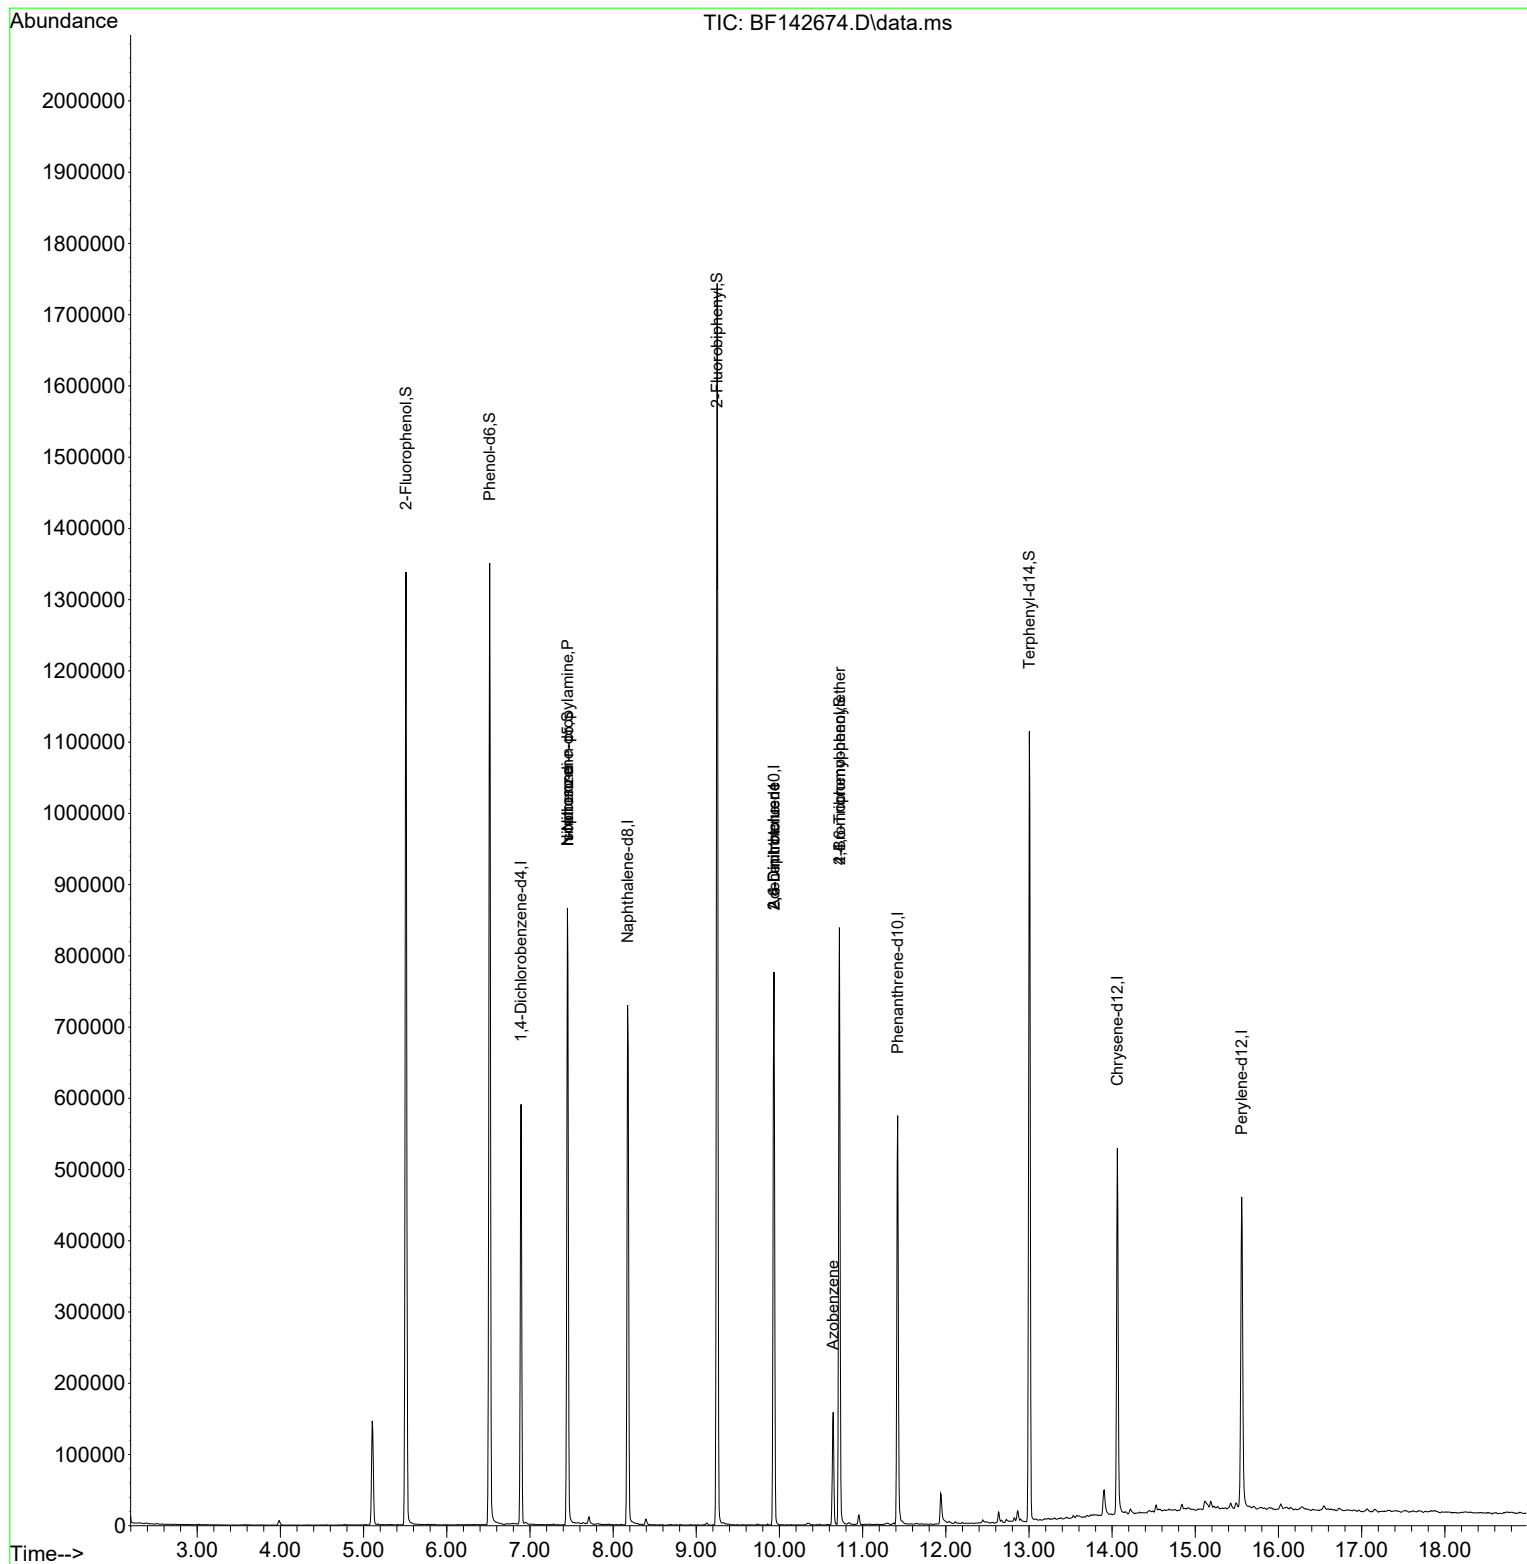




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.893 min Scan# 79
Delta R.T. -0.011 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC

Tgt Ion:152 Resp: 127322
Ion Ratio Lower Upper
152 100
150 158.0 128.2 192.4
115 56.4 48.3 72.5

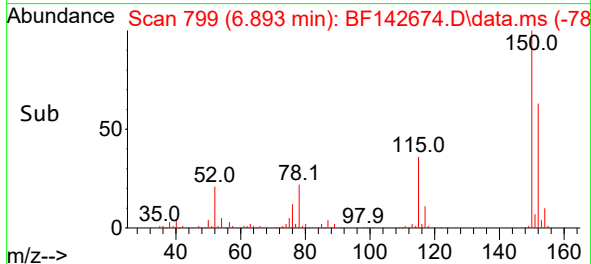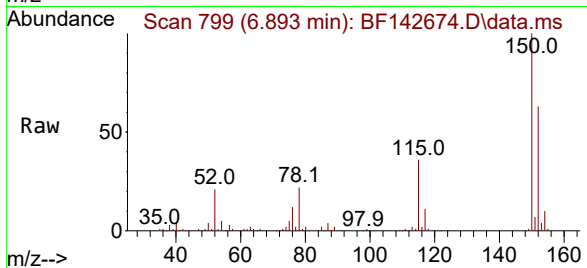

#5
2-Fluorophenol
Concen: 68.052 ng
RT: 5.510 min Scan# 564
Delta R.T. -0.006 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion:112 Resp: 514287
Ion Ratio Lower Upper
112 100
64 58.0 47.5 71.3
63 29.6 24.9 37.3


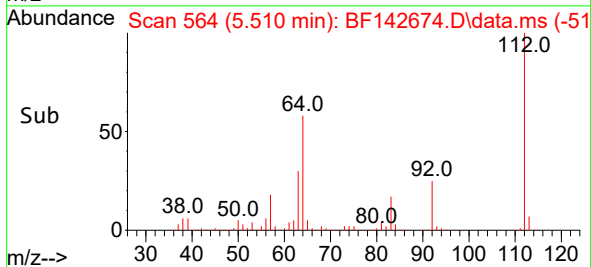

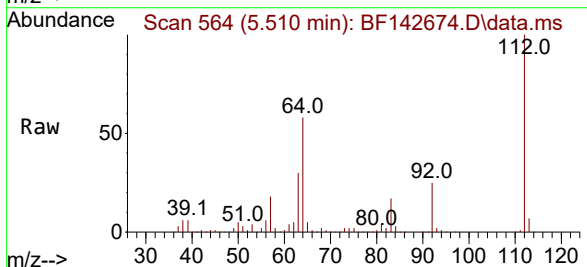




#7
Phenol-d6
Concen: 70.318 ng
RT: 6.516 min Scan# 71
Delta R.T. -0.017 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC

Tgt Ion: 99 Resp: 639693
Ion Ratio Lower Upper
99 100
42 18.8 16.2 24.2
71 32.6 27.3 40.9

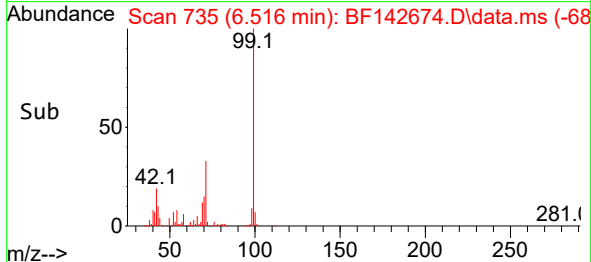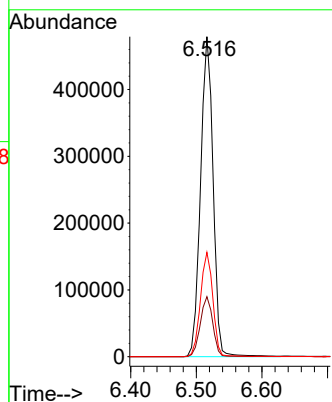

#19
n-Nitroso-di-n-propylamine
Concen: 8.892 ng
RT: 7.451 min Scan# 894
Delta R.T. 0.124 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion: 70 Resp: 50135
Ion Ratio Lower Upper
70 100
42 51.8 52.4 78.6#
101 0.0 7.8 11.8#
130 2.4 18.0 27.0#


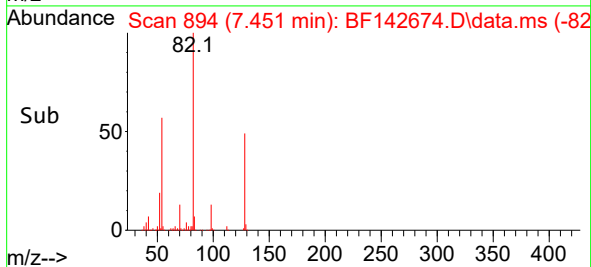

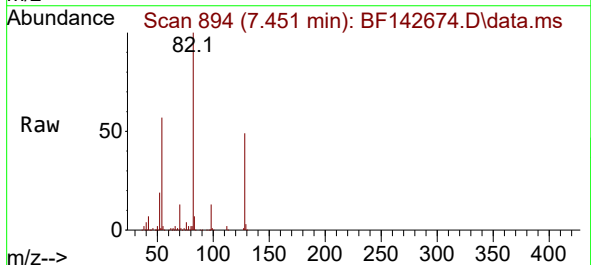




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.175 min Scan# 1017
Delta R.T. -0.012 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC

Tgt Ion:136 Resp: 485551
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 8.3 6.6 10.0
68 5.6 4.1 6.1

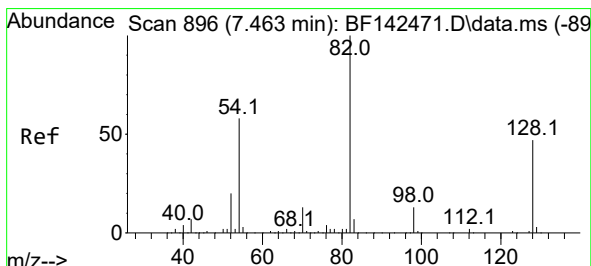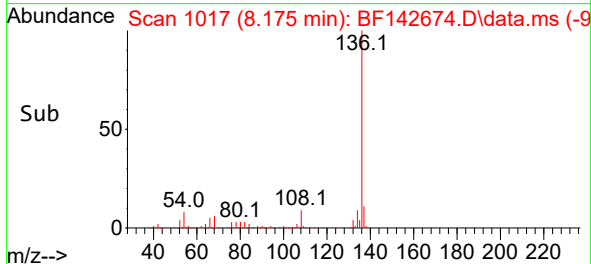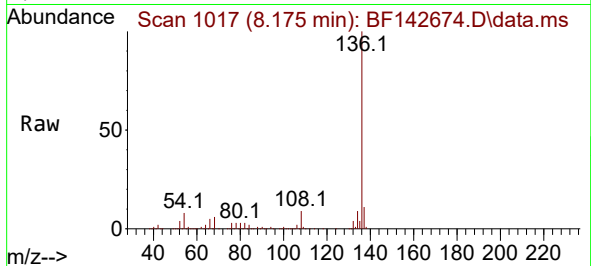

#23
Nitrobenzene-d5
Concen: 41.776 ng
RT: 7.451 min Scan# 894
Delta R.T. -0.023 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion: 82 Resp: 371998
Ion Ratio Lower Upper
82 100
128 48.9 37.4 56.2
54 57.2 46.6 70.0


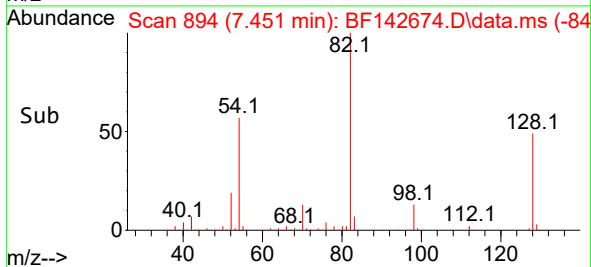

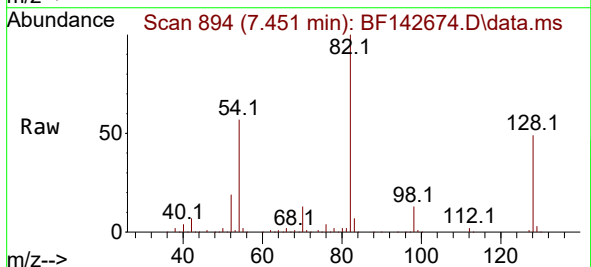




#25
Isophorone
Concen: 24.062 ng
RT: 7.451 min Scan# 894
Delta R.T. -0.282 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC


Tgt Ion: 82 Resp: 358226
Ion Ratio Lower Upper
82 100
95 0.0 6.0 9.0#
138 0.0 15.5 23.3#

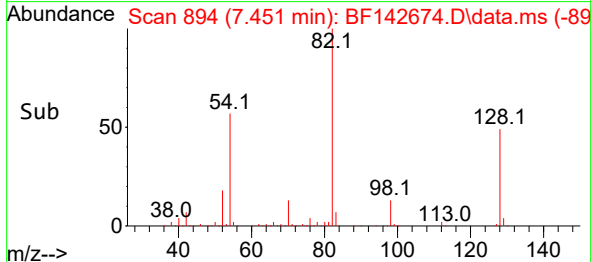

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1316
Delta R.T. -0.012 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion:164 Resp: 232600
Ion Ratio Lower Upper
164 100
162 99.7 80.2 120.4
160 44.8 35.6 53.4


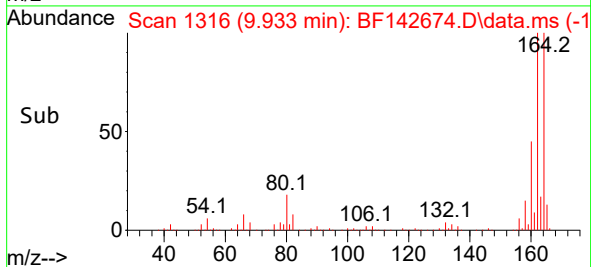

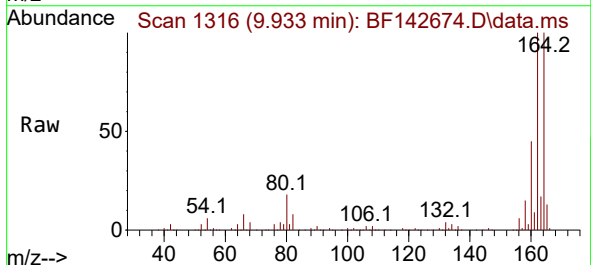


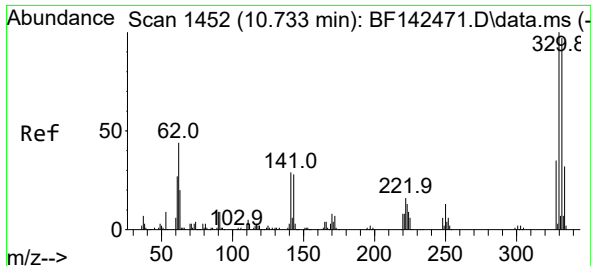

#42
2,4,6-Tribromophenol
Concen: 57.564 ng
RT: 10.722 min Scan# 1450
Delta R.T. -0.017 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC


Tgt Ion:330 Resp: 148605
Ion Ratio Lower Upper
330 100
332 97.0 77.6 116.4
141 29.1 24.6 36.8

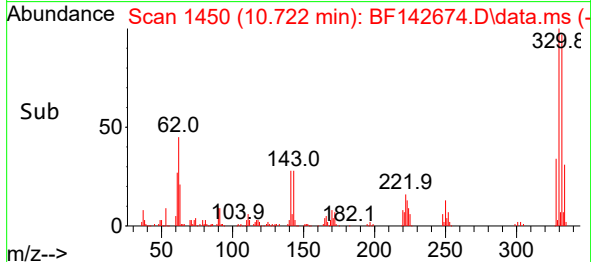

#45
2-Fluorobiphenyl
Concen: 45.377 ng
RT: 9.251 min Scan# 1200
Delta R.T. -0.017 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion:172 Resp: 786562
Ion Ratio Lower Upper
172 100
171 35.0 28.6 42.8
170 22.7 18.9 28.3

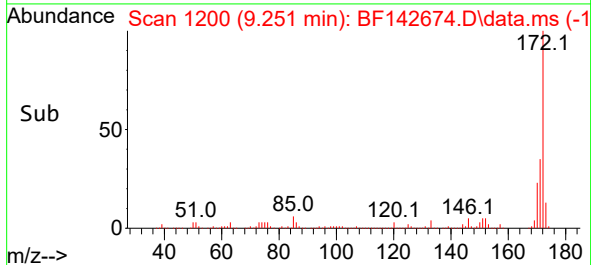

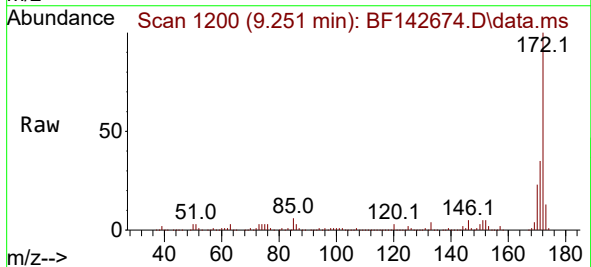


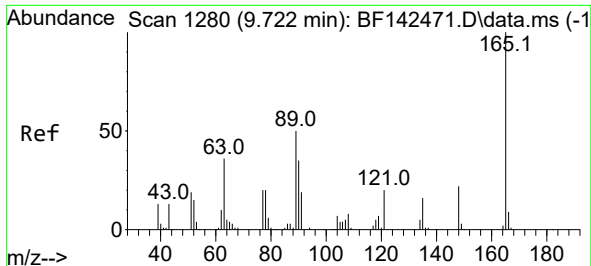

#51
2,6-Dinitrotoluene
Concen: 9.019 ng
RT: 9.933 min Scan# 1316
Delta R.T. 0.206 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC


Tgt Ion:165 Resp: 29875
Ion Ratio Lower Upper
165 100
63 0.9 42.9 64.3#
89 0.8 40.2 60.4#

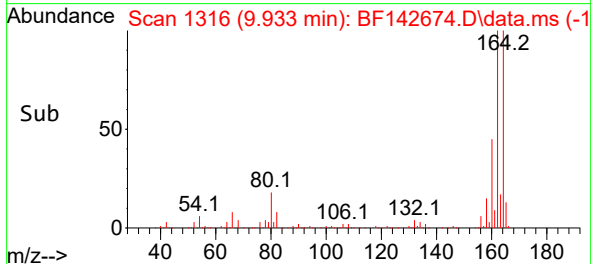

#57
2,4-Dinitrotoluene
Concen: 6.906 ng
RT: 9.933 min Scan# 1316
Delta R.T. -0.200 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion:165 Resp: 29875
Ion Ratio Lower Upper
165 100
63 0.9 33.6 50.4#
89 0.8 50.2 75.4#
182 0.0 2.2 3.4#


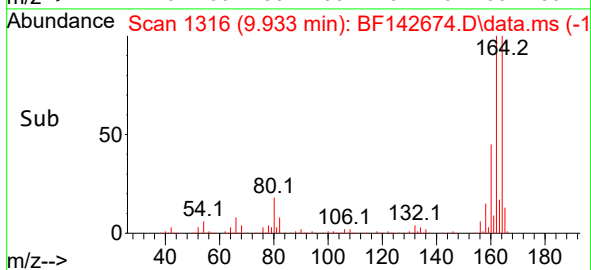

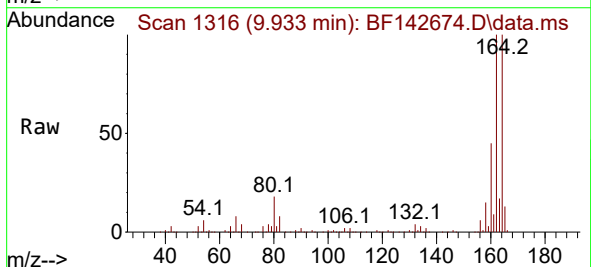


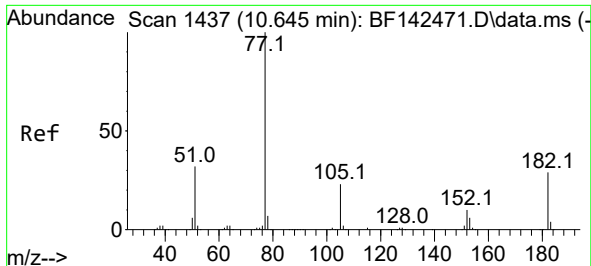

#63
Azobenzene
Concen: 2.799 ng
RT: 10.645 min Scan# 1437
Delta R.T. 0.000 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC


Tgt Ion: 77 Resp: 37688
Ion Ratio Lower Upper
77 100
182 94.3 9.0 49.0#
105 169.8 2.4 42.4#
51 42.8 13.5 53.5

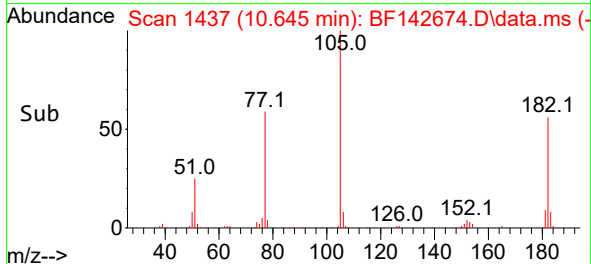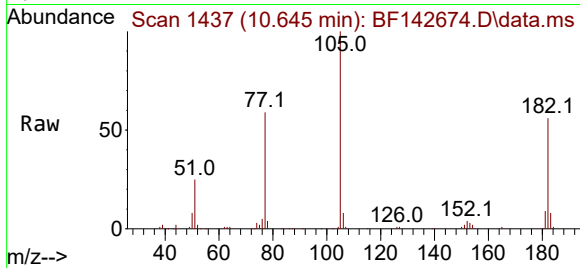

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.422 min Scan# 1569
Delta R.T. -0.012 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion:188 Resp: 313857
Ion Ratio Lower Upper
188 100
94 8.9 6.6 10.0
80 9.3 7.4 11.0


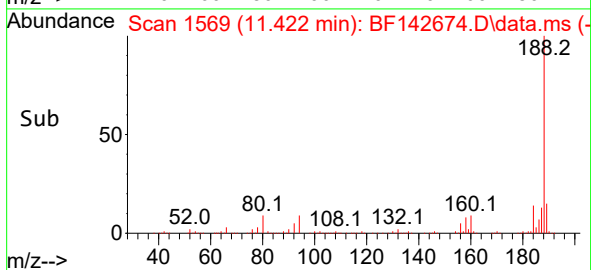

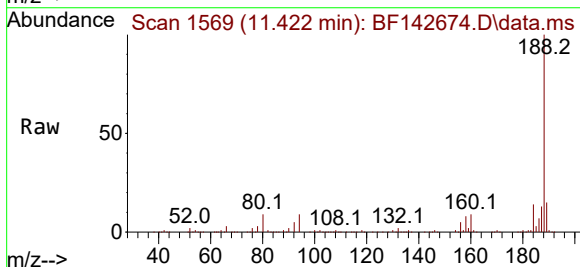


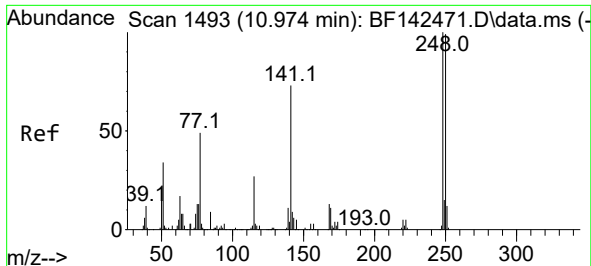

#67
4-Bromophenyl-phenylether
Concen: 2.457 ng
RT: 10.722 min Scan# 14
Delta R.T. -0.253 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35




Instrument :
BNA_F
ClientSampleId :
TP07-MHH-WC


Tgt Ion:248 Resp: 9119
Ion Ratio Lower Upper
248 100
250 196.5 79.0 118.4#
141 442.9 58.4 87.6#

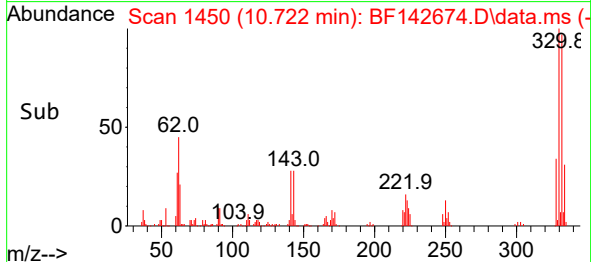

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.063 min Scan# 2018
Delta R.T. -0.012 min
Lab File: BF142674.D
Acq: 07 Jun 2025 06:35

Tgt Ion:240 Resp: 258549
Ion Ratio Lower Upper
240 100
120 11.2 7.5 11.3
236 25.0 19.6 29.4


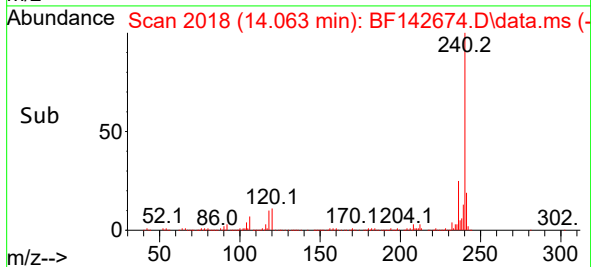

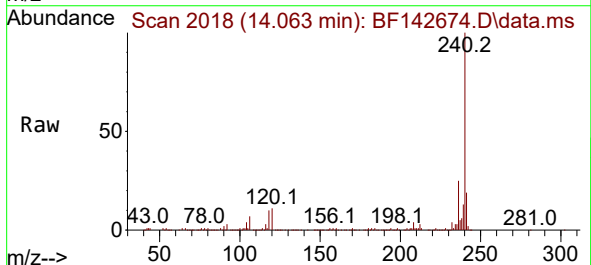


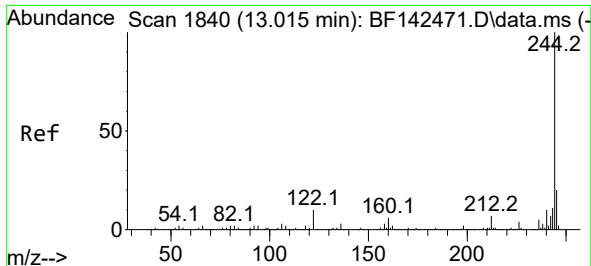

#79
 Terphenyl-d14
 Concen: 29.138 ng
 RT: 13.004 min Scan# 1838
 Delta R.T. -0.012 min
 Lab File: BF142674.D
 Acq: 07 Jun 2025 06:35

Instrument :
 BNA_F
 ClientSampleId :
 TP07-MHH-WC

Tgt Ion:244 Resp: 551285
 Ion Ratio Lower Upper
 244 100
 212 6.3 5.3 7.9
 122 11.1 8.2 12.2

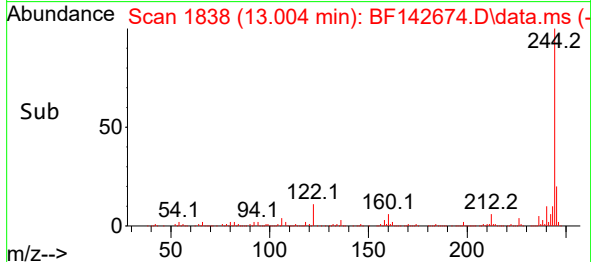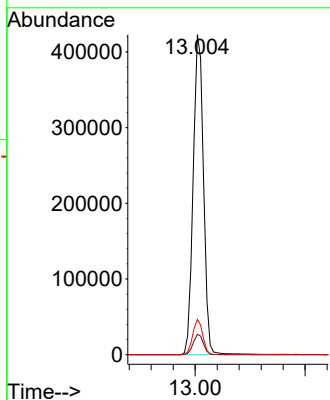

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.557 min Scan# 2272
 Delta R.T. -0.012 min
 Lab File: BF142674.D
 Acq: 07 Jun 2025 06:35

Tgt Ion:264 Resp: 270848
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.6 28.0
 265 21.2 17.7 26.5

