
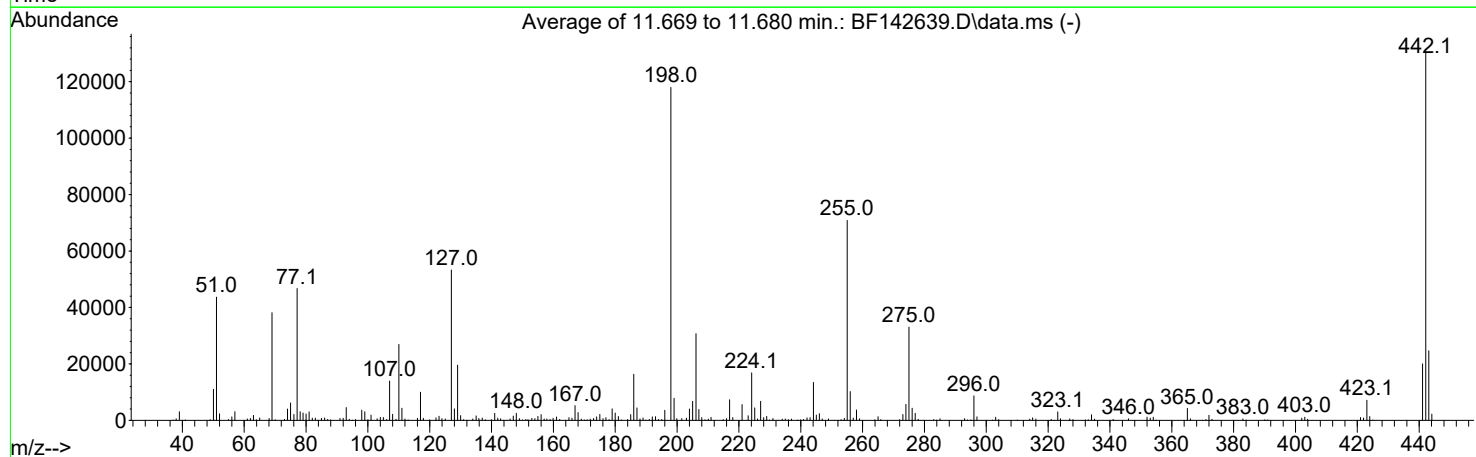


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
Data File : BF142639.D
Acq On : 06 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

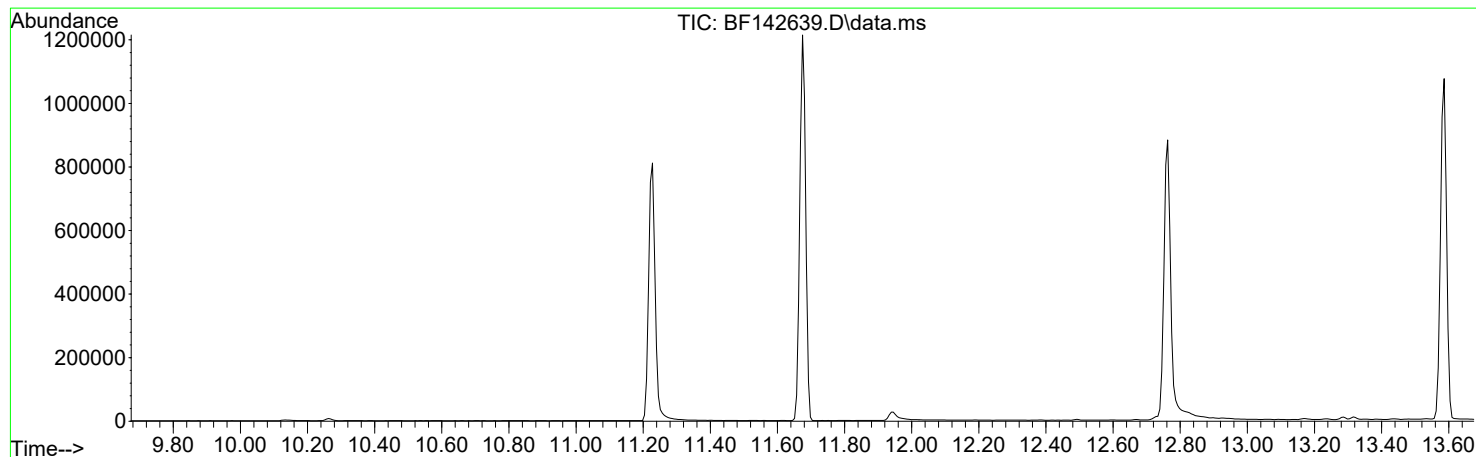

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	37.0	43683	PASS
68	69	0.00	2	1.8	699	PASS
69	198	0.00	100	32.3	38139	PASS
70	69	0.00	2	0.6	236	PASS
127	198	10	80	45.2	53288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117984	PASS
199	198	5	9	6.6	7844	PASS
275	198	10	60	28.0	33067	PASS
365	198	1	100	3.6	4253	PASS
441	198	0.01	100	17.0	20023	PASS
442	442	50	100	100.0	130333	PASS
443	442	15	24	18.9	24653	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2025	BNA_F	<u>BF142639.D</u>
Compound Name	Response	Retention Time
DDT	279400	13.586
DDD	5638	13.286
DDE	586	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6224	285624	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
Data File : BF142639.D
Acq On : 06 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 06 12:07:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

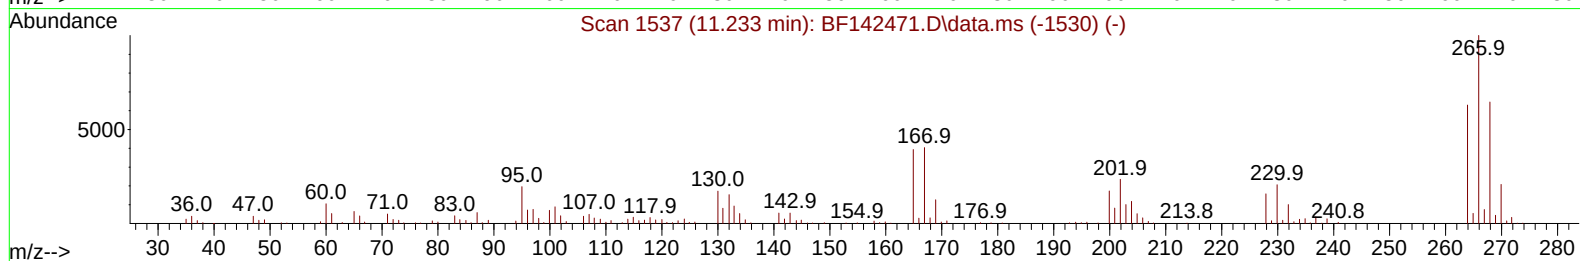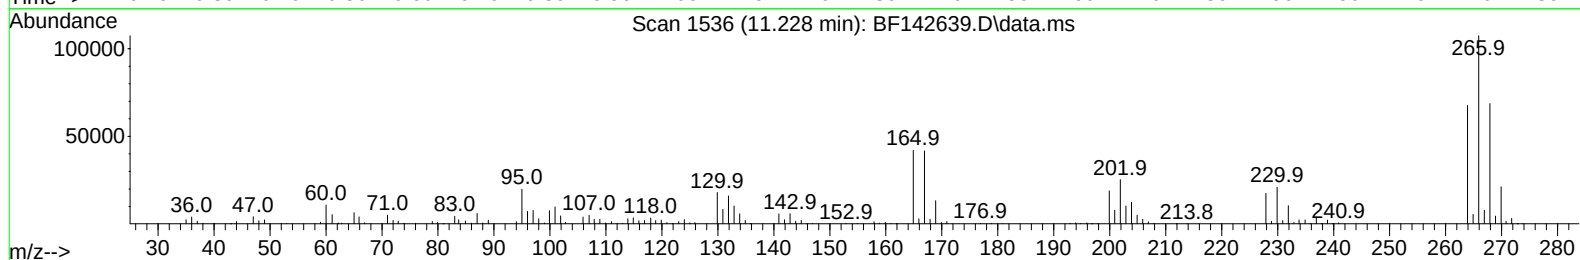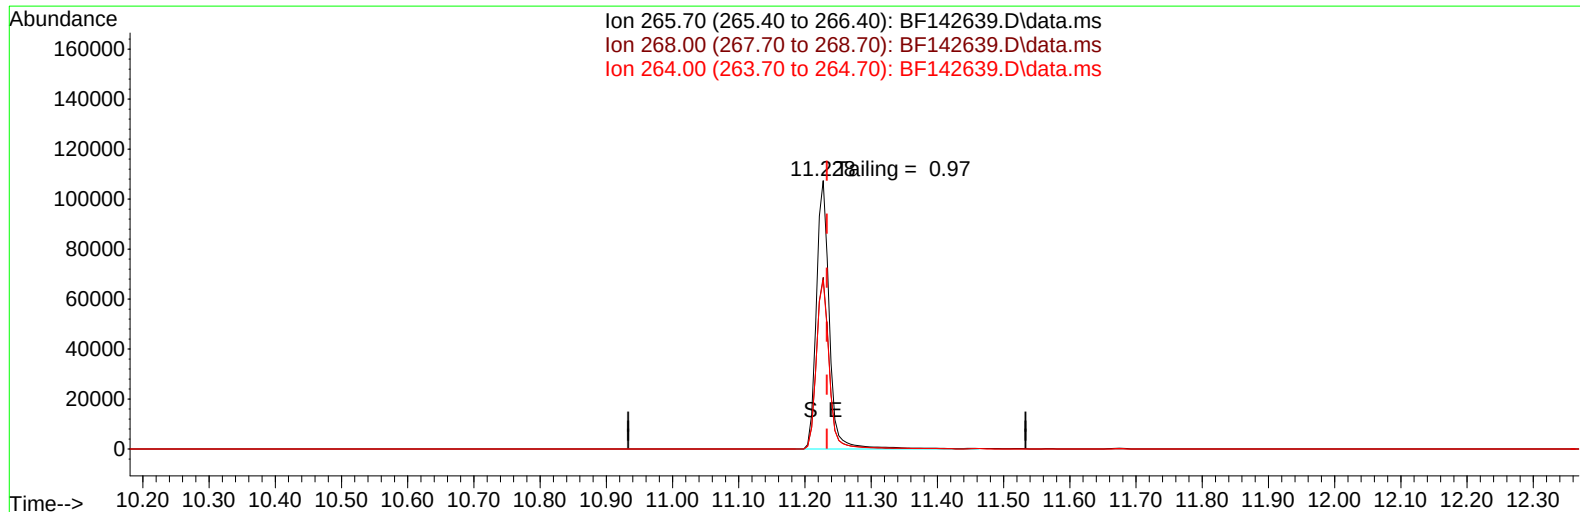

TIC: BF142639.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.006) 29628.01 ng




response 145695

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.93
264.00	63.00	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
Data File : BF142639.D
Acq On : 06 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 06 12:07:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

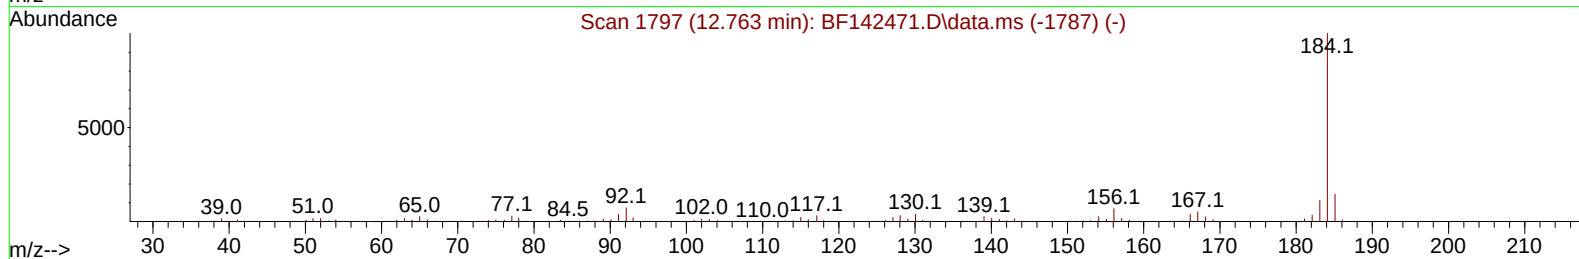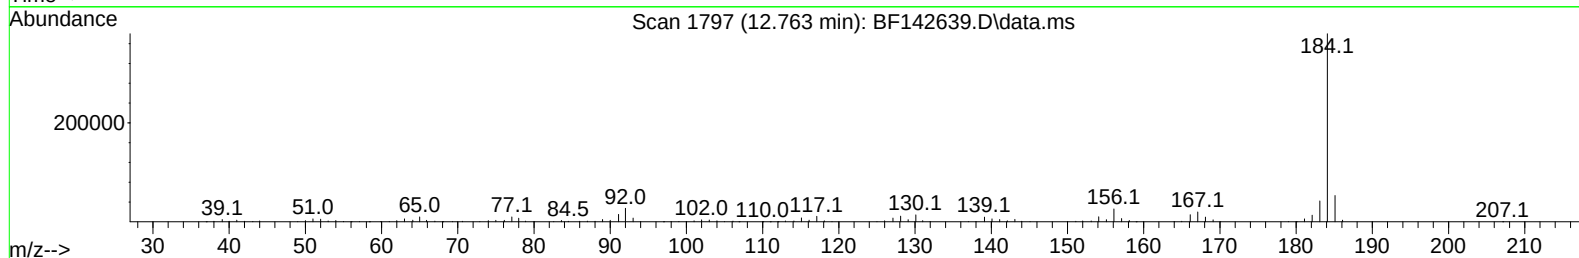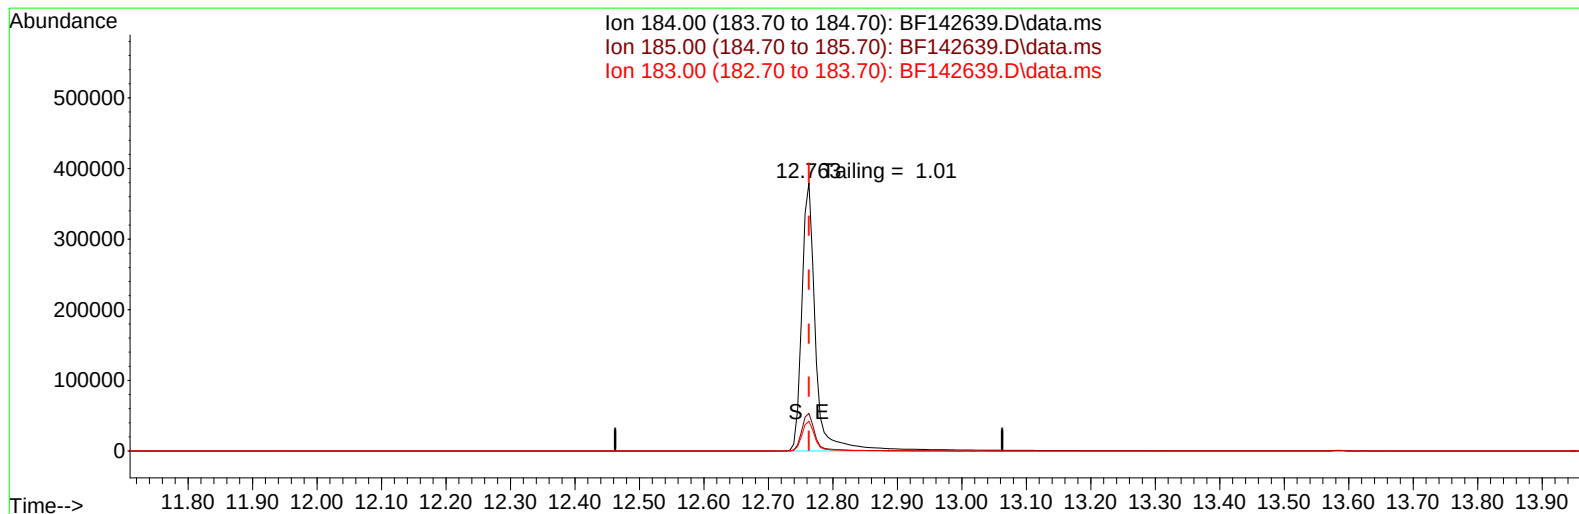

TIC: BF142639.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 566505

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.01
183.00	11.20	11.13
0.00	0.00	0.00