
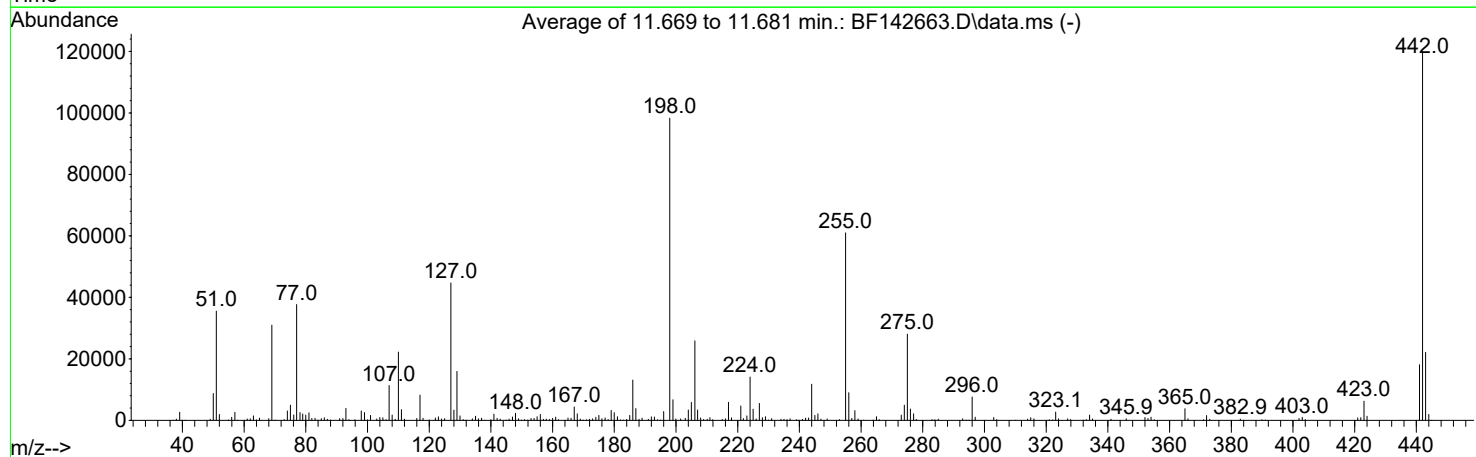


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
Data File : BF142663.D
Acq On : 07 Jun 2025 00:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

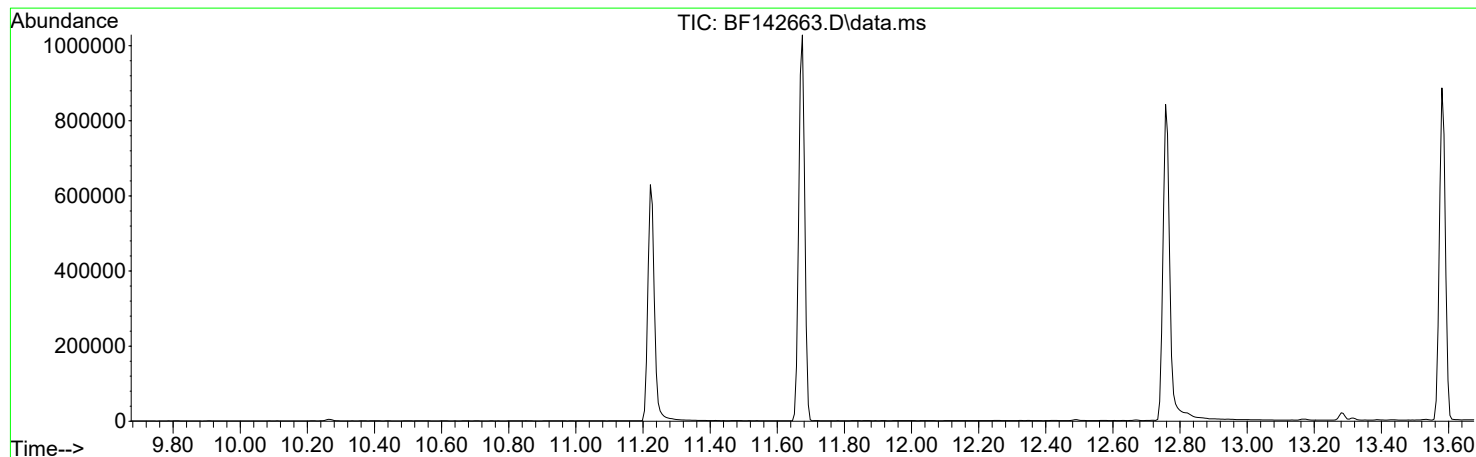

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	35552	PASS
68	69	0.00	2	1.9	577	PASS
69	198	0.00	100	31.5	30987	PASS
70	69	0.00	2	0.4	125	PASS
127	198	10	80	45.5	44688	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98304	PASS
199	198	5	9	6.8	6697	PASS
275	198	10	60	28.5	28053	PASS
365	198	1	100	3.9	3795	PASS
441	198	0.01	100	18.4	18134	PASS
442	442	50	100	100.0	119651	PASS
443	442	15	24	18.5	22107	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2025	BNA_F	<u>BF142663.D</u>
Compound Name	Response	Retention Time
DDT	227515	13.58
DDD	8386	13.28
DDE	397	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8783	236298	3.72

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060625\
Data File : BF142663.D
Acq On : 07 Jun 2025 00:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 04:18:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

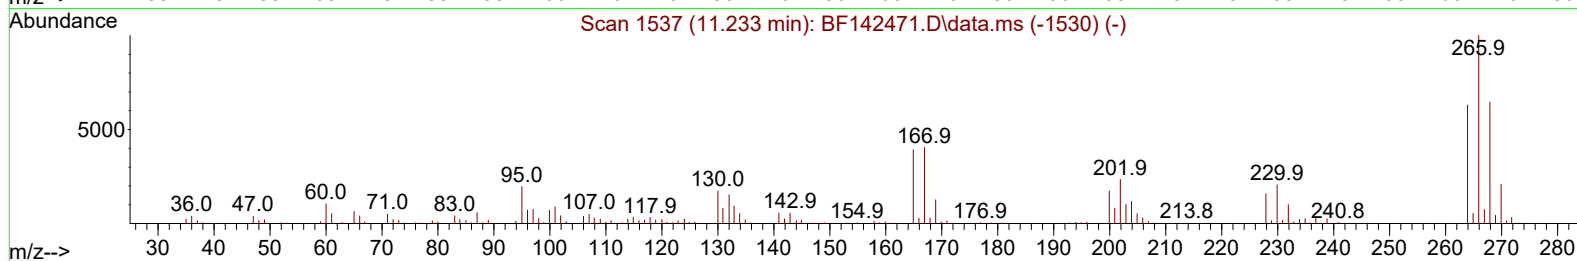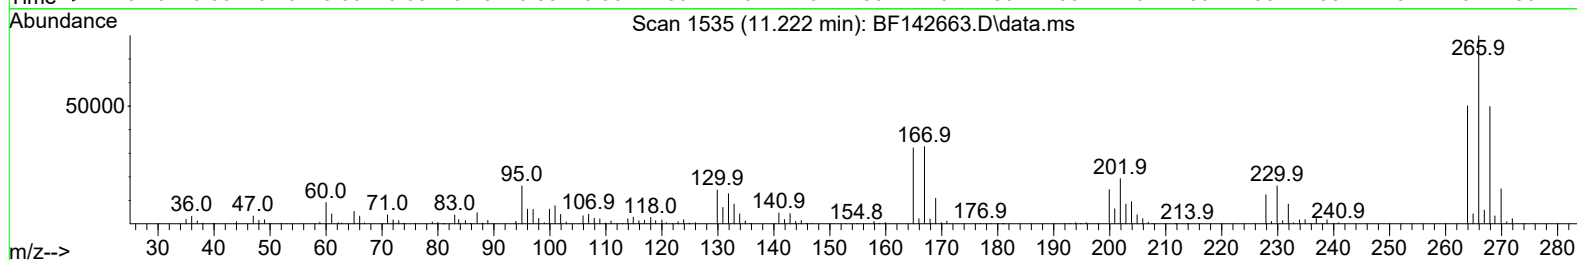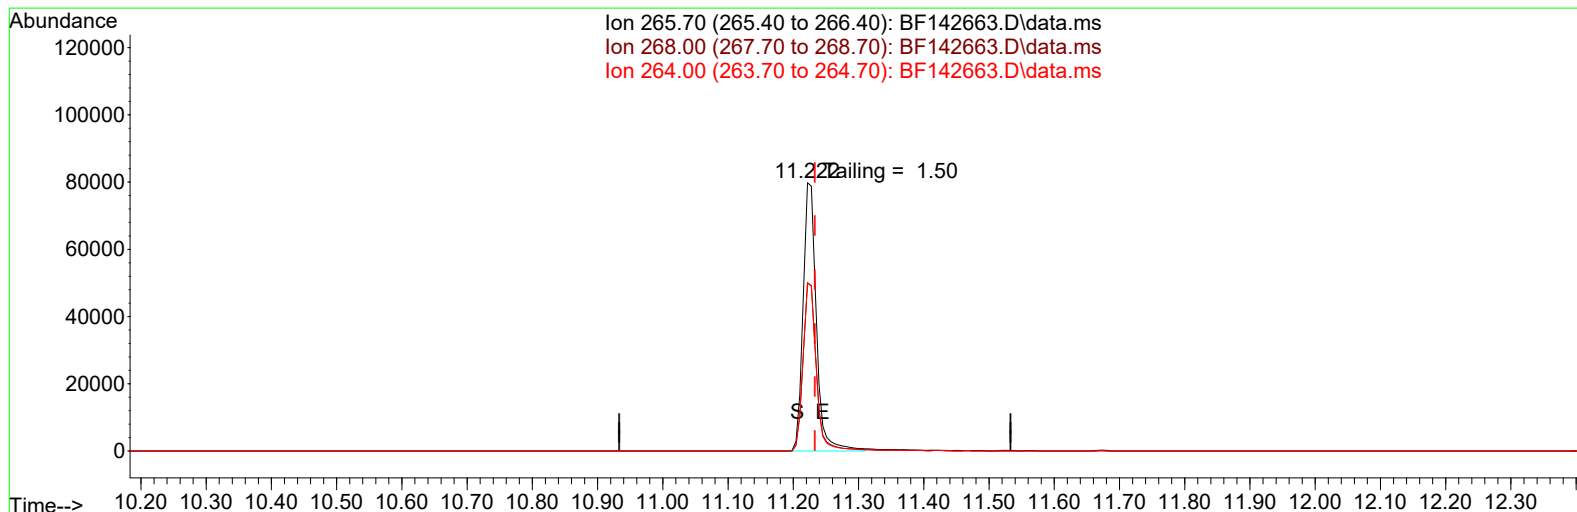

TIC: BF142663.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.011) 33068.85 ng

response 115491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	62.43
264.00	63.00	62.84
0.00	0.00	0.00

BNA F

ClientSampleId :

DFTPP


Quant Time: Jun 07 04:18:30 2025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue May 20 16:26:47 2025

Response via : Initial Calibration




Ion 185.00 (184.70 to 185.70): BF142663.D\data.ms

Ion 183.00 (182.70 to 183.70): BF142663.D\data.ms

$$12.75 \text{ trailing} = 1.41$$

S E

E



184.1

Scan 1797 (12.763 min): BF142471.D\data.ms (-1787) (-)

184.1



12.757min (-0.006) 0.00 ng

response **539096**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.50	14.31
--------	-------	-------

183.00	11.20	11.17
--------	-------	-------

0.00 0.00 0.00