

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
 Data File : BF133618.D
 Acq On : 07 Jun 2023 10:58
 Operator : CG\JU
 Sample : PB153236BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153236BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	501	508	515	rBV	40174	59240	1.28%	0.222%
2	5.457	567	573	576	rBV	3162191	3411081	73.85%	12.772%
3	6.463	738	744	747	rBV	2859181	3495448	75.67%	13.088%
4	6.834	803	807	811	rBV	906659	716868	15.52%	2.684%
5	7.404	897	904	907	rBV	2162223	2272982	49.21%	8.511%
6	8.116	1020	1025	1029	rBV	1060528	938838	20.33%	3.515%
7	9.198	1203	1209	1212	rBV	4376189	3981999	86.21%	14.910%
8	9.875	1320	1324	1328	rBV	1340251	1055450	22.85%	3.952%
9	10.669	1454	1459	1462	rBV	2947768	2747204	59.47%	10.286%
10	11.363	1573	1577	1581	rBV	1453996	1203603	26.06%	4.507%
11	12.963	1843	1849	1852	rBV	4435578	4619107	100.00%	17.295%
12	14.010	2023	2027	2031	rBV	1272445	1120200	24.25%	4.194%
13	15.474	2271	2276	2281	rBV	857737	1085575	23.50%	4.065%




Sum of corrected areas: 26707595

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
Data File : BF133618.D
Acq On : 07 Jun 2023 10:58
Operator : CG\JU
Sample : PB153236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153236BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

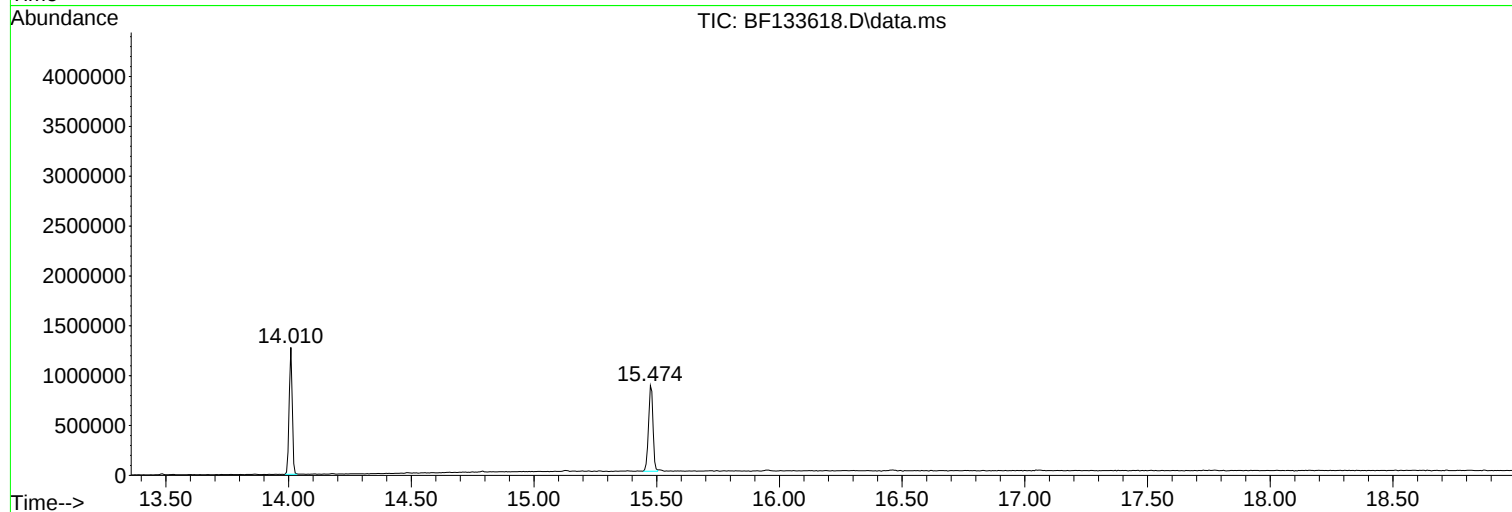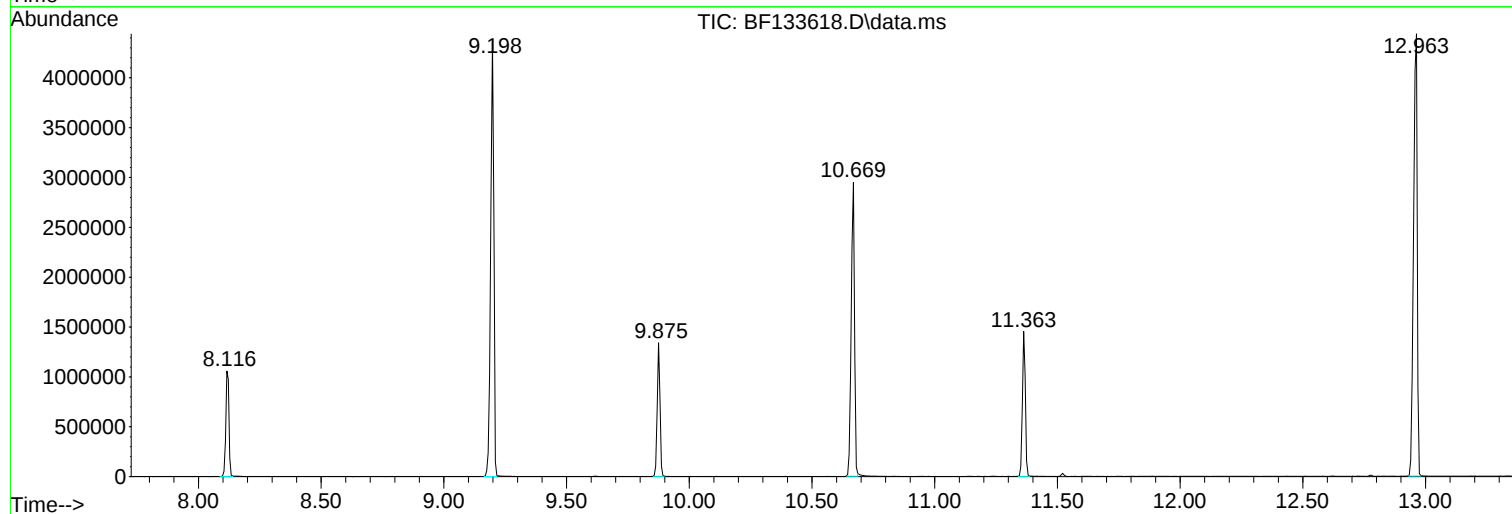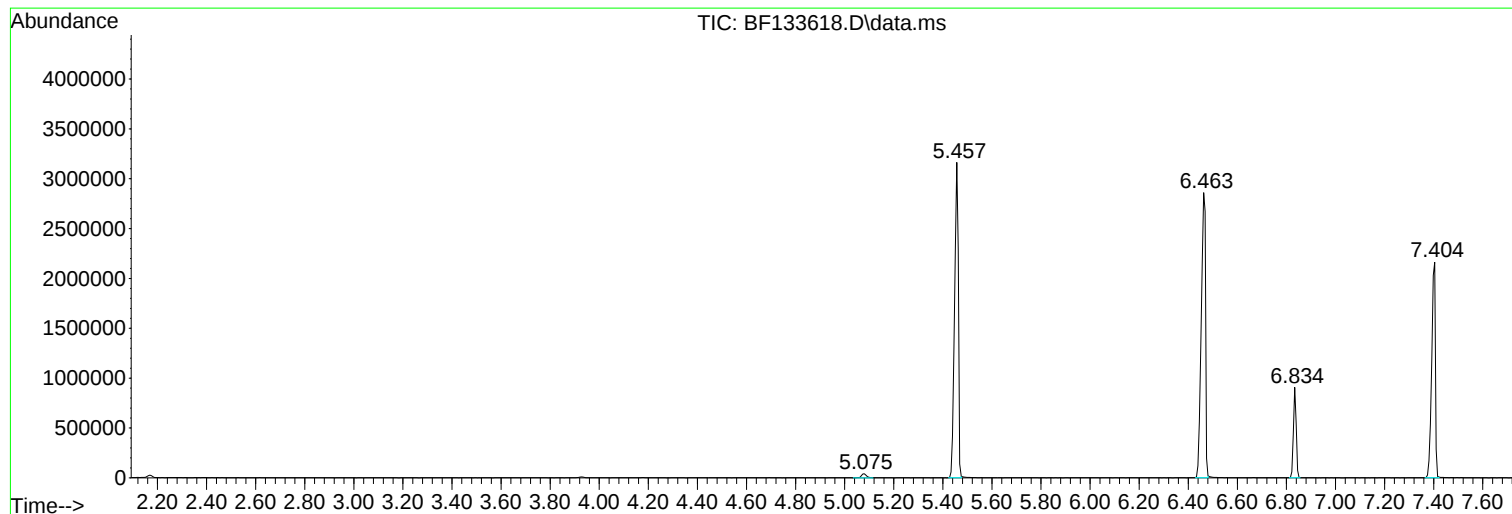

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
Data File : BF133618.D
Acq On : 07 Jun 2023 10:58
Operator : CG\JU
Sample : PB153236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153236BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
Data File : BF133618.D
Acq On : 07 Jun 2023 10:58
Operator : CG\JU
Sample : PB153236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153236BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------