


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
 Data File : BF133616.D
 Acq On : 07 Jun 2023 09:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 07 11:27:15 2023

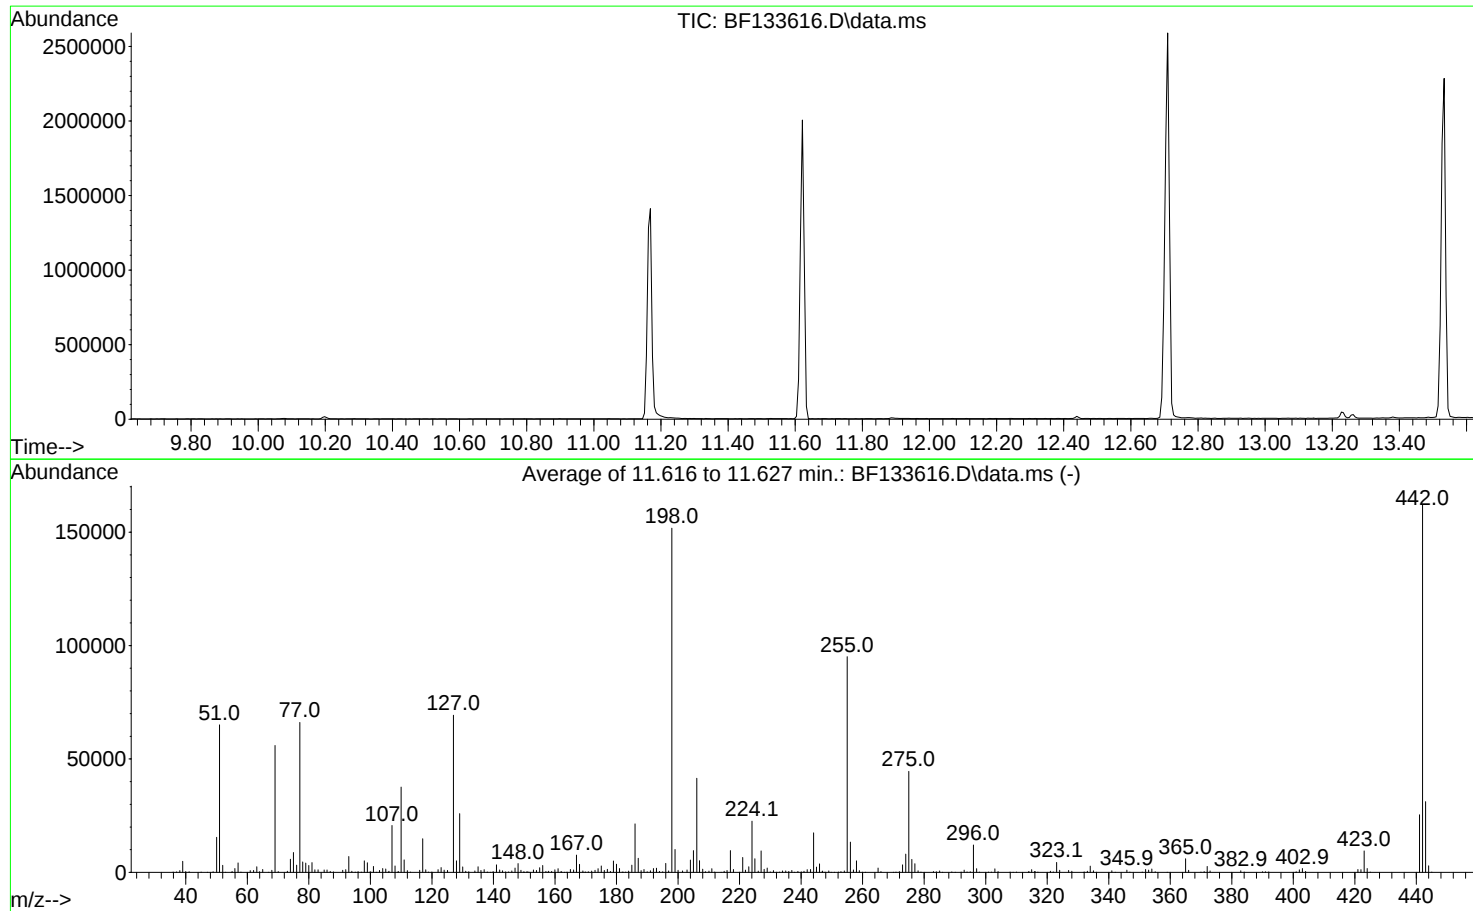

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	65020	PASS
68	69	0.00	2	1.7	926	PASS
69	198	0.00	100	36.9	55965	PASS
70	69	0.00	2	0.6	362	PASS
127	198	10	80	45.7	69309	PASS
197	198	0.00	2	0.4	613	PASS
198	198	100	100	100.0	151771	PASS
199	198	5	9	6.6	10070	PASS
275	198	10	60	29.4	44552	PASS
365	198	1	100	4.0	6033	PASS
441	198	0.01	100	16.7	25420	PASS
442	442	50	100	100.0	162195	PASS
443	442	15	24	19.2	31209	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/7/2023	BNA_F	<u>BF133616.D</u>
Compound Name	Response	Retention Time
DDT	395907	13.533
DDD	11588	13.233
DDE	272	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11860	407767	2.91

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
Data File : BF133616.D
Acq On : 07 Jun 2023 09:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 11:07:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 14:05:12 2023
Response via : Initial Calibration

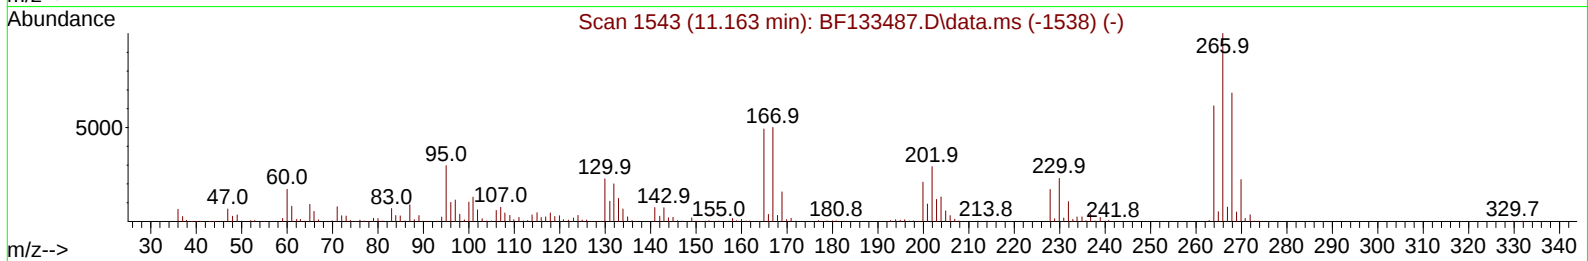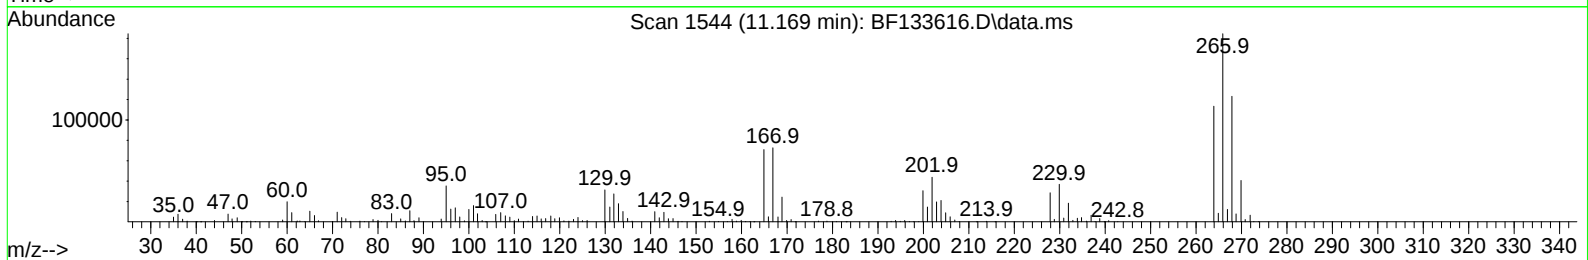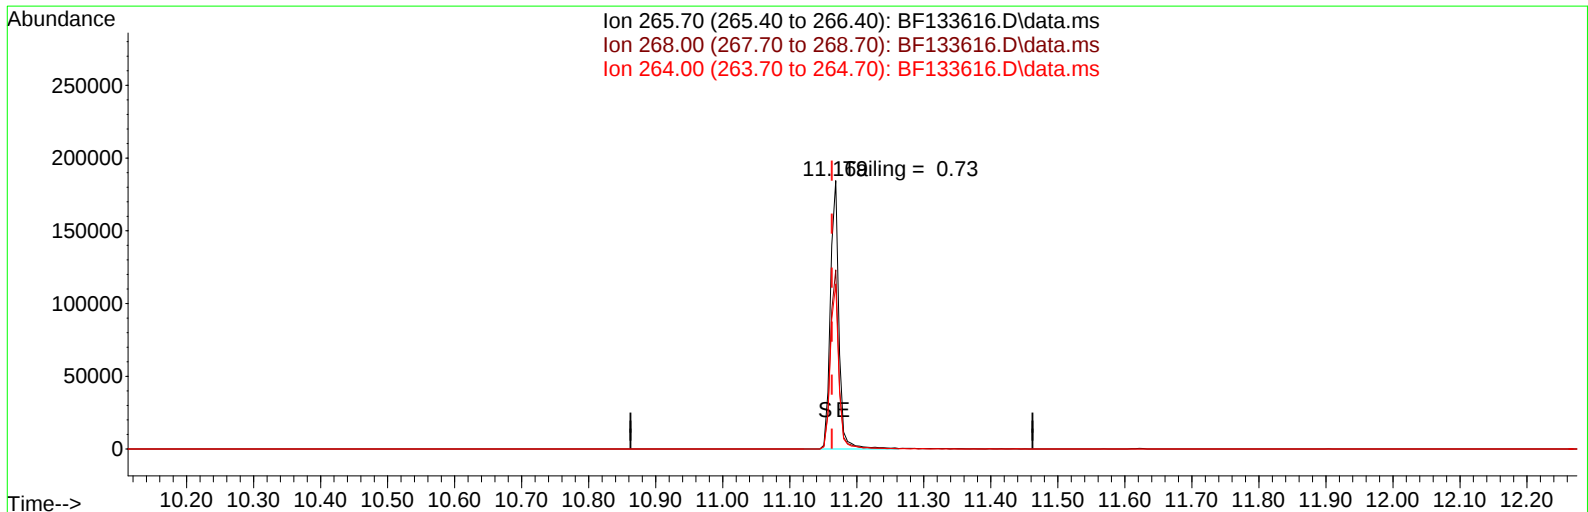

TIC: BF133616.D\data.ms

(70) Pentachlorophenol (C)

11.169min (+ 0.006) 105508.54 ng




response 164648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	66.72
264.00	61.50	61.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060723\
Data File : BF133616.D
Acq On : 07 Jun 2023 09:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 11:07:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 14:05:12 2023
Response via : Initial Calibration

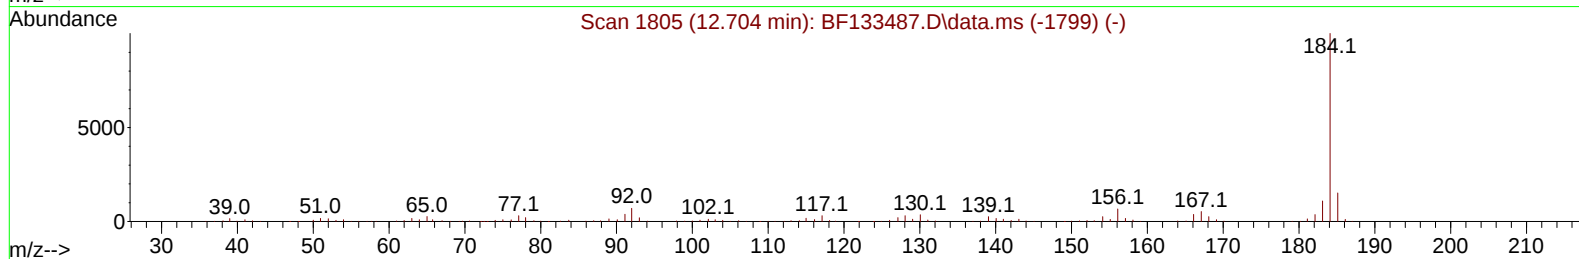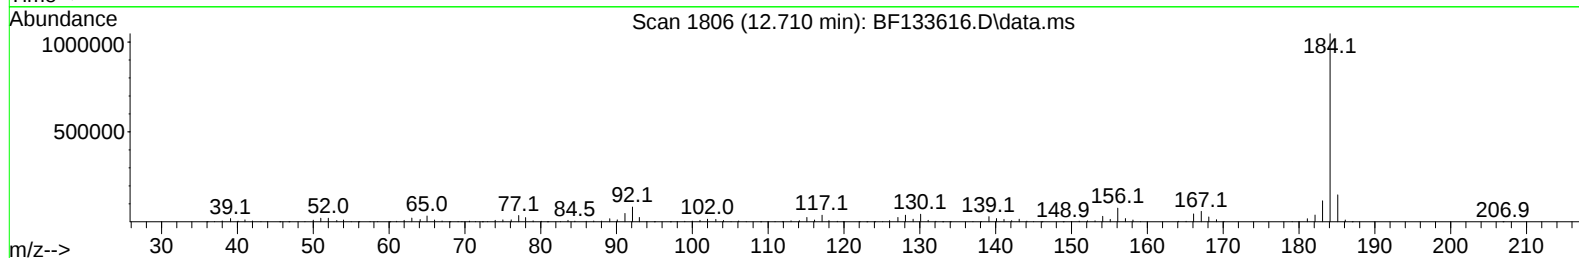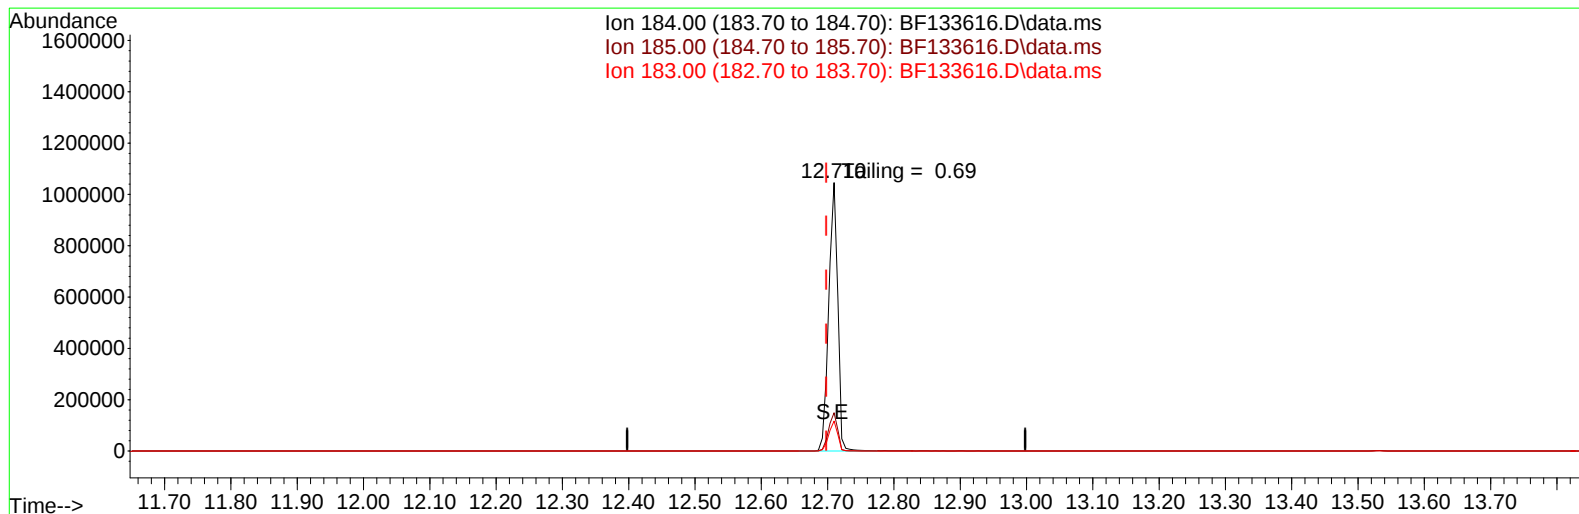

TIC: BF133616.D\data.ms

(77) Benzidine

12.710min (+ 0.012) 121954.46 ng m

response 988025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.28
183.00	10.90	11.14
0.00	0.00	0.00