
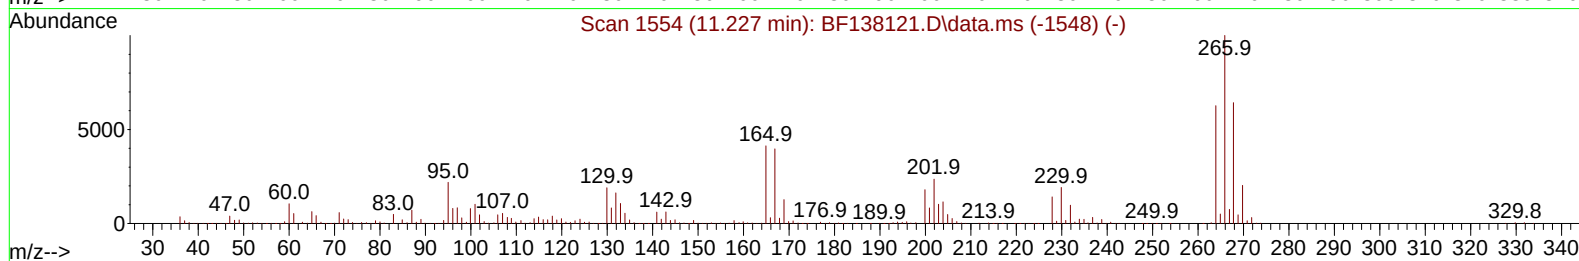
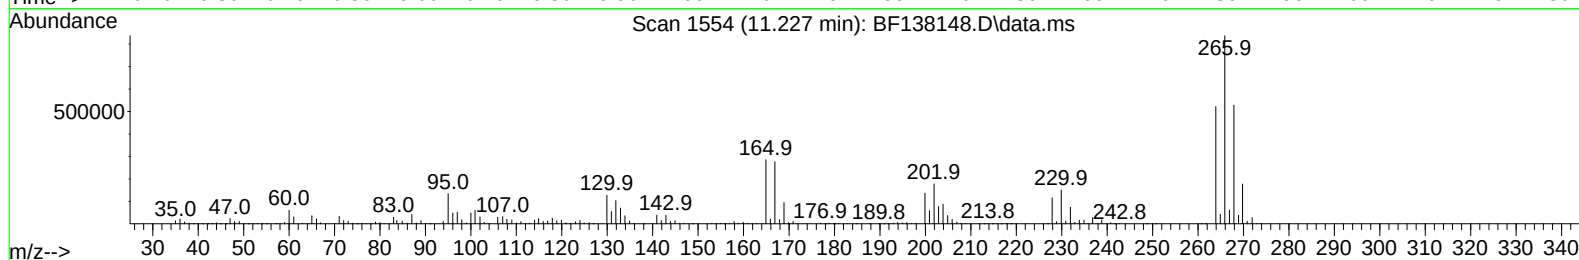


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138148.D
Acq On : 07 Jun 2024 09:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 12:46:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

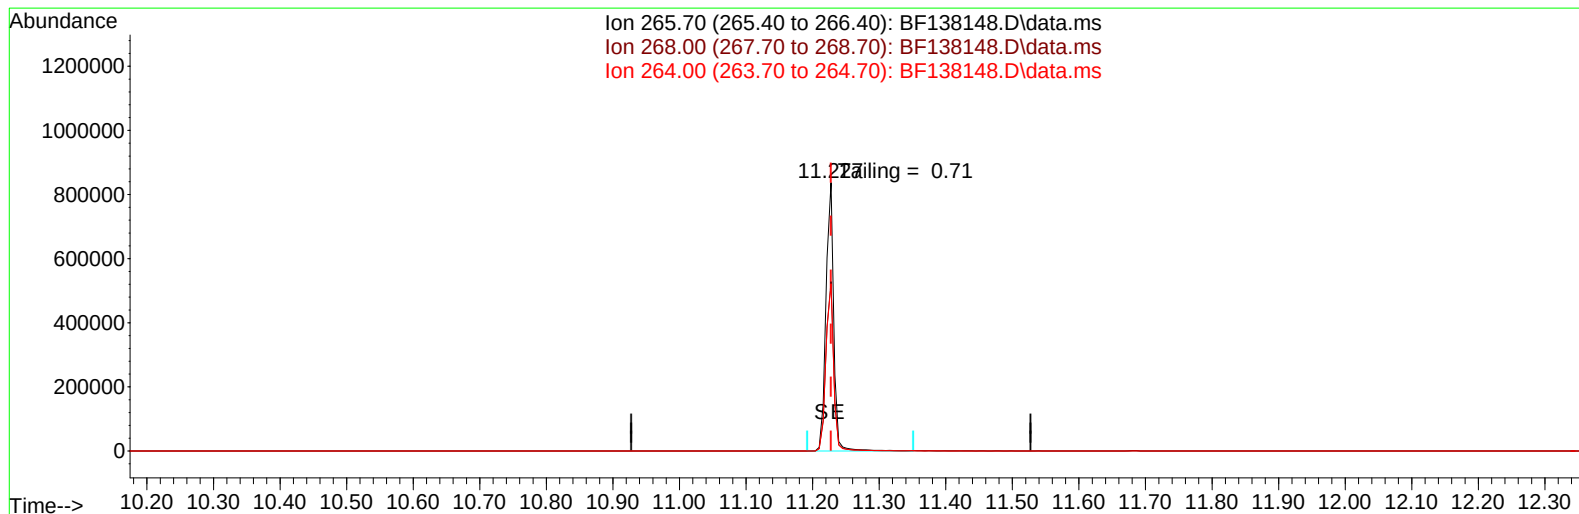

TIC: BF138148.D\data.ms

(70) Pentachlorophenol (C)




11.227min (+ 0.000) 555959.62 ng

response 681542

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.09
264.00	62.60	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138148.D
Acq On : 07 Jun 2024 09:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 12:46:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

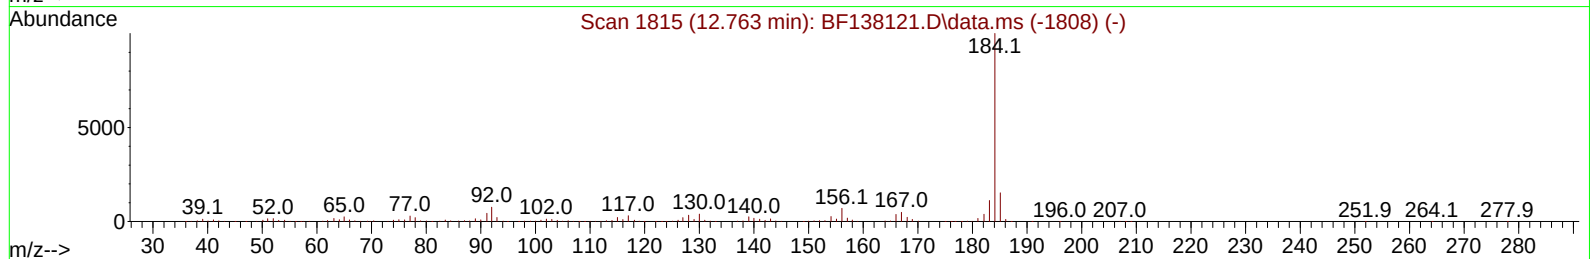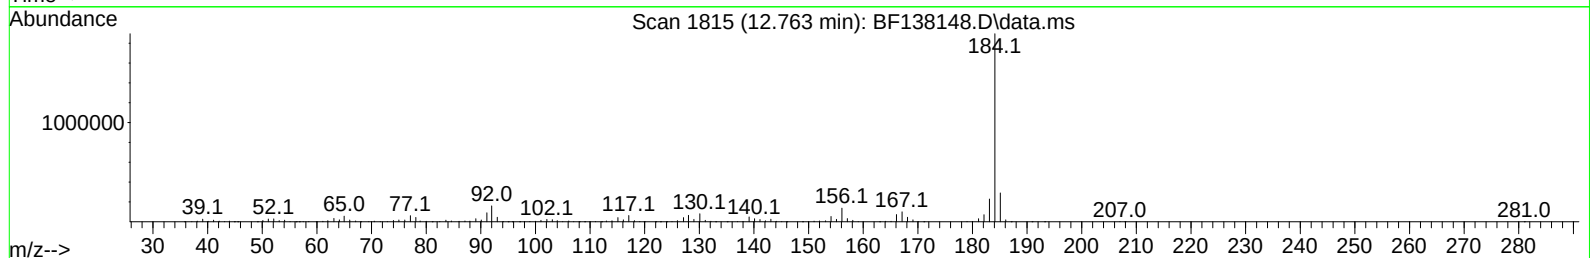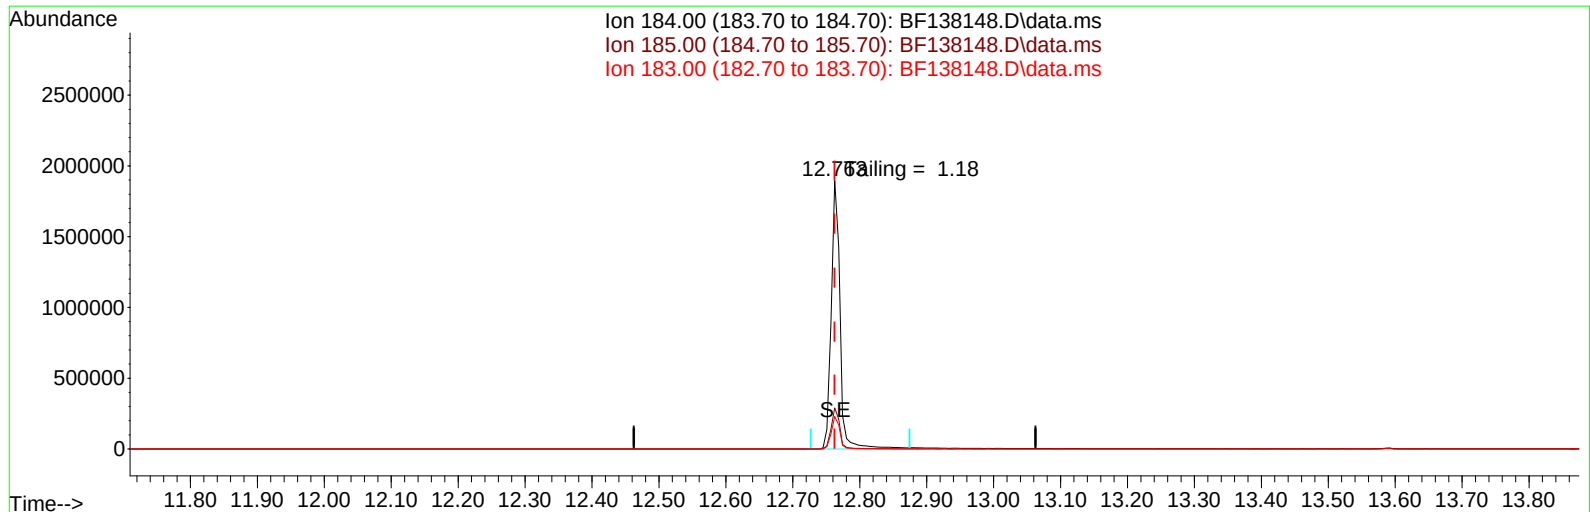

TIC: BF138148.D\data.ms

(77) Benzidine**12.763min (+ 0.000) 146941.18 ng****response 1746493**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.33
183.00	11.20	12.09
0.00	0.00	0.00