

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
 Data File : BF138153.D
 Acq On : 07 Jun 2024 11:33
 Operator : CG\JU
 Sample : PB161307BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB161307BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.316	34	39	45	rVB	190578	269609	1.95%	0.353%
2	2.428	52	58	67	rVB	109156	148869	1.08%	0.195%
3	5.540	581	587	590	rBV	8721276	9716427	70.31%	12.718%
4	6.534	749	756	759	rBV	8307292	9596800	69.45%	12.561%
5	6.904	815	819	822	rBV	2852193	2151218	15.57%	2.816%
6	7.469	909	915	918	rBV	6034053	6310312	45.67%	8.259%
7	8.186	1032	1037	1040	rBV	3215133	2868026	20.75%	3.754%
8	9.263	1214	1220	1223	rBV	12264860	12577262	91.02%	16.462%
9	9.939	1329	1335	1338	rBV	4207372	3446697	24.94%	4.511%
10	10.727	1462	1469	1472	rBV	7978823	7708839	55.79%	10.090%
11	11.427	1584	1588	1591	rBV	4190110	3634640	26.30%	4.757%
12	13.016	1853	1858	1861	rBV	12529593	13818593	100.00%	18.087%
13	14.063	2032	2036	2051	rBV	2999300	2595712	18.78%	3.397%
14	15.545	2281	2288	2305	rBV	1158294	1558819	11.28%	2.040%




Sum of corrected areas: 76401823

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138153.D
Acq On : 07 Jun 2024 11:33
Operator : CG\JU
Sample : PB161307BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161307BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

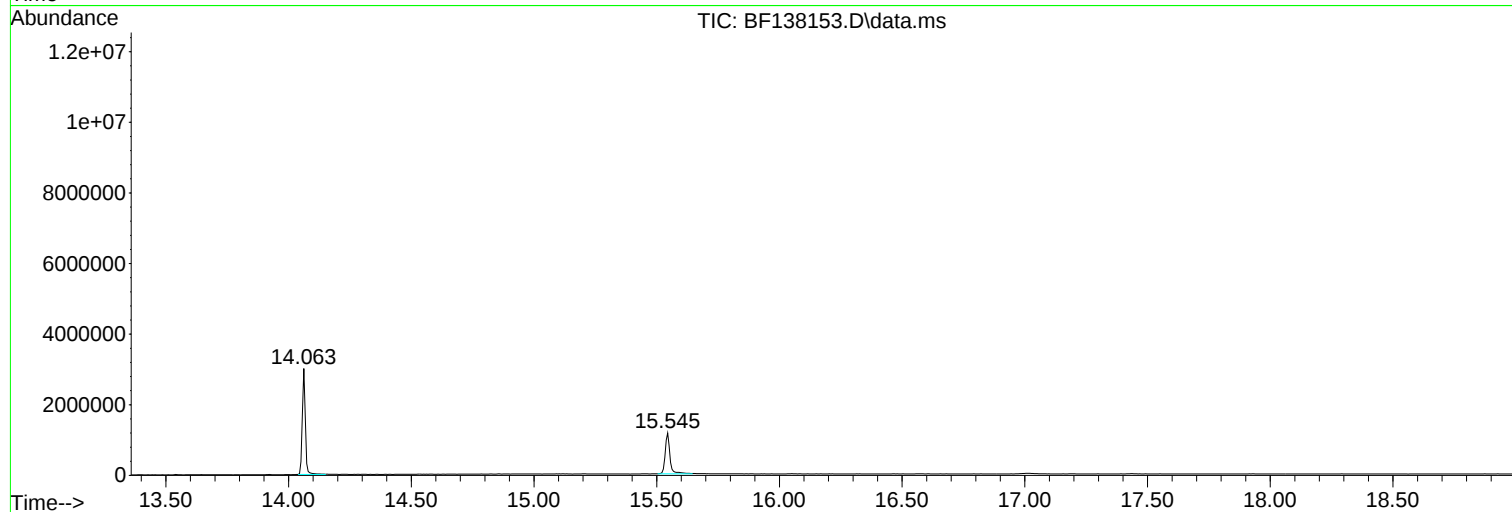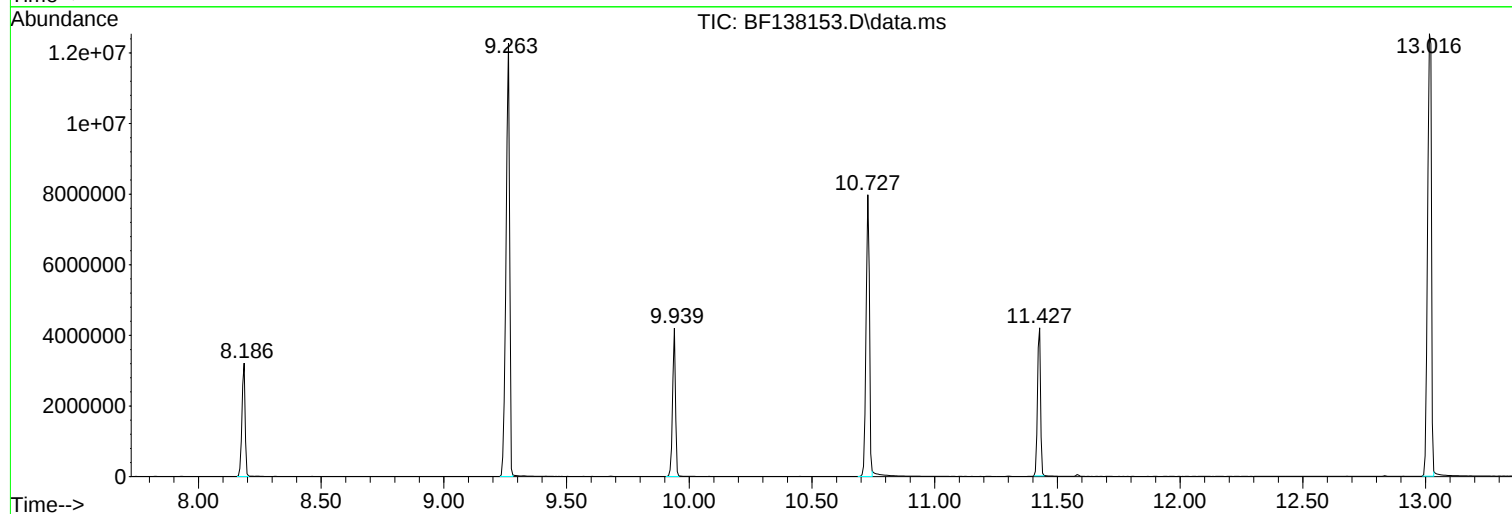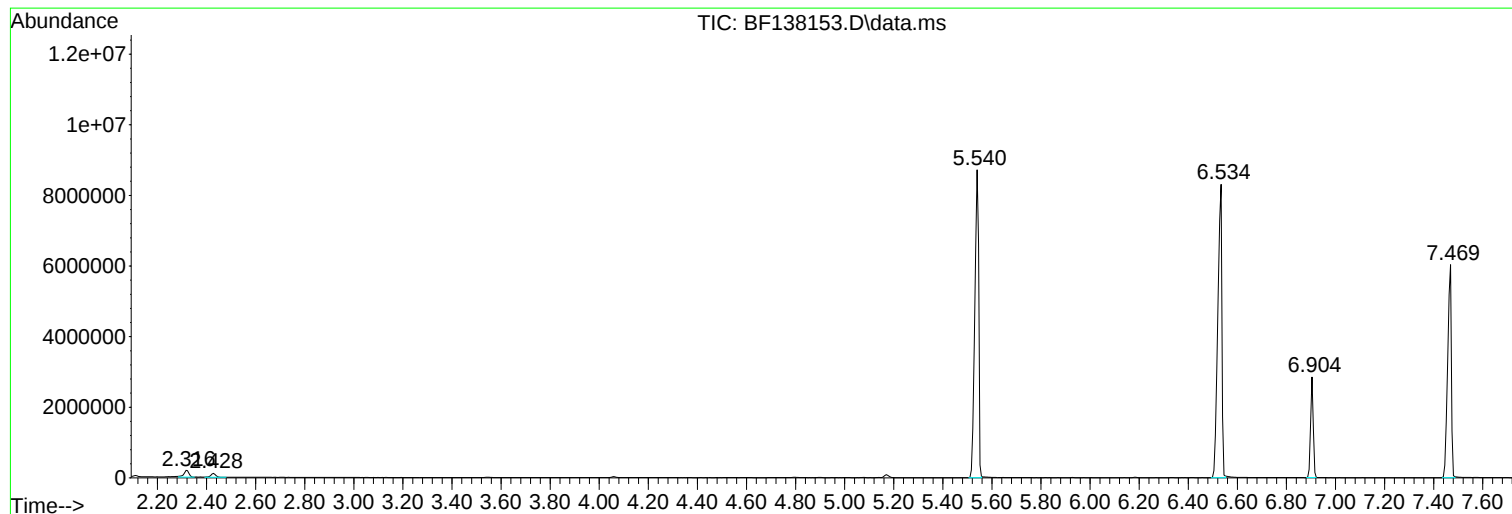

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138153.D
Acq On : 07 Jun 2024 11:33
Operator : CG\JU
Sample : PB161307BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161307BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.316	2.51 ng	269609	1,4-Dichlorobenzene-d4	6.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

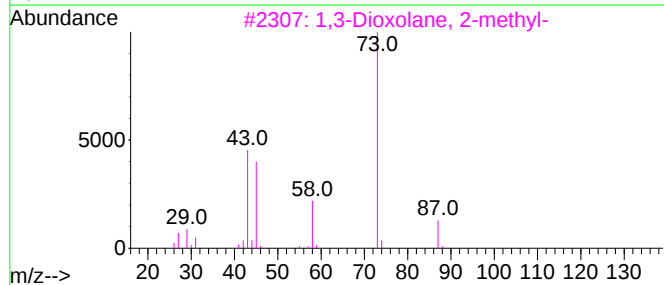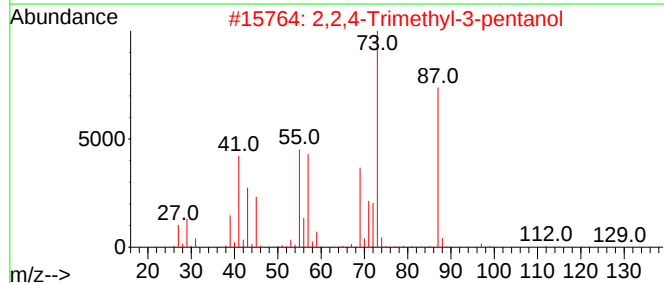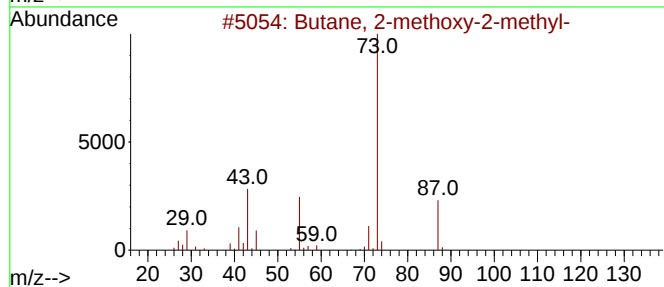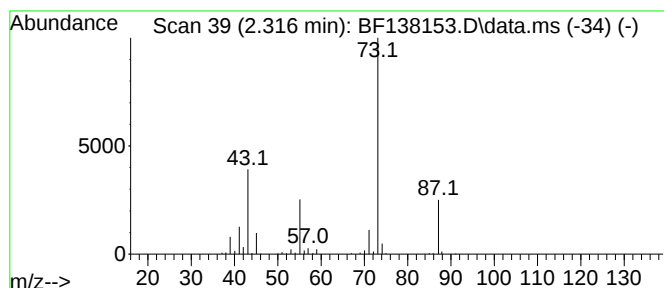

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138153.D
Acq On : 07 Jun 2024 11:33
Operator : CG\JU
Sample : PB161307BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161307BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.316	2.5	ng	269609	1	6.904	2151220	20.0