
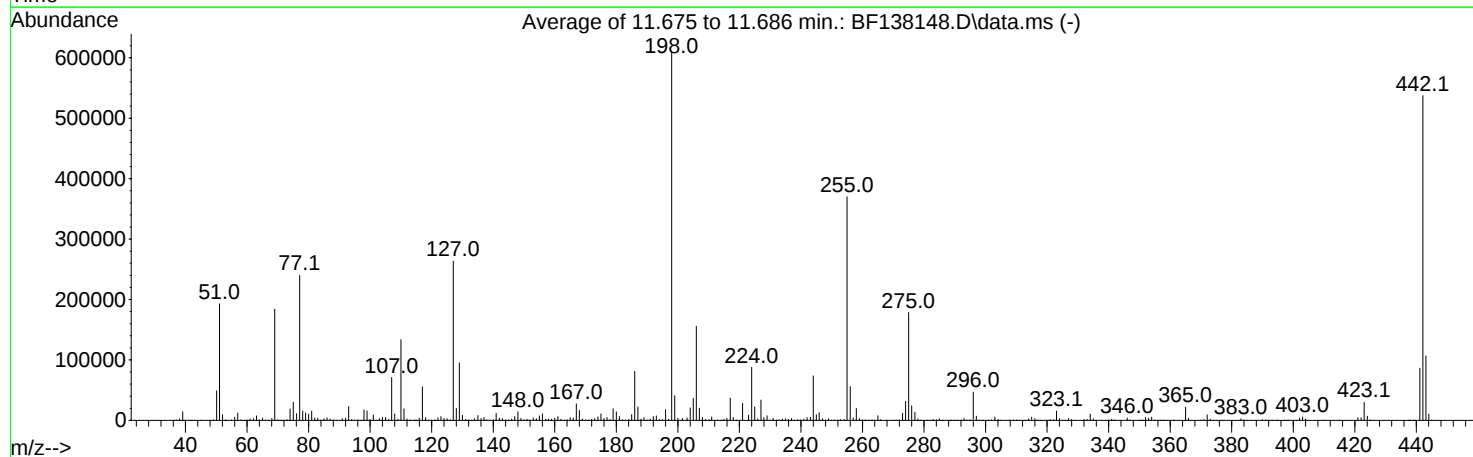


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138148.D
Acq On : 07 Jun 2024 09:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 06 05:19:29 2024

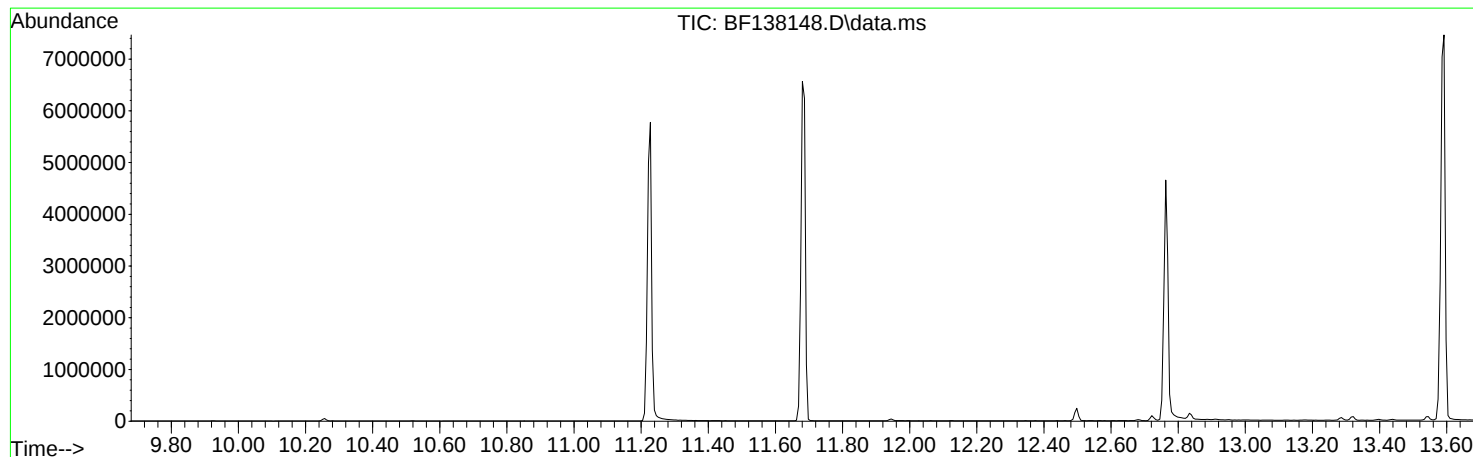




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	192729	PASS
68	69	0.00	2	1.7	3108	PASS
69	198	0.00	100	30.3	184208	PASS
70	69	0.00	2	0.5	1012	PASS
127	198	10	80	43.3	263531	PASS
197	198	0.00	2	0.3	1893	PASS
198	198	100	100	100.0	608853	PASS
199	198	5	9	6.7	40672	PASS
275	198	10	60	29.3	178435	PASS
365	198	1	100	3.6	21750	PASS
441	198	0.01	100	14.2	86493	PASS
442	442	50	100	100.0	537624	PASS
443	442	15	24	19.9	106771	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138148.D
Acq On : 07 Jun 2024 09:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 12:46:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

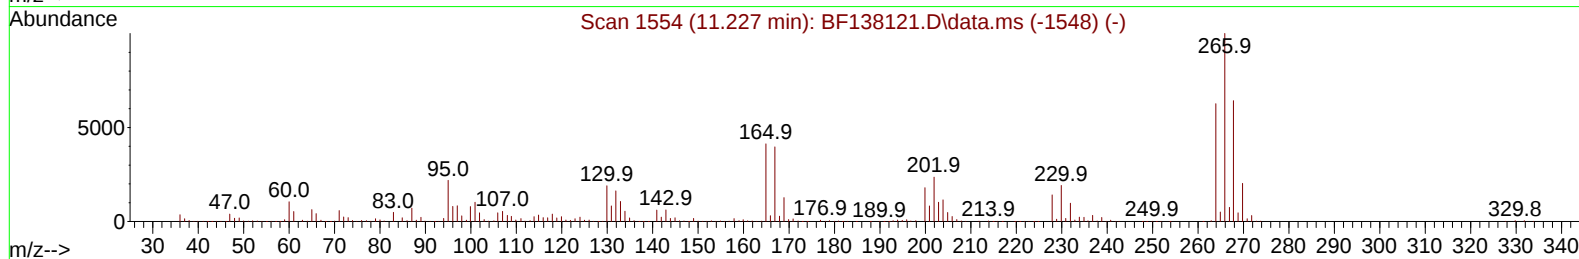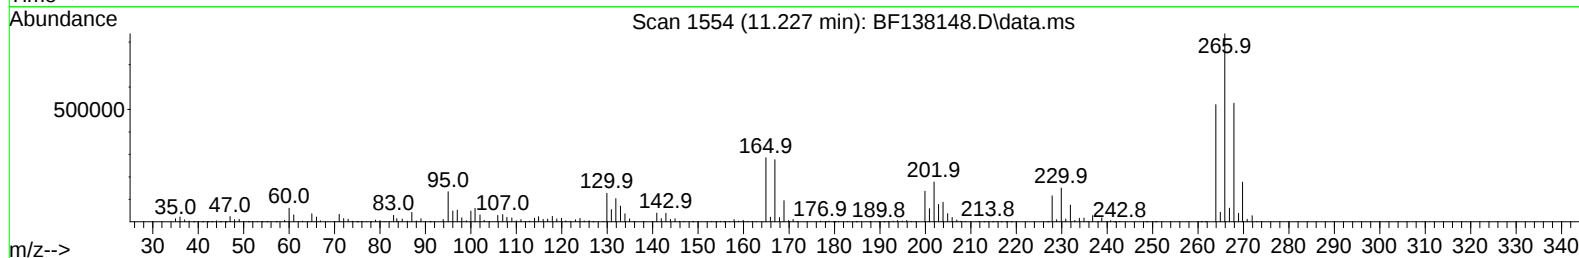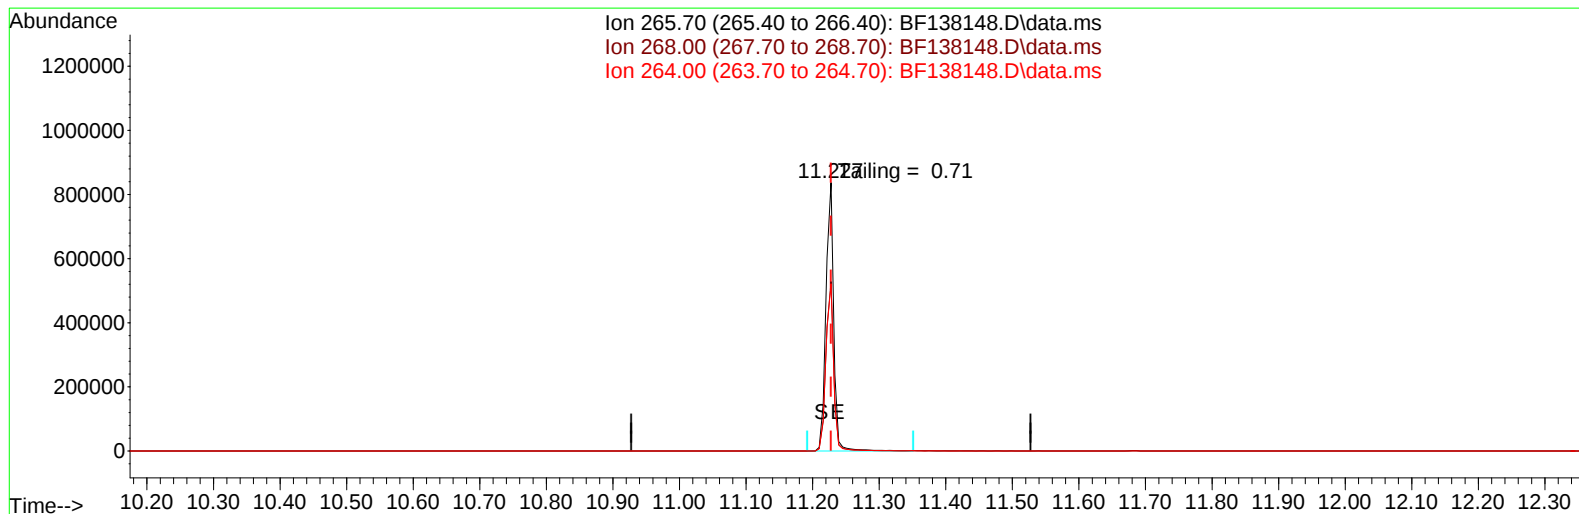

TIC: BF138148.D\data.ms

(70) Pentachlorophenol (C)

11.227min (+ 0.000) 555959.62 ng




response 681542

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.09
264.00	62.60	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060724\
Data File : BF138148.D
Acq On : 07 Jun 2024 09:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 12:46:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

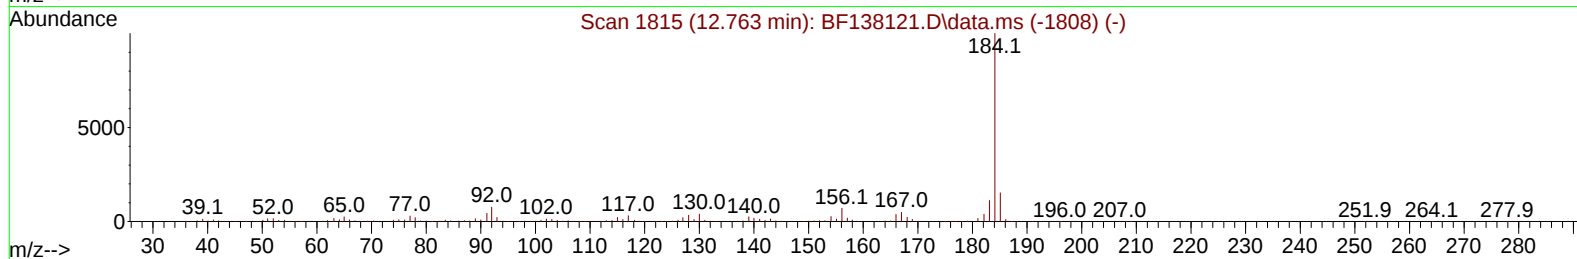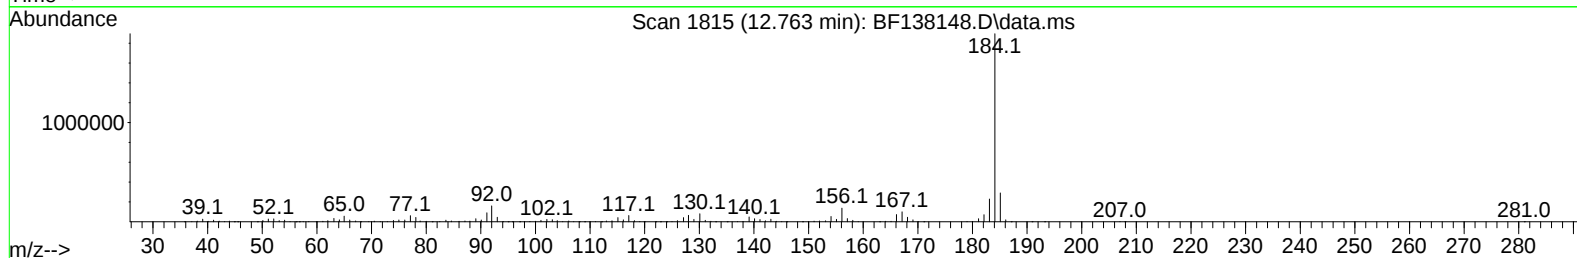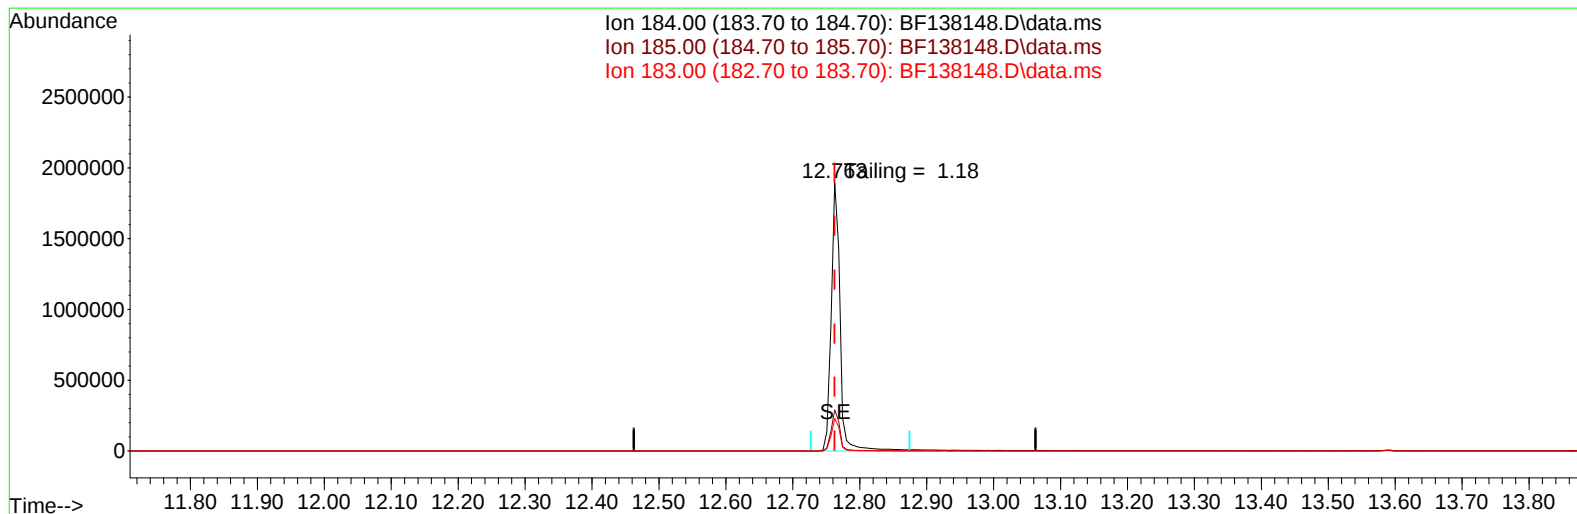

TIC: BF138148.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 146941.18 ng

response 1746493

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.33
183.00	11.20	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2024	BNA_F	<u>BF138148.D</u>
Compound Name	Response	Retention Time
DDT	1359140	13.592
DDD	18840	13.321
DDE	571	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19411	1378551	1.41

Instrument :
BNA_F
ClientSampleId :
DFTPP